


Data Path : Z:\HPCHEM1\BNA F\DATA\BF040416\
 Data File : BF086059.D
 Acq On : 5 Apr 2016 2:48
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 01 23:17:06 2016

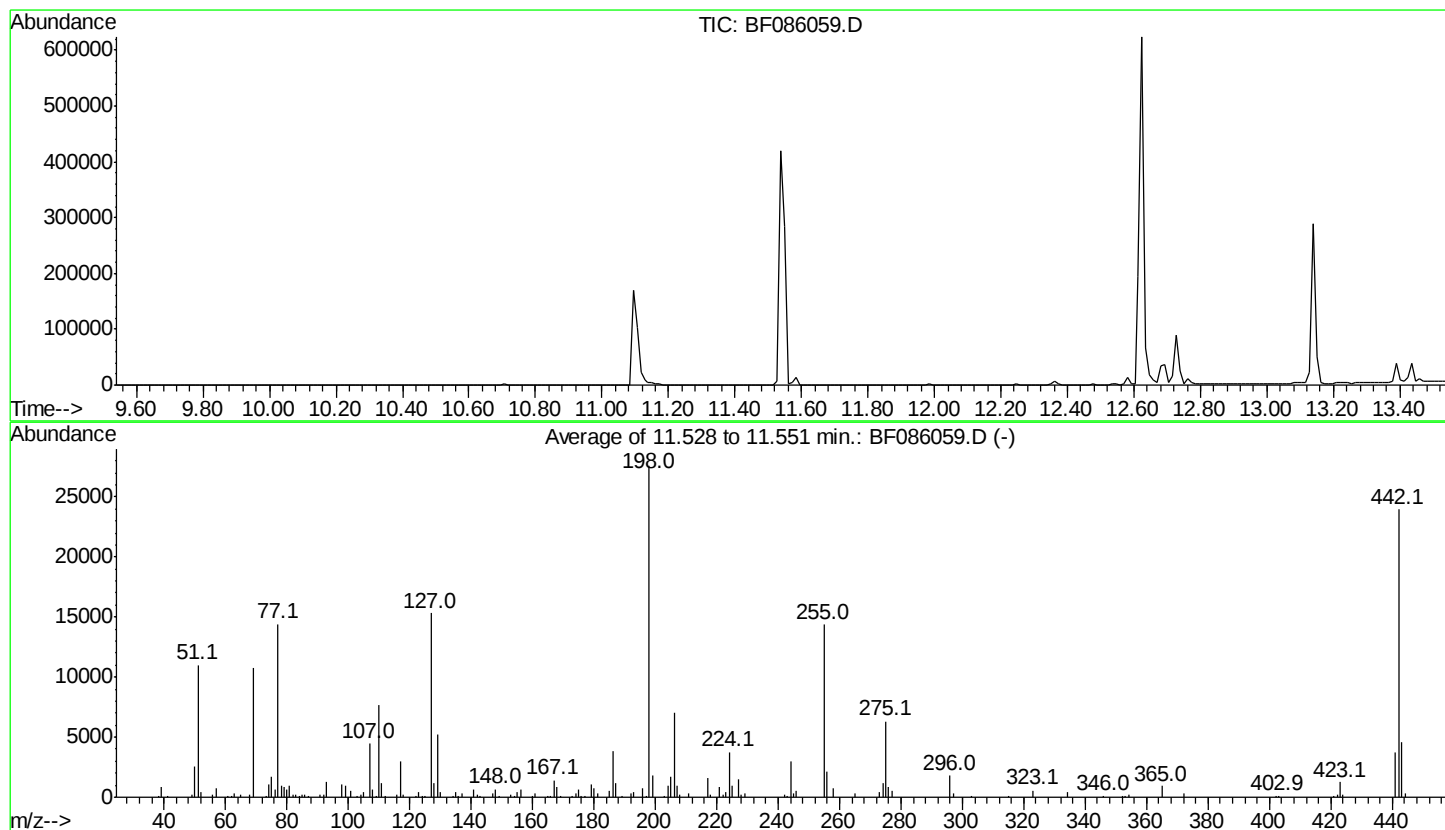

AutoFind: Scans 826, 827, 828; Background Corrected with Scan 823

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.8	10977	PASS
68	69	0.00	2	1.7	182	PASS
69	198	0.00	100	38.8	10711	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	55.5	15305	PASS
197	198	0.00	2	0.5	140	PASS
198	198	100	100	100.0	27597	PASS
199	198	5	9	6.7	1855	PASS
275	198	10	60	22.8	6301	PASS
365	198	1	100	3.4	947	PASS
441	442	0.01	24	15.7	3769	PASS
442	198	50	100	86.8	23964	PASS
443	442	15	24	19.1	4578	PASS