
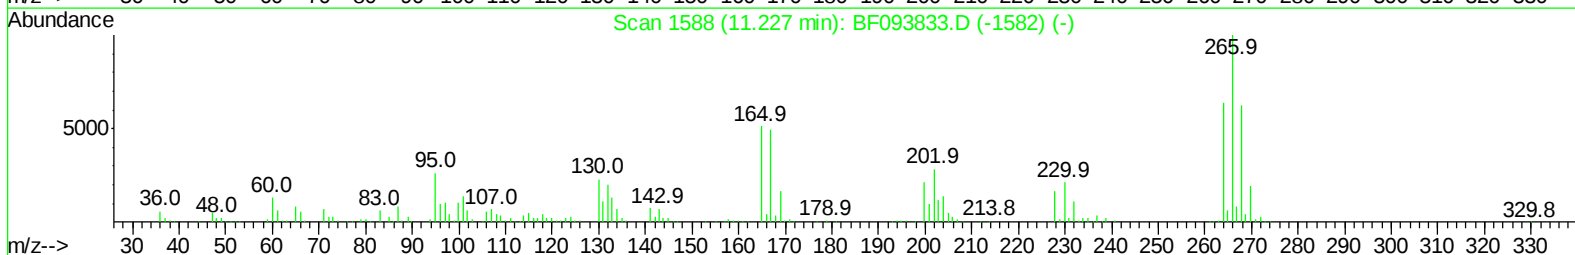
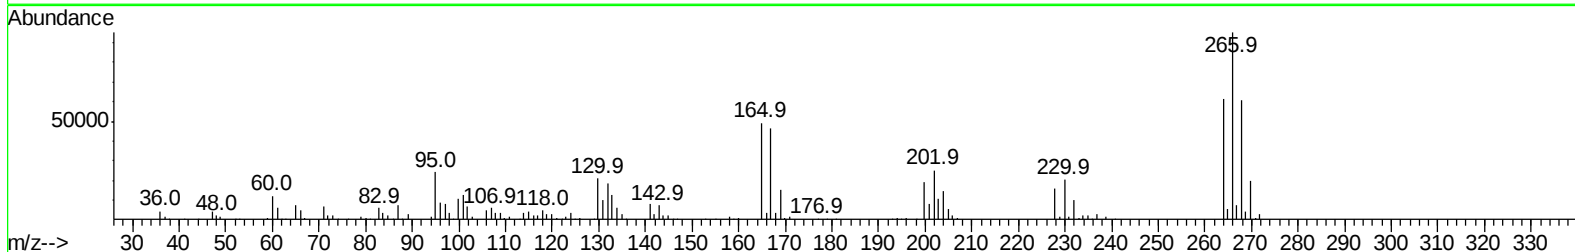


Data Path : Z:\HPCHEM1\BNA F\Data\BF040417\
Data File : BF094168.D
Acq On : 4 Apr 2017 15:29
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 05:32:34 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 14:38:29 2017
Response via : Initial Calibration

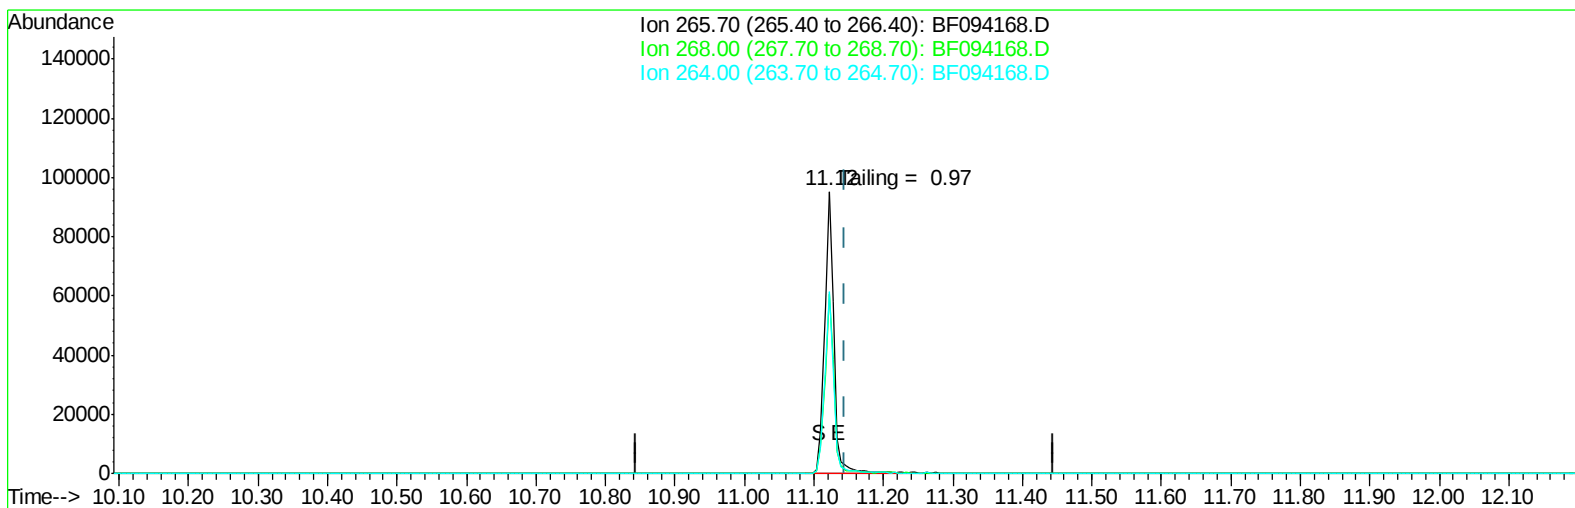

TIC: BF094168.D

(69) Pentachlorophenol (C)




11.122min (-0.024) 0.00ng

response 87734

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.68
264.00	64.60	64.55
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF040417\
Data File : BF094168.D
Acq On : 4 Apr 2017 15:29
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 05:32:34 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 31 14:38:29 2017
Response via : Initial Calibration

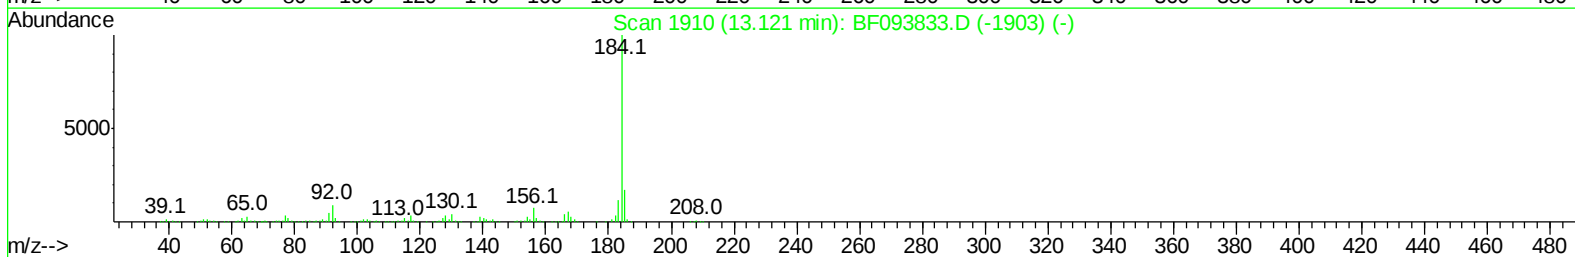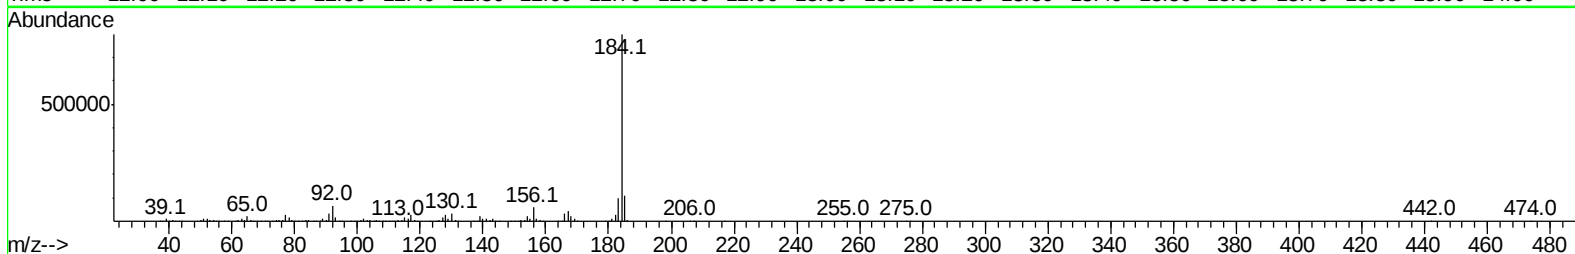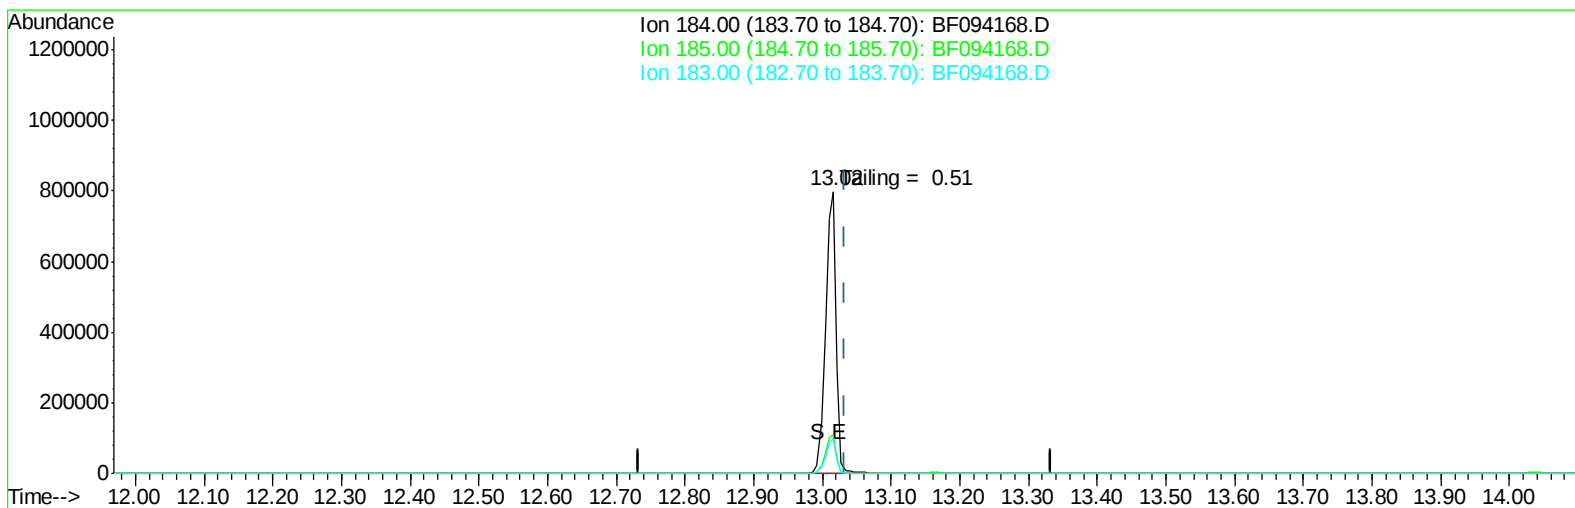

TIC: BF094168.D

(76) Benzidine

13.016min (-0.018) 0.00ng

response 867759

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	13.69#
183.00	12.20	12.20
0.00	0.00	0.00