

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040417\
 Data File : BF094186.D
 Acq On : 5 Apr 2017 00:04
 Operator : SJ/MA
 Sample : I2495-08 5X
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LSS-SP04-COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.257	59	63	67	rBV	22904	26840	2.24%	0.203%
2	3.069	197	201	211	rVB	27365	36579	3.05%	0.276%
3	3.998	354	359	366	rBV	82513	85843	7.16%	0.648%
4	4.263	400	404	407	rBV	17707	16433	1.37%	0.124%
5	4.369	419	422	424	rBV	49090	53457	4.46%	0.404%
6	4.404	424	428	432	rVB	853189	848359	70.80%	6.405%
7	4.628	460	466	471	rBV2	26105	27673	2.31%	0.209%
8	5.351	585	589	592	rBV	29132	27987	2.34%	0.211%
9	5.381	592	594	599	rVB	20037	18238	1.52%	0.138%
10	5.434	599	603	606	rBV2	15877	19399	1.62%	0.146%
11	5.475	606	610	616	rBV	995424	873903	72.93%	6.598%
12	5.616	630	634	638	rBV	1050419	920424	76.81%	6.949%
13	5.681	642	645	648	rBV	51270	44857	3.74%	0.339%
14	5.875	674	678	682	rBV	908576	832136	69.45%	6.283%
15	6.051	704	708	711	rBV	802206	709639	59.22%	5.358%
16	6.251	739	742	745	rBV	25348	21852	1.82%	0.165%
17	6.516	781	787	792	rBV	593320	569860	47.56%	4.303%
18	6.810	834	837	841	rVB2	18640	15982	1.33%	0.121%
19	7.069	876	881	888	rBV6	15995	29151	2.43%	0.220%
20	7.275	913	916	922	rBV2	32165	34915	2.91%	0.264%
21	7.380	928	934	937	rBV	1119992	1132474	94.51%	8.550%
22	7.404	937	938	943	rVB2	43358	26234	2.19%	0.198%
23	7.810	1000	1007	1009	rBV4	23031	31576	2.64%	0.238%
24	8.245	1077	1081	1084	rBV	50402	44411	3.71%	0.335%
25	8.310	1088	1092	1099	rVV	38853	51550	4.30%	0.389%
26	8.363	1099	1101	1105	rVB	28356	23417	1.95%	0.177%
27	8.698	1153	1158	1162	rBV	1214673	1039970	86.79%	7.852%
28	9.010	1209	1211	1216	rVB5	10867	16535	1.38%	0.125%
29	9.198	1240	1243	1247	rVB	58126	53247	4.44%	0.402%
30	9.339	1263	1267	1273	rBV2	22872	29461	2.46%	0.222%
31	9.416	1275	1280	1286	rBV4	22593	39822	3.32%	0.301%
32	9.516	1290	1297	1302	rBV2	1134169	1198237	100.00%	9.047%
33	9.774	1337	1341	1346	rBV5	13787	24401	2.04%	0.184%
34	9.827	1347	1350	1356	rBV7	11262	16908	1.41%	0.128%

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040417\
Data File : BF094186.D
Acq On : 5 Apr 2017 00:04
Operator : SJ/MA
Sample : I2495-08 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP04-COMP

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.110	1396	1398	1401	rVB	28704	23817	1.99%	0.180%
36	10.192	1409	1412	1416	rBV3	21139	28862	2.41%	0.218%
37	10.486	1458	1462	1469	rBV	544866	533991	44.56%	4.032%
38	10.692	1495	1497	1499	rBV2	34340	36004	3.00%	0.272%
39	11.092	1562	1565	1568	rVB5	30284	32968	2.75%	0.249%
40	11.251	1590	1592	1595	rVB4	36949	30380	2.54%	0.229%
41	11.286	1596	1598	1602	rBV2	30874	40719	3.40%	0.307%
42	11.339	1603	1607	1610	rVV	1005773	1049326	87.57%	7.923%
43	11.368	1610	1612	1615	rVB	121382	103991	8.68%	0.785%
44	11.433	1621	1623	1625	rVB	44117	34926	2.91%	0.264%
45	12.092	1733	1735	1738	rBV2	57903	60947	5.09%	0.460%
46	12.833	1858	1861	1864	rBV	177123	178916	14.93%	1.351%
47	13.110	1905	1908	1912	rVB	189521	198222	16.54%	1.497%
48	13.315	1940	1943	1949	rVB	623742	665152	55.51%	5.022%
49	14.598	2157	2161	2164	rBV	608867	639230	53.35%	4.826%
50	16.233	2436	2439	2445	rVB	554592	645596	53.88%	4.874%


Sum of corrected areas: 13244817

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040417\
Data File : BF094186.D
Acq On : 5 Apr 2017 00:04
Operator : SJ/MA
Sample : I2495-08 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP04-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

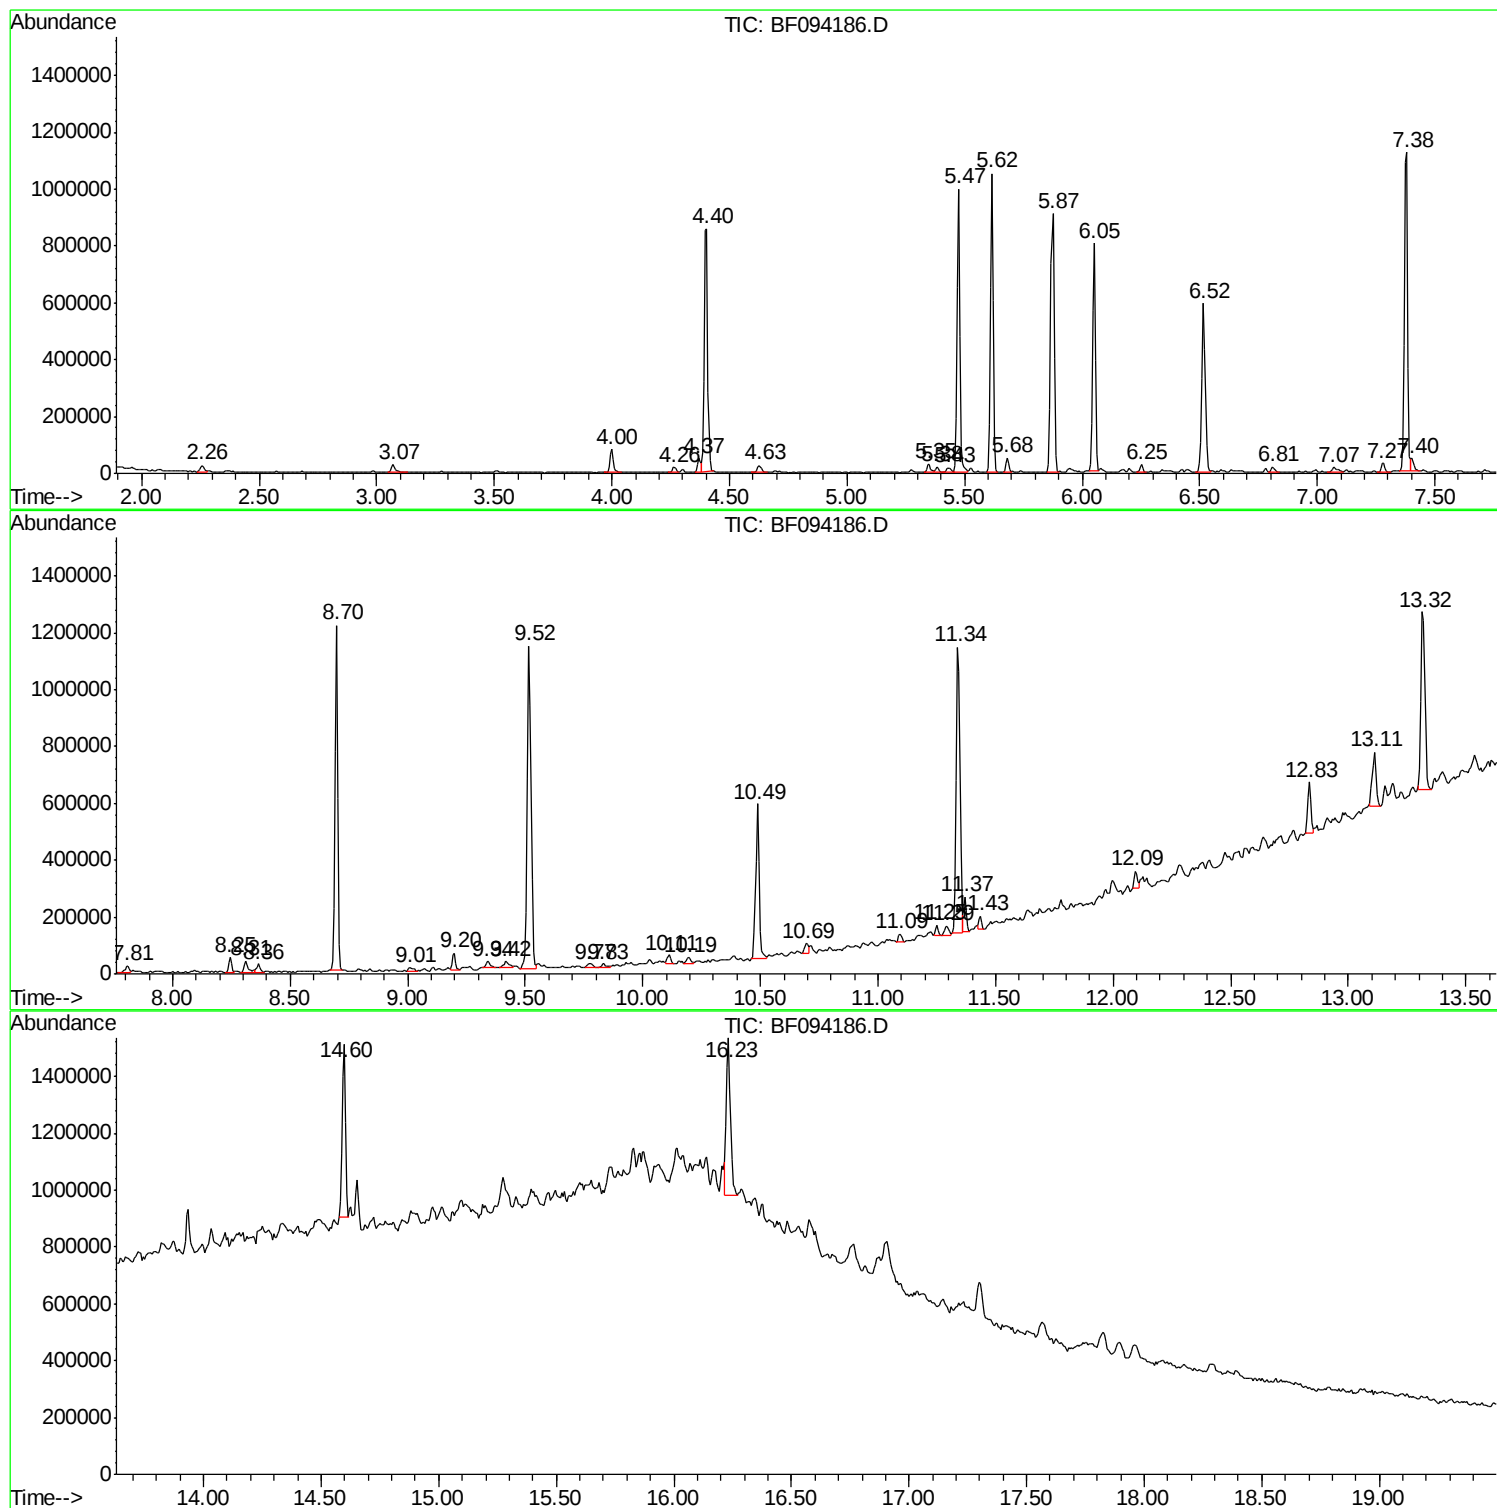

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040417\
Data File : BF094186.D
Acq On : 5 Apr 2017 00:04
Operator : SJ/MA
Sample : I2495-08 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP04-COMP










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.00	2.06 ng	85843	1,4-Dichlorobenzene-d4	5.87

Hit# of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	45	
2	Butyl aldoxime, 3-methyl-, syn-	101	C5H11NO	005780-40-5	35	
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	16	
4	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9	
5	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	9	

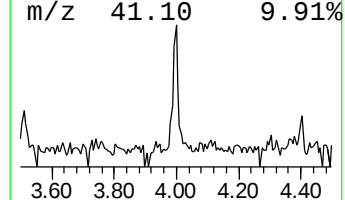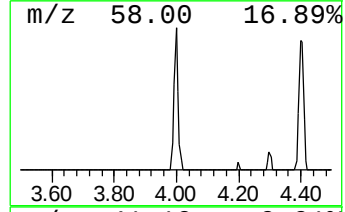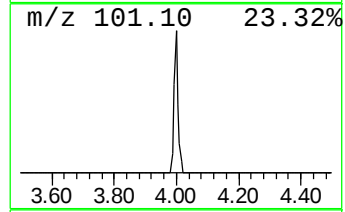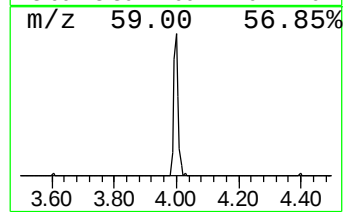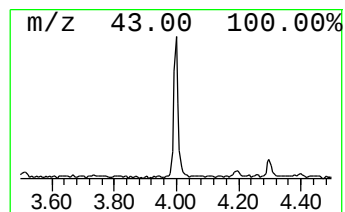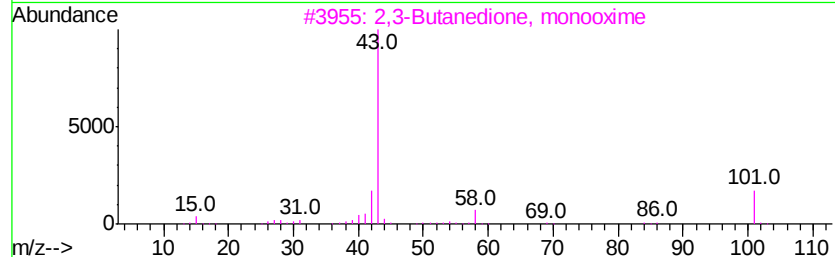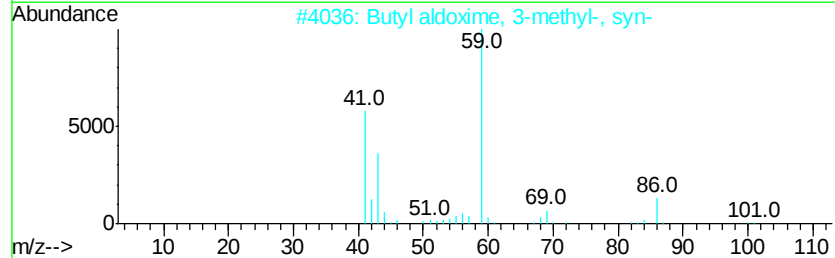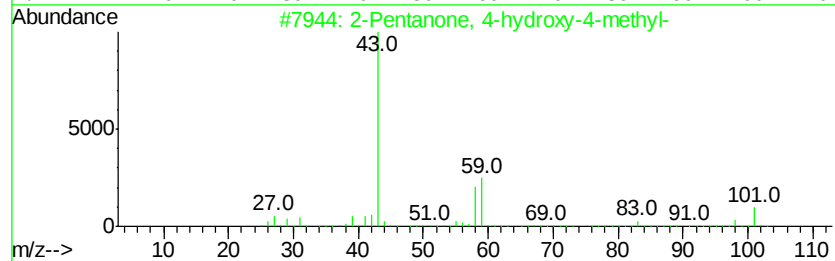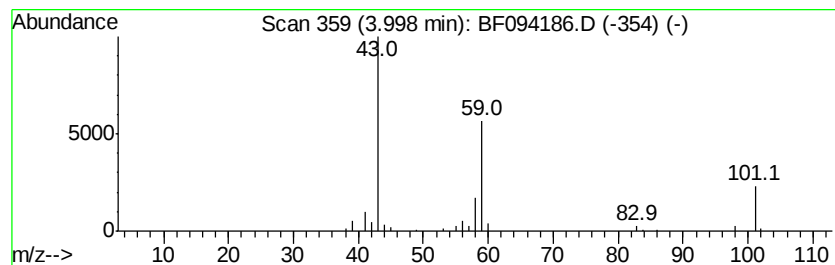

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040417\
Data File : BF094186.D
Acq On : 5 Apr 2017 00:04
Operator : SJ/MA
Sample : I2495-08 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP04-COMP










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown5.62 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.62	22.12 ng	920424	1,4-Dichlorobenzene-d4	5.87

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	16
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		Tranvlcyproline-propionyl	189	C12H15NO	1000123-86-3	10
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

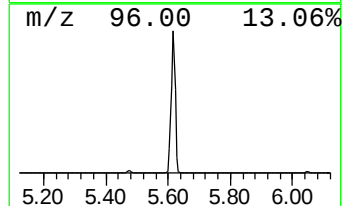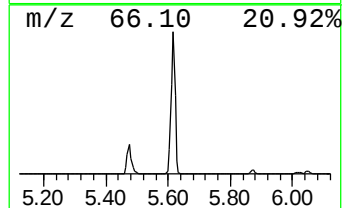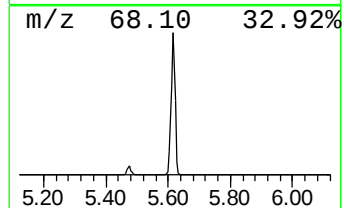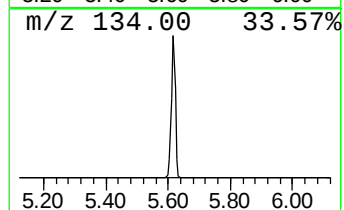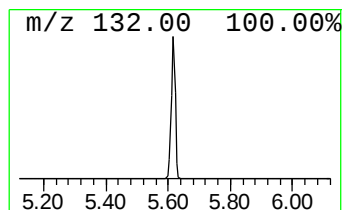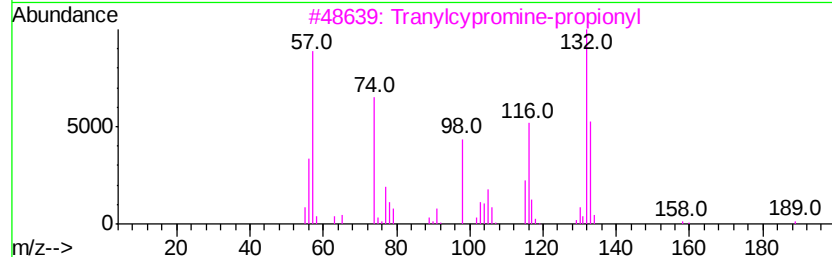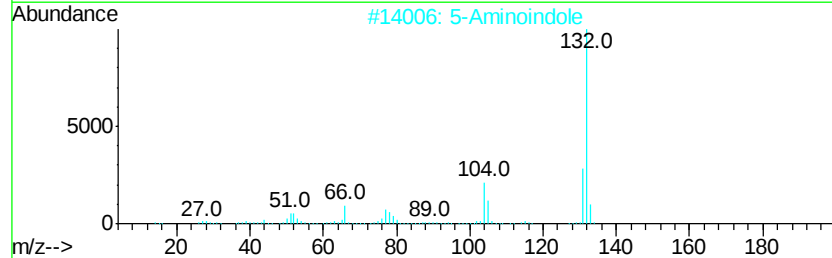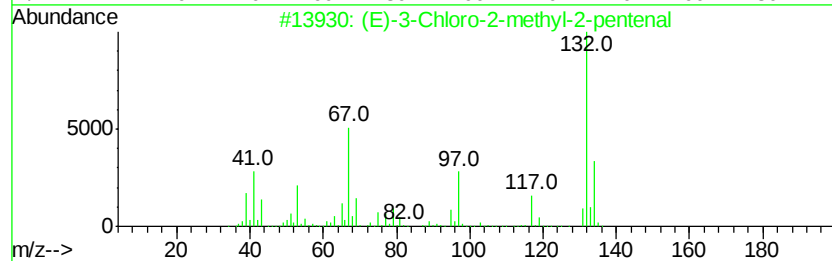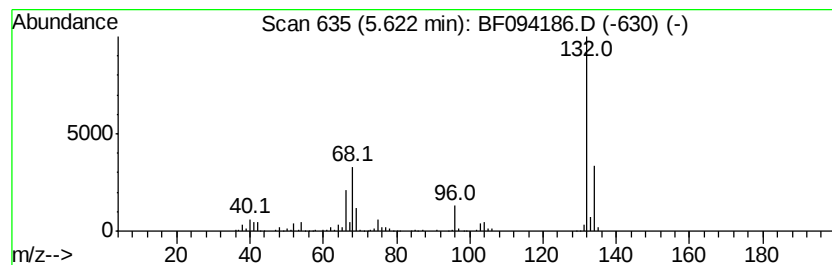

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040417\
Data File : BF094186.D
Acq On : 5 Apr 2017 00:04
Operator : SJ/MA
Sample : I2495-08 5X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LSS-SP04-COMP

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	4.00	2.1	ng	85843	1	5.87	832136	20.0
unknown5.62	5.62	22.1	ng	920424	1	5.87	832136	20.0