
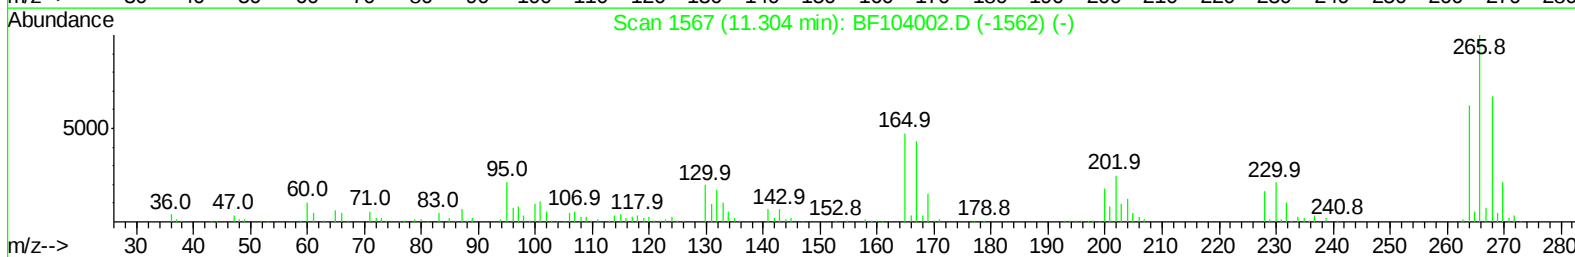
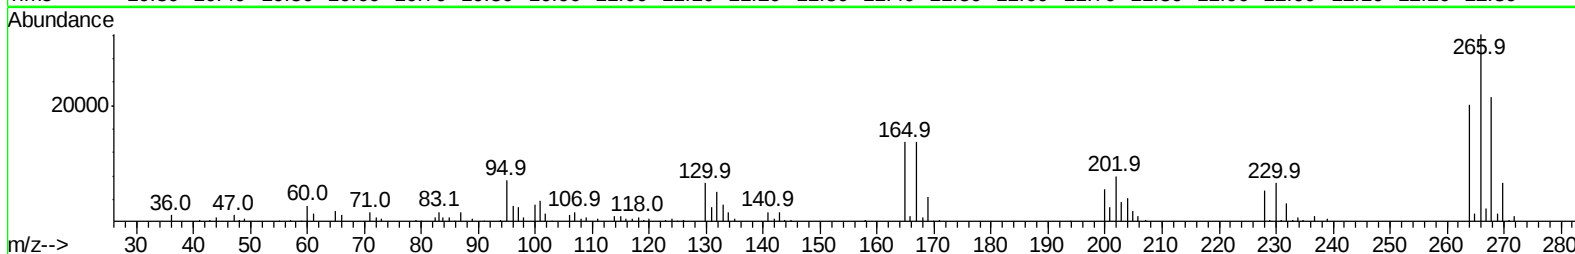


Data Path : Z:\HPCHEM1\BNA F\DATA\BF040418\
Data File : BF104223.D
Acq On : 4 Apr 2018 13:51
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 04:39:47 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 04 18:06:58 2018
Response via : Initial Calibration

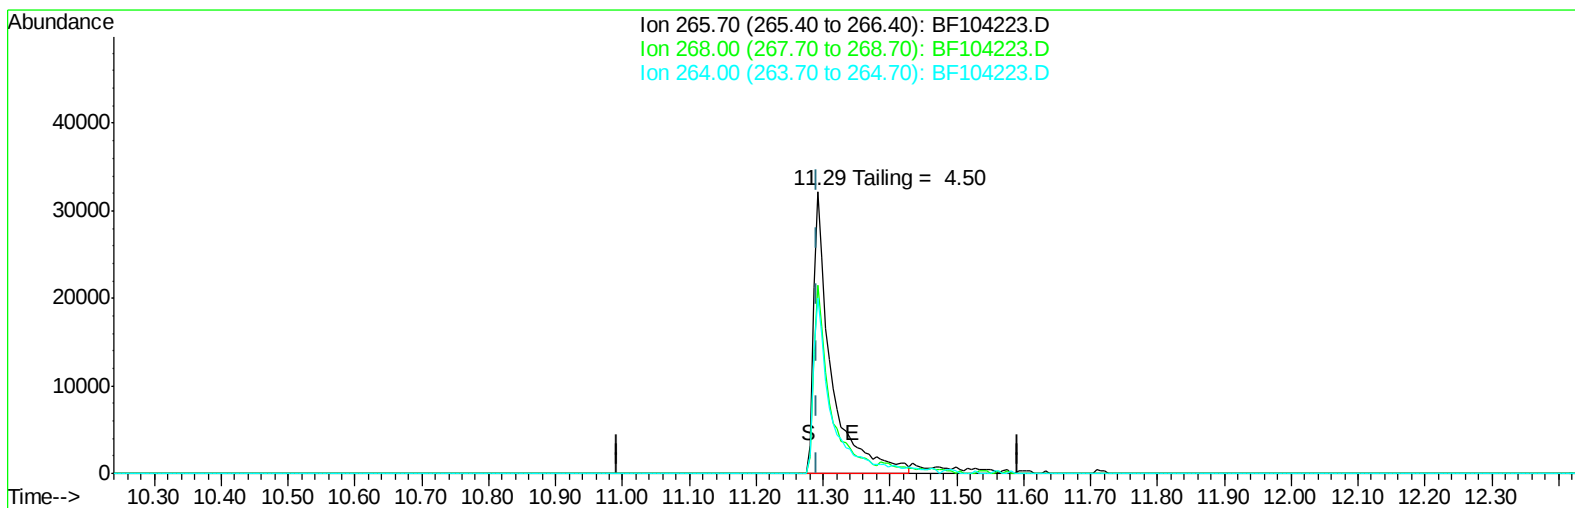

TIC: BF104223.D

(69) Pentachlorophenol (C)




11.292min (+0.000) 65487.40ng

response 59427

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.70
264.00	61.90	62.37
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040418\
Data File : BF104223.D
Acq On : 4 Apr 2018 13:51
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 04:39:47 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 04 18:06:58 2018
Response via : Initial Calibration

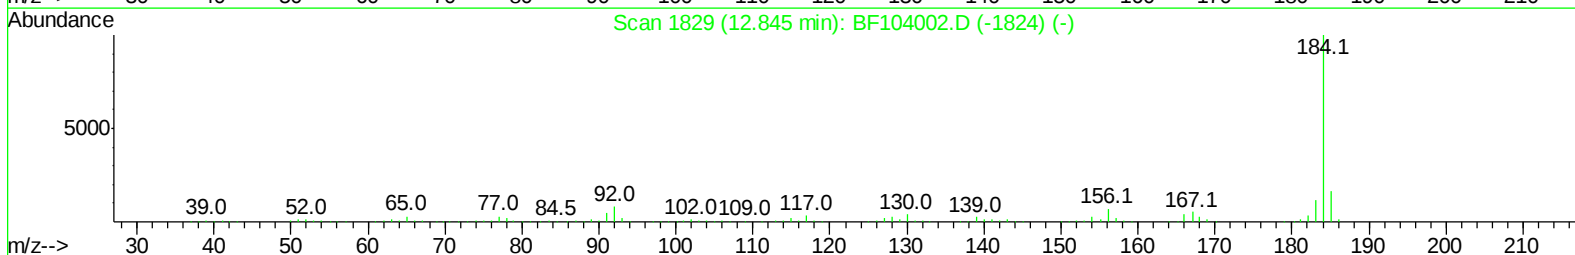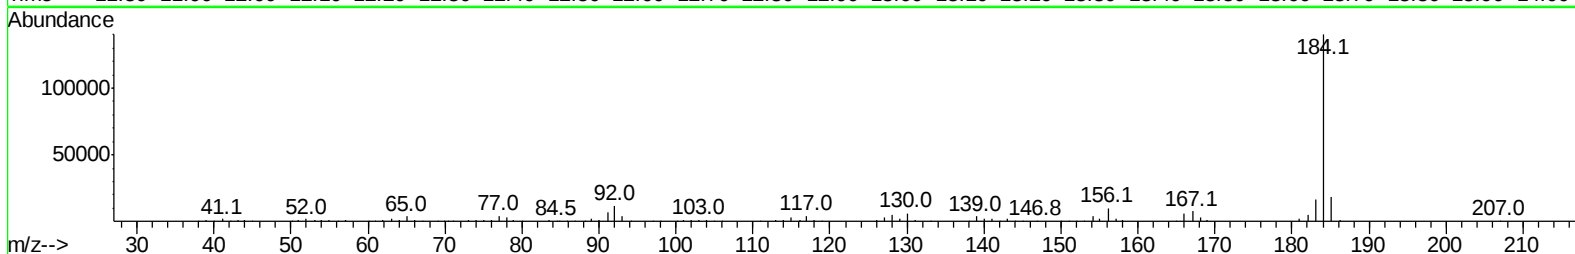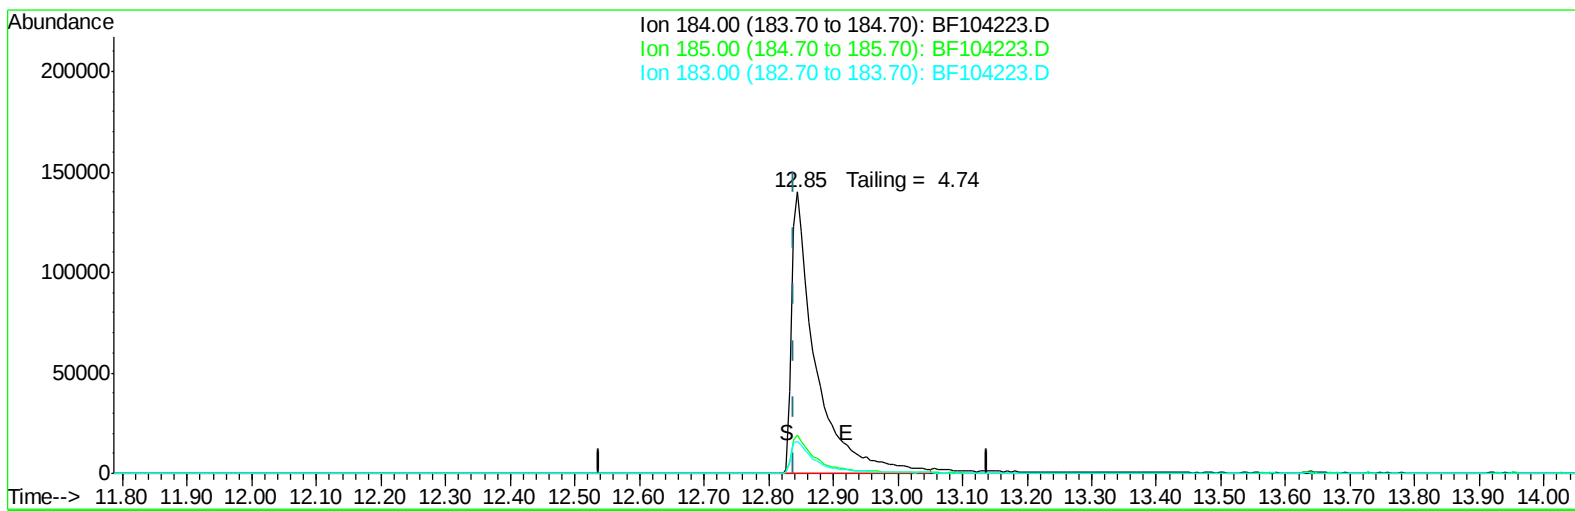

TIC: BF104223.D

(76) Benzidine

12.845min (+0.006) 0.00ng

response 359206

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.52
183.00	11.60	11.57
0.00	0.00	0.00