
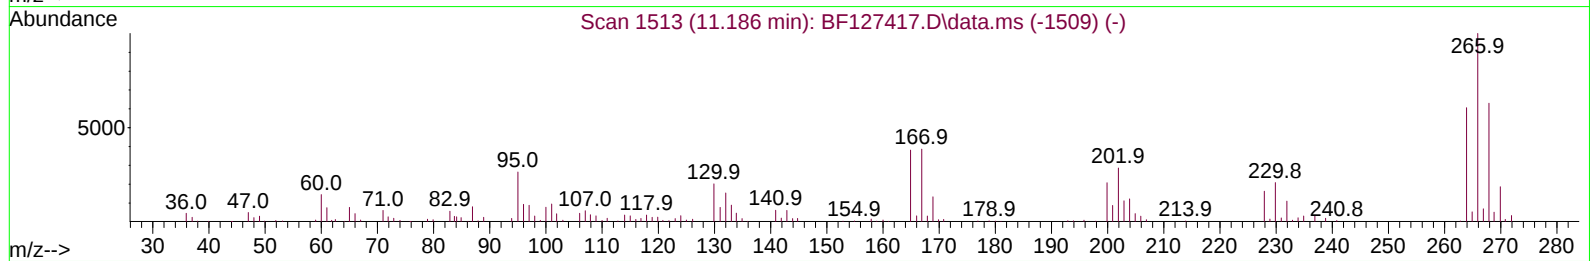
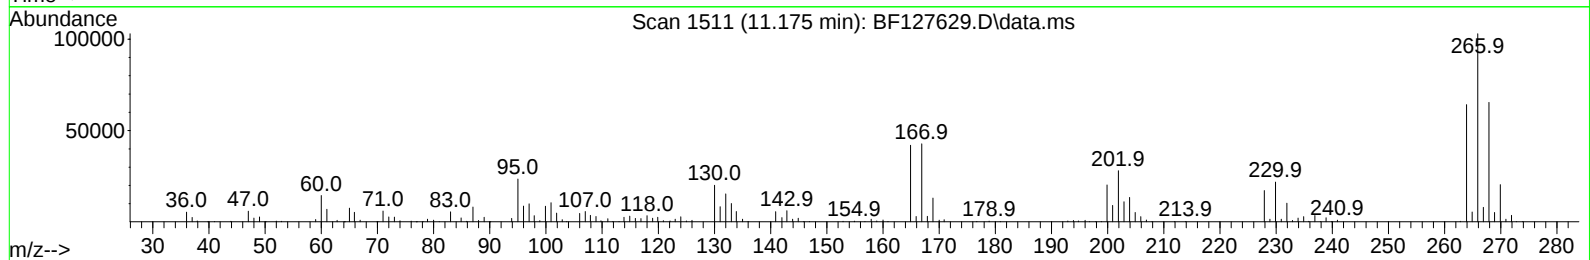


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040422\
Data File : BF127629.D
Acq On : 04 Apr 2022 09:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 16:23:01 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 29 07:13:31 2022
Response via : Initial Calibration

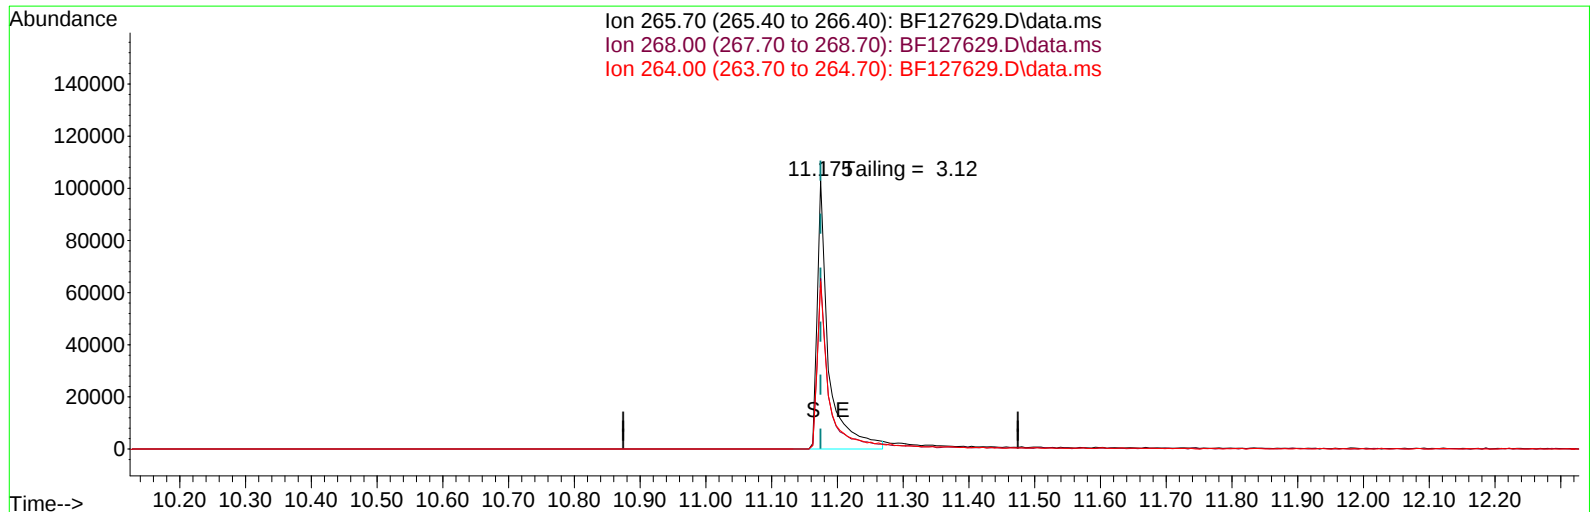

TIC: BF127629.D\data.ms

(70) Pentachlorophenol (C)




11.175min (+ 0.000) 38029.82 ng

response 131779

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.52
264.00	60.60	62.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040422\
 Data File : BF127629.D
 Acq On : 04 Apr 2022 09:57
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 04 16:23:01 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 29 07:13:31 2022
 Response via : Initial Calibration

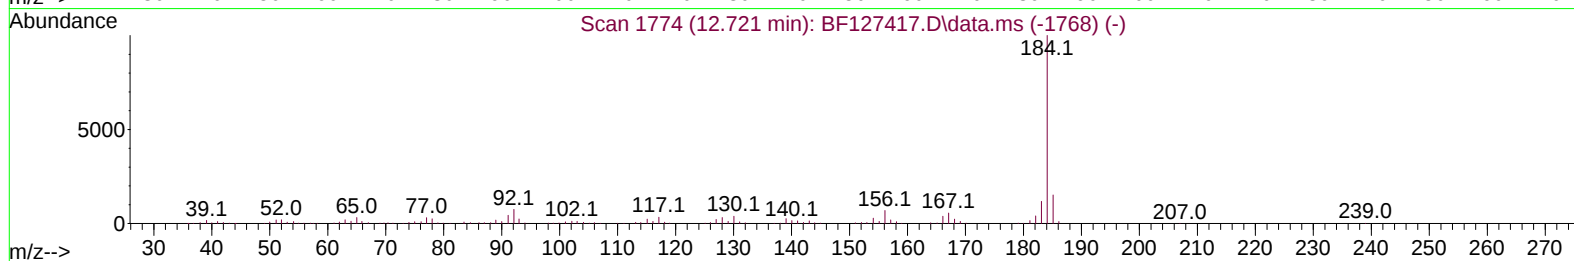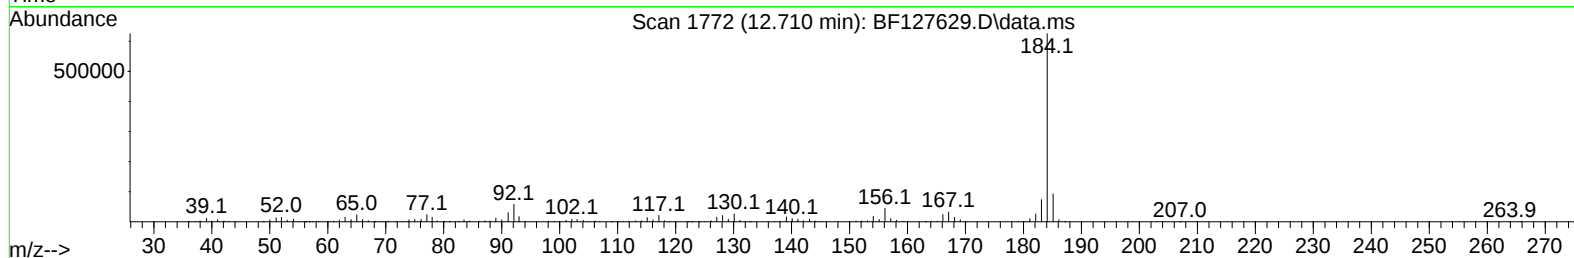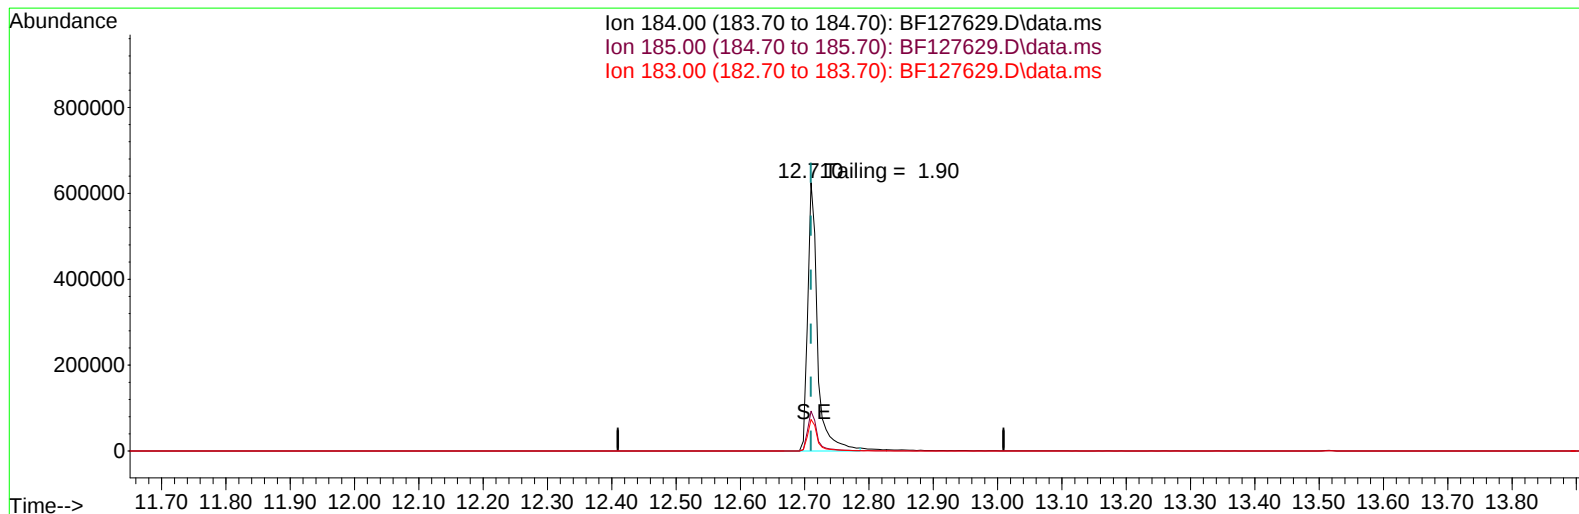

TIC: BF127629.D\data.ms

(77) Benzidine**12.710min (+ 0.000) 445532.47 ng****response 679888**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.86
183.00	11.70	11.78
0.00	0.00	0.00