

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040422\
 Data File : BF127631.D
 Acq On : 04 Apr 2022 11:48
 Operator : CG\JU
 Sample : PB143792BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143792BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127631.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	477	481	499	rBV	22306	44771	1.06%	0.171%
2	5.469	537	541	572	rBV	3222559	3449662	81.69%	13.145%
3	6.481	708	713	740	rBV	3012355	3533409	83.68%	13.464%
4	6.834	770	773	788	rVB	739251	693355	16.42%	2.642%
5	7.404	866	870	891	rBV	2313928	2413825	57.16%	9.198%
6	8.116	987	991	1002	rBV	954958	904060	21.41%	3.445%
7	9.192	1168	1174	1177	rBV	3774756	3832146	90.75%	14.602%
8	9.869	1286	1289	1303	rVB	1071037	1042110	24.68%	3.971%
9	10.669	1421	1425	1451	rBV	2364391	2419455	57.30%	9.219%
10	11.363	1540	1543	1554	rBV	1122635	1097294	25.99%	4.181%
11	12.751	1776	1779	1784	rVB	88278	66868	1.58%	0.255%
12	12.951	1808	1813	1817	rBV	3881582	4222691	100.00%	16.090%
13	13.457	1896	1899	1904	rBV	68104	57199	1.35%	0.218%
14	14.015	1991	1994	2009	rBV	1051103	1058106	25.06%	4.032%
15	14.751	2115	2119	2123	rBV	52874	50338	1.19%	0.192%
16	15.086	2172	2176	2181	rBV	68574	76598	1.81%	0.292%
17	15.462	2235	2240	2243	rBV	75775	88370	2.09%	0.337%
18	15.504	2243	2247	2262	rVV	610351	912250	21.60%	3.476%
19	15.892	2308	2313	2320	rBV	63838	91490	2.17%	0.349%
20	16.392	2393	2398	2404	rBV	44898	73369	1.74%	0.280%
21	16.980	2492	2498	2506	rVB2	25376	50234	1.19%	0.191%
22	17.133	2515	2524	2527	rBV8	22706	66205	1.57%	0.252%




Sum of corrected areas: 26243805

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040422\
Data File : BF127631.D
Acq On : 04 Apr 2022 11:48
Operator : CG\JU
Sample : PB143792BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143792BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

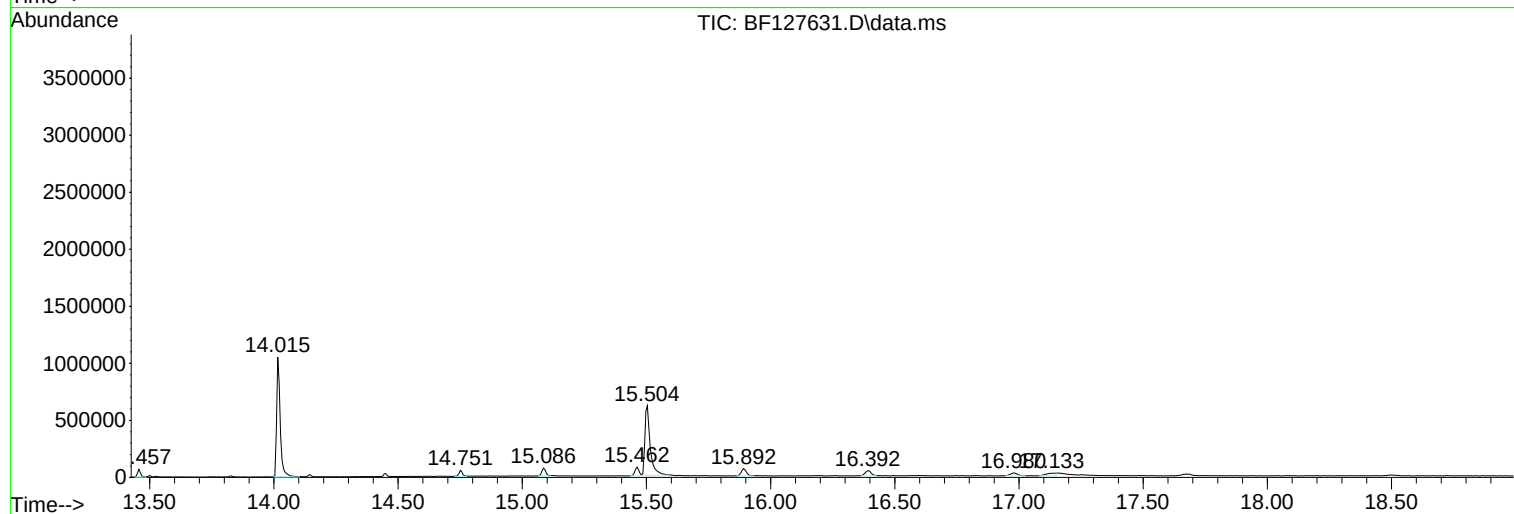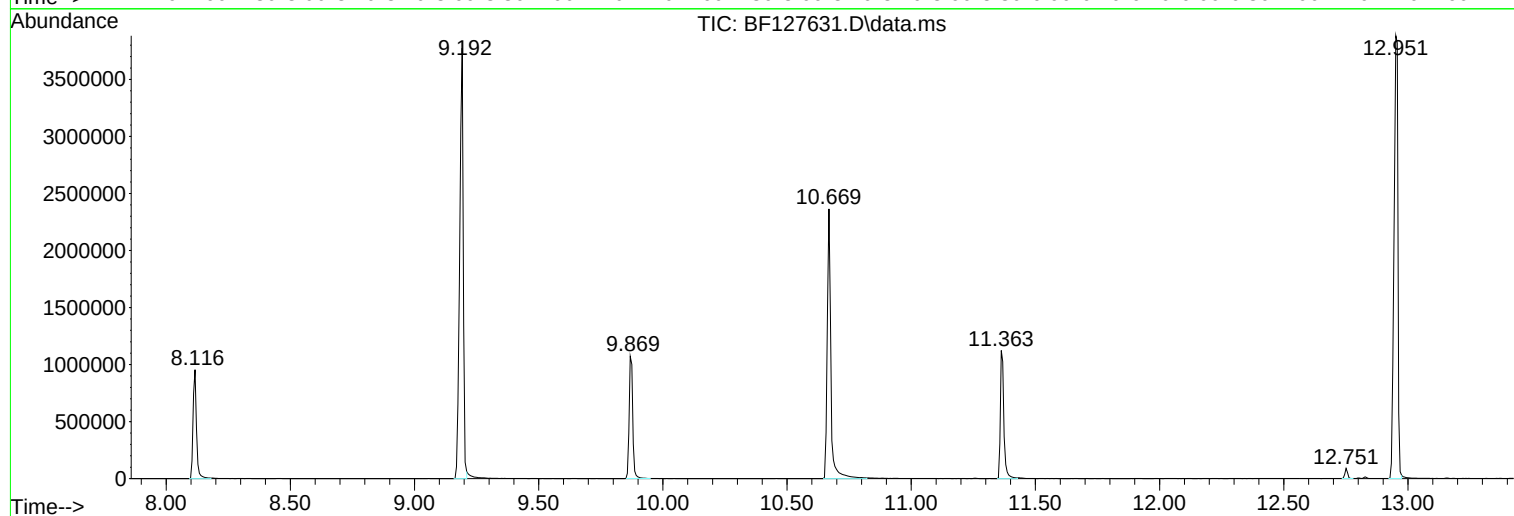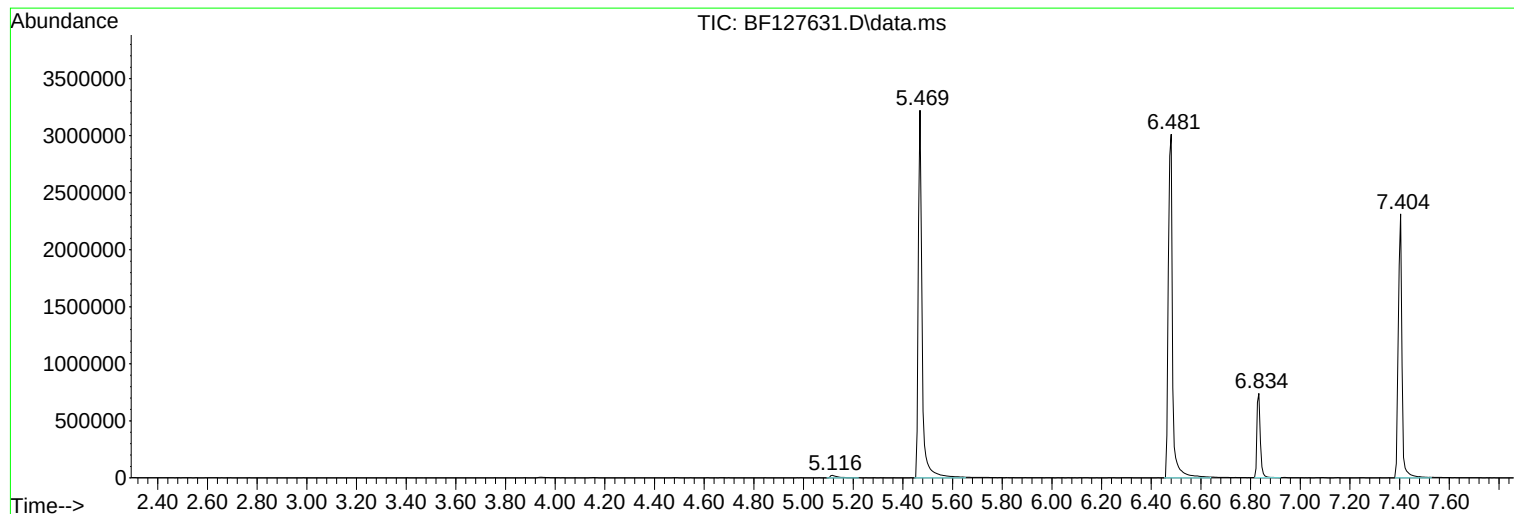

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040422\
Data File : BF127631.D
Acq On : 04 Apr 2022 11:48
Operator : CG\JU
Sample : PB143792BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143792BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Tetradecane, 1-iodo- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.892	2.01 ng	91490	Perylene-d12	15.504

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tetradecane, 1-iodo-	324	C14H29I	019218-94-1	91
2			Heneicosane	296	C21H44	000629-94-7	87
3			Hexadecane, 1-iodo-	352	C16H33I	000544-77-4	80
4			Octacosane	394	C28H58	000630-02-4	76
5			1-Iodoundecane	282	C11H23I	004282-44-4	74

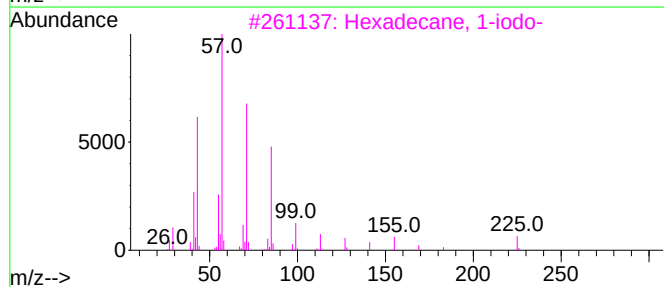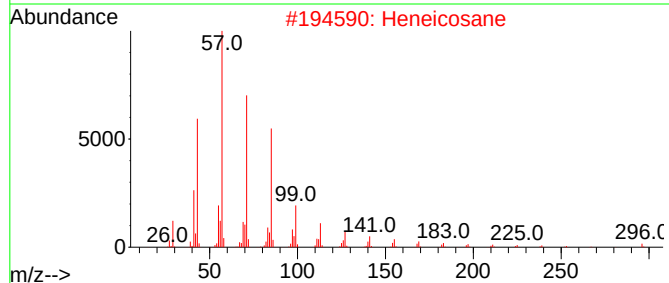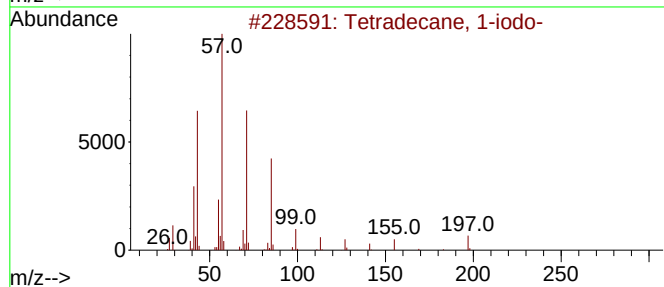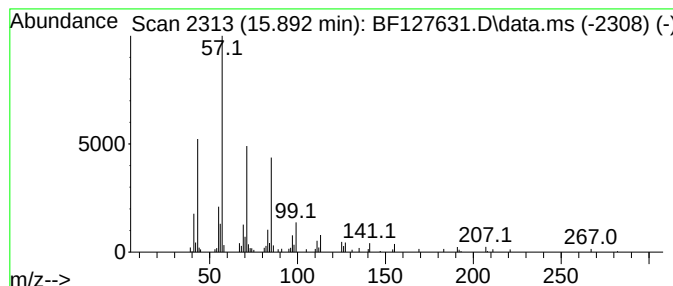

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040422\
Data File : BF127631.D
Acq On : 04 Apr 2022 11:48
Operator : CG\JU
Sample : PB143792BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143792BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF032122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Tetradecane, 1-...	15.892	2.0	ng	91490	6	15.504	912250	20.0