
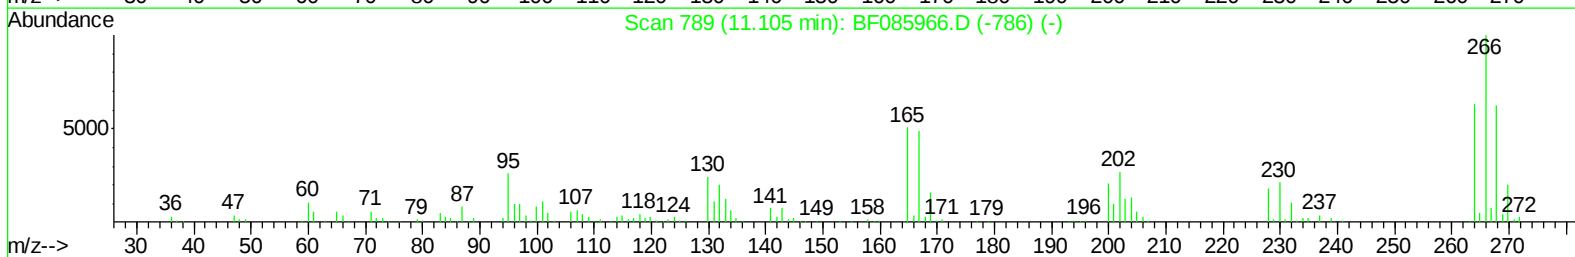
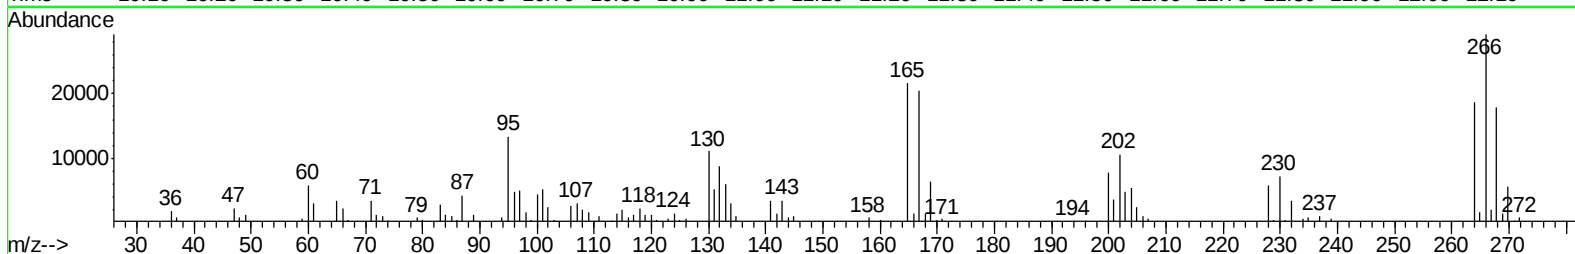


Data Path : Z:\HPCHEM1\BNA_F\Data\BF040516\
Data File : BF086080.D
Acq On : 5 Apr 2016 16:58
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 05:38:51 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

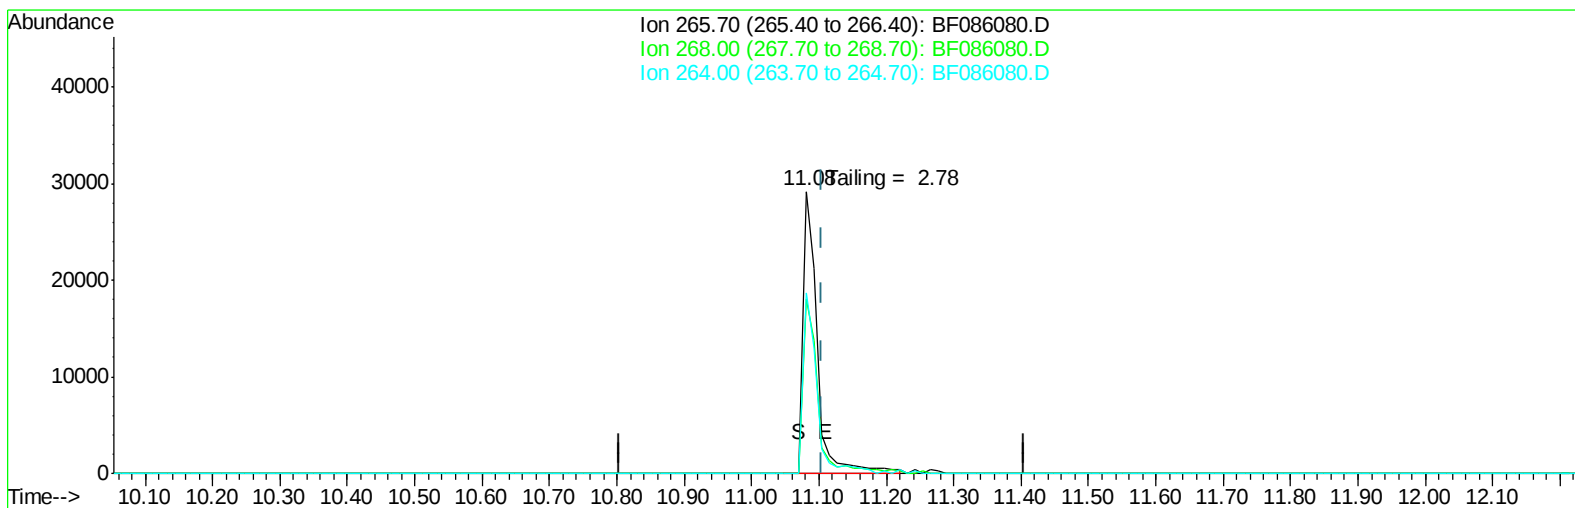

TIC: BF086080.D

(69) Pentachlorophenol (C)




11.082min (-0.023) 40915.95ng

response 42515

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	61.64
264.00	63.30	64.22
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF040516\
Data File : BF086080.D
Acq On : 5 Apr 2016 16:58
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 05:38:51 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

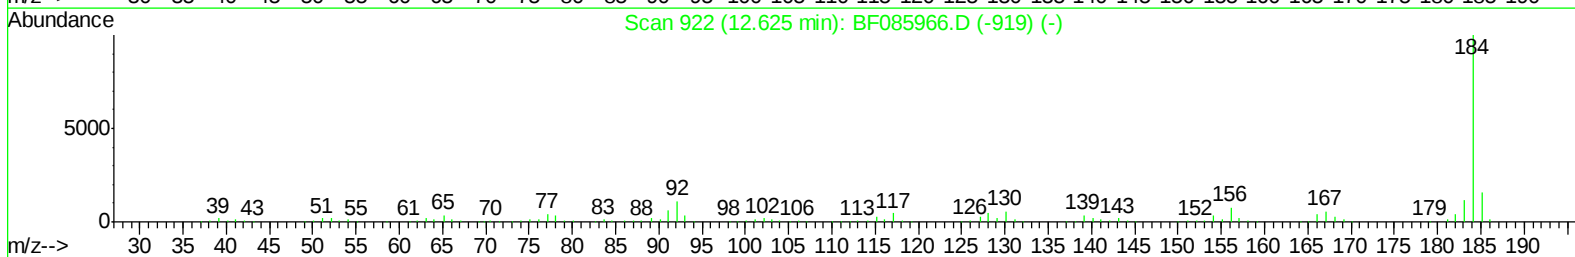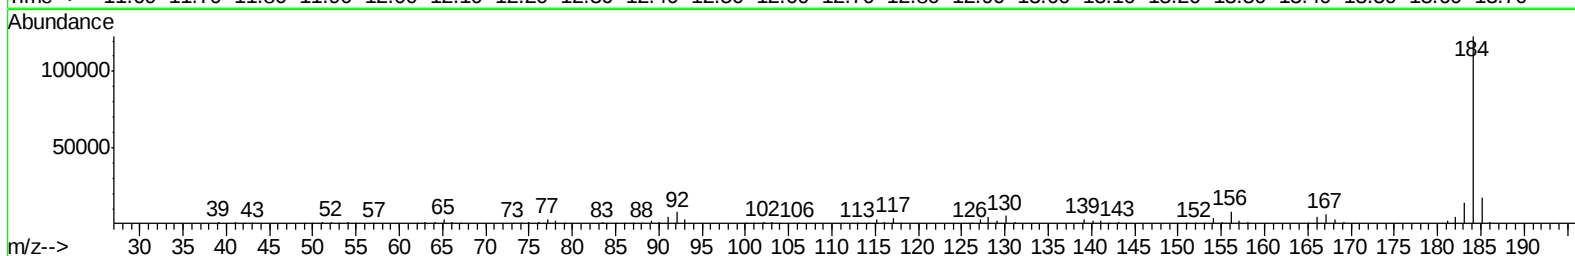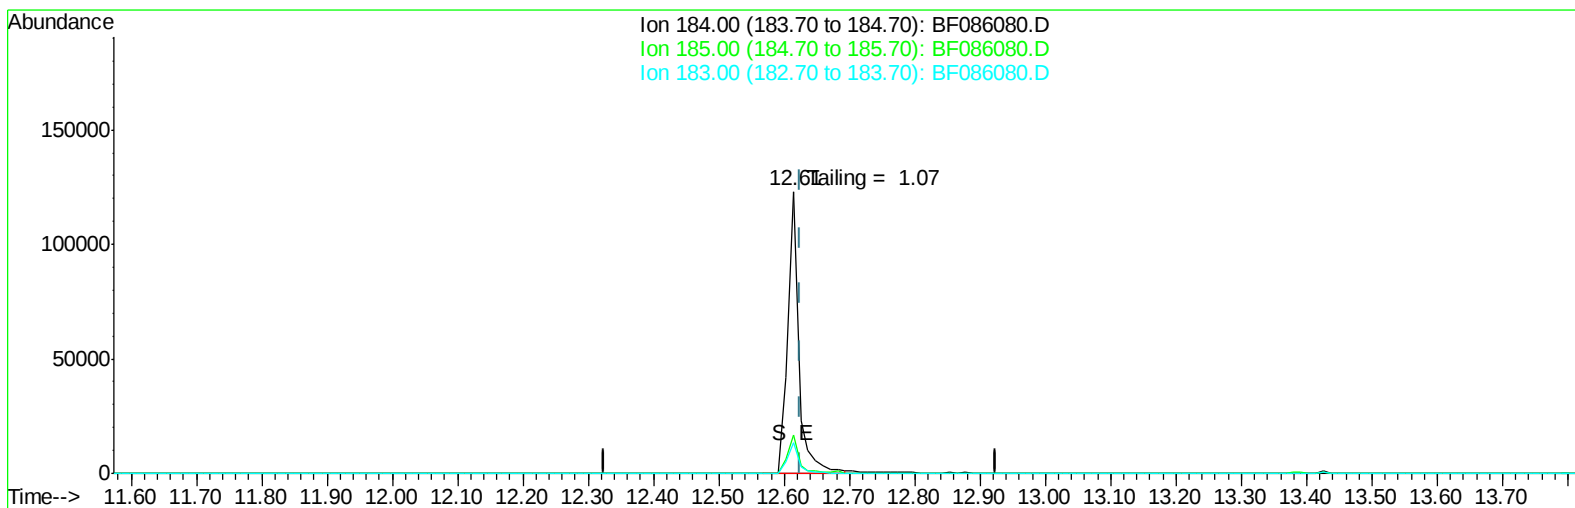

TIC: BF086080.D

(76) Benzidine

12.614min (-0.011) 0.00ng

response 148326

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	13.74
183.00	11.80	10.87
0.00	0.00	0.00