
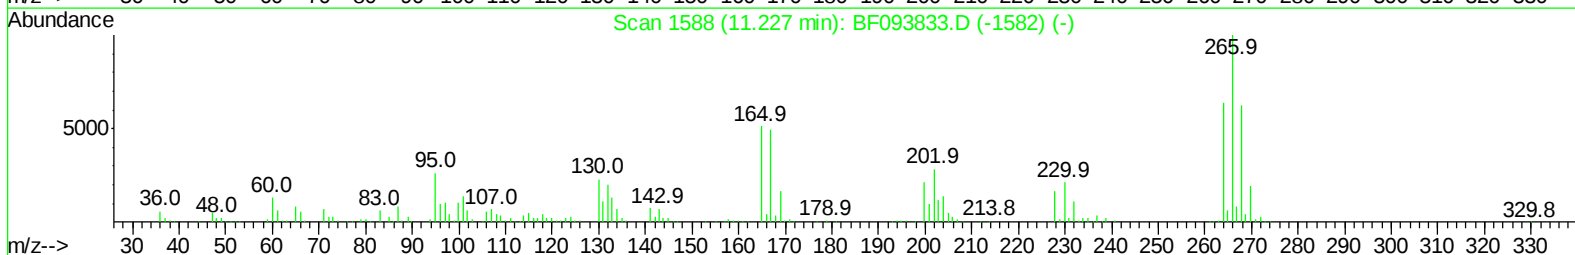
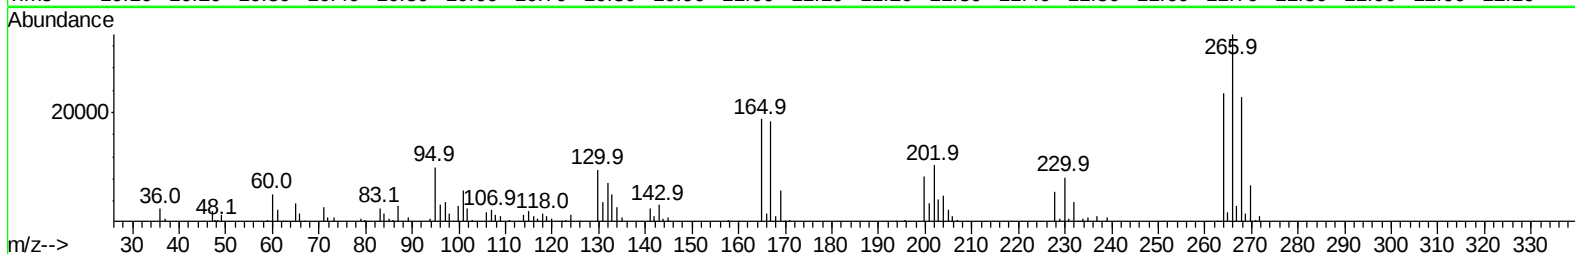


Data Path : Z:\HPCHEM1\BNA F\DATA\BF040517\  
Data File : BF094212.D  
Acq On : 6 Apr 2017 2:43  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 07:05:10 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 31 14:38:29 2017  
Response via : Initial Calibration

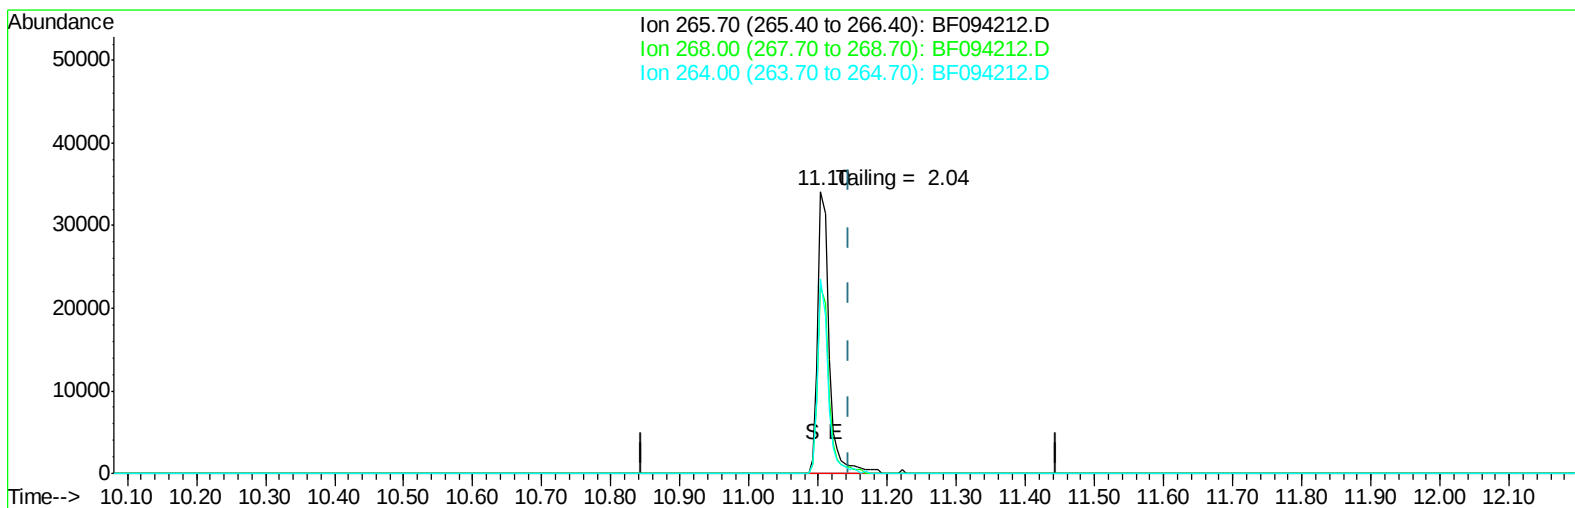

TIC: BF094212.D

(69) Pentachlorophenol (C)




11.104min (-0.041) 33629.06ng

response 38553

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 66.59 |
| 264.00 | 64.60 | 68.91 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040517\  
Data File : BF094212.D  
Acq On : 6 Apr 2017 2:43  
Operator : SJ/MA  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 07:05:10 2017  
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Mar 31 14:38:29 2017  
Response via : Initial Calibration

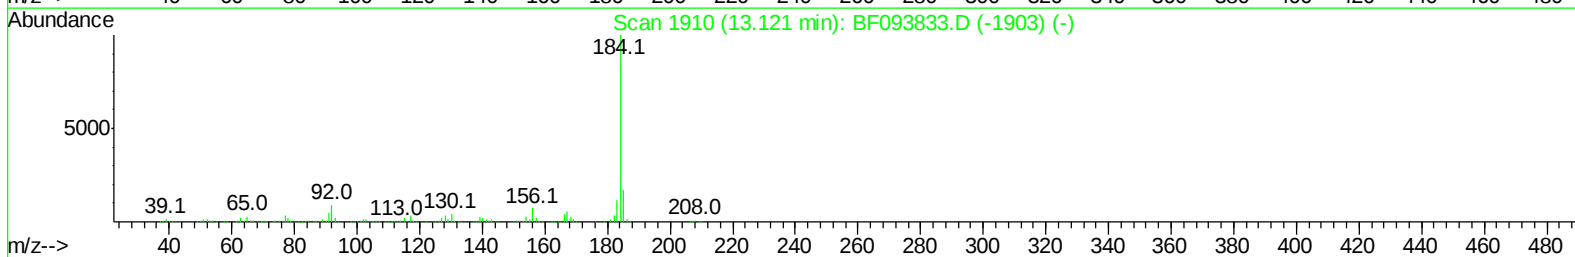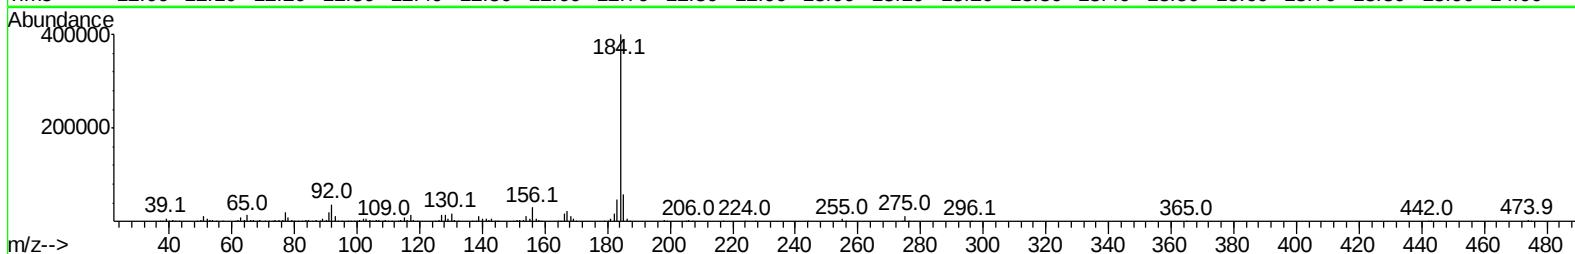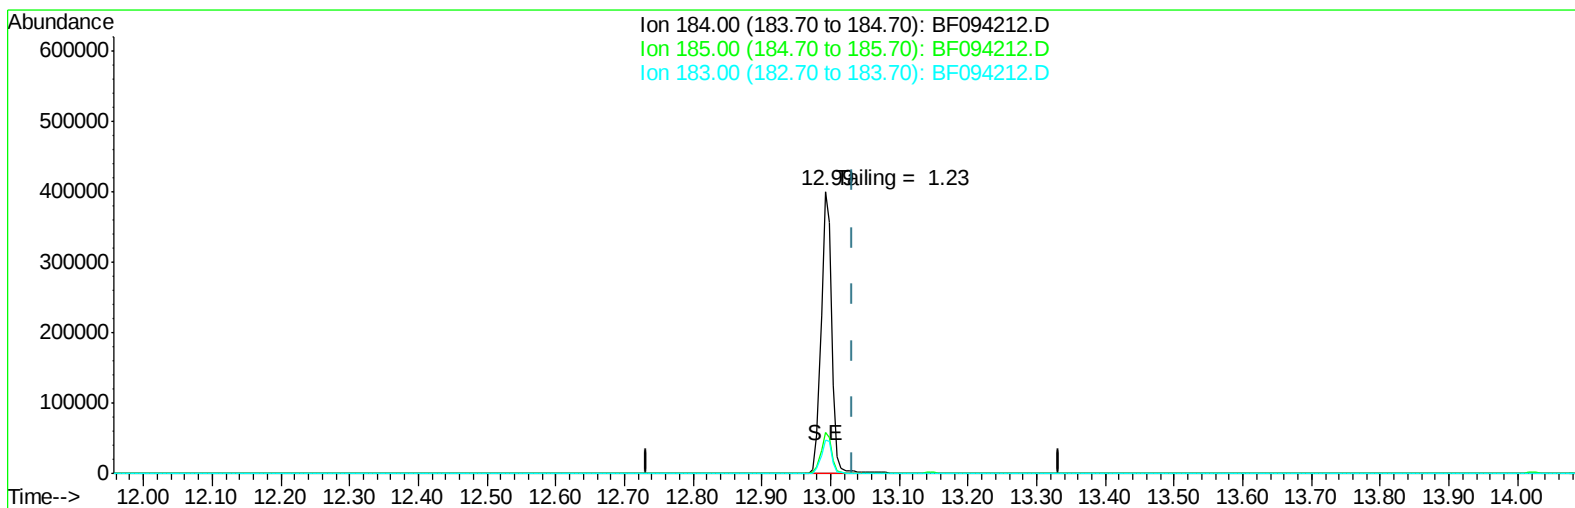

TIC: BF094212.D

(76) Benzidine

12.992min (-0.041) 73317.12ng

response 429461

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 184.00 | 100   | 100    |
| 185.00 | 19.40 | 14.67# |
| 183.00 | 12.20 | 11.73  |
| 0.00   | 0.00  | 0.00   |