

Data Path : Z:\HPCHEM1\BNA F\Data\BF040517\
 Data File : BF094211.D
 Acq On : 6 Apr 2017 1:19
 Operator : SJ/MA
 Sample : I2522-13 10X
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 BASING-7(0-2)

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.981	353	356	364	rVB	41125	43120	3.32%	0.493%
2	4.251	399	402	406	rVB	22493	22579	1.74%	0.258%
3	4.387	421	425	435	rVB	364729	328732	25.30%	3.761%
4	4.604	457	462	466	rBV	79052	71140	5.48%	0.814%
5	5.463	604	608	617	rVB	346982	342439	26.36%	3.918%
6	5.604	628	632	637	rBV	410460	353065	27.18%	4.040%
7	5.863	672	676	680	rBV	1122389	1010105	77.75%	11.558%
8	6.039	702	706	710	rBV	322379	277510	21.36%	3.175%
9	6.504	781	785	791	rBV	218611	195264	15.03%	2.234%
10	7.369	926	932	935	rBV	1420366	1299150	100.00%	14.865%
11	8.686	1152	1156	1160	rVB	448194	377169	29.03%	4.316%
12	9.186	1238	1241	1244	rVB	18451	16370	1.26%	0.187%
13	9.504	1288	1295	1302	rBV2	1165477	1262292	97.16%	14.443%
14	10.474	1456	1460	1464	rBV	152103	139785	10.76%	1.599%
15	10.686	1491	1496	1497	rBV2	13654	15339	1.18%	0.176%
16	10.704	1497	1499	1503	rVB	18916	17357	1.34%	0.199%
17	11.327	1601	1605	1609	rBV	1030852	1030479	79.32%	11.791%
18	12.821	1856	1859	1862	rVB	26658	27893	2.15%	0.319%
19	13.098	1902	1906	1909	rVB	27987	32272	2.48%	0.369%
20	13.304	1937	1941	1946	rVB	272181	268048	20.63%	3.067%
21	14.580	2154	2158	2162	rBV	912082	931044	71.67%	10.653%
22	16.209	2431	2435	2443	rVB	594734	678379	52.22%	7.762%


Sum of corrected areas: 8739531

Data Path : Z:\HPCHEM1\BNA F\Data\BF040517\
Data File : BF094211.D
Acq On : 6 Apr 2017 1:19
Operator : SJ/MA
Sample : I2522-13 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BASING-7(0-2)

Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

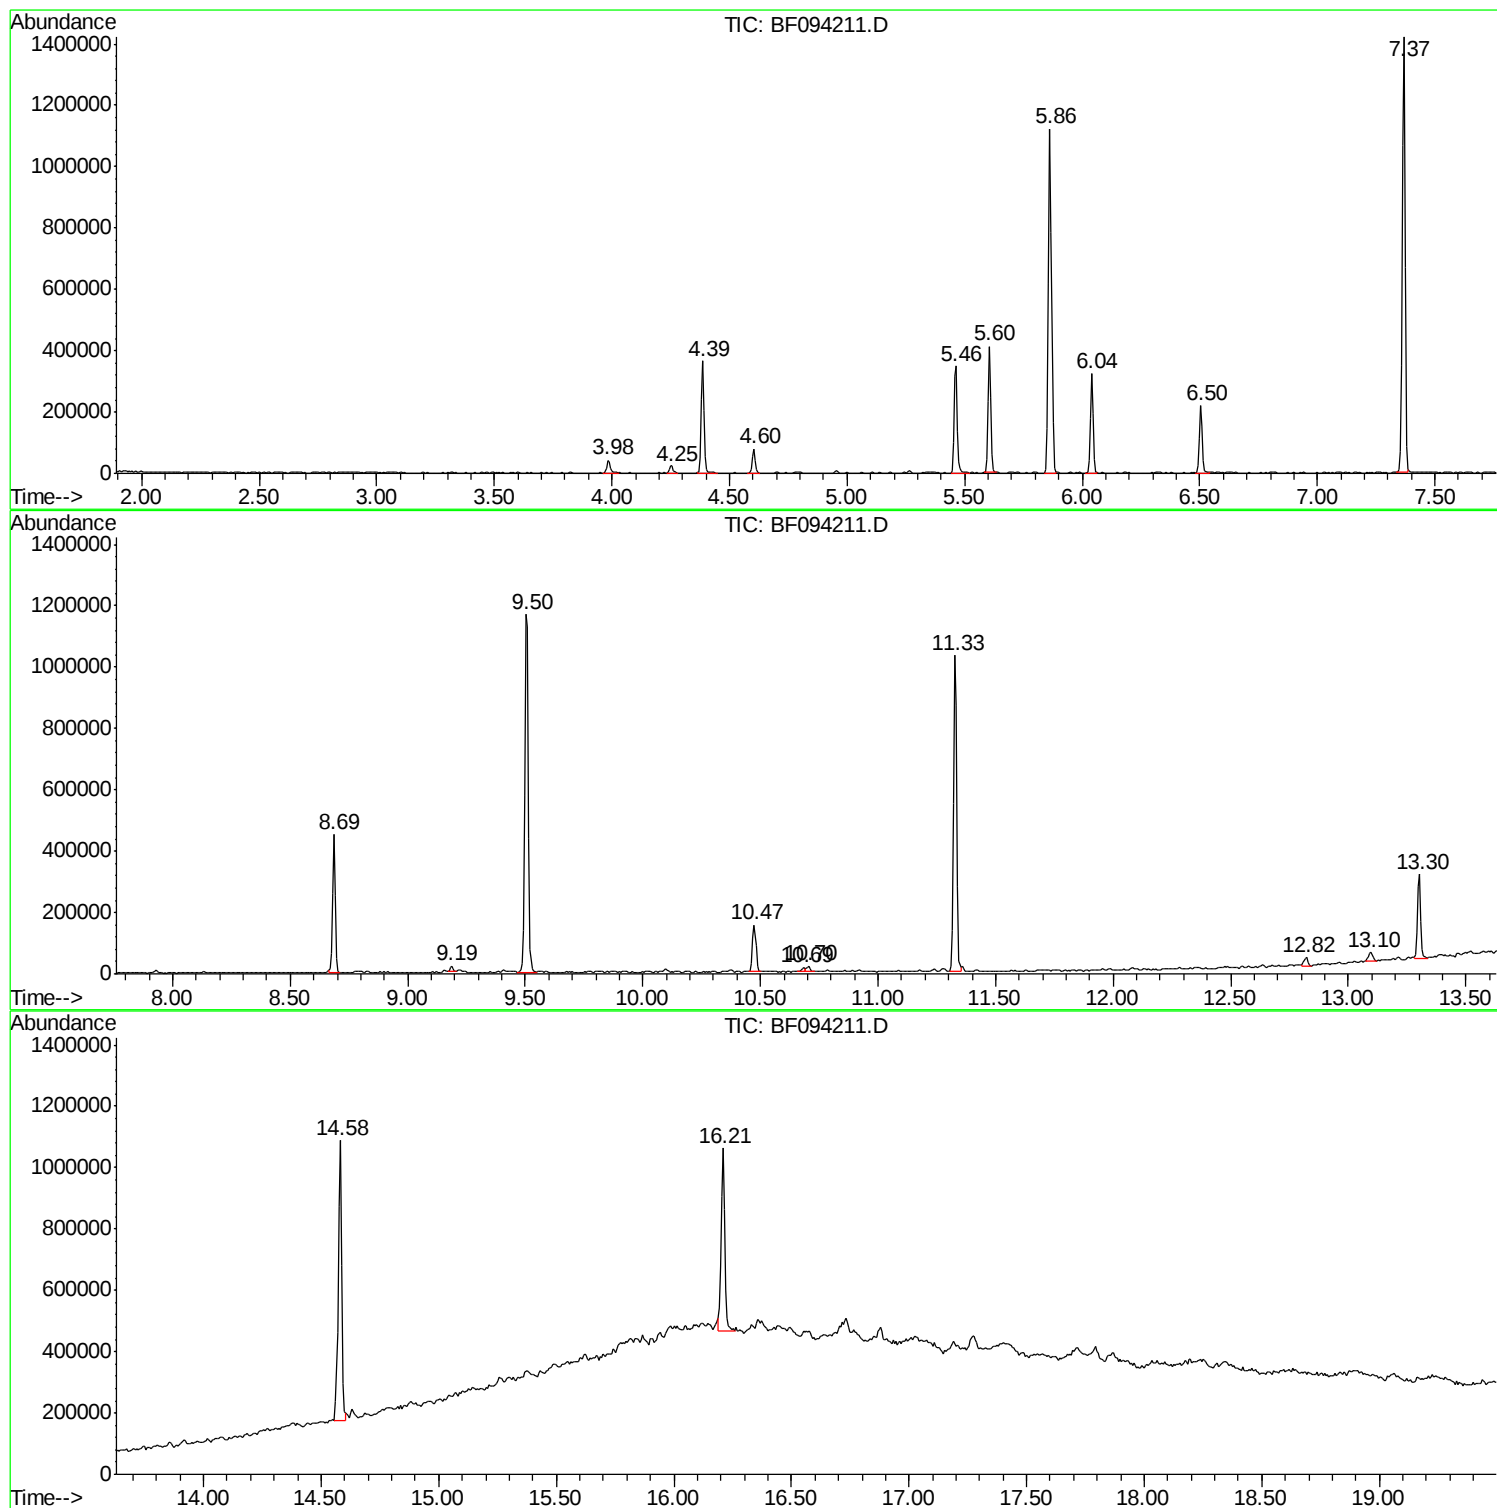

Data Path : Z:\HPCHEM1\BNA_F\Data\BF040517\
Data File : BF094211.D
Acq On : 6 Apr 2017 1:19
Operator : SJ/MA
Sample : I2522-13 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BASING-7(0-2)










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.60 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.60	6.99 ng	353065	1,4-Dichlorobenzene-d4	5.86

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	27
2		5-Aminoindole	132	C8H8N2	005192-03-0	12
3		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9
4		1-Methylpyrrolo[1,2-a]pyrazine	132	C8H8N2	064608-59-9	9
5		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9

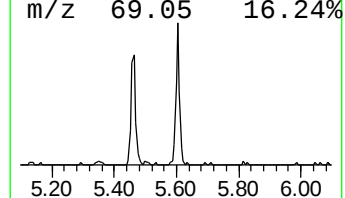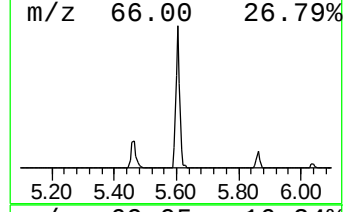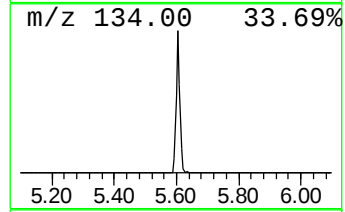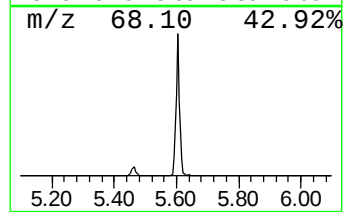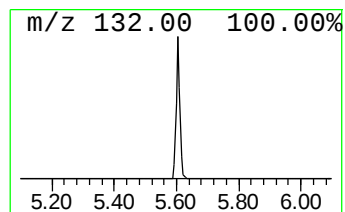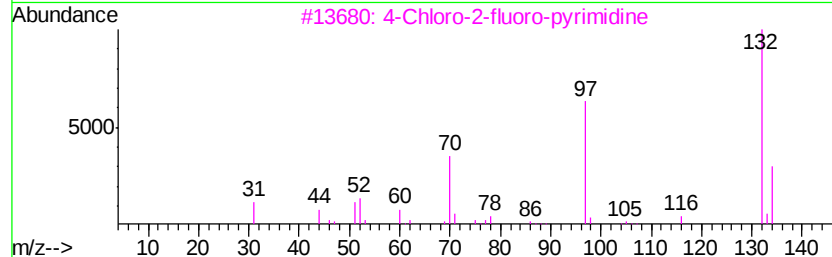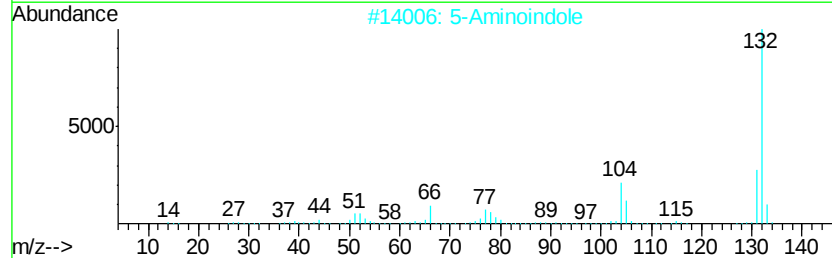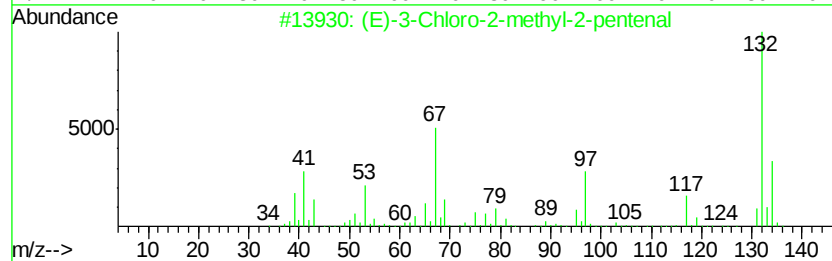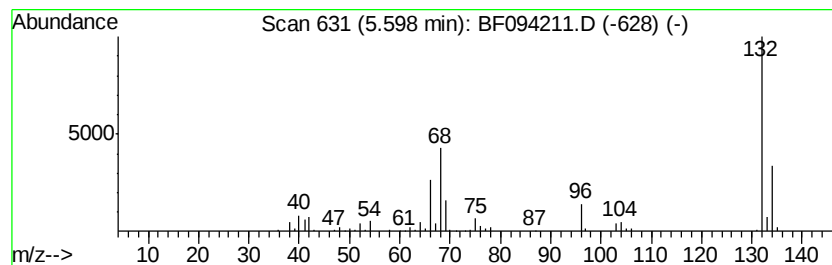

Data Path : Z:\HPCHEM1\BNA_F\Data\BF040517\
Data File : BF094211.D
Acq On : 6 Apr 2017 1:19
Operator : SJ/MA
Sample : I2522-13 10X
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
BASING-7(0-2)

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.60	5.60	7.0	ng	353065	1	5.86	1010110	20.0