
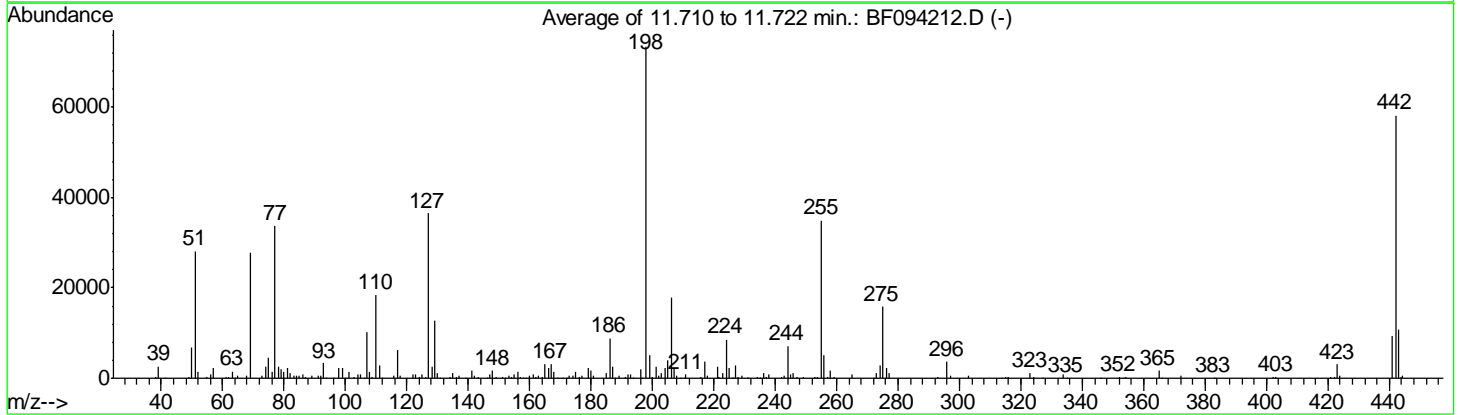


Data Path : Z:\HPCHEM1\BNA F\Data\BF040517\  
 Data File : BF094212.D  
 Acq On : 6 Apr 2017 2:43  
 Operator : SJ/MA  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF032217.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Mar 31 14:38:29 2017

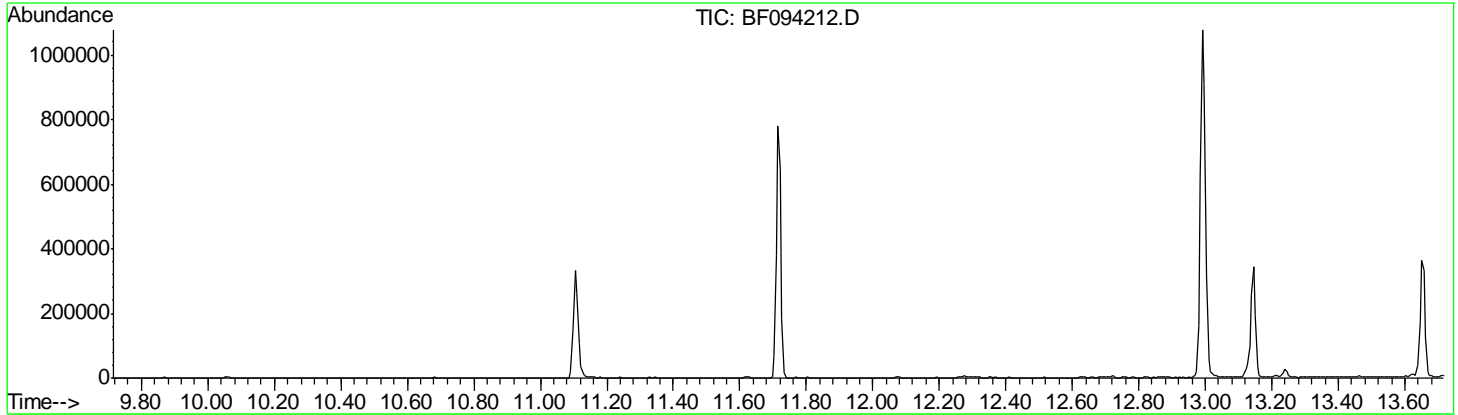

AutoFind: Scans 1670, 1671, 1672; Background Corrected with Scan 1665

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.3	28122	PASS
68	69	0.00	2	1.9	512	PASS
69	198	0.00	100	37.7	27656	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.6	36405	PASS
197	198	0.00	2	0.2	134	PASS
198	198	100	100	100.0	73360	PASS
199	198	5	9	7.1	5188	PASS
275	198	10	60	21.6	15842	PASS
365	198	1	100	2.2	1647	PASS
441	442	0.01	24	15.9	9231	PASS
442	198	50	100	79.1	58056	PASS
443	442	15	24	18.7	10837	PASS