
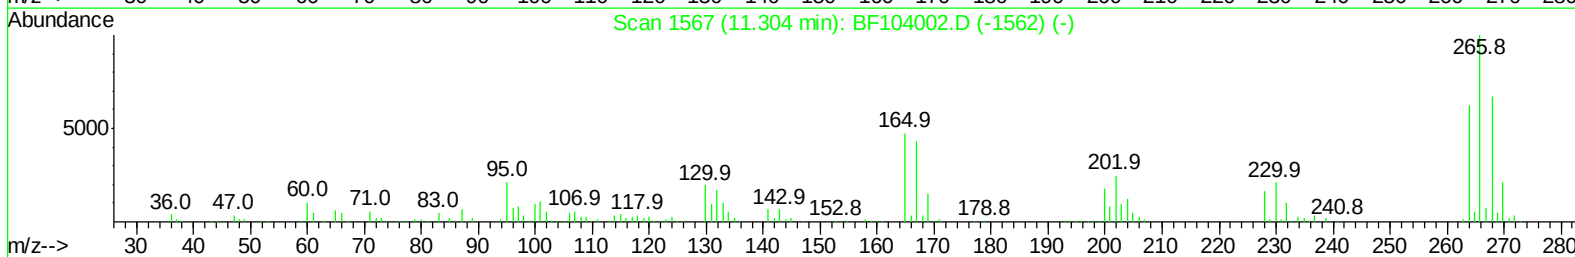
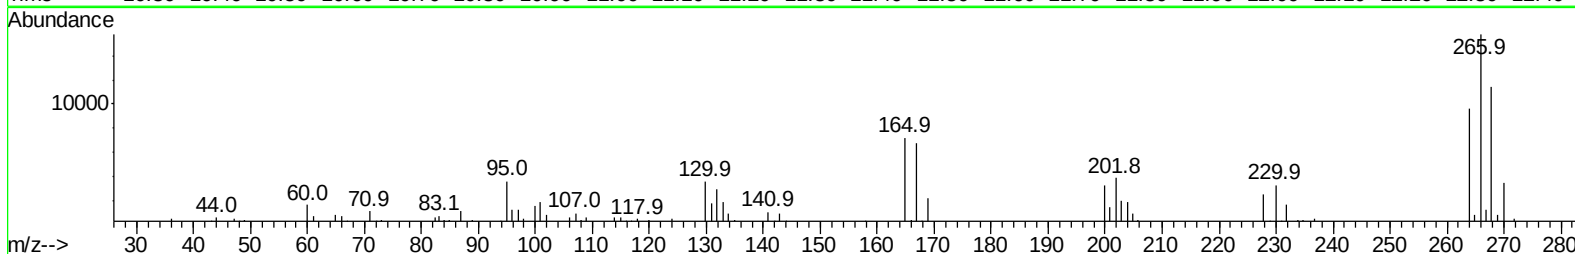


Data Path : Z:\HPCHEM1\BNA F\Data\BF040518\
Data File : BF104271.D
Acq On : 5 Apr 2018 15:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 06:06:44 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 04 18:06:58 2018
Response via : Initial Calibration

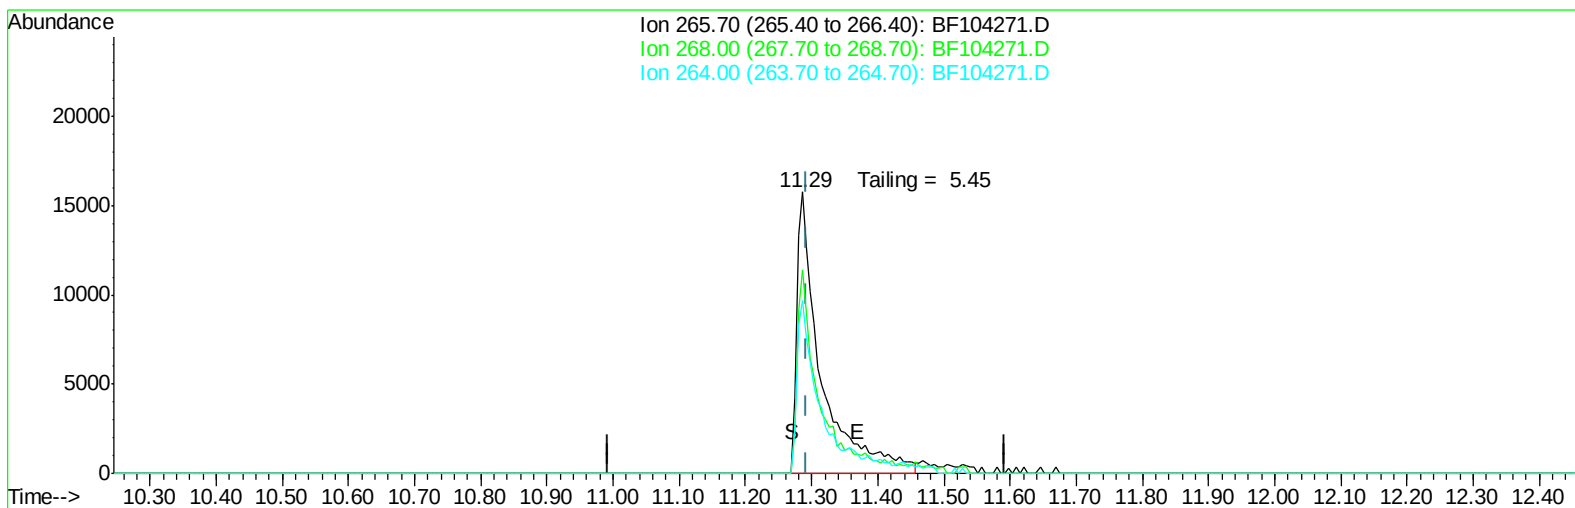

TIC: BF104271.D

(69) Pentachlorophenol (C)




11.286min (-0.006) 21268.58ng

response 40185

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	72.23
264.00	61.90	61.26
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF040518\
Data File : BF104271.D
Acq On : 5 Apr 2018 15:09
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 06:06:44 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 04 18:06:58 2018
Response via : Initial Calibration

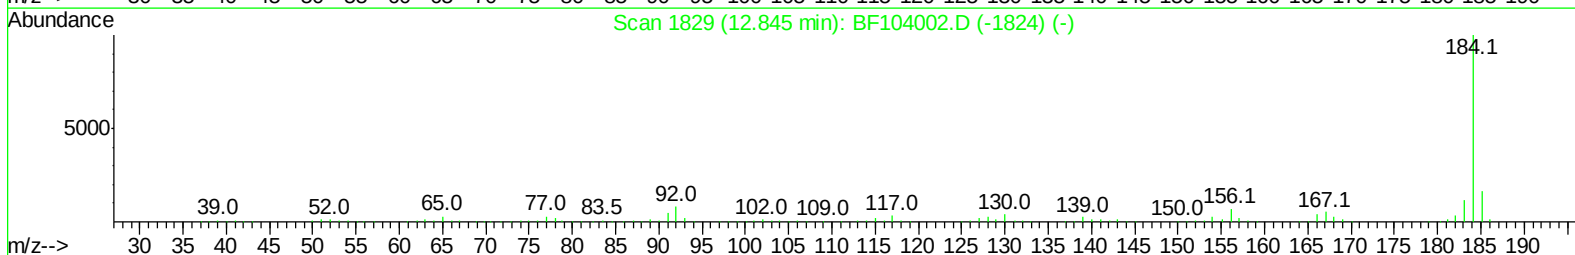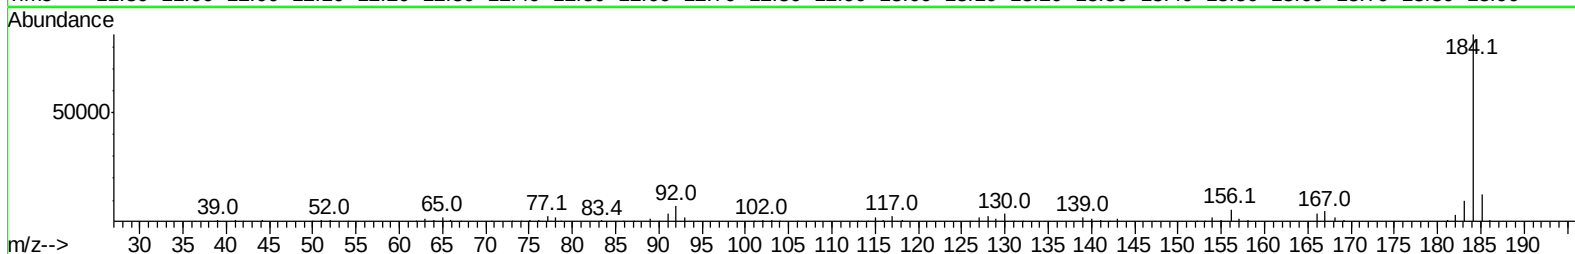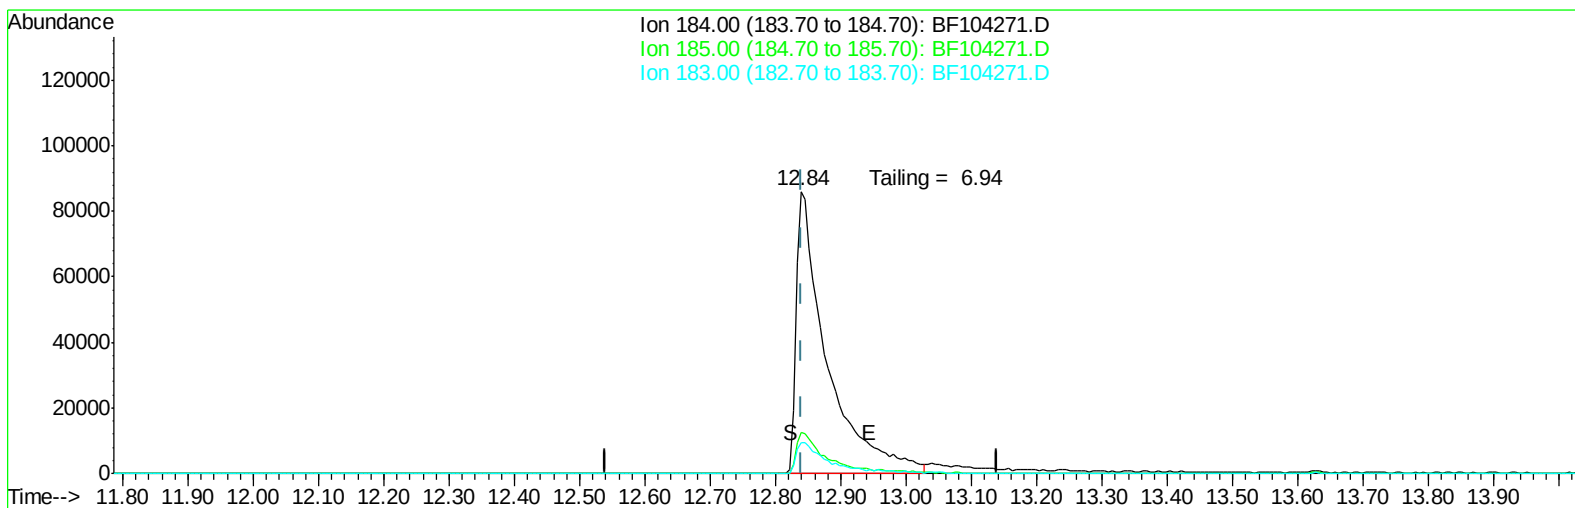

TIC: BF104271.D

(76) Benzidine

12.839min (-0.000) 0.00ng

response 280079

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.46
183.00	11.60	10.99
0.00	0.00	0.00