


Data Path : Z:\HPCHEM1\BNA_F\Data\BF040518\
 Data File : BF104271.D
 Acq On : 5 Apr 2018 15:09
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032818.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 04 18:06:58 2018

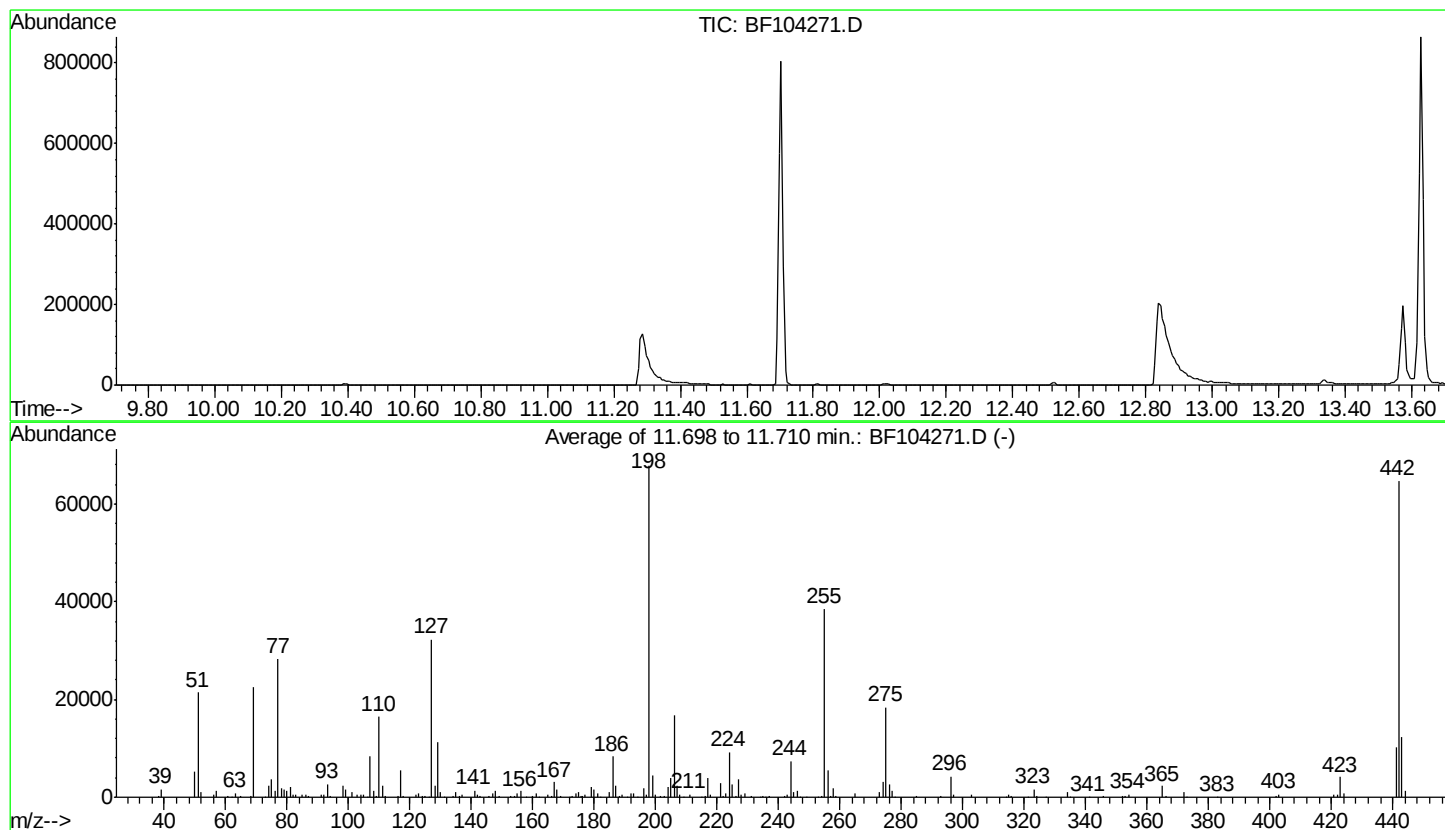

AutoFind: Scans 1634, 1635, 1636; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	21417	PASS
68	69	0.00	2	1.7	393	PASS
69	198	0.00	100	33.2	22537	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.5	32236	PASS
197	198	0.00	2	0.7	497	PASS
198	198	100	100	100.0	67858	PASS
199	198	5	9	6.5	4394	PASS
275	198	10	60	27.2	18457	PASS
365	198	1	100	3.4	2297	PASS
441	443	0.01	100	84.3	10325	PASS
442	198	50	100	95.4	64752	PASS
443	442	15	24	18.9	12255	PASS