

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040519\
 Data File : BF113628.D
 Acq On : 5 Apr 2019 21:24
 Operator : JU/SJ
 Sample : K2245-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Apr 05 23:26:03 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 04:05:31 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.68	152	113728	20.00	ng	0.00
21) Naphthalene-d8	7.96	136	439200	20.00	ng	0.00
39) Acenaphthene-d10	9.71	164	219906	20.00	ng	-0.01
64) Phenanthrene-d10	11.19	188	461779	20.00	ng	-0.01
76) Chrysene-d12	13.82	240	367300	20.00	ng	-0.02
87) Perylene-d12	15.22	264	310207	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	651021	97.61	ng	0.00
7) Phenol-d6	6.33	99	769786	93.65	ng	0.00
23) Nitrobenzene-d5	7.25	82	544565	72.63	ng	-0.01
42) 2,4,6-Tribromophenol	10.50	330	299673	113.44	ng	-0.01
45) 2-Fluorobiphenyl	9.04	172	1045502	76.54	ng	-0.01
79) Terphenyl-d14	12.77	244	1312822	72.77	ng	-0.02
Target Compounds						
19) n-Nitroso-di-n-propylamine	7.25	70	71266	14.060	ng	# 74
25) Isophorone	7.25	82	544559	37.701	ng	# 64
51) 2,6-Dinitrotoluene	9.71	165	28169	7.884	ng	# 26
57) 2,4-Dinitrotoluene	9.71	165	28169	6.518	ng	# 23
67) 4-Bromophenyl-phenylether	10.50	248	17130	3.308	ng	# 1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF040519\
Data File : BF113628.D
Acq On : 5 Apr 2019 21:24
Operator : JU/SJ
Sample : K2245-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :

Quant Time: Apr 05 23:26:03 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

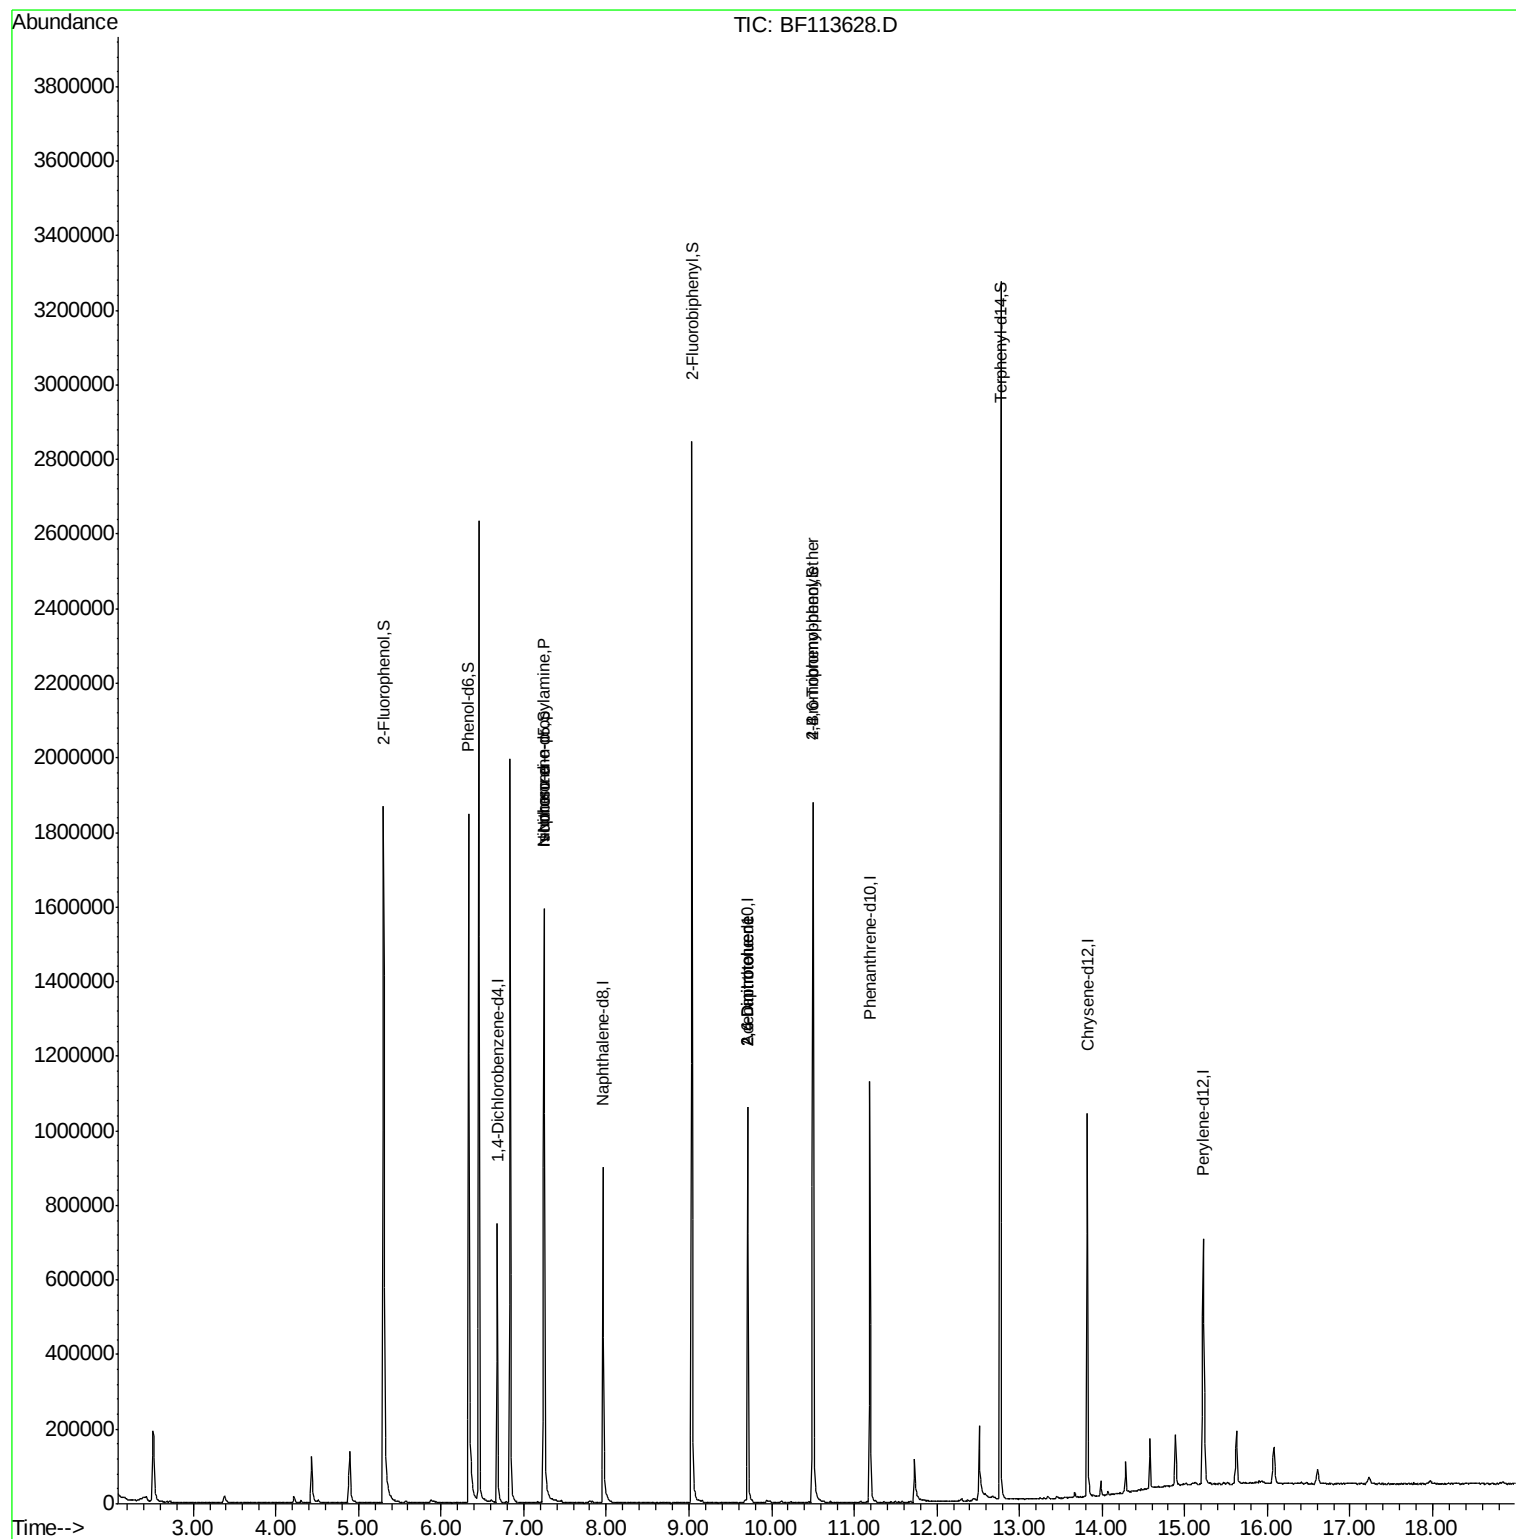




#1



1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.68 min Scan# 781
 Delta R.T. -0.01 min
 Lab File: BF113628.D
 Acq: 5 Apr 2019 21:24

Instrument :
 BNA_F
 ClientSampleId :

Tot Ion:152 Resp: 113728
 Ion Ratio Lower Upper
 152 100
 150 157.9 124.7 187.1
 115 56.6 46.0 69.0

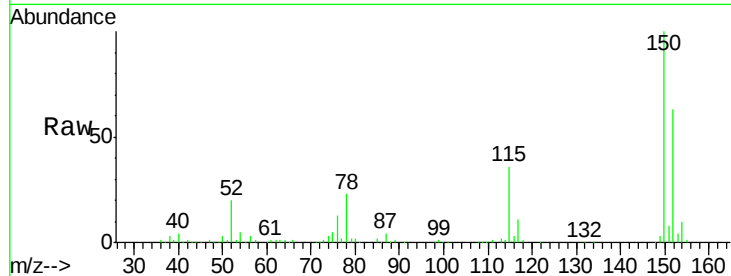


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

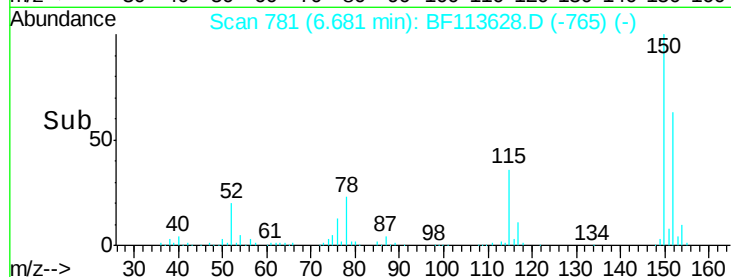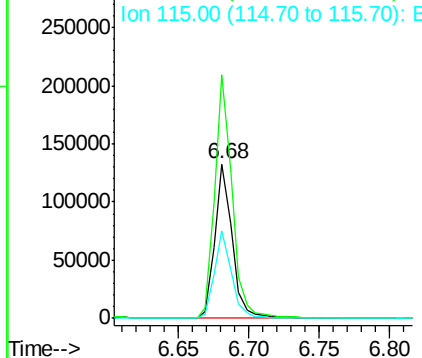



#5


2-Fluorophenol
 Concen: 97.614 ng
 RT: 5.30 min Scan# 547
 Delta R.T. 0.01 min
 Lab File: BF113628.D
 Acq: 5 Apr 2019 21:24

Tgt Ion:112 Resp: 651021
 Ion Ratio Lower Upper
 112 100
 64 59.7 49.2 73.8
 63 30.2 24.9 37.3

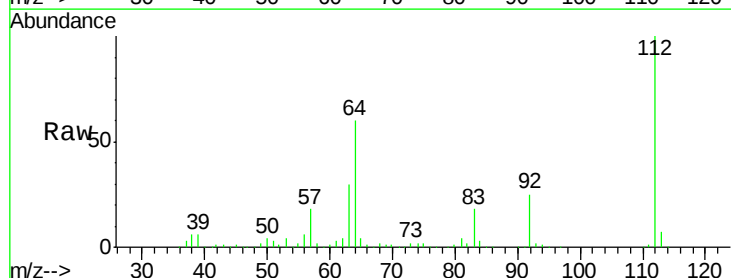

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

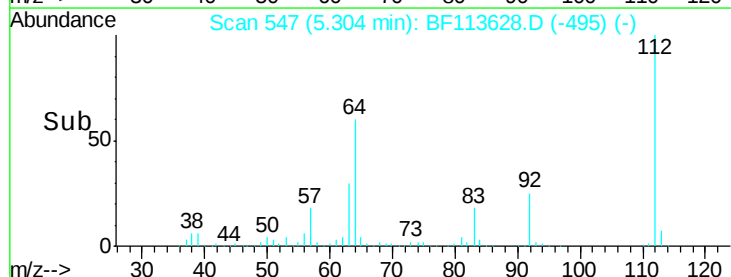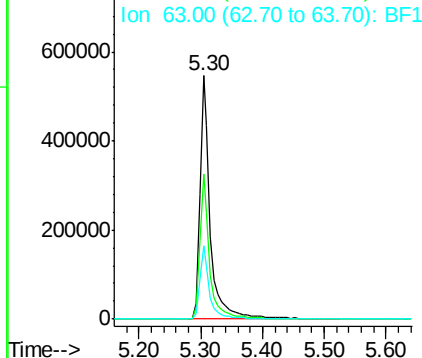

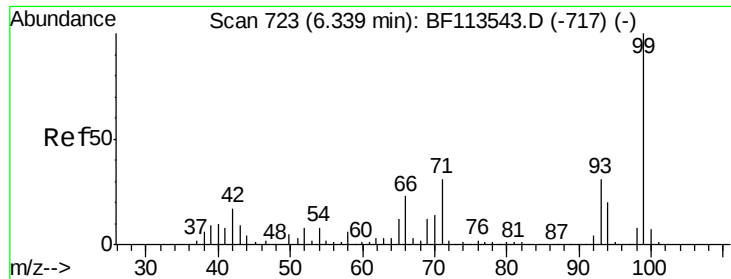

#7

Phenol-d6

Concen: 93.648 ng

RT: 6.33 min Scan# 722

Delta R.T. -0.01 min

Lab File: BF113628.D

Acq: 5 Apr 2019 21:24

Instrument :

BNA_F

ClientSampled :


Tot Ion: 99 Resp: 769786

Ion Ratio Lower Upper

99 100

42 18.1 14.8 22.2




71 31.1 24.9 37.3

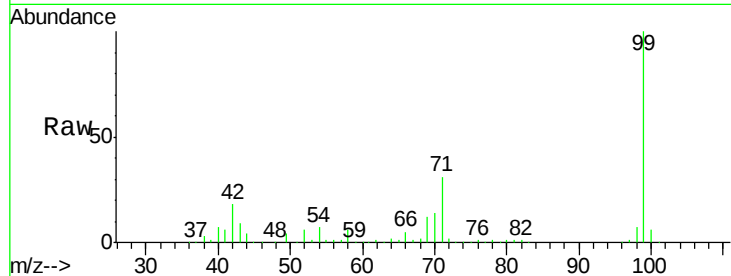

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

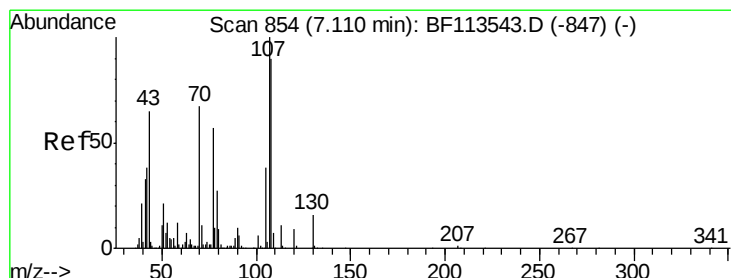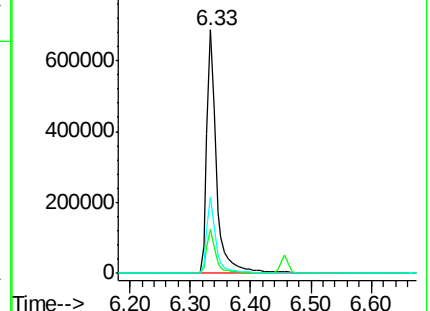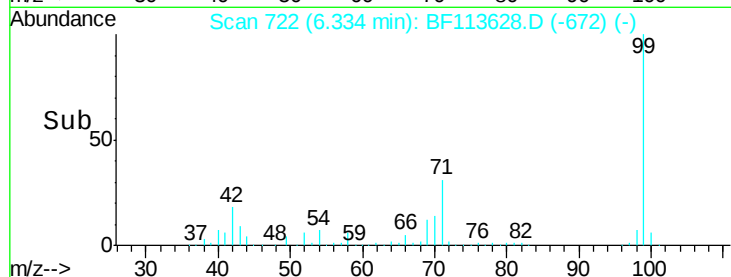

#19

n-Nitroso-di-n-propylamine

Concen: 14.060 ng

RT: 7.25 min Scan# 877

Delta R.T. 0.14 min

Lab File: BF113628.D

Acq: 5 Apr 2019 21:24

Tgt Ion: 70 Resp: 71266


Ion Ratio Lower Upper

70 100

42 45.3 48.4 72.6#

101 0.0 7.8 11.8#

130 2.1 18.2 27.4#


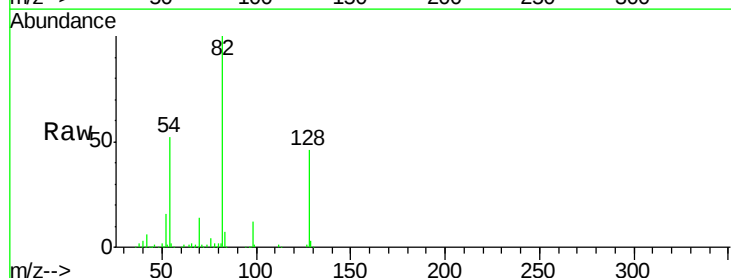


Abundance Ion 70.00 (69.70 to 70.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 101.00 (100.70 to 101.70): BF1

Ion 130.00 (129.70 to 130.70): BF1

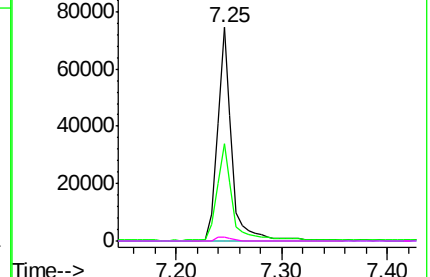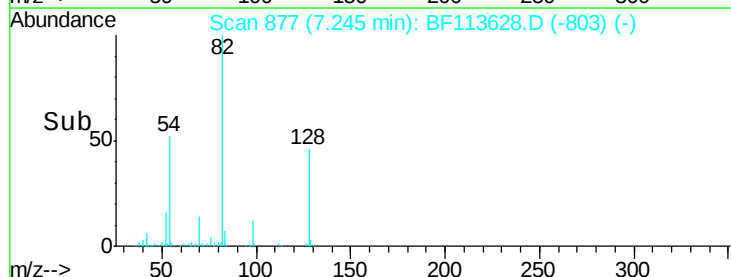



#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.96 min Scan# 999

Delta R.T. -0.01 min

Lab File: BF113628.D

Acq: 5 Apr 2019 21:24

Instrument :

BNA_F

ClientSampleId :

Tot Ion:136 Resp: 439200


Ion Ratio Lower Upper

136 100

137 10.5 8.9 13.3

54 7.8 7.0 10.6

68 6.1 4.8 7.2


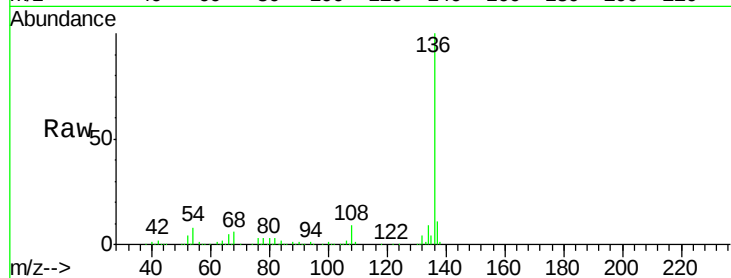


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

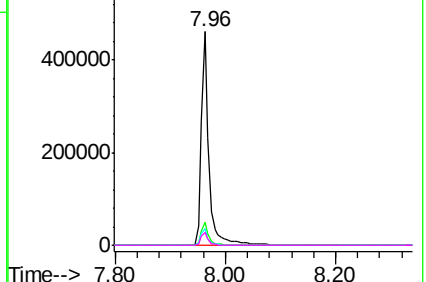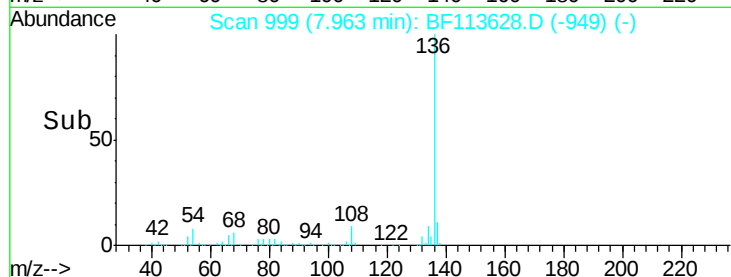

#23

Nitrobenzene-d5

Concen: 72.628 ng

RT: 7.25 min Scan# 877

Delta R.T. -0.01 min

Lab File: BF113628.D

Acq: 5 Apr 2019 21:24


Tgt Ion: 82 Resp: 544565

Ion Ratio Lower Upper

82 100

128 46.0 36.5 54.7



54 52.2 42.2 63.2

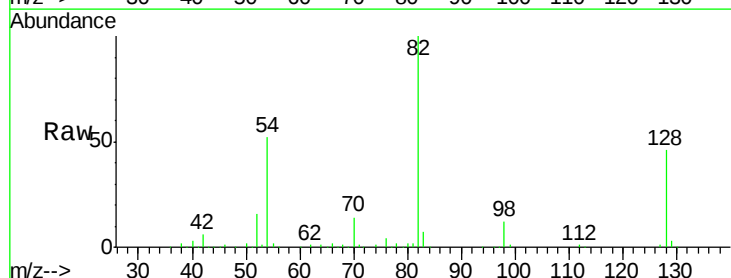


Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BF1

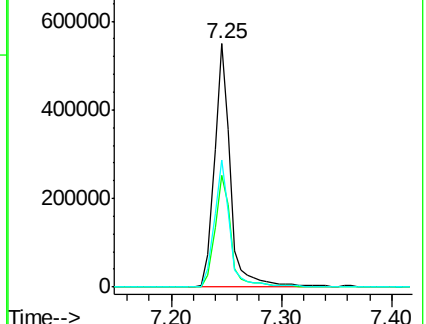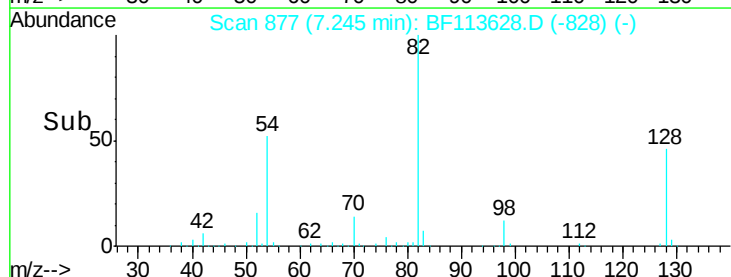

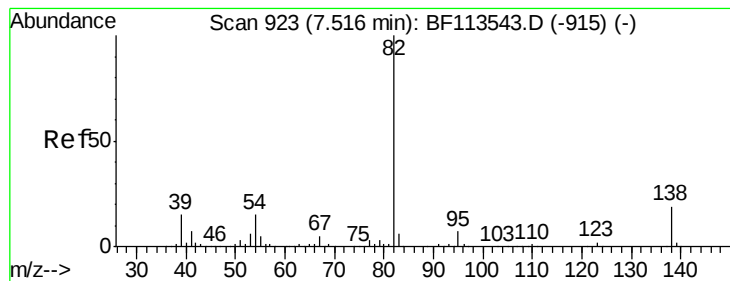

#25

Isophorone

Concen: 37.701 ng

RT: 7.25 min Scan# 877

Delta R.T. -0.27 min

Lab File: BF113628.D

Acq: 5 Apr 2019 21:24

Instrument :

BNA_F

ClientSampleId :


Tot Ion: 82 Resp: 544559

Ion Ratio Lower Upper

82 100

95 0.0 5.5 8.3#




138 0.0 15.2 22.8#

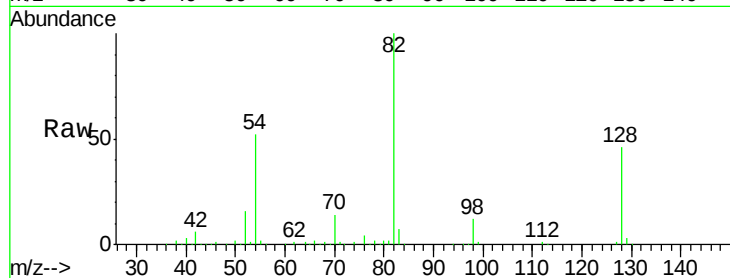

Abundance Ion 82.00 (81.70 to 82.70): BF1

Ion 95.00 (94.70 to 95.70): BF1

Ion 138.00 (137.70 to 138.70): BF1

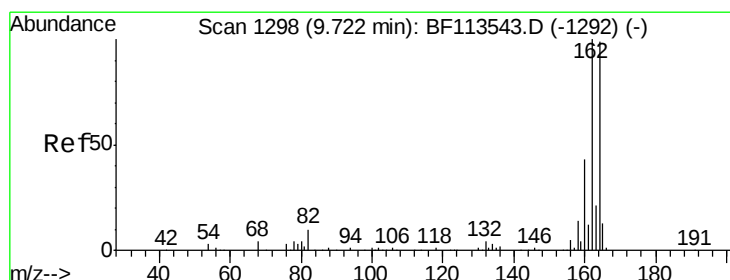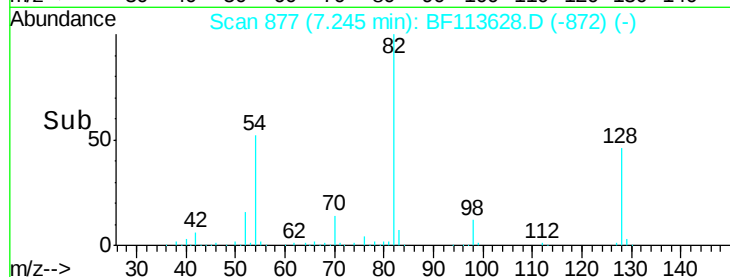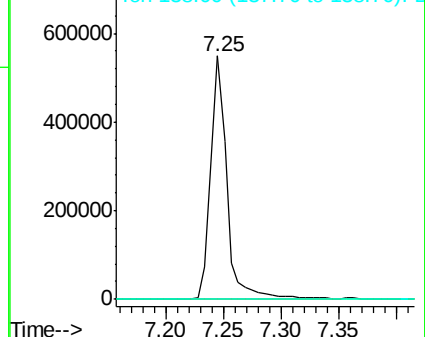

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.71 min Scan# 1296

Delta R.T. -0.01 min

Lab File: BF113628.D

Acq: 5 Apr 2019 21:24


Tgt Ion:164 Resp: 219906

Ion Ratio Lower Upper

164 100

162 100.2 81.8 122.6



160 43.9 36.4 54.6

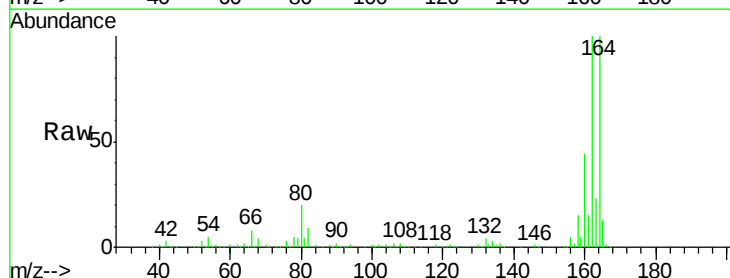

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E



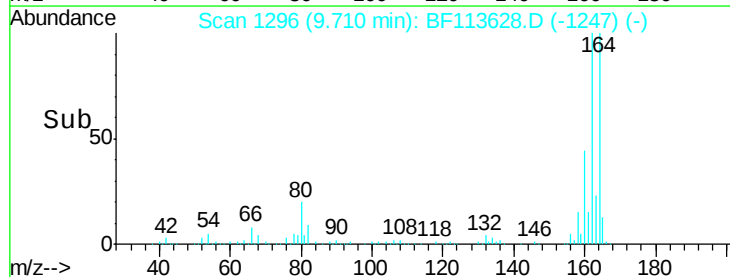
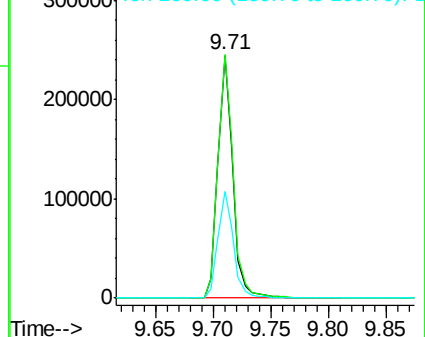




#42
 2,4,6-Tribromophenol
 Concen: 113.443 ng
 RT: 10.50 min Scan# 1431
 Delta R.T. -0.01 min
 Lab File: BF113628.D
 Acq: 5 Apr 2019 21:24




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
330	100		
332	96.9	77.8	116.6
141	27.8	22.7	34.1

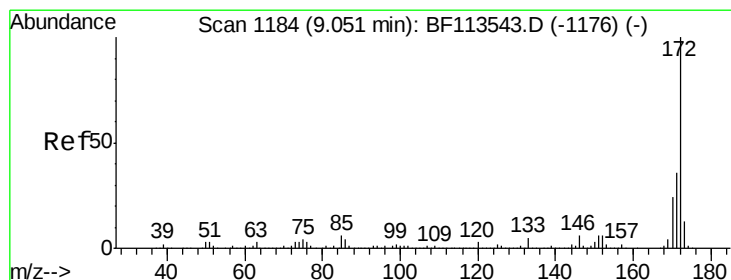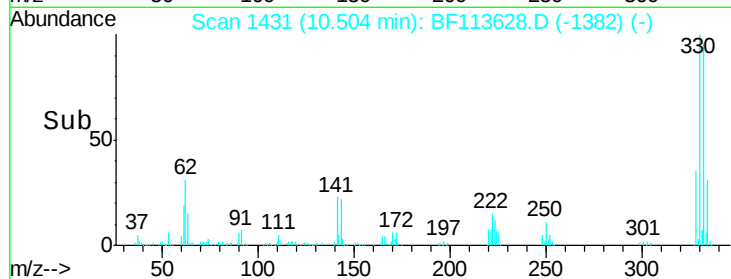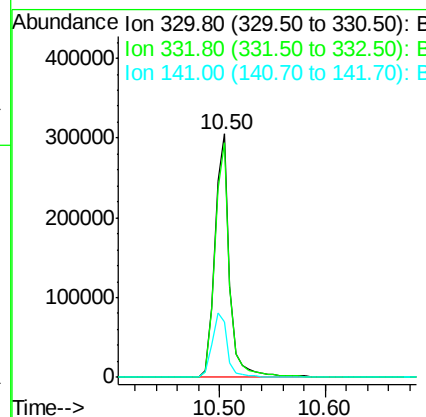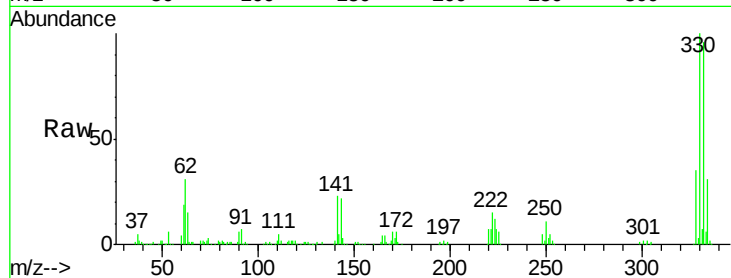

#45
 2-Fluorobiphenyl
 Concen: 76.539 ng
 RT: 9.04 min Scan# 1182
 Delta R.T. -0.01 min
 Lab File: BF113628.D
 Acq: 5 Apr 2019 21:24

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.2	29.0	43.6
170	23.9	19.5	29.3


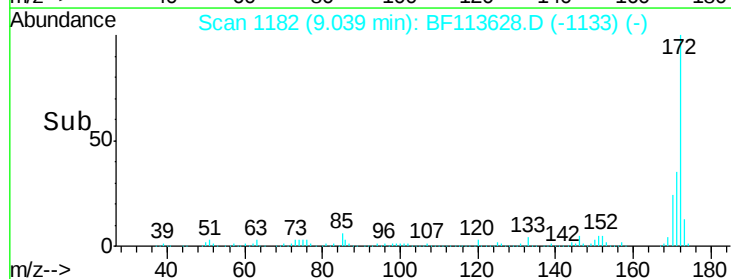
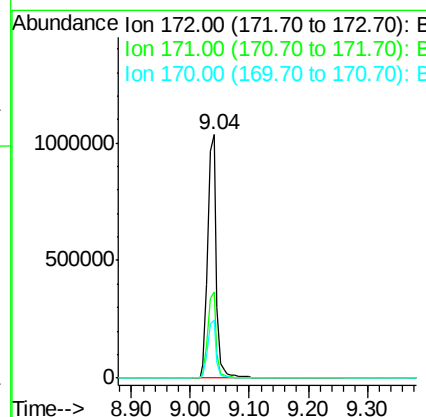
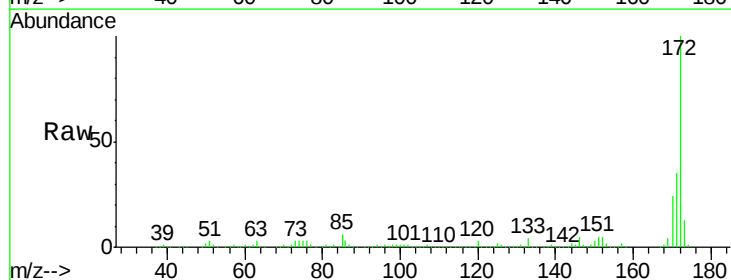


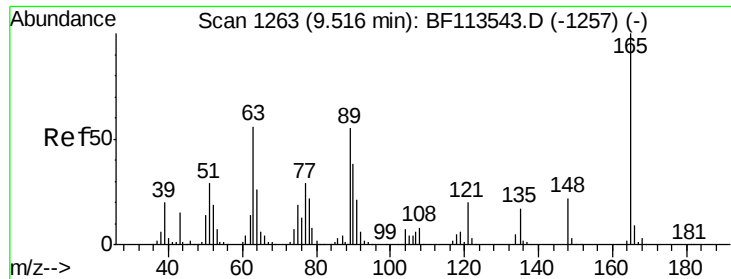

#51
 2,6-Dinitrotoluene
 Concen: 7.884 ng
 RT: 9.71 min Scan# 1296
 Delta R.T. 0.19 min
 Lab File: BF113628.D
 Acq: 5 Apr 2019 21:24




Instrument :
 BNA_F
 ClientSampleId :


Tot Ion	Ratio	Lower	Upper
165	100		
63	1.0	43.4	65.0#
89	1.4	43.1	64.7#

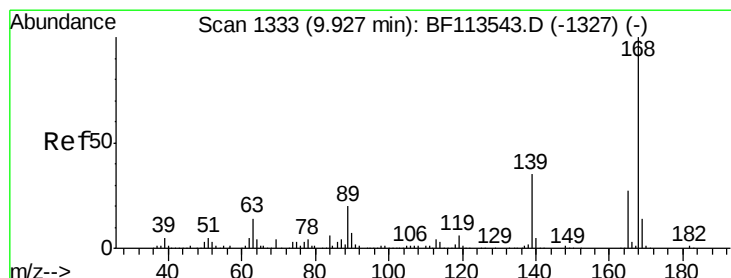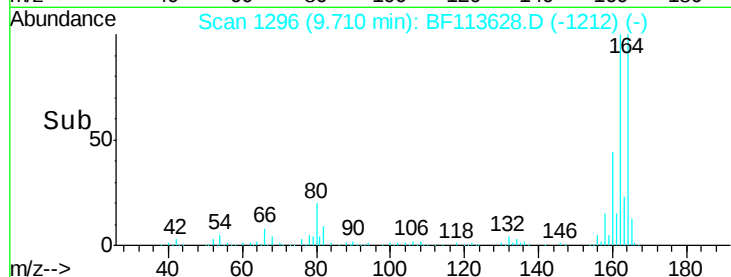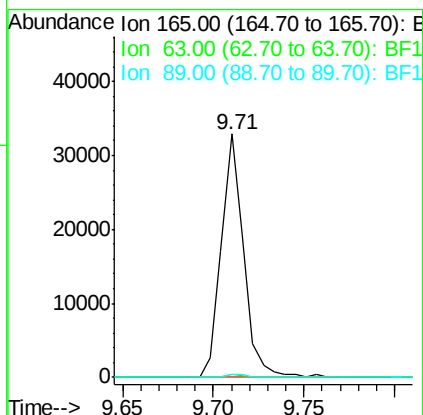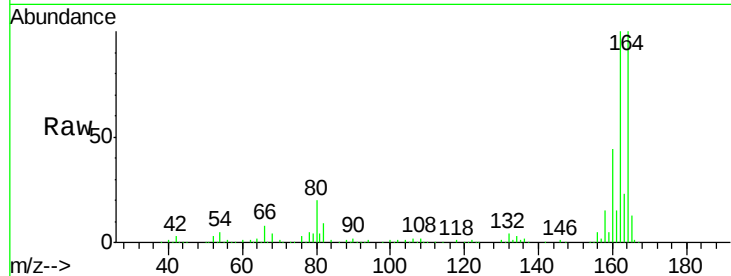

#57
 2,4-Dinitrotoluene
 Concen: 6.518 ng
 RT: 9.71 min Scan# 1296
 Delta R.T. -0.22 min
 Lab File: BF113628.D
 Acq: 5 Apr 2019 21:24

Tgt Ion	Ratio	Lower	Upper
165	100		
63	1.0	37.5	56.3#
89	1.4	57.4	86.2#
182	0.0	2.0	3.0#


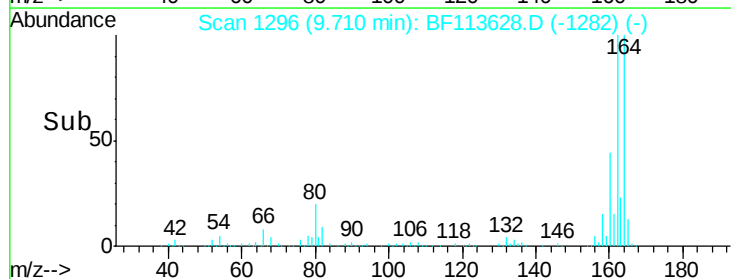
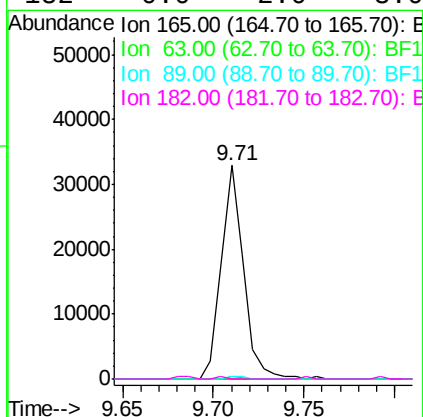
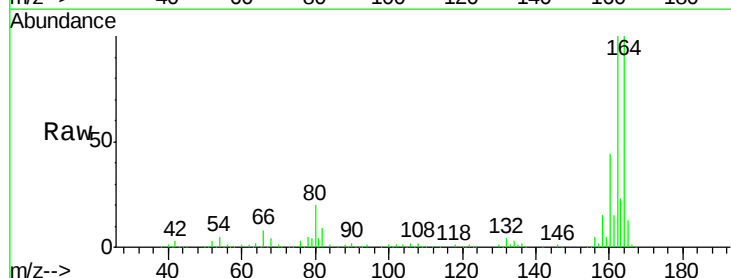


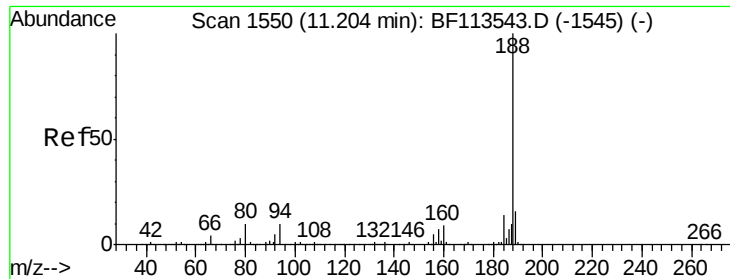

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.19 min Scan# 1548
Delta R.T. -0.01 min
Lab File: BF113628.D
Acq: 5 Apr 2019 21:24




Instrument :
BNA_F
ClientSampleId :


Tot Ion:188 Resp: 461779
Ion Ratio Lower Upper
188 100
94 9.0 7.0 10.6
80 8.7 7.7 11.5

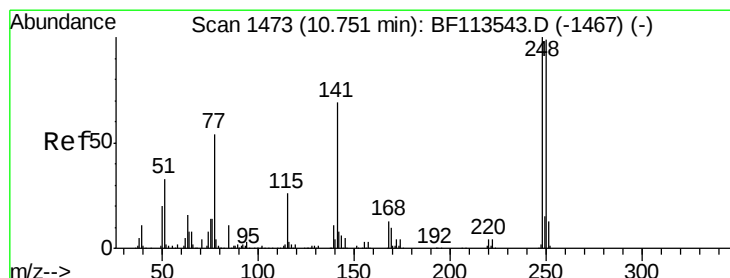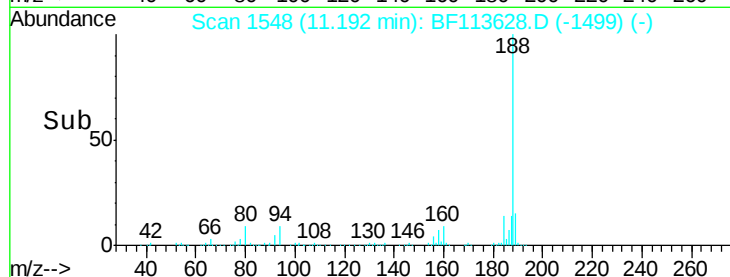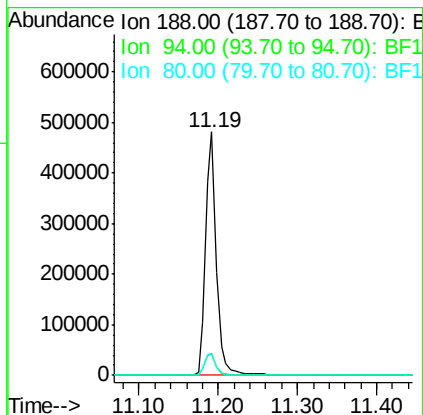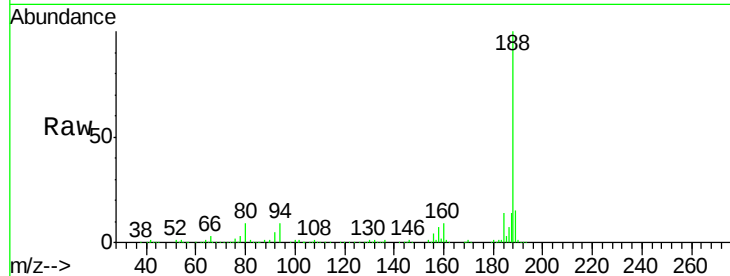

#67
4-Bromophenyl-phenylether
Concen: 3.308 ng
RT: 10.50 min Scan# 1431
Delta R.T. -0.25 min
Lab File: BF113628.D
Acq: 5 Apr 2019 21:24

Tgt Ion:248 Resp: 17130
Ion Ratio Lower Upper
248 100
250 198.9 78.3 117.5#
141 420.8 56.2 84.4#


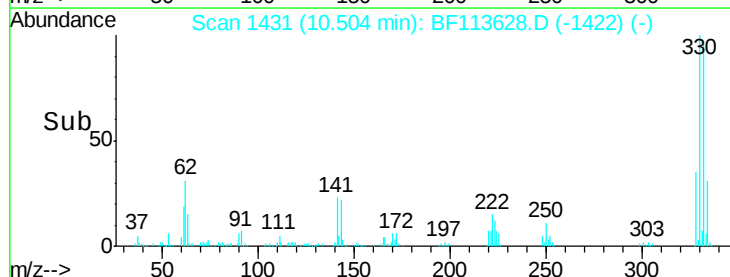
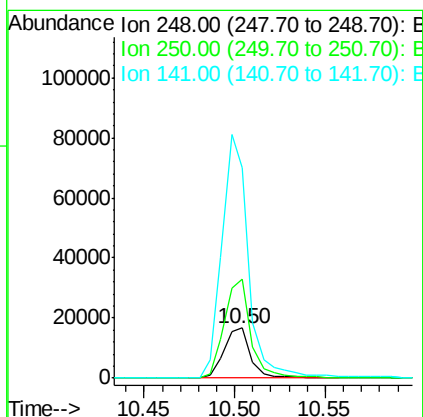
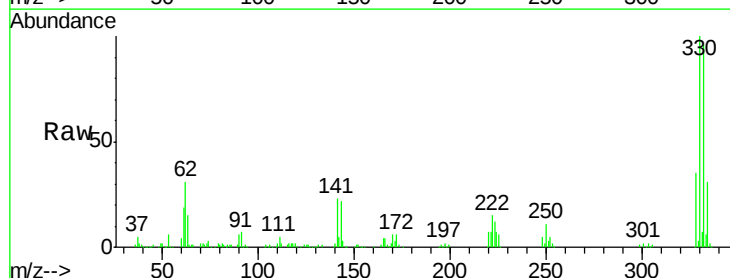


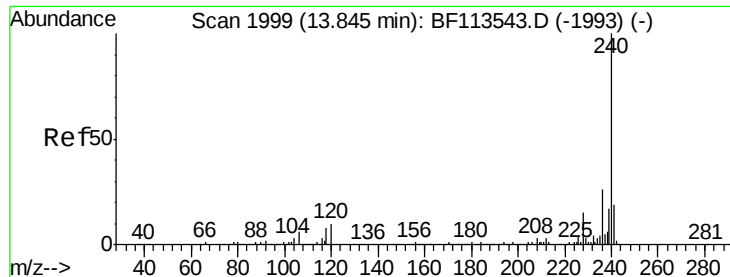

#76
 Chrysene-d12
 Concen: 20.000 ng
 RT: 13.82 min Scan# 1995
 Delta R.T. -0.02 min
 Lab File: BF113628.D
 Acq: 5 Apr 2019 21:24




Instrument :
 BNA_F
 ClientSampleID :




Tot Ion:240 Resp: 367300
 Ion Ratio Lower Upper
 240 100
 120 10.0 8.8 13.2
 236 25.7 20.9 31.3

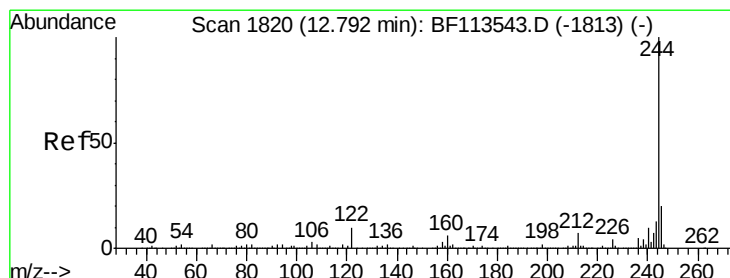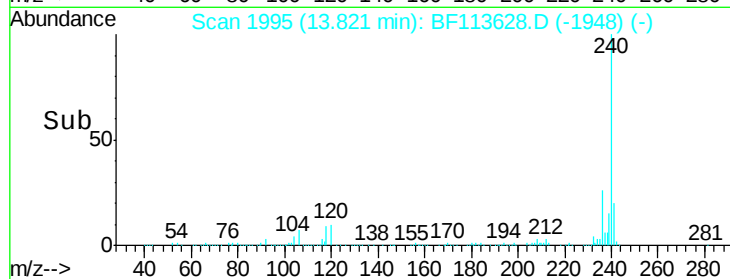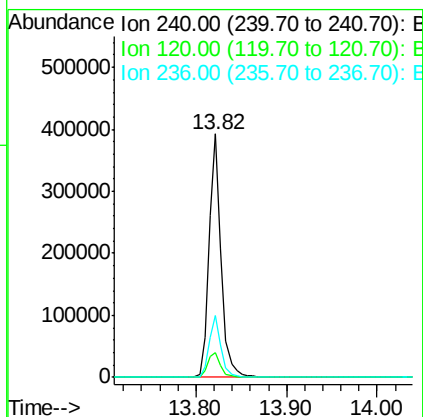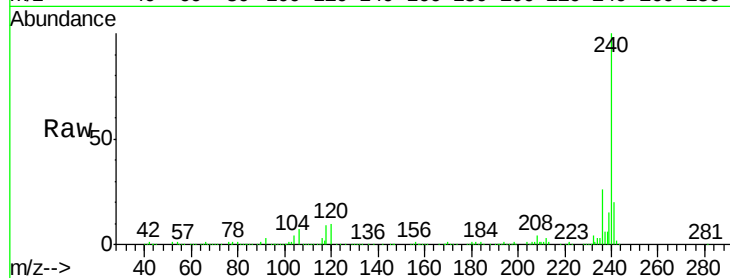

#79
 Terphenyl-d14
 Concen: 72.772 ng
 RT: 12.77 min Scan# 1817
 Delta R.T. -0.02 min
 Lab File: BF113628.D
 Acq: 5 Apr 2019 21:24

Tgt Ion:244 Resp: 1312822
 Ion Ratio Lower Upper
 244 100
 212 6.4 5.5 8.3
 122 9.8 8.6 13.0

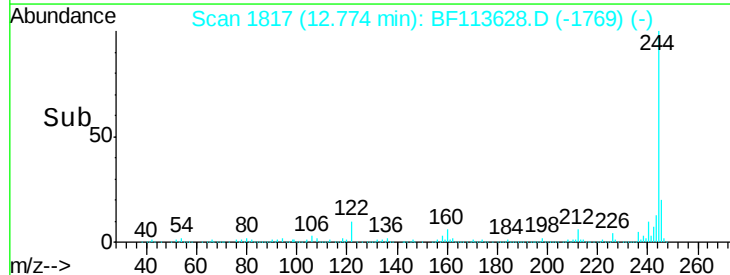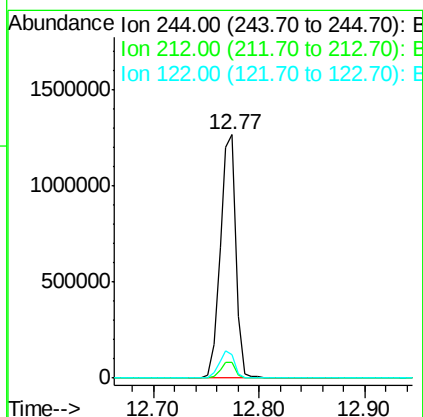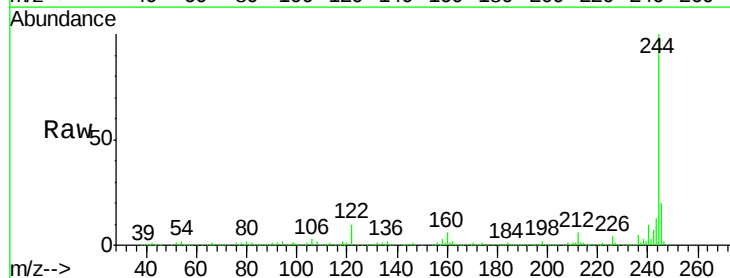

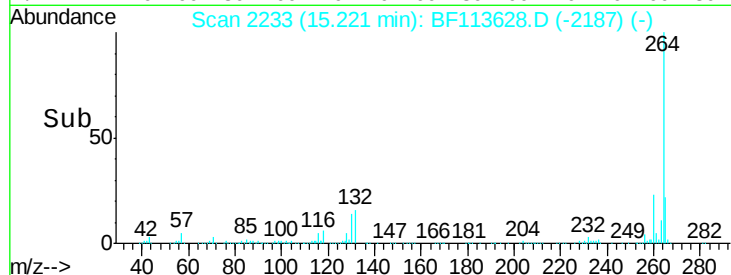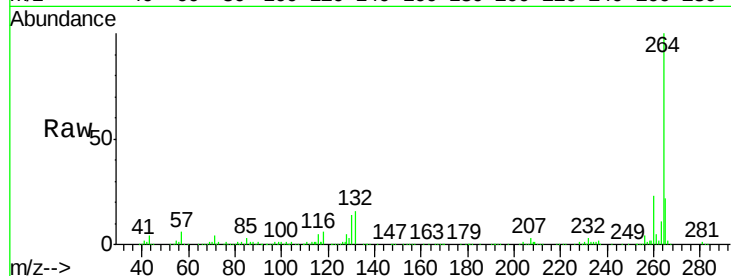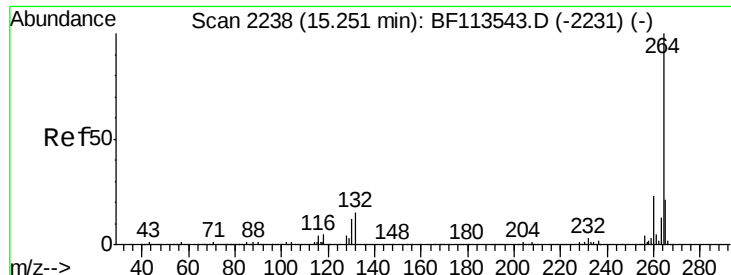

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.22 min Scan# 2233
Delta R.T. -0.03 min
Lab File: BF113628.D
Acq: 5 Apr 2019 21:24

Instrument :
BNA_F
ClientSampleId :

Tot Ion:	264	Resp:	310207
Ion	Ratio	Lower	Upper
264	100		
260	23.4	19.1	28.7
265	21.5	17.1	25.7

