
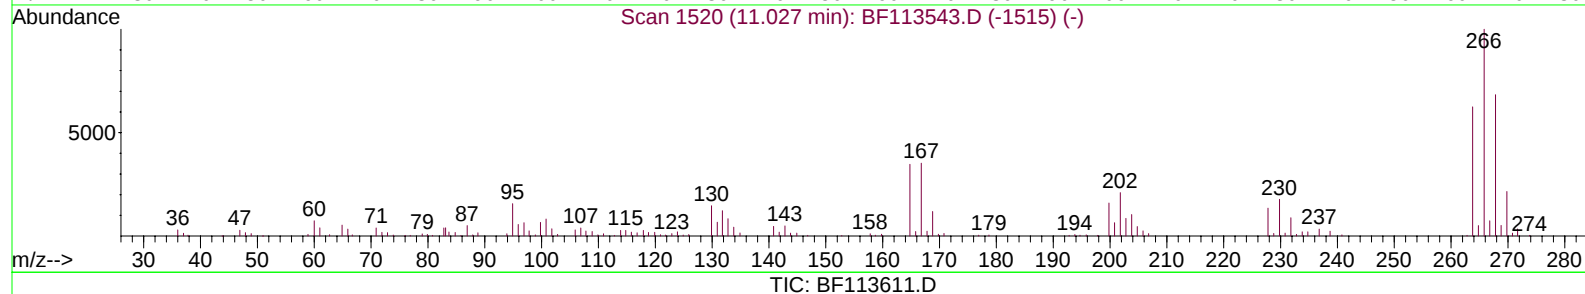
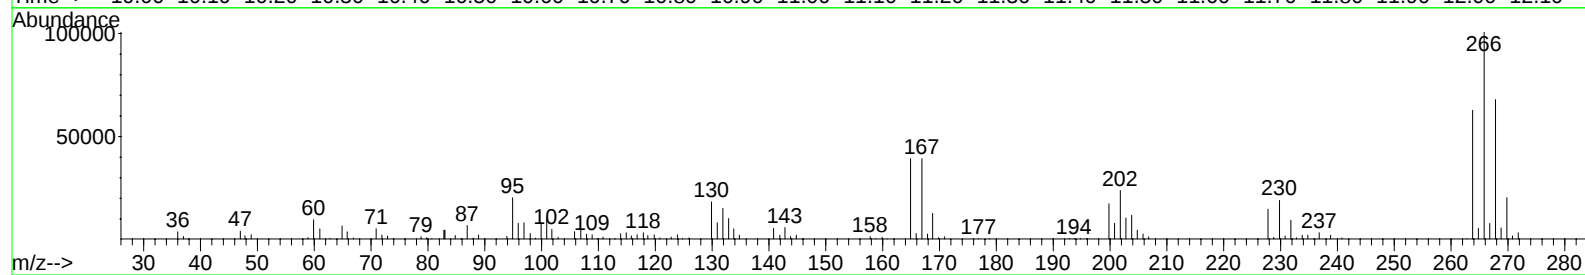


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF040519\
Data File : BF113611.D
Acq On : 5 Apr 2019 9:16
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 19:08:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

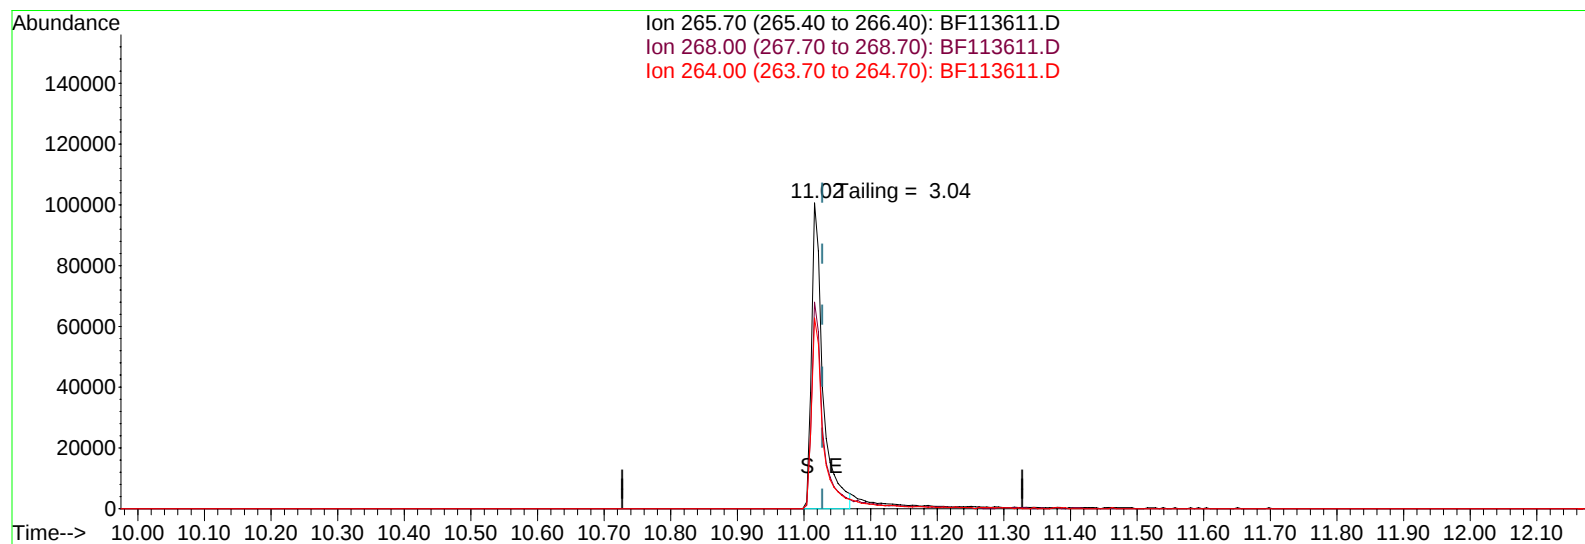

(70) Pentachlorophenol (C)




11.016min (-0.012) 52643.07ng

response 132293

Ion	Exp%	Act%
265.70	100	100
268.00	67.20	67.53
264.00	61.50	62.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF040519\
Data File : BF113611.D
Acq On : 5 Apr 2019 9:16
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 05 19:08:08 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

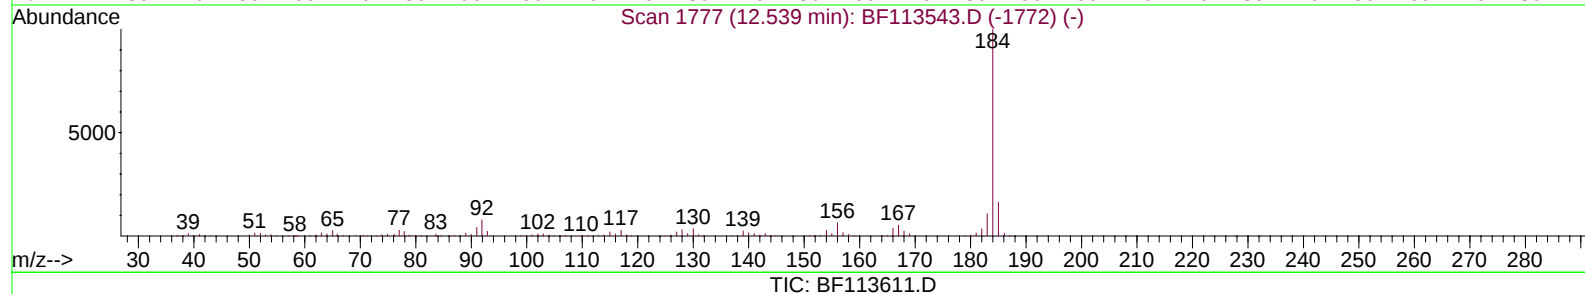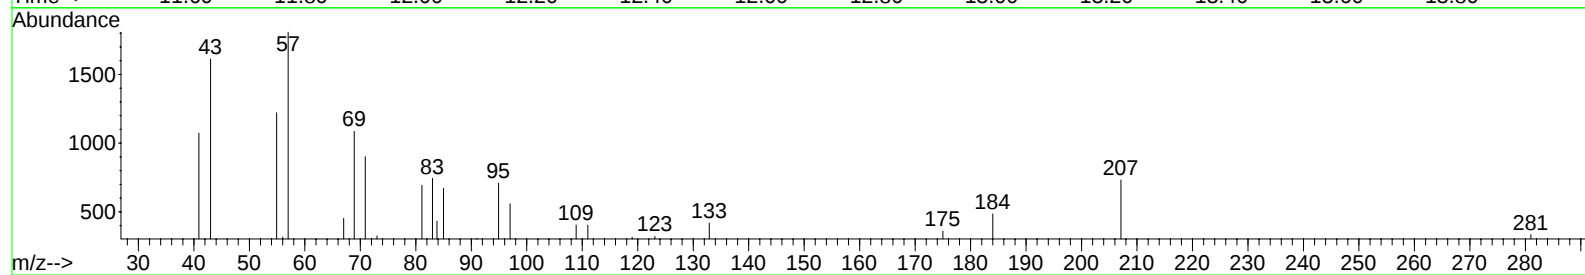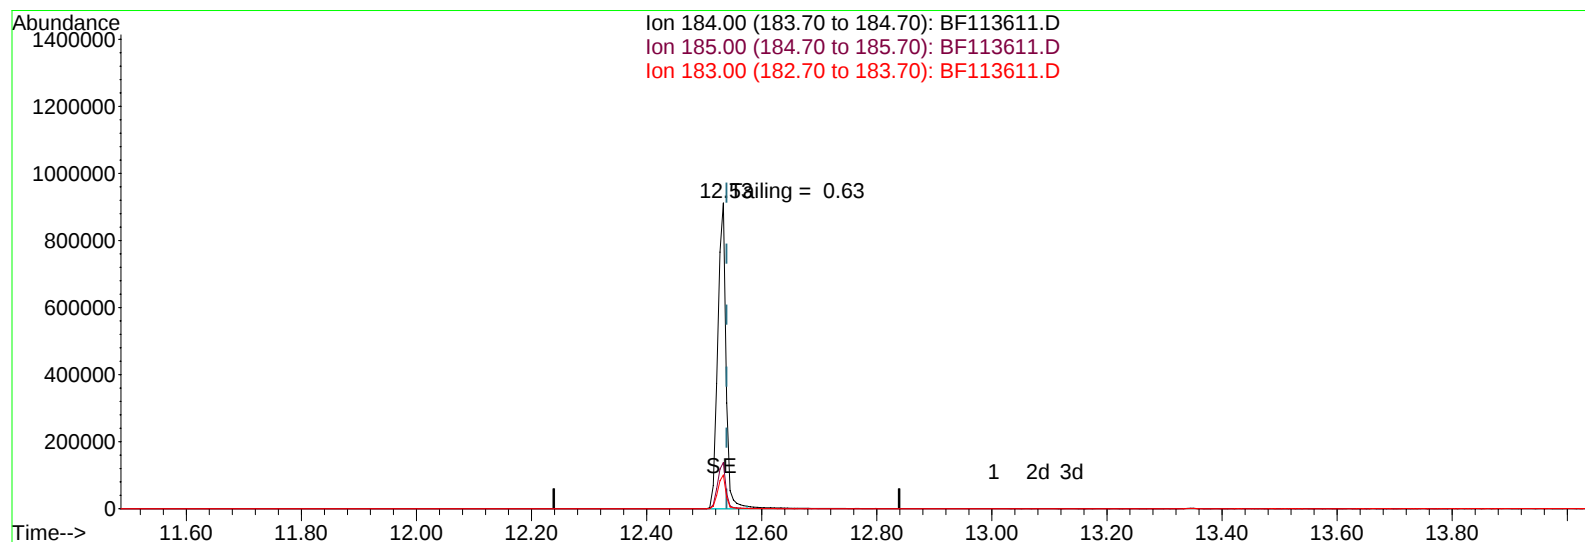

(77) Benzidine

13.004min (+0.465) 239.84ng

response 990

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	0.00#
183.00	11.20	0.00#
0.00	0.00	0.00