

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040519\
 Data File : BF113631.D
 Acq On : 5 Apr 2019 22:49
 Operator : JU/SJ
 Sample : K2245-16
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TP-3D

Quant Time: Apr 06 01:41:58 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 04 04:05:31 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.68	152	118997	20.00	ng	0.00
21) Naphthalene-d8	7.96	136	458690	20.00	ng	0.00
39) Acenaphthene-d10	9.71	164	227494	20.00	ng	-0.01
64) Phenanthrene-d10	11.19	188	476258	20.00	ng	-0.01
76) Chrysene-d12	13.82	240	370658	20.00	ng	-0.02
87) Perylene-d12	15.22	264	326437	20.00	ng	-0.03
System Monitoring Compounds						
5) 2-Fluorophenol	5.30	112	710435	101.81	ng	0.00
7) Phenol-d6	6.33	99	809217	94.09	ng	0.00
23) Nitrobenzene-d5	7.25	82	656414	83.82	ng	-0.01
42) 2,4,6-Tribromophenol	10.50	330	346151	126.67	ng	-0.01
45) 2-Fluorobiphenyl	9.04	172	1203454	85.16	ng	-0.01
79) Terphenyl-d14	12.77	244	1455677	79.96	ng	-0.02


Target Compounds	Qvalue
------------------	--------

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040519\
Data File : BF113631.D
Acq On : 5 Apr 2019 22:49
Operator : JU/SJ
Sample : K2245-16
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TP-3D

Quant Time: Apr 06 01:41:58 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 04 04:05:31 2019
Response via : Initial Calibration

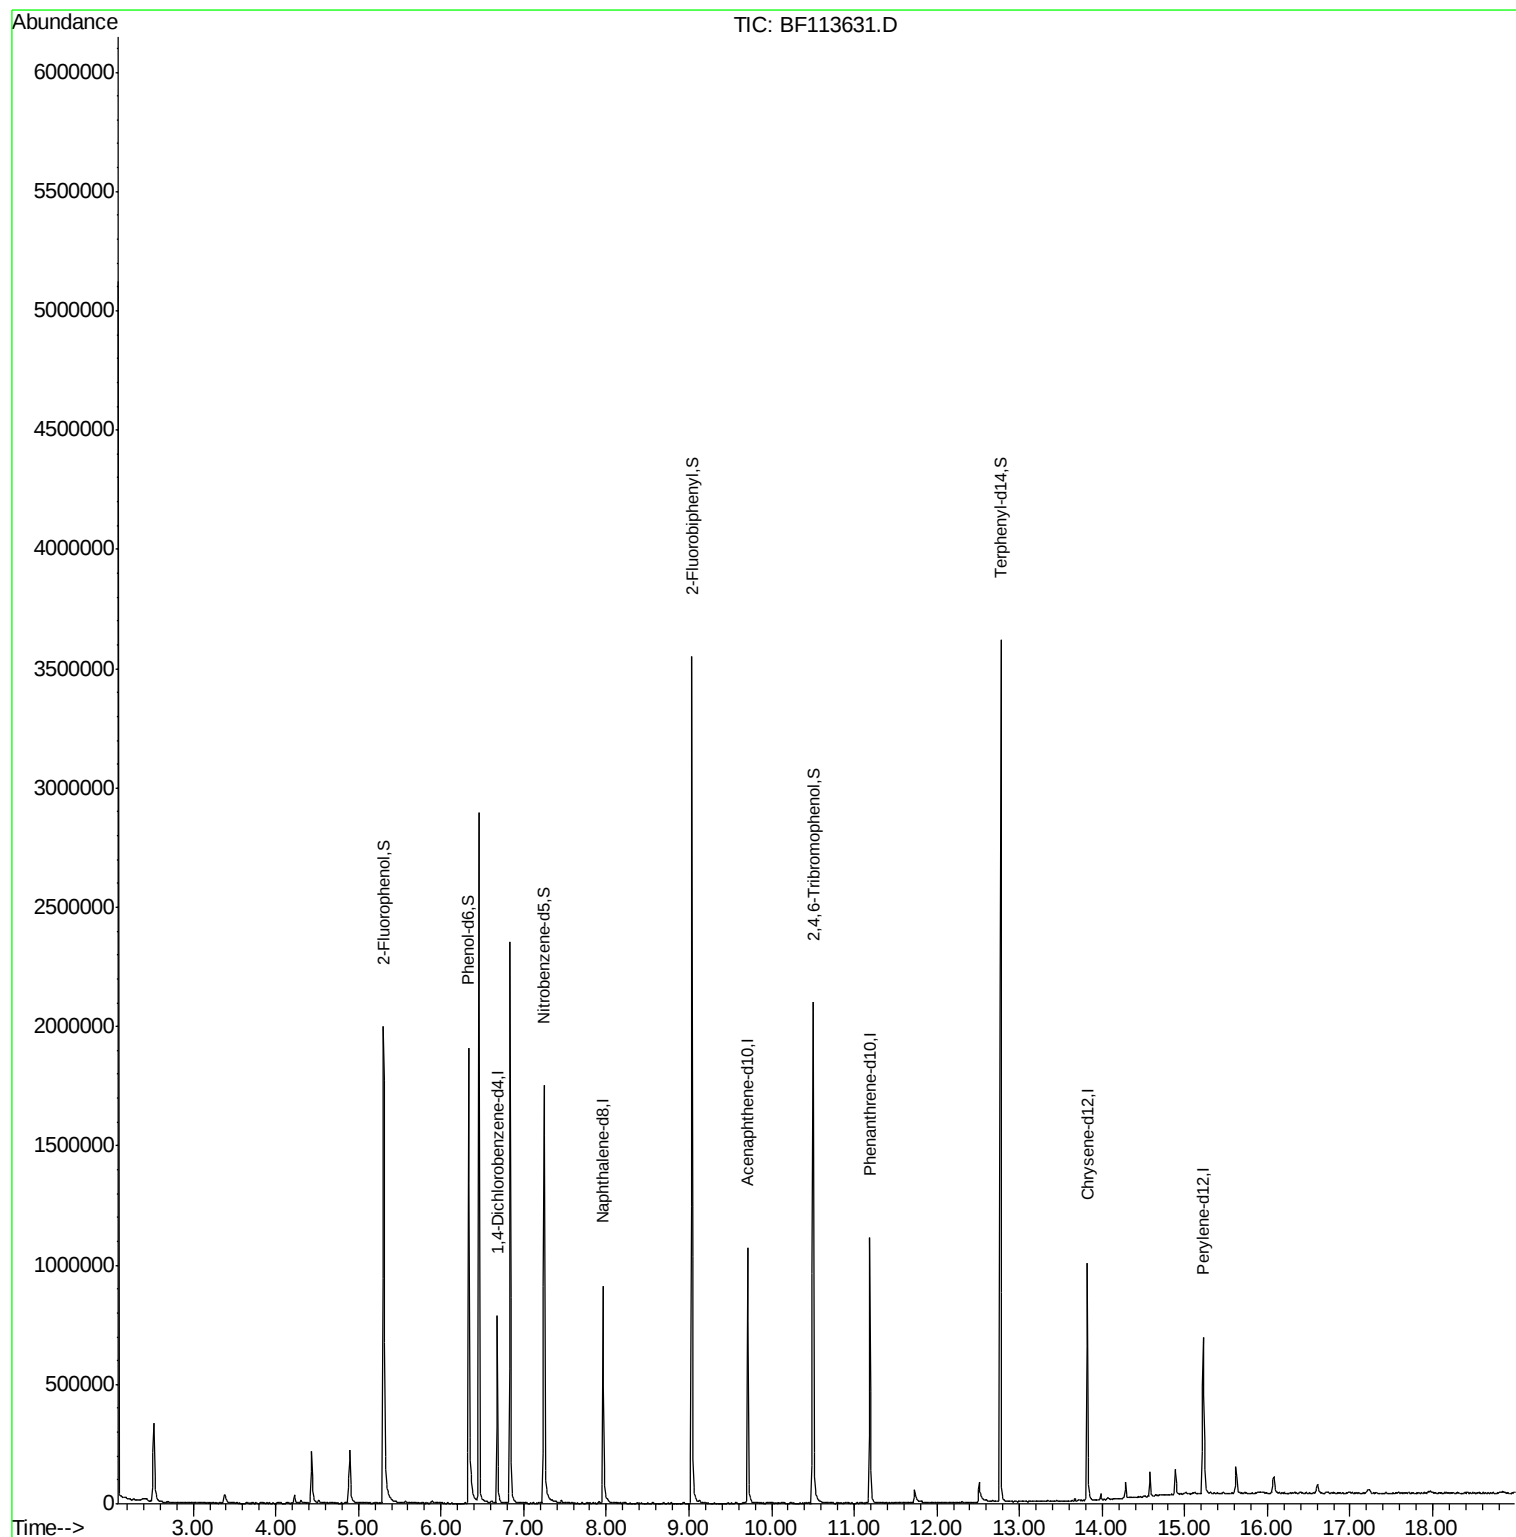







#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.68 min Scan# 781
 Delta R.T. -0.01 min
 Lab File: BF113631.D
 Acq: 5 Apr 2019 22:49

Instrument :
 BNA_F
 ClientSampleId :
 TP-3D

Tgt Ion:152 Resp: 118997
 Ion Ratio Lower Upper
 152 100
 150 158.9 124.7 187.1
 115 56.9 46.0 69.0

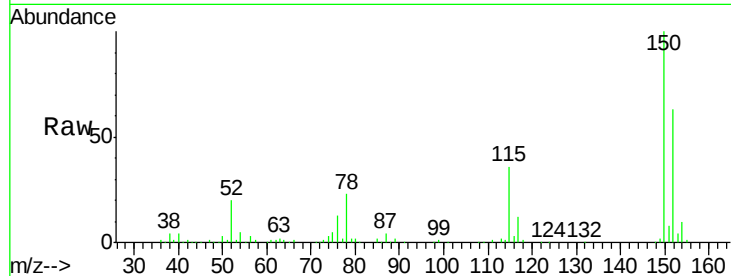


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

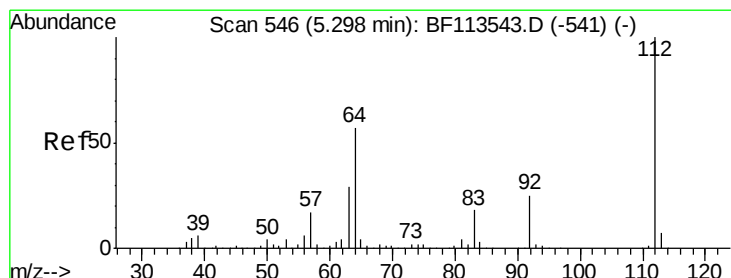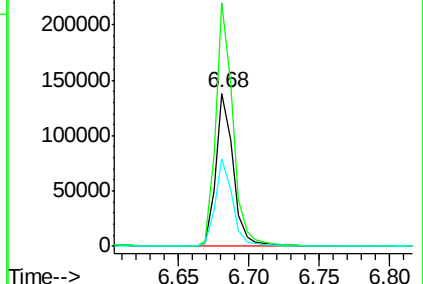
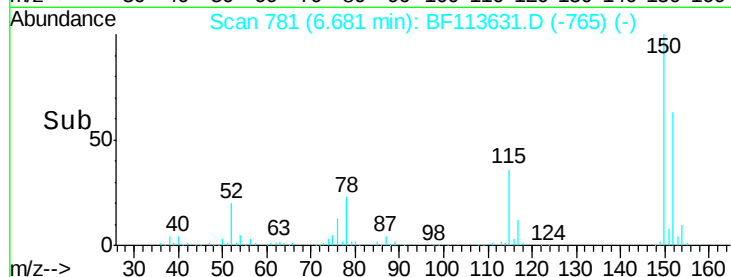



#5
 2-Fluorophenol
 Concen: 101.806 ng
 RT: 5.30 min Scan# 547
 Delta R.T. 0.01 min
 Lab File: BF113631.D
 Acq: 5 Apr 2019 22:49

Tgt Ion:112 Resp: 710435
 Ion Ratio Lower Upper
 112 100
 64 60.2 49.2 73.8
 63 30.7 24.9 37.3

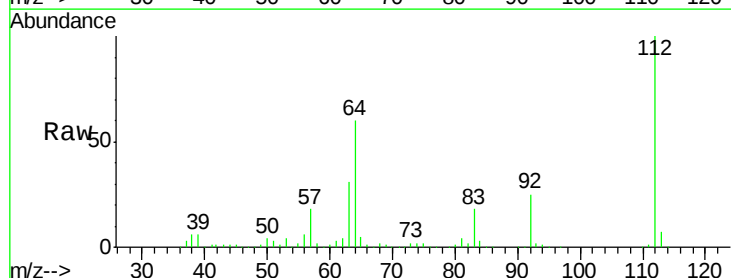

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

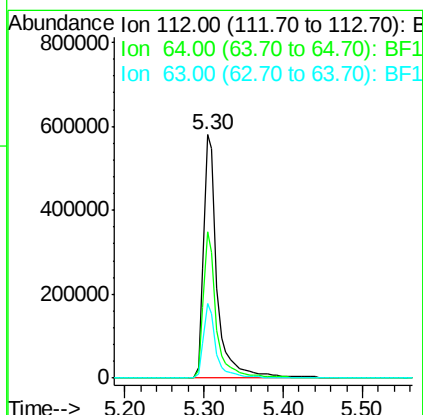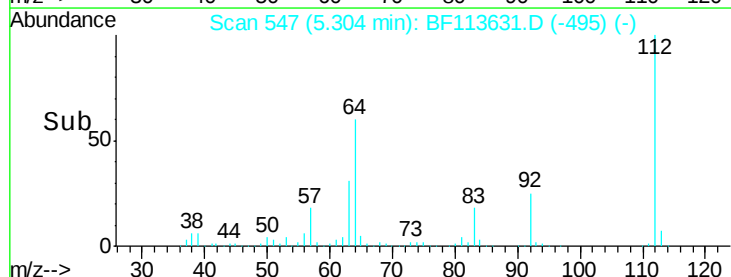

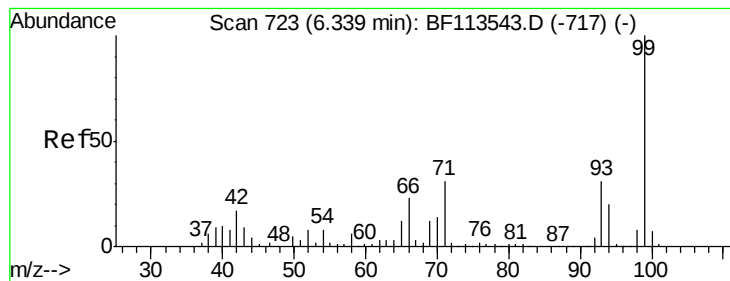

#7

Phenol-d6

Concen: 94.086 ng

RT: 6.33 min Scan# 722

Delta R.T. -0.01 min

Lab File: BF113631.D

Acq: 5 Apr 2019 22:49

Instrument :

BNA_F

ClientSampleId :

TP-3D


Tgt Ion: 99 Resp: 809217

Ion Ratio Lower Upper

99 100

42 18.0 14.8 22.2




71 31.1 24.9 37.3

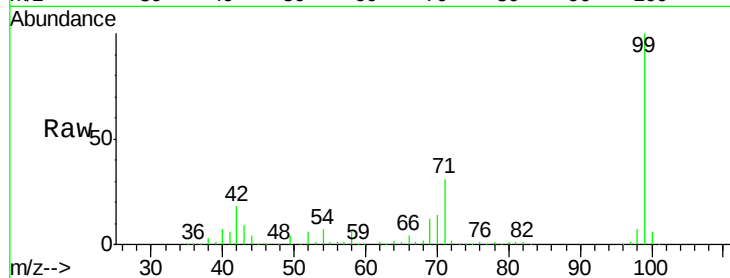

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

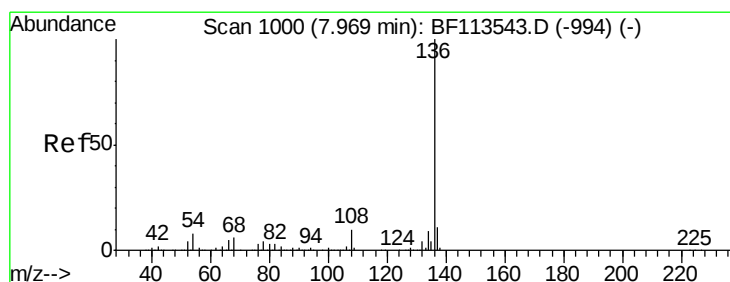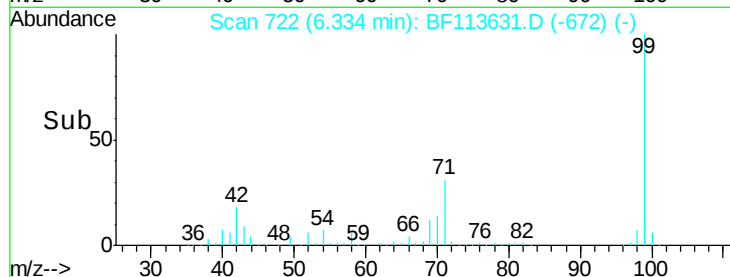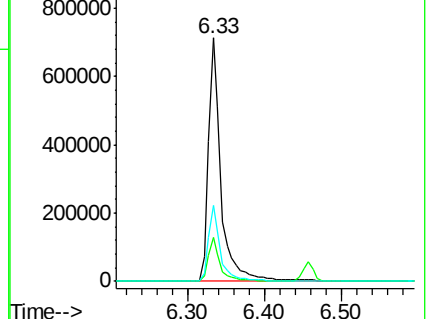

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.96 min Scan# 999

Delta R.T. -0.01 min

Lab File: BF113631.D

Acq: 5 Apr 2019 22:49

Tgt Ion: 136 Resp: 458690


Ion Ratio Lower Upper

136 100

137 10.6 8.9 13.3

54 7.7 7.0 10.6

68 5.7 4.8 7.2


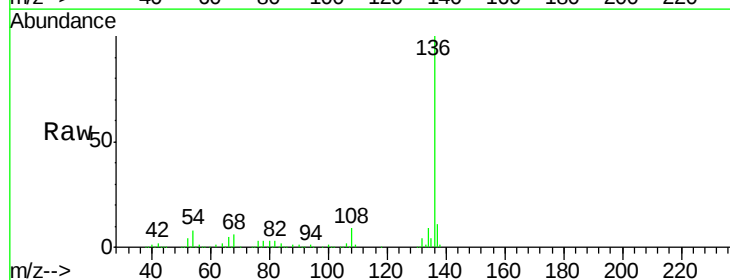


Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

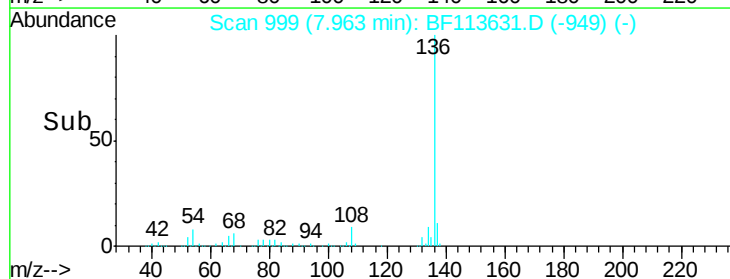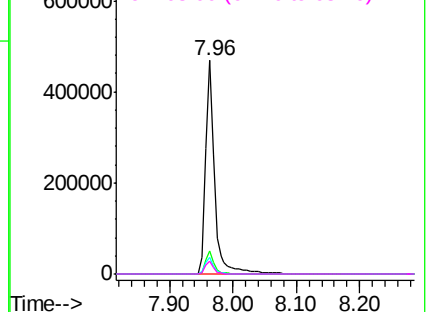







#23
Nitrobenzene-d5
Concen: 83.825 ng
RT: 7.25 min Scan# 877
Delta R.T. -0.01 min
Lab File: BF113631.D
Acq: 5 Apr 2019 22:49

Instrument :
BNA_F
ClientSampleId :
TP-3D

Tgt Ion: 82 Resp: 656414
Ion Ratio Lower Upper
82 100
128 45.8 36.5 54.7
54 51.7 42.2 63.2

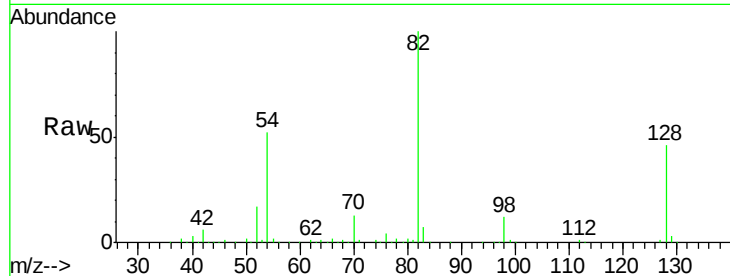


Abundance Ion 82.00 (81.70 to 82.70): BF1
Ion 128.00 (127.70 to 128.70): BF1
Ion 54.00 (53.70 to 54.70): BF1

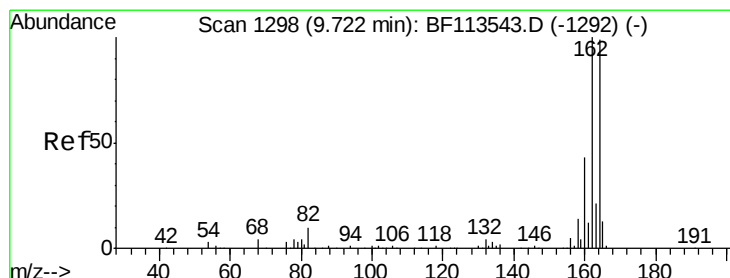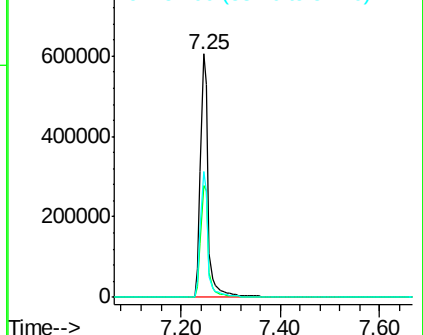
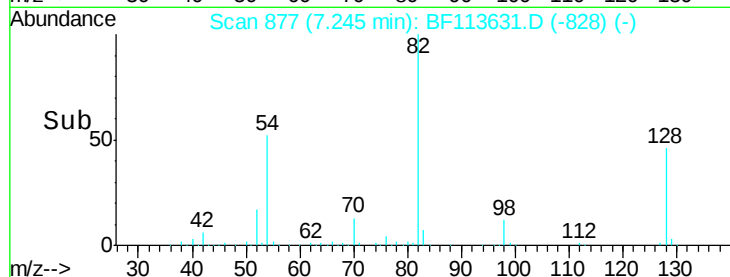


#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.71 min Scan# 1296
Delta R.T. -0.01 min
Lab File: BF113631.D
Acq: 5 Apr 2019 22:49

Tgt Ion: 164 Resp: 227494
Ion Ratio Lower Upper
164 100
162 100.7 81.8 122.6
160 43.5 36.4 54.6

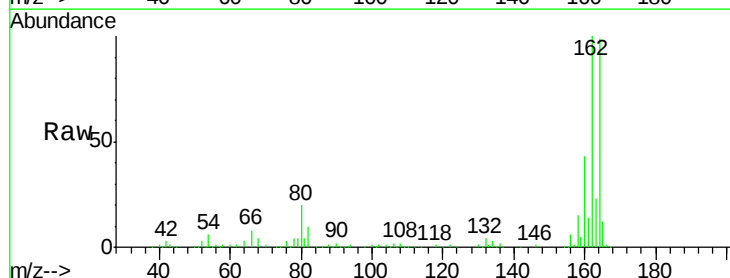

Abundance Ion 164.00 (163.70 to 164.70): BF1
Ion 162.00 (161.70 to 162.70): BF1
Ion 160.00 (159.70 to 160.70): BF1

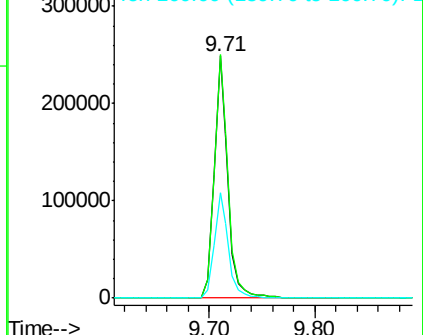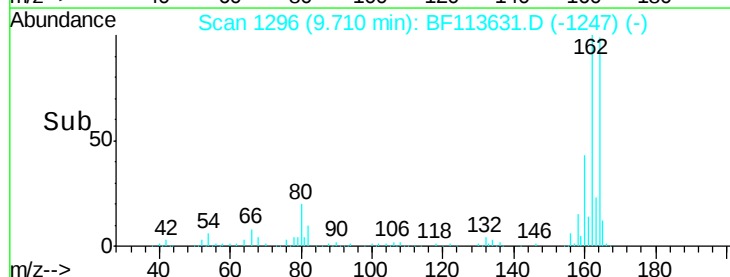







#42
 2,4,6-Tribromophenol
 Concen: 126.667 ng
 RT: 10.50 min Scan# 1431
 Delta R.T. -0.01 min
 Lab File: BF113631.D
 Acq: 5 Apr 2019 22:49

Instrument :
 BNA_F
 ClientSampleId :
 TP-3D

Tgt Ion:330 Resp: 346151
 Ion Ratio Lower Upper
 330 100
 332 95.2 77.8 116.6
 141 27.2 22.7 34.1

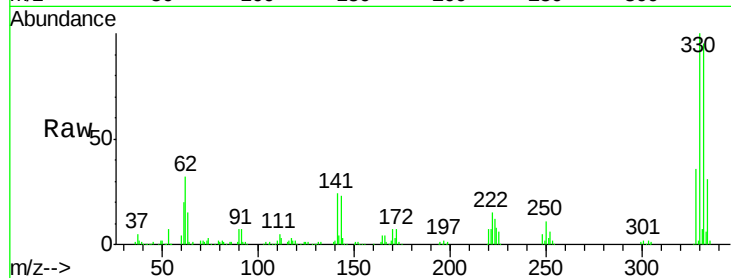


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

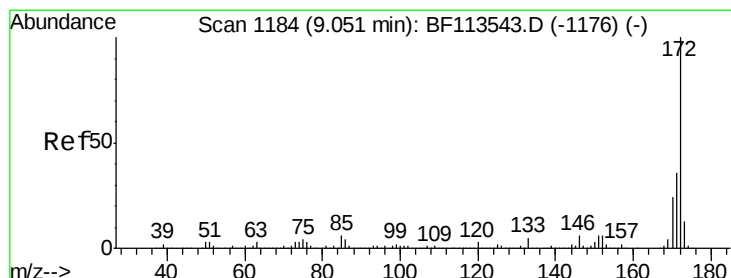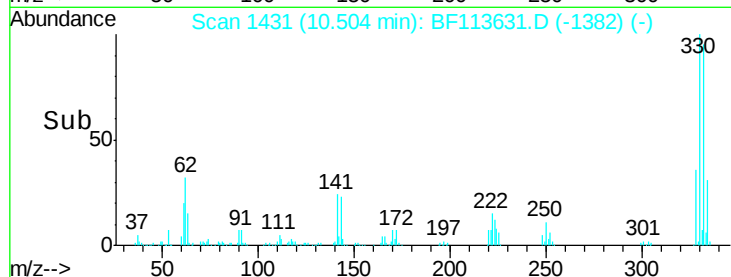
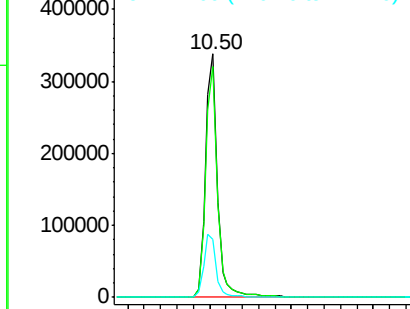



#45
 2-Fluorobiphenyl
 Concen: 85.164 ng
 RT: 9.04 min Scan# 1182
 Delta R.T. -0.01 min
 Lab File: BF113631.D
 Acq: 5 Apr 2019 22:49

Tgt Ion:172 Resp: 1203454
 Ion Ratio Lower Upper
 172 100
 171 35.9 29.0 43.6
 170 24.4 19.5 29.3

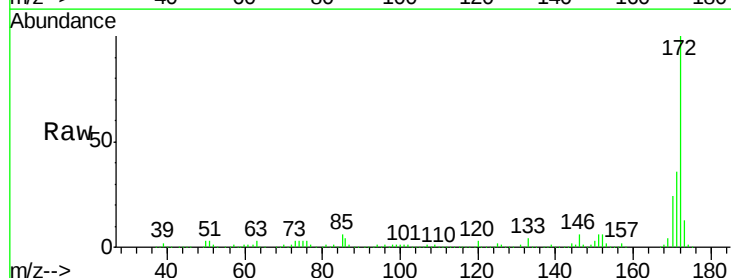

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

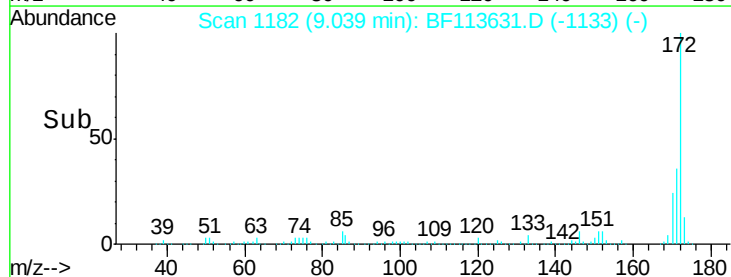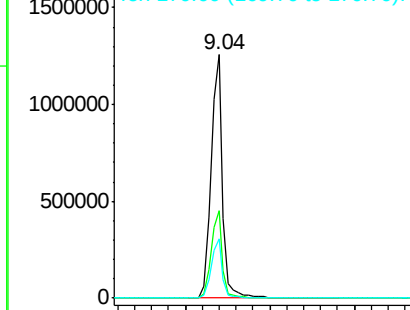

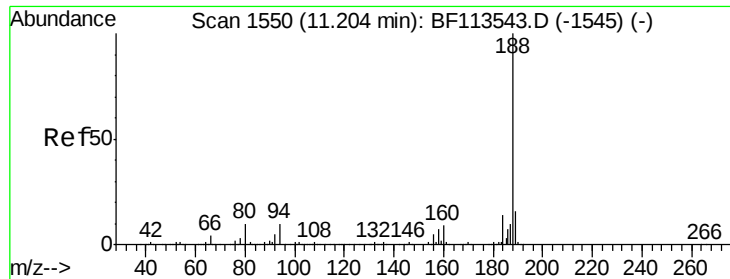

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.19 min Scan# 1548

Delta R.T. -0.01 min

Lab File: BF113631.D

Acq: 5 Apr 2019 22:49

Instrument :

BNA_F

ClientSampleId :

TP-3D


Tgt Ion:188 Resp: 476258

Ion Ratio Lower Upper

188 100

94 8.5 7.0 10.6




80 8.7 7.7 11.5

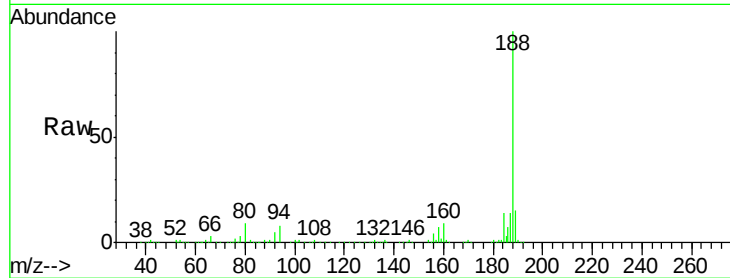

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

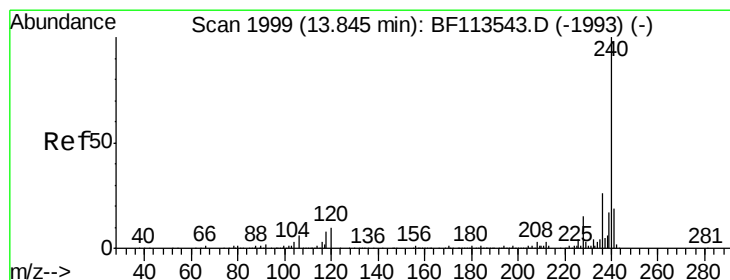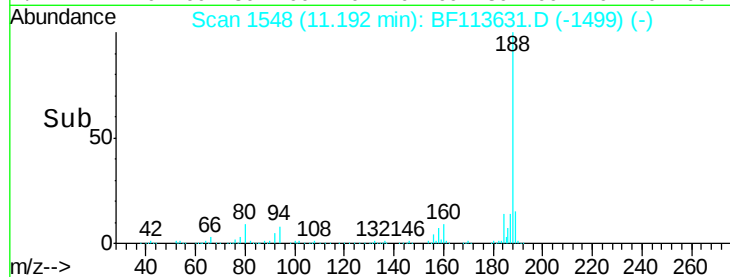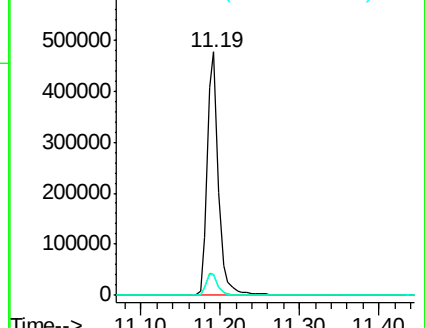

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.82 min Scan# 1995

Delta R.T. -0.02 min

Lab File: BF113631.D

Acq: 5 Apr 2019 22:49


Tgt Ion:240 Resp: 370658

Ion Ratio Lower Upper

240 100

120 10.5 8.8 13.2



236 25.3 20.9 31.3

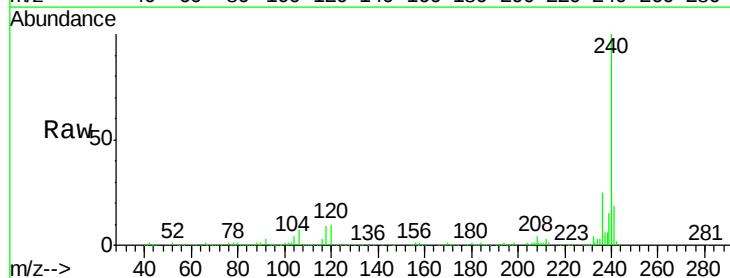


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

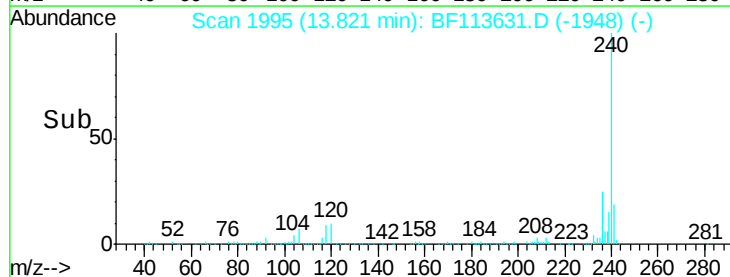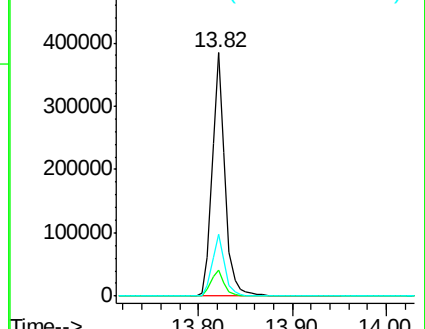

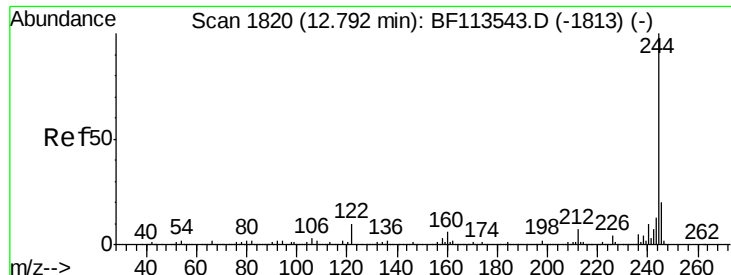

#79

Terphenyl-d14

Concen: 79.960 ng

RT: 12.77 min Scan# 1817

Delta R.T. -0.02 min

Lab File: BF113631.D

Acq: 5 Apr 2019 22:49

Instrument :

BNA_F

ClientSampleId :

TP-3D


Tgt Ion:244 Resp: 1455677

Ion Ratio Lower Upper

244 100

212 6.7 5.5 8.3




122 10.1 8.6 13.0

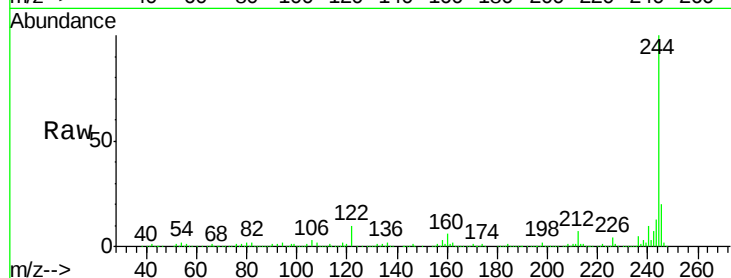

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

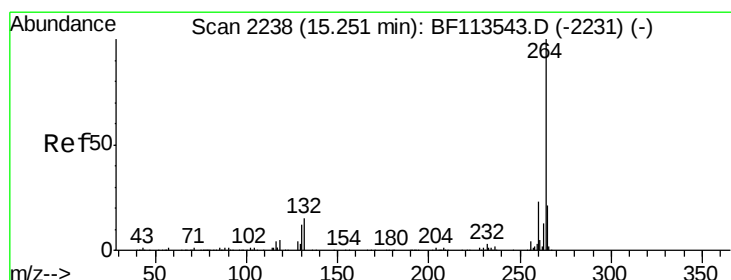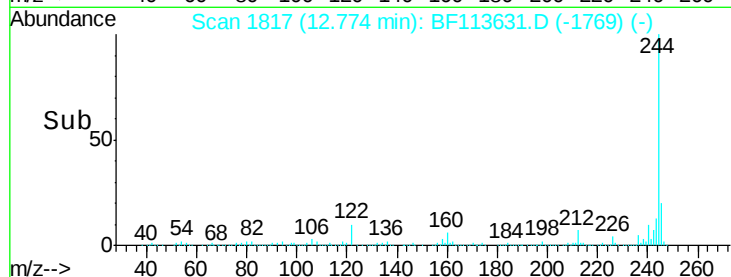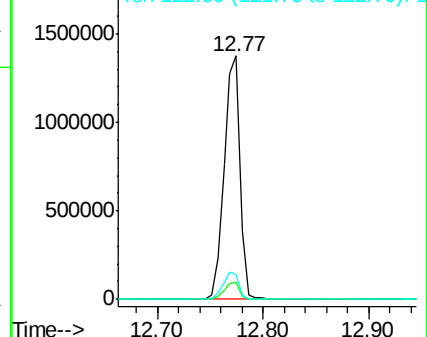

#87

Perylene-d12

Concen: 20.000 ng

RT: 15.22 min Scan# 2233

Delta R.T. -0.03 min

Lab File: BF113631.D

Acq: 5 Apr 2019 22:49


Tgt Ion:264 Resp: 326437

Ion Ratio Lower Upper

264 100

260 23.8 19.1 28.7

265 22.0 17.1 25.7

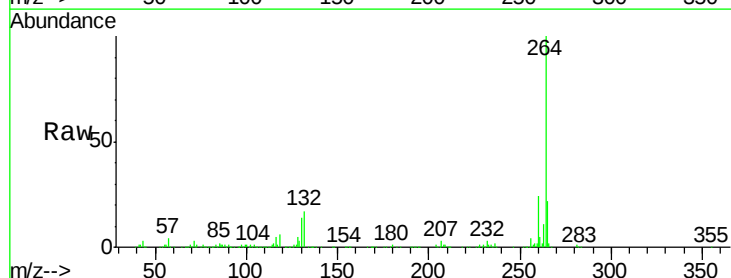

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

