

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040519\
 Data File : BF113614.D
 Acq On : 5 Apr 2019 10:45
 Operator : JU/SJ
 Sample : PB118551BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB118551BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.310	544	548	574	rBV	2468290	2562272	71.40%	9.507%
2	6.334	718	722	739	rBV	2378610	2683163	74.77%	9.956%
3	6.457	739	743	758	rVB	2910115	2701351	75.27%	10.023%
4	6.681	778	781	793	rBV	752464	706284	19.68%	2.621%
5	6.840	804	808	824	rBV	2330090	2150860	59.93%	7.981%
6	7.245	873	877	904	rBV	1507847	1721204	47.96%	6.387%
7	7.963	995	999	1020	rBV	883595	922923	25.72%	3.425%
8	9.039	1177	1182	1185	rBV	3359606	3226885	89.92%	11.973%
9	9.716	1292	1297	1311	rBV	1081588	1066063	29.71%	3.956%
10	10.504	1427	1431	1452	rBV	2090284	2151912	59.96%	7.985%
11	11.198	1545	1549	1570	rVB	1141054	1174434	32.73%	4.358%
12	12.775	1812	1817	1821	rBV	3339043	3588743	100.00%	13.316%
13	13.827	1992	1996	2004	rBV	1217334	1158163	32.27%	4.297%
14	14.586	2122	2125	2130	rVB	38974	36699	1.02%	0.136%
15	14.898	2175	2178	2182	rVB	47740	51286	1.43%	0.190%
16	15.233	2230	2235	2246	rVB	743394	988150	27.53%	3.667%
17	15.633	2300	2303	2308	rVB3	44242	59869	1.67%	0.222%


Sum of corrected areas: 26950261

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040519\
Data File : BF113614.D
Acq On : 5 Apr 2019 10:45
Operator : JU/SJ
Sample : PB118551BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118551BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

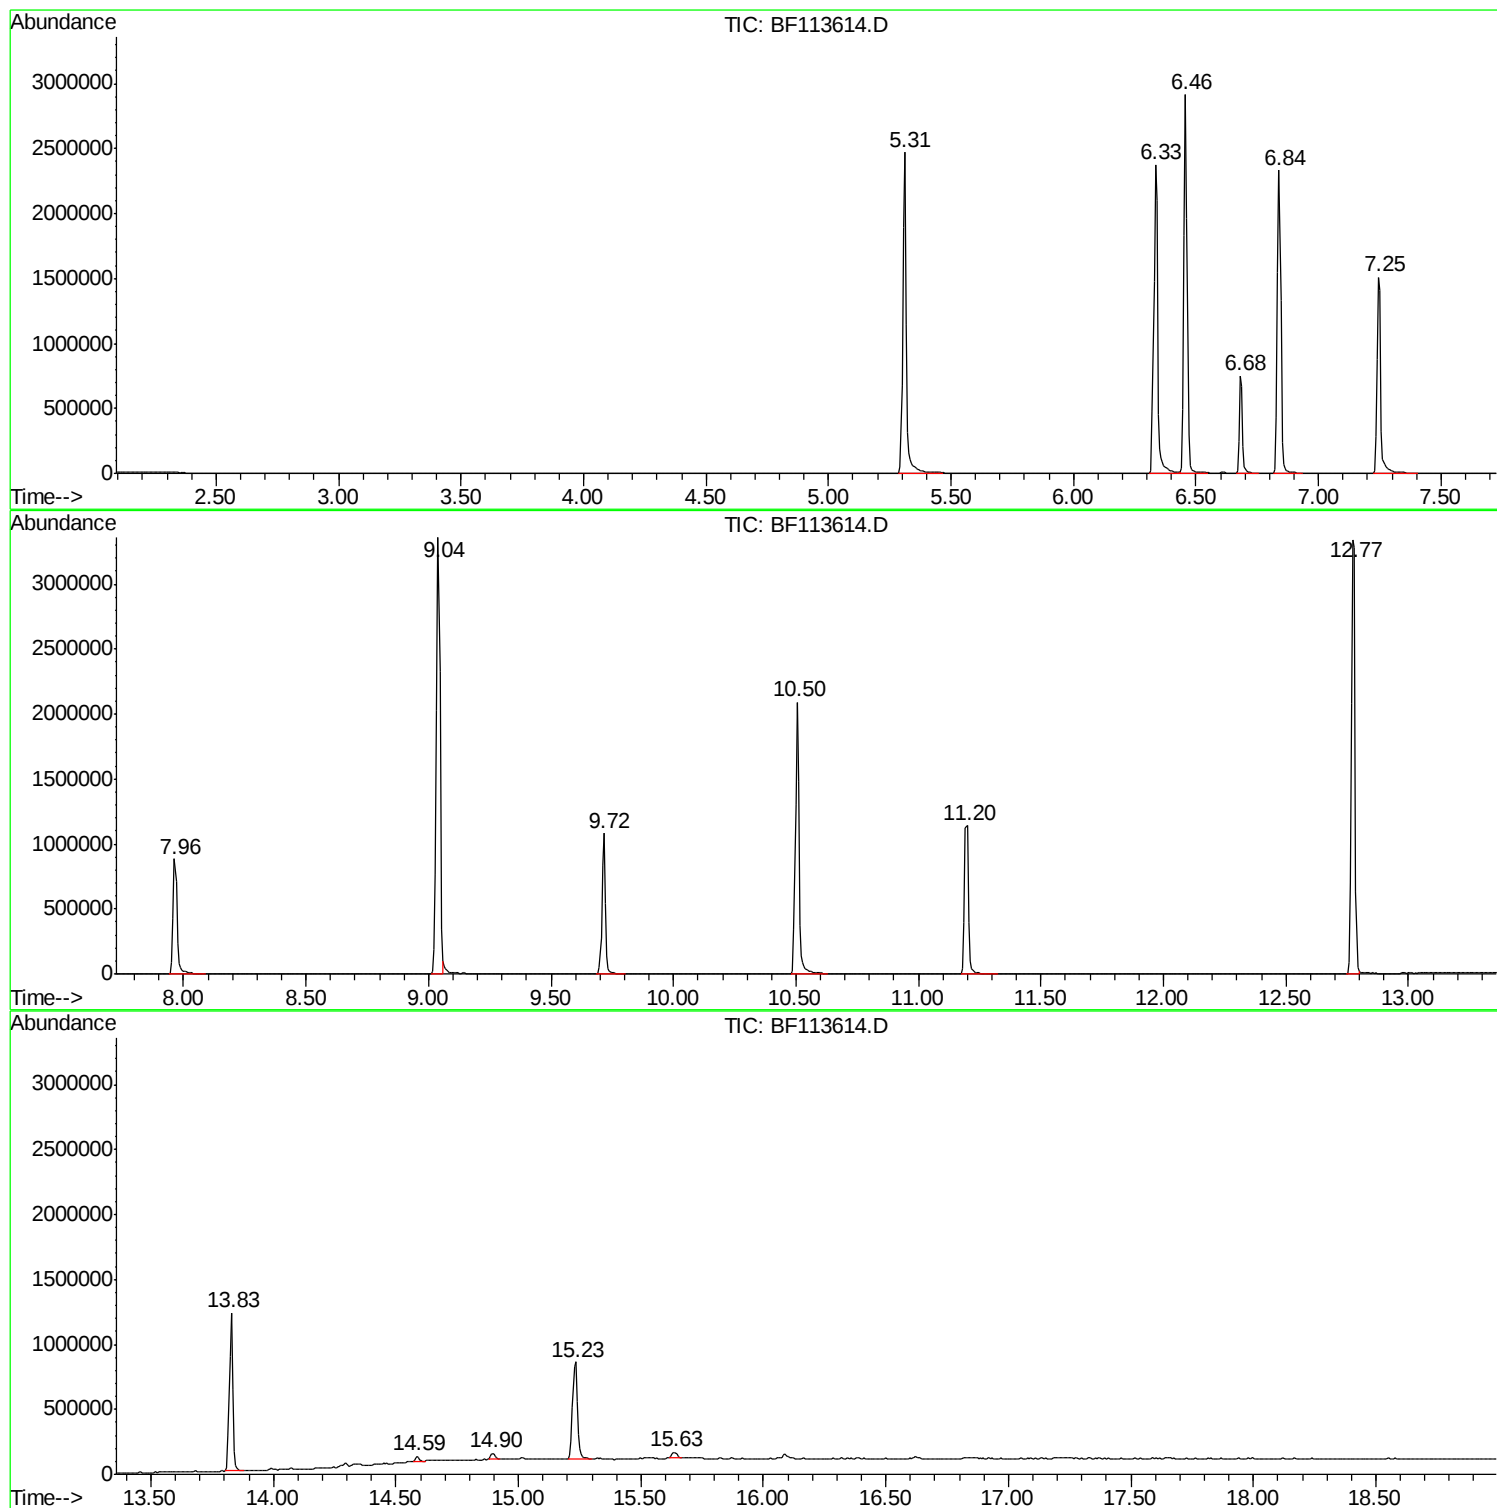

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040519\
Data File : BF113614.D
Acq On : 5 Apr 2019 10:45
Operator : JU/SJ
Sample : PB118551BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118551BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.46 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.46	76.49 ng	2701350	1,4-Dichlorobenzene-d4	6.68

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranlylcypropine-propionyl	189	C12H15NO	1000123-86-3	12
3		Amphetaminil	250	C17H18N2	017590-01-1	12
4		5-Aminoindole	132	C8H8N2	005192-03-0	12
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	12

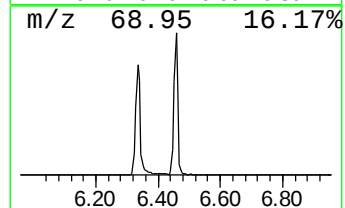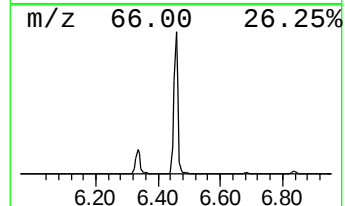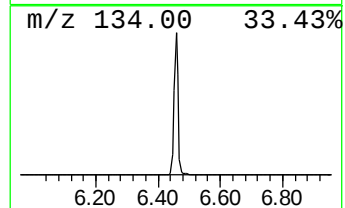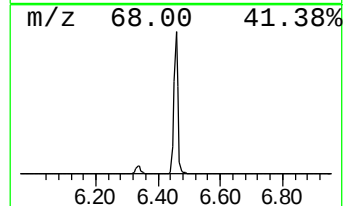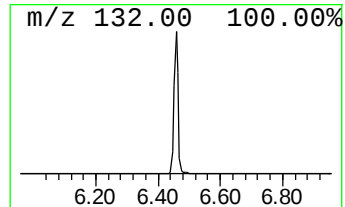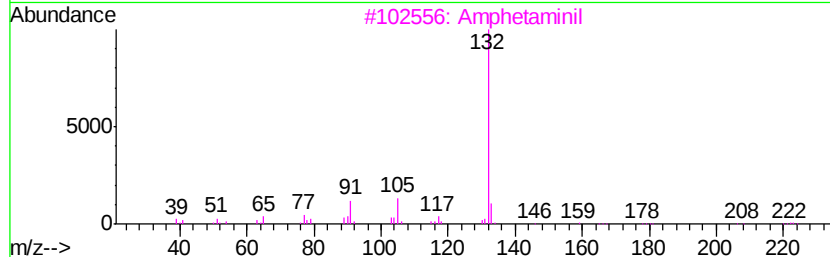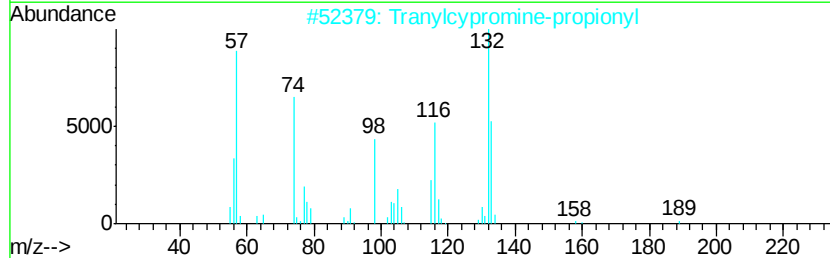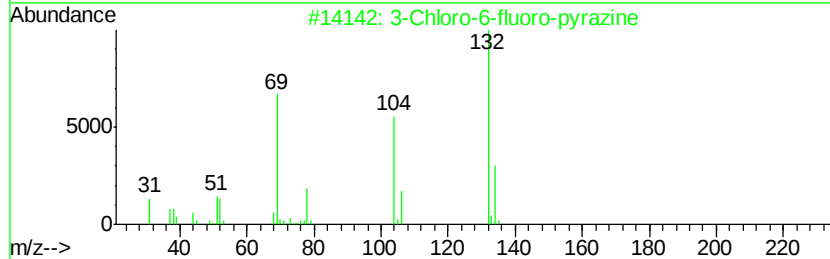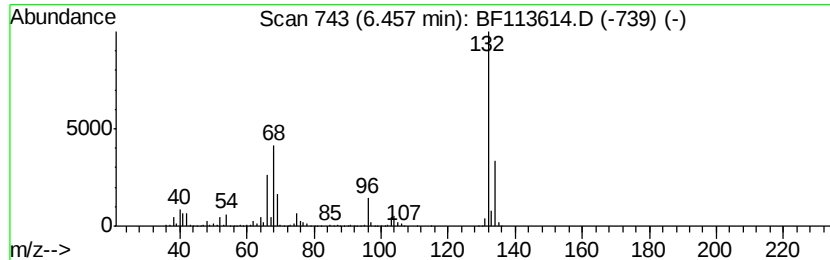

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF040519\
Data File : BF113614.D
Acq On : 5 Apr 2019 10:45
Operator : JU/SJ
Sample : PB118551BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB118551BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.46	6.46	76.5	ng	2701350	1	6.68	706284	20.0