


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040519\
 Data File : BF113611.D
 Acq On : 5 Apr 2019 9:16
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF040319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 04 04:05:31 2019

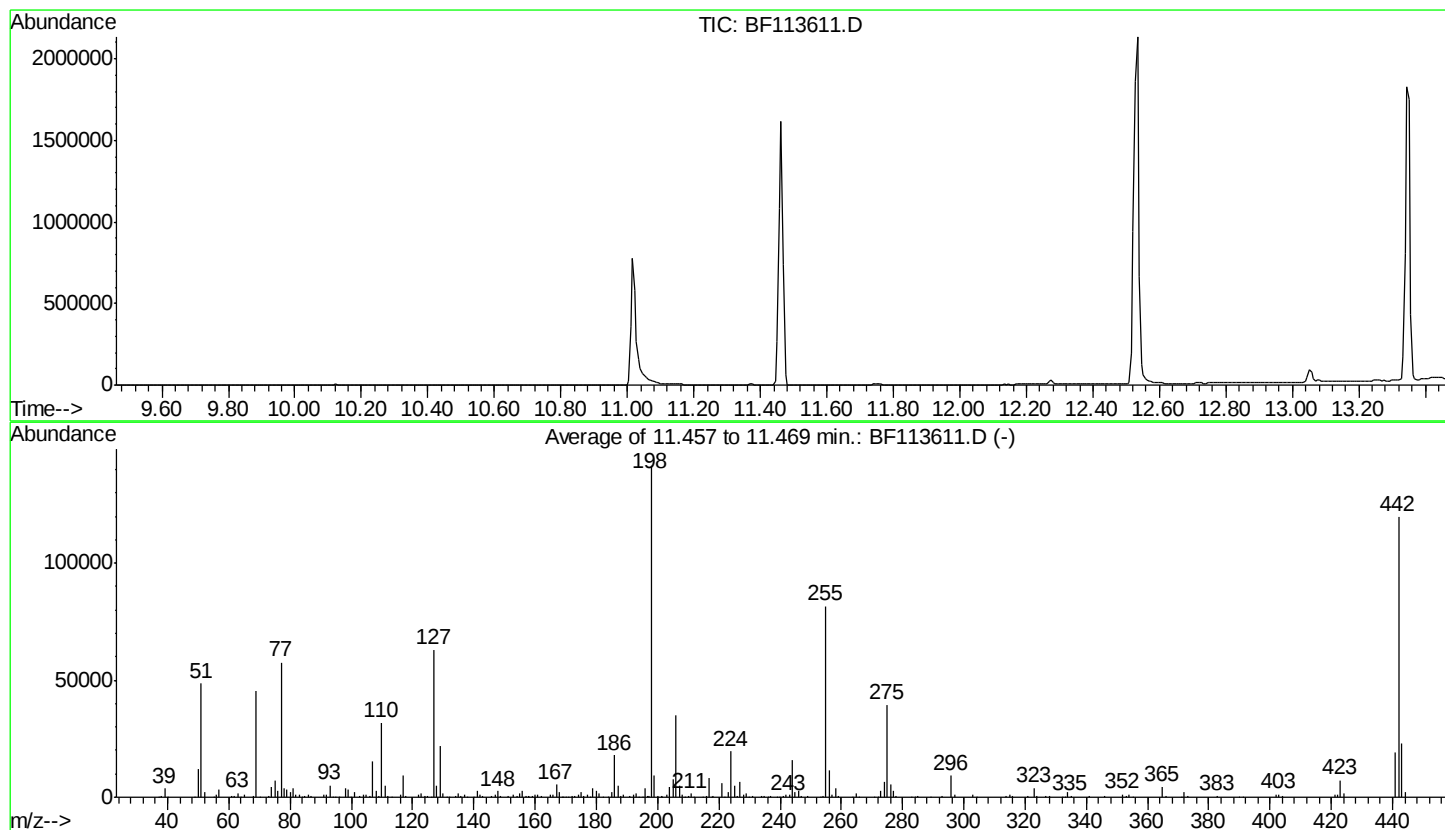

AutoFind: Scans 1593, 1594, 1595; Background Corrected with Scan 1588

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	48474	PASS
68	69	0.00	2	1.5	660	PASS
69	198	0.00	100	32.1	45498	PASS
70	69	0.00	2	0.5	247	PASS
127	198	10	80	44.5	63013	PASS
197	198	0.00	2	0.3	426	PASS
198	198	100	100	100.0	141696	PASS
199	198	5	9	6.5	9175	PASS
275	198	10	60	27.9	39552	PASS
365	198	1	100	3.1	4427	PASS
441	198	0.01	100	13.4	18949	PASS
442	198	50	100	84.6	119880	PASS
443	442	15	24	19.3	23171	PASS