

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040615\
 Data File : BF078262.D
 Acq On : 6 Apr 2015 17:45
 Operator : TP/IZ
 Sample : G1710-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 W-19

Quant Time: Apr 07 01:26:11 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 07 02:08:45 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.98	152	52056	20.00	ng	0.00
21) Naphthalene-d8	8.56	136	212609	20.00	ng	0.00
38) Acenaphthene-d10	10.72	164	106007	20.00	ng	0.00
63) Phenanthrene-d10	12.55	188	212172	20.00	ng	-0.01
75) Chrysene-d12	15.84	240	221031	20.00	ng	-0.01
86) Perylene-d12	17.63	264	205182	20.00	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.26	112	160419	50.81	ng	0.00
7) Phenol-d6	6.58	99	119661	30.24	ng	0.00
23) Nitrobenzene-d5	7.68	82	272823	77.78	ng	0.00
41) 2,4,6-Tribromophenol	11.70	330	120045	136.54	ng	0.00
44) 2-Fluorobiphenyl	9.90	172	602092	81.19	ng	0.00
78) Terphenyl-d14	14.55	244	666558	68.14	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040615\
Data File : BF078262.D
Acq On : 6 Apr 2015 17:45
Operator : TP/IZ
Sample : G1710-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
W-19

Quant Time: Apr 07 01:26:11 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 02:08:45 2015
Response via : Initial Calibration

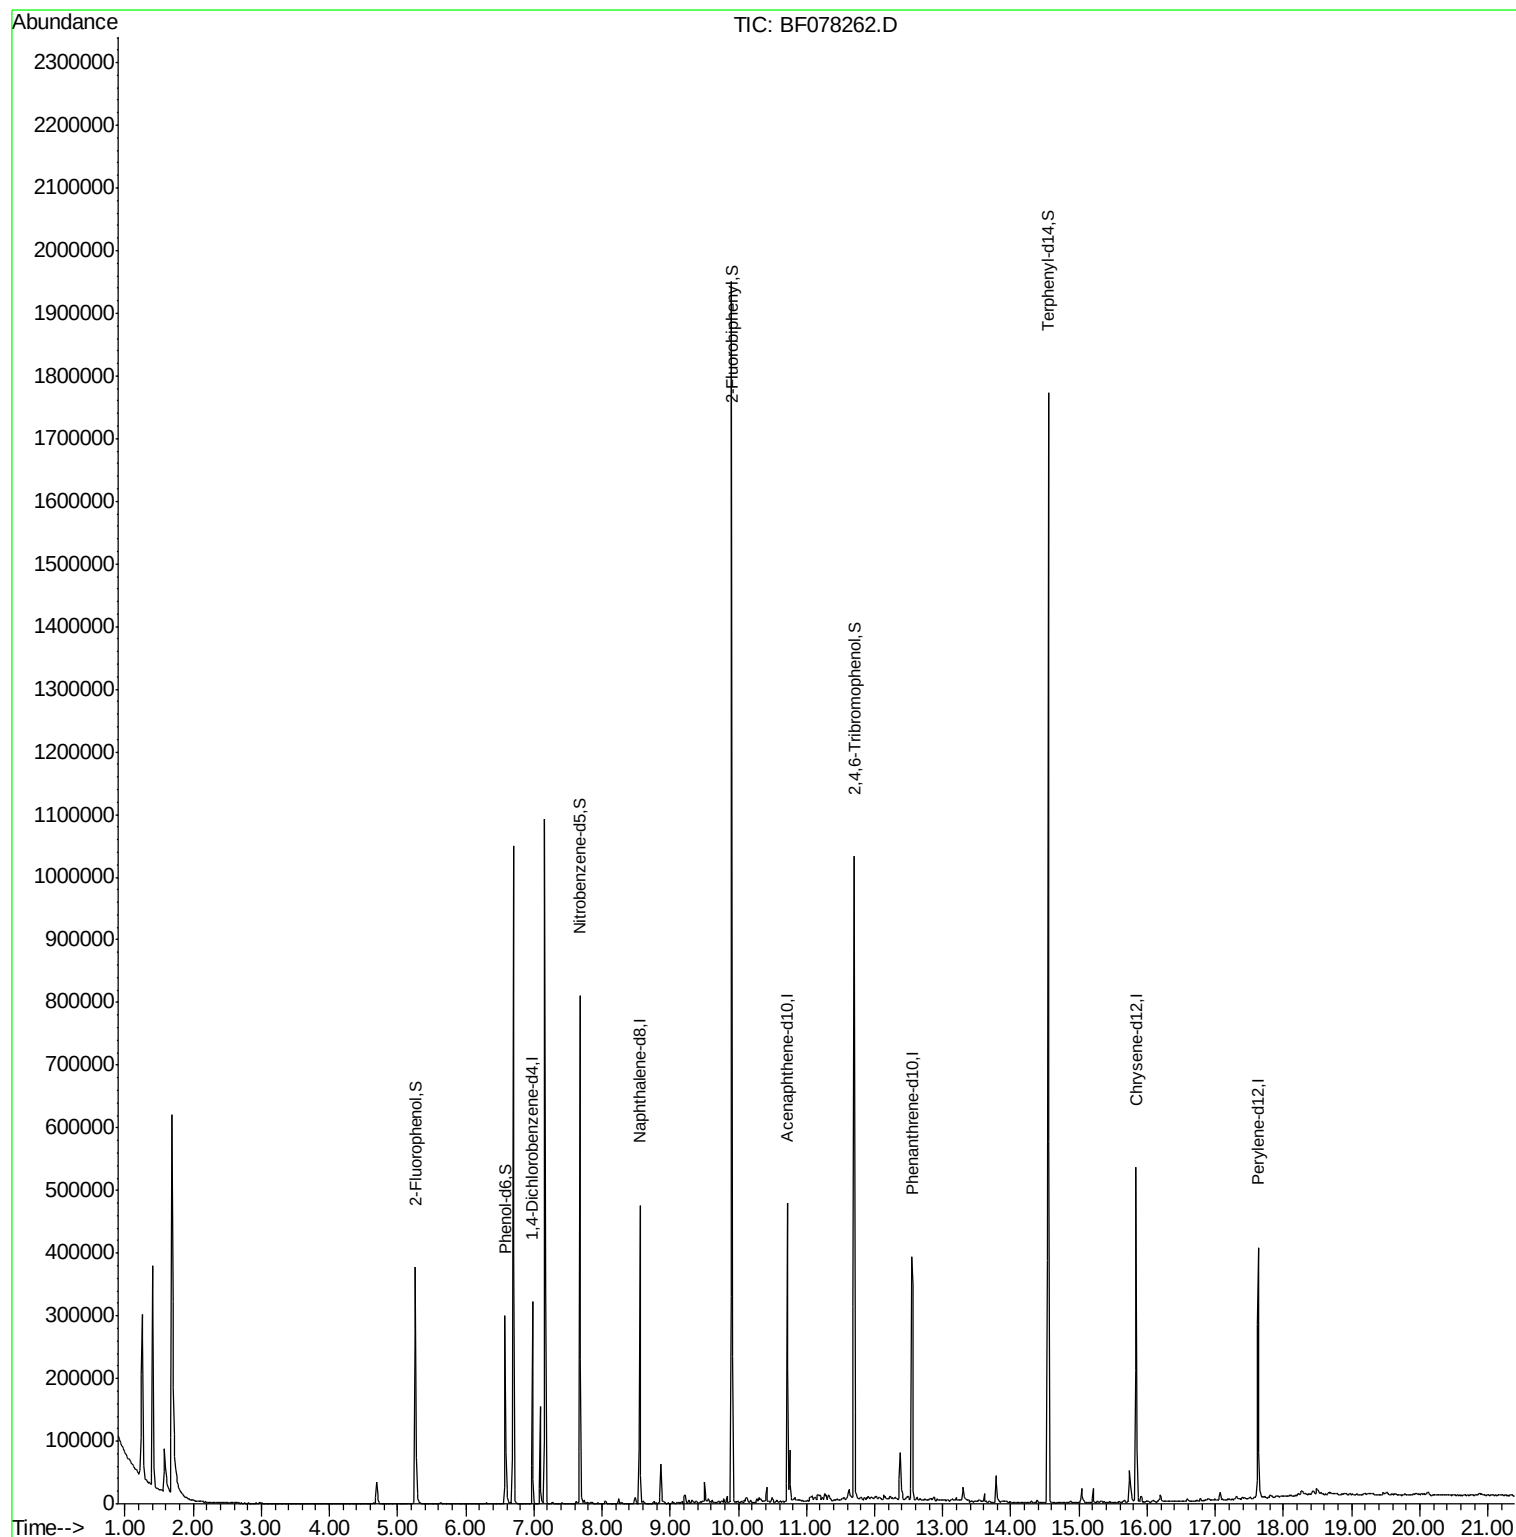

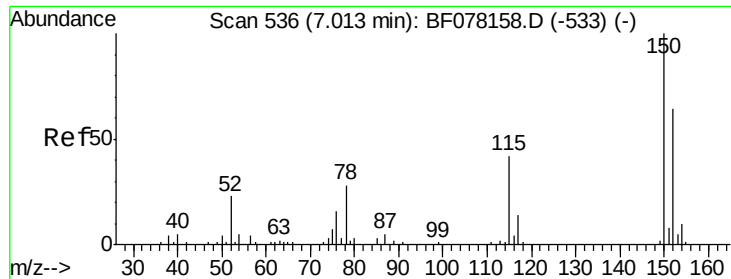


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.98 min Scan# 533
Delta R.T. -0.00 min
Lab File: BF078262.D
Acq: 6 Apr 2015 17:45

Instrument :
BNA_F
ClientSampleId :
W-19

Tgt Ion:152 Resp: 52056
Ion Ratio Lower Upper
152 100
150 154.2 125.9 188.9
115 58.0 52.7 79.1

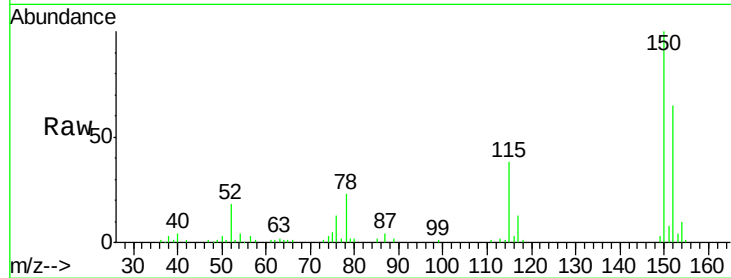


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

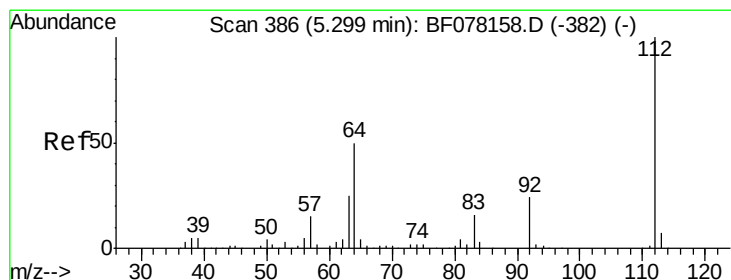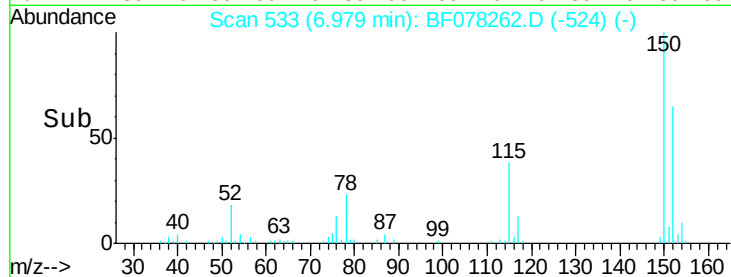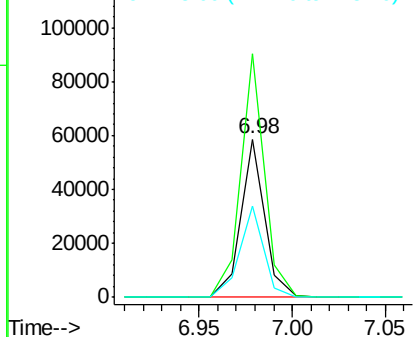



#5


2-Fluorophenol
Concen: 50.81 ng
RT: 5.26 min Scan# 383
Delta R.T. 0.00 min
Lab File: BF078262.D
Acq: 6 Apr 2015 17:45

Tgt Ion:112 Resp: 160419
Ion Ratio Lower Upper
112 100
64 51.6 39.9 59.9
63 25.2 20.2 30.4

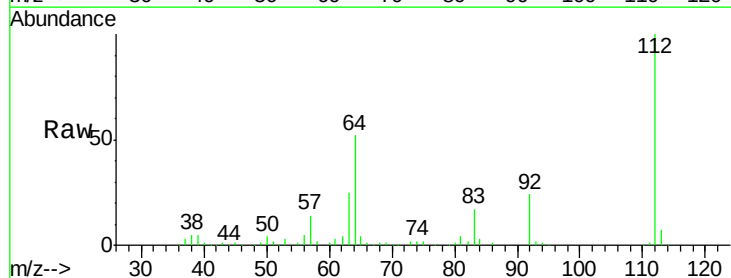

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

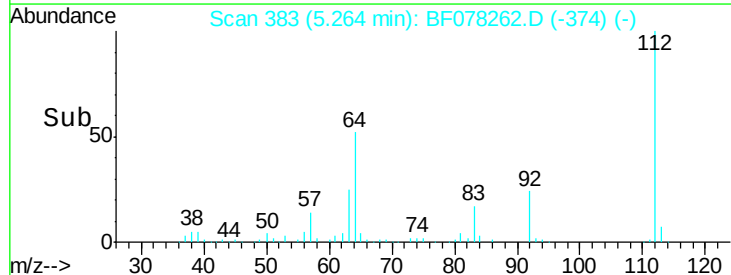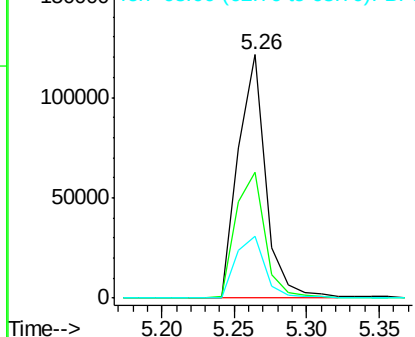

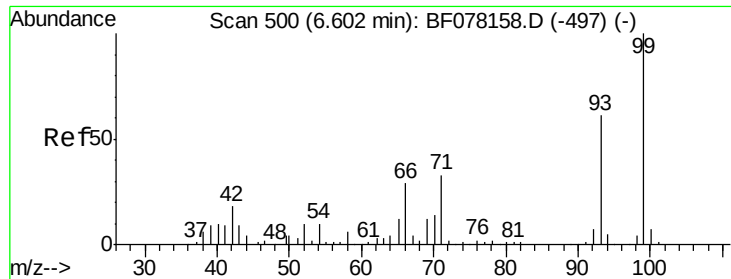

#7

Phenol-d6

Concen: 30.24 ng

RT: 6.58 min Scan# 498

Delta R.T. 0.00 min

Lab File: BF078262.D

Acq: 6 Apr 2015 17:45

Instrument :

BNA_F

ClientSampleId :

W-19


Tgt Ion: 99 Resp: 119661

Ion Ratio Lower Upper

99 100

42 15.9 14.8 22.2




71 30.9 26.6 39.8

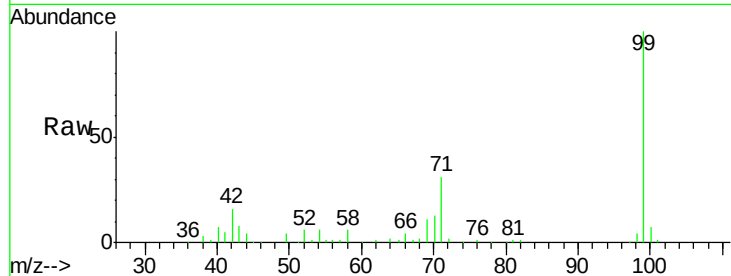

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

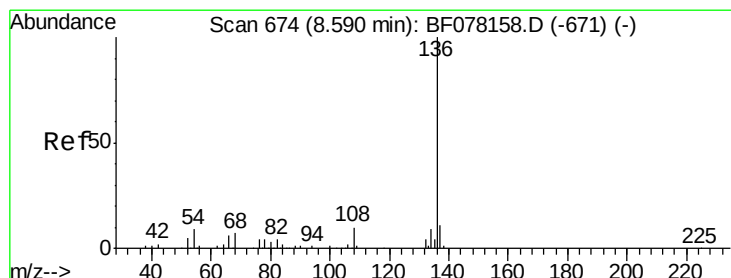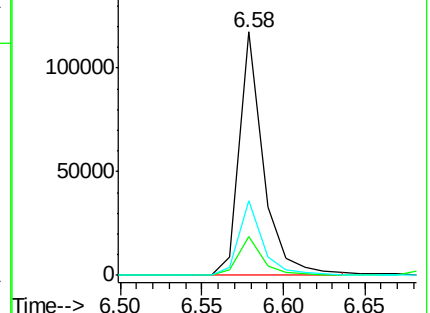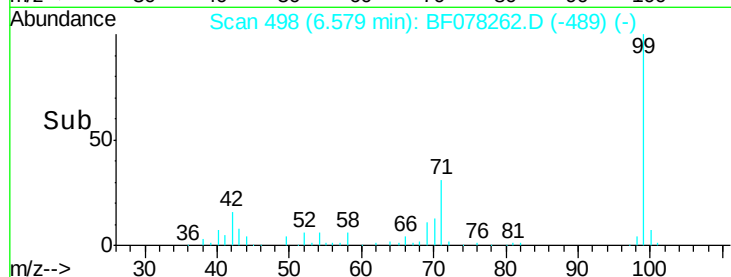

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.56 min Scan# 671

Delta R.T. -0.00 min

Lab File: BF078262.D

Acq: 6 Apr 2015 17:45

Tgt Ion: 136 Resp: 212609


Ion Ratio Lower Upper

136 100

137 10.5 9.0 13.4

54 6.6 7.0 10.6#

68 5.5 5.4 8.2


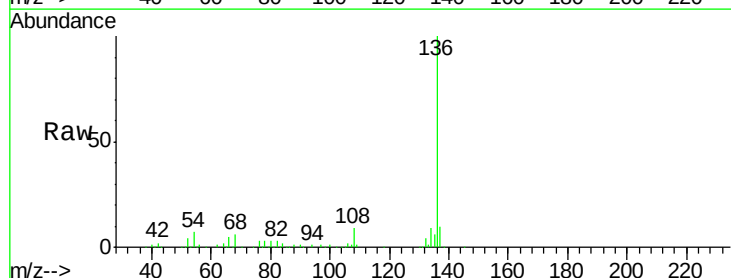



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

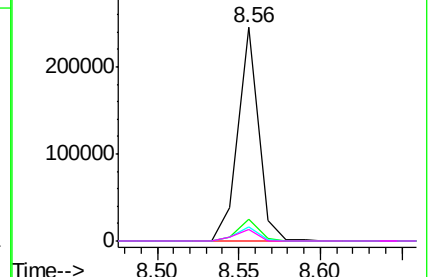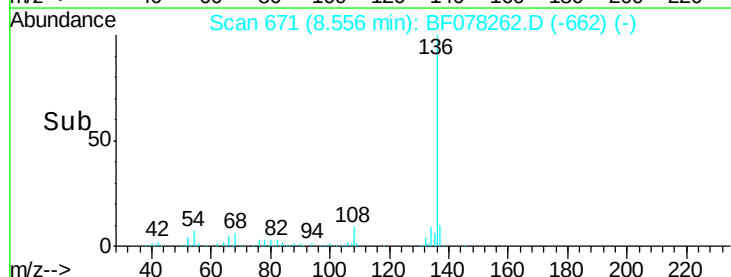


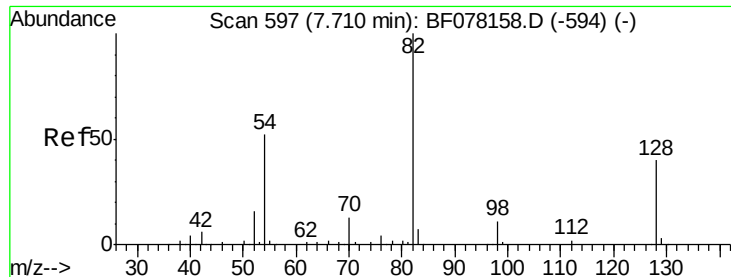




#23
 Nitrobenzene-d5
 Concen: 77.78 ng
 RT: 7.68 min Scan# 594
 Delta R.T. 0.00 min
 Lab File: BF078262.D
 Acq: 6 Apr 2015 17:45

Instrument :
 BNA_F
 ClientSampleId :
 W-19

Tgt Ion: 82 Resp: 272823
 Ion Ratio Lower Upper
 82 100
 128 42.7 31.8 47.8
 54 49.2 41.5 62.3

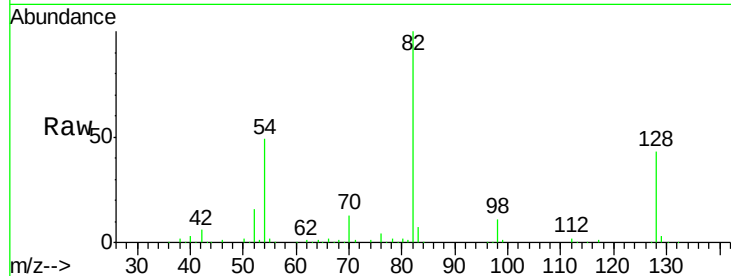


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF0

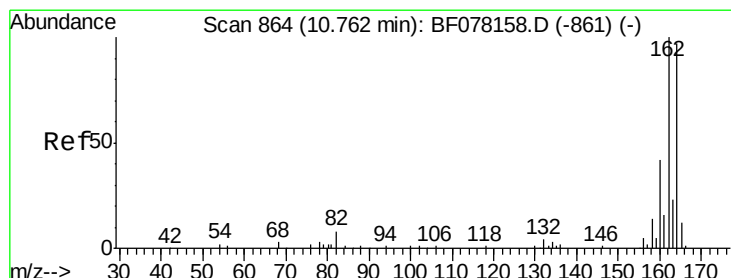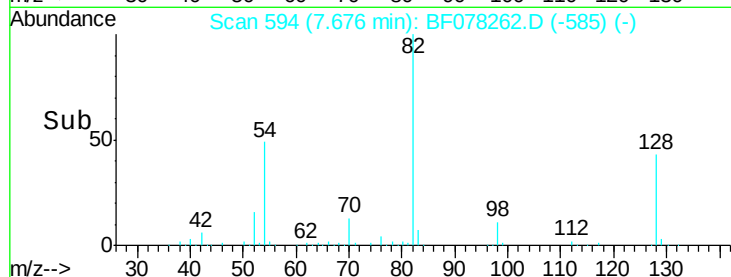
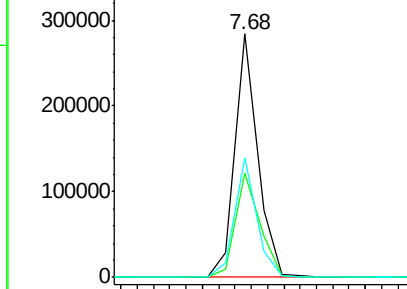



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 10.72 min Scan# 860
 Delta R.T. -0.00 min
 Lab File: BF078262.D
 Acq: 6 Apr 2015 17:45

Tgt Ion: 164 Resp: 106007
 Ion Ratio Lower Upper
 164 100
 162 103.9 82.2 123.2
 160 43.6 34.7 52.1

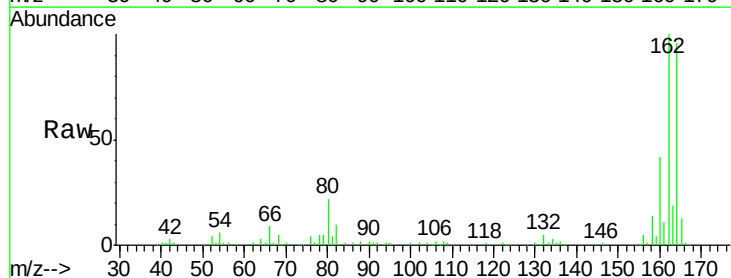

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E



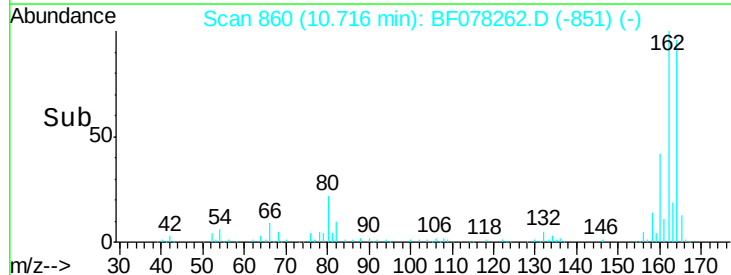
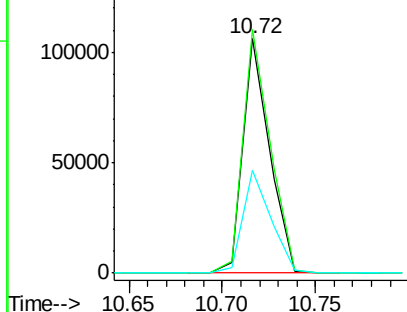


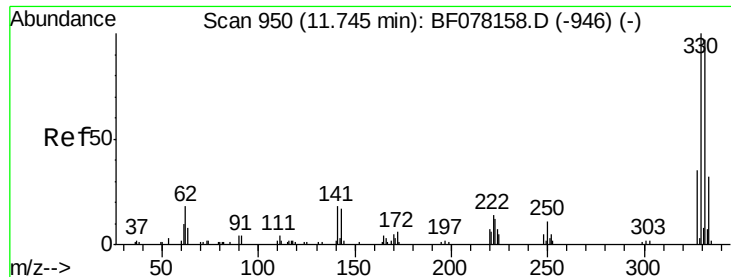

#41
 2,4,6-Tribromophenol
 Concen: 136.54 ng
 RT: 11.70 min Scan# 946
 Delta R.T. -0.00 min
 Lab File: BF078262.D
 Acq: 6 Apr 2015 17:45




Instrument :
 BNA_F
 ClientSampleId :
 W-19


Tgt Ion	Ratio	Lower	Upper
330	100		
332	95.4	78.6	117.8
141	39.7	31.2	46.8

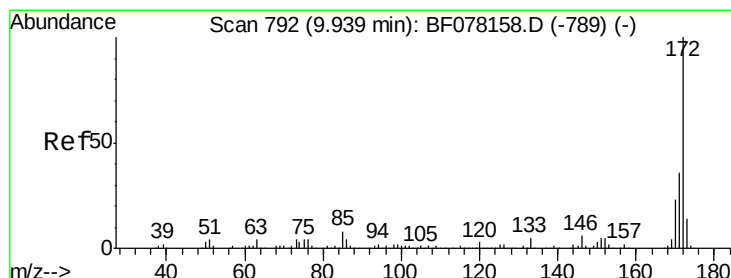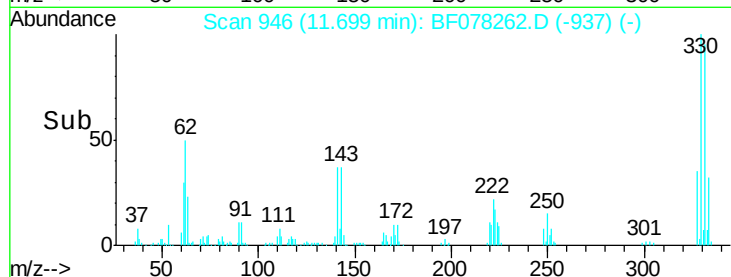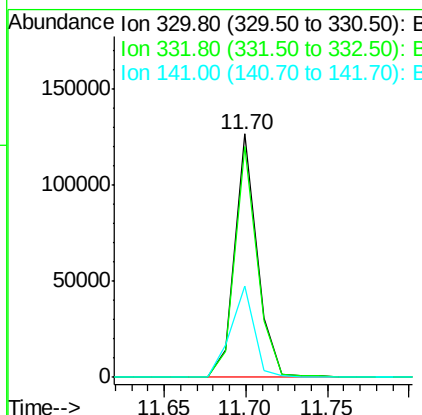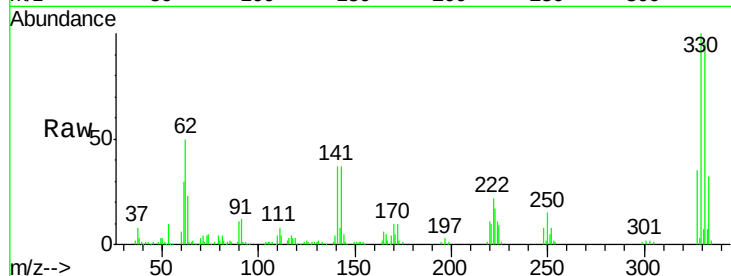

#44
 2-Fluorobiphenyl
 Concen: 81.19 ng
 RT: 9.90 min Scan# 789
 Delta R.T. -0.00 min
 Lab File: BF078262.D
 Acq: 6 Apr 2015 17:45

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.4	28.6	42.8
170	23.7	18.5	27.7

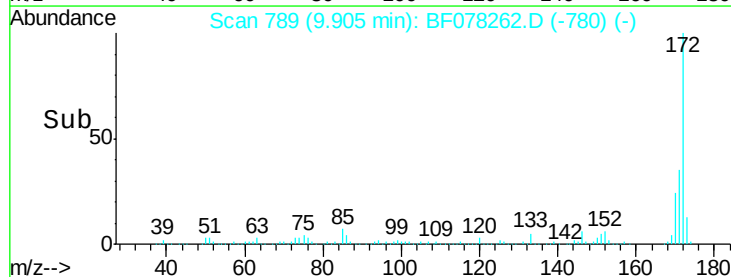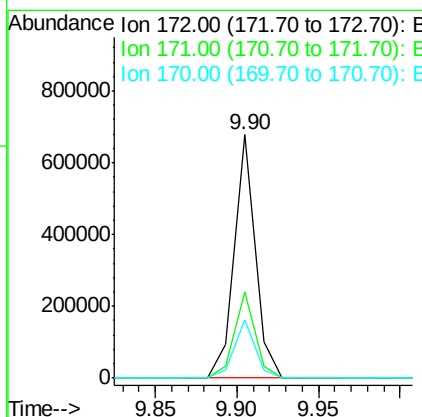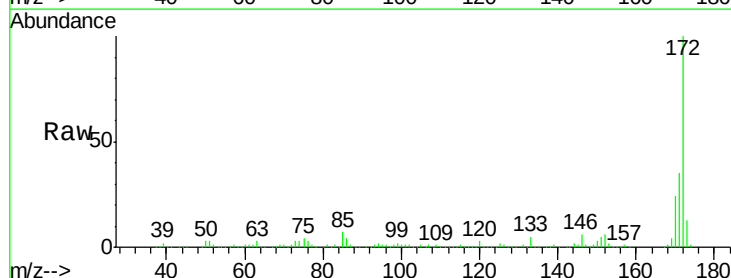


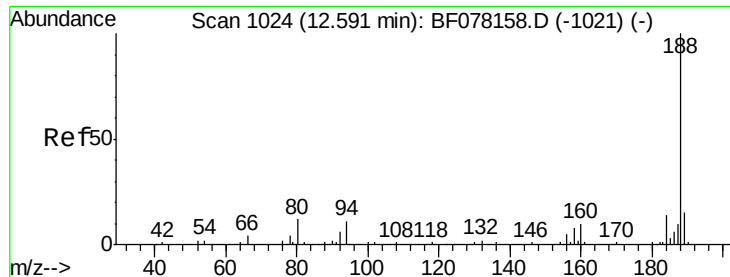




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.55 min Scan# 1020
Delta R.T. -0.01 min
Lab File: BF078262.D
Acq: 6 Apr 2015 17:45

Instrument :
BNA_F
ClientSampleId :
W-19

Tgt Ion:188 Resp: 212172
Ion Ratio Lower Upper
188 100
94 12.7 9.0 13.4
80 14.0 9.5 14.3

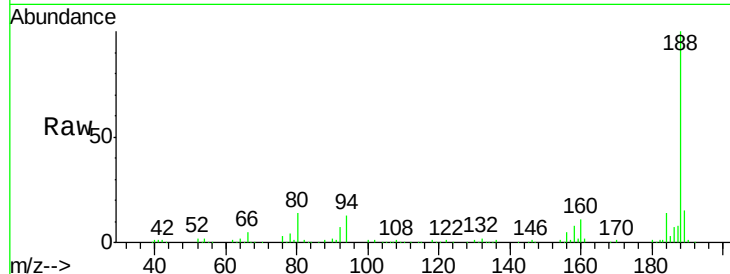


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

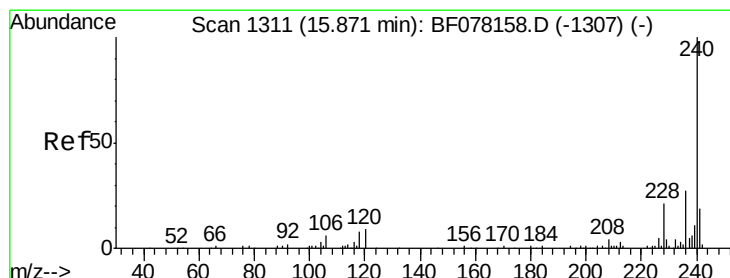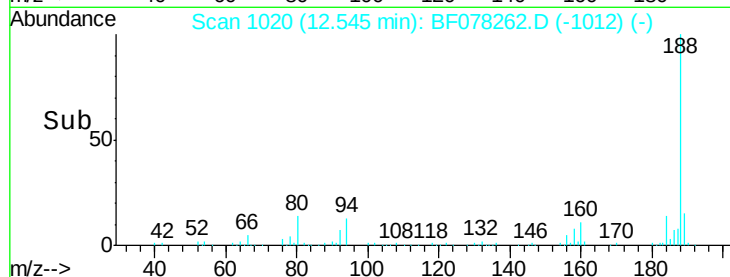
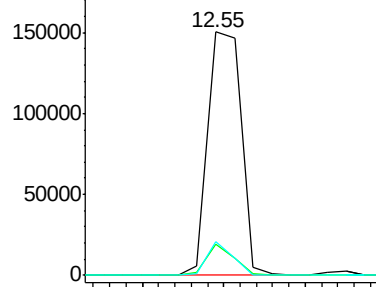



#75
Chrysene-d12
Concen: 20.00 ng
RT: 15.84 min Scan# 1308
Delta R.T. -0.01 min
Lab File: BF078262.D
Acq: 6 Apr 2015 17:45

Tgt Ion:240 Resp: 221031
Ion Ratio Lower Upper
240 100
120 11.4 7.1 10.7#
236 24.8 21.4 32.2

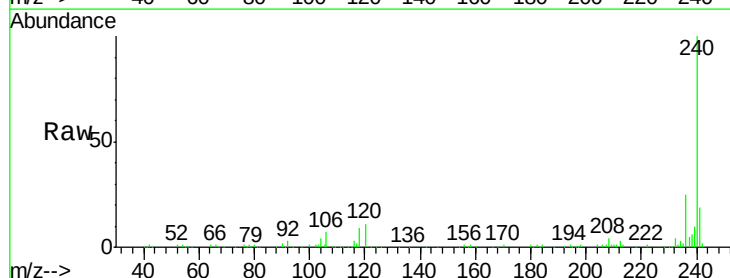

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



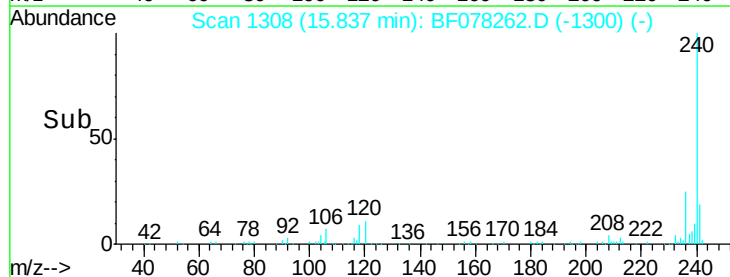
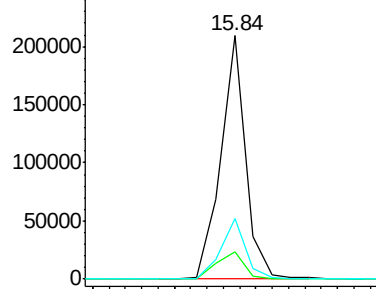


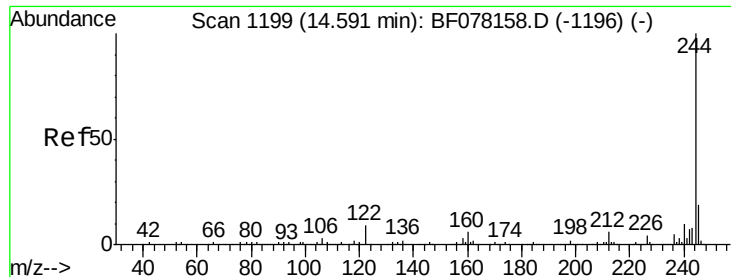

#78
 Terphenyl-d14
 Concen: 68.14 ng
 RT: 14.55 min Scan# 1195
 Delta R.T. -0.00 min
 Lab File: BF078262.D
 Acq: 6 Apr 2015 17:45

Instrument :
 BNA_F
 ClientSampleId :
 W-19

Tgt Ion	Ratio	Lower	Upper
244	100		
212	6.9	5.0	7.4
122	13.2	7.1	10.7#

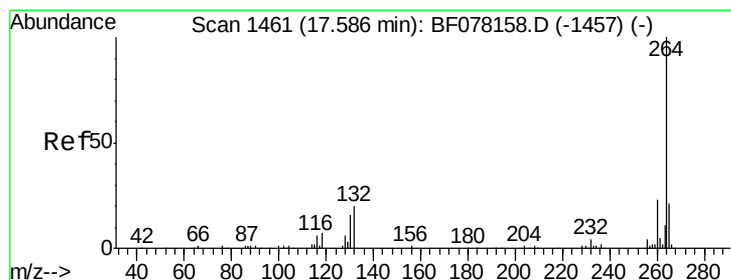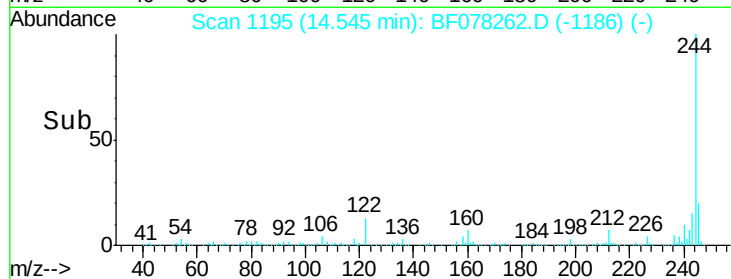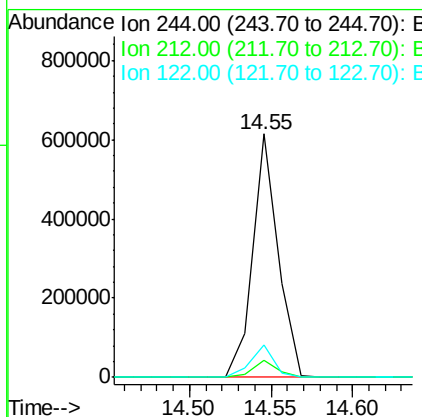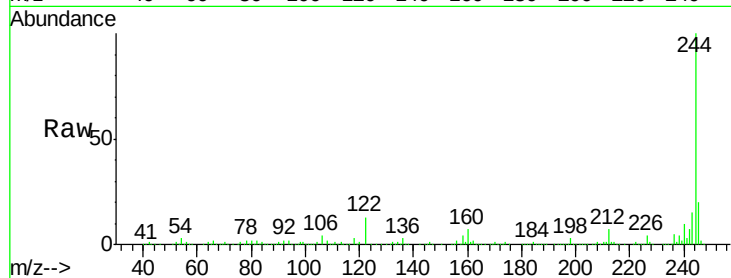

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.63 min Scan# 1465
 Delta R.T. -0.01 min
 Lab File: BF078262.D
 Acq: 6 Apr 2015 17:45

Tgt Ion	Ratio	Lower	Upper
264	100		
260	23.3	18.6	27.8
265	21.3	17.0	25.6

