


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040615\
 Data File : BF078272.D
 Acq On : 6 Apr 2015 23:22
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Apr 07 02:08:45 2015

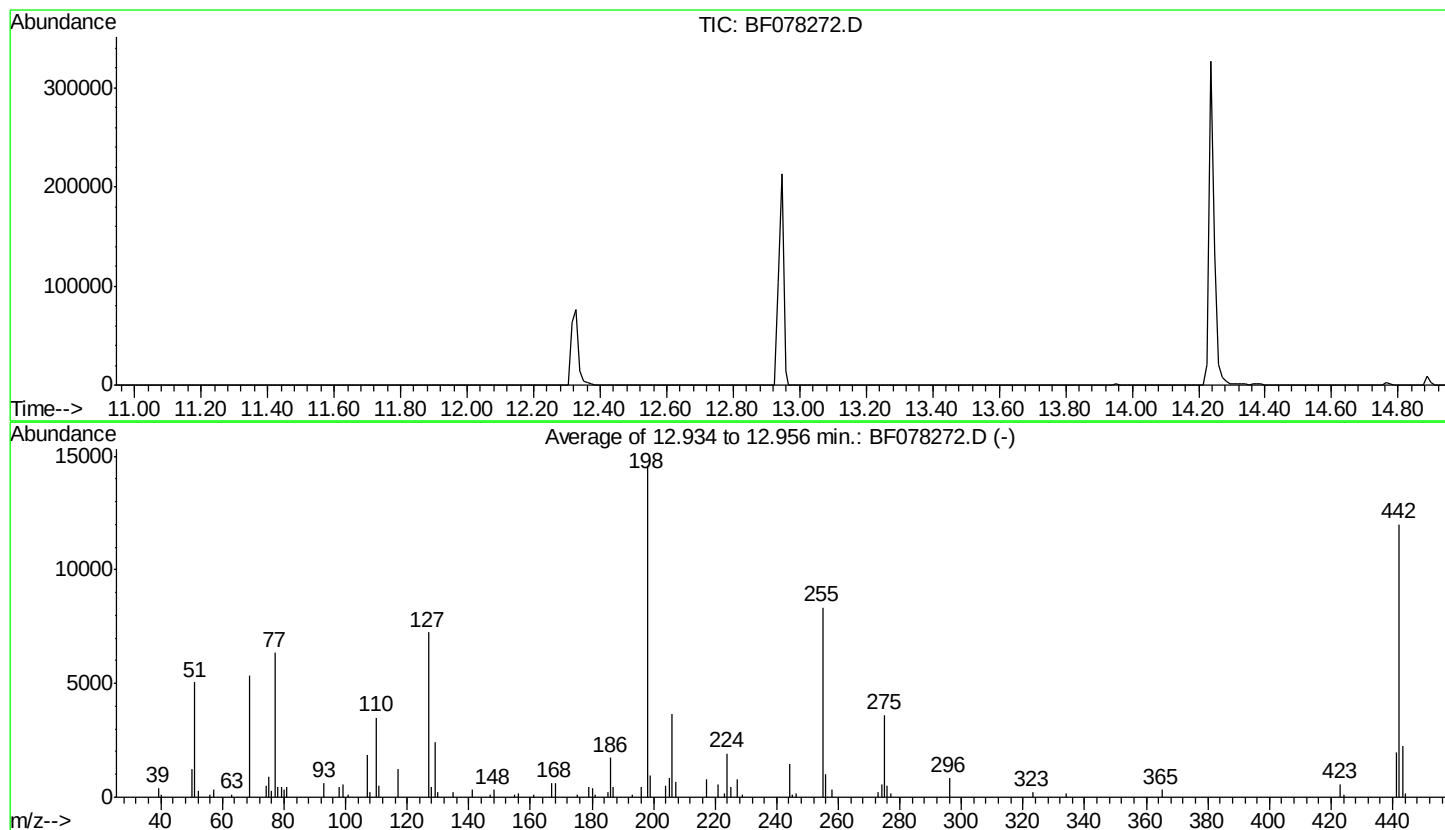

AutoFind: Scans 1054, 1055, 1056; Background Corrected with Scan 1051

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	5049	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.5	5323	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	49.8	7257	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	14580	PASS
199	198	5	9	6.6	965	PASS
275	198	10	60	24.7	3606	PASS
365	198	1	100	2.3	329	PASS
441	442	0.01	24	16.2	1947	PASS
442	198	50	100	82.3	11999	PASS
443	442	15	24	18.9	2270	PASS