
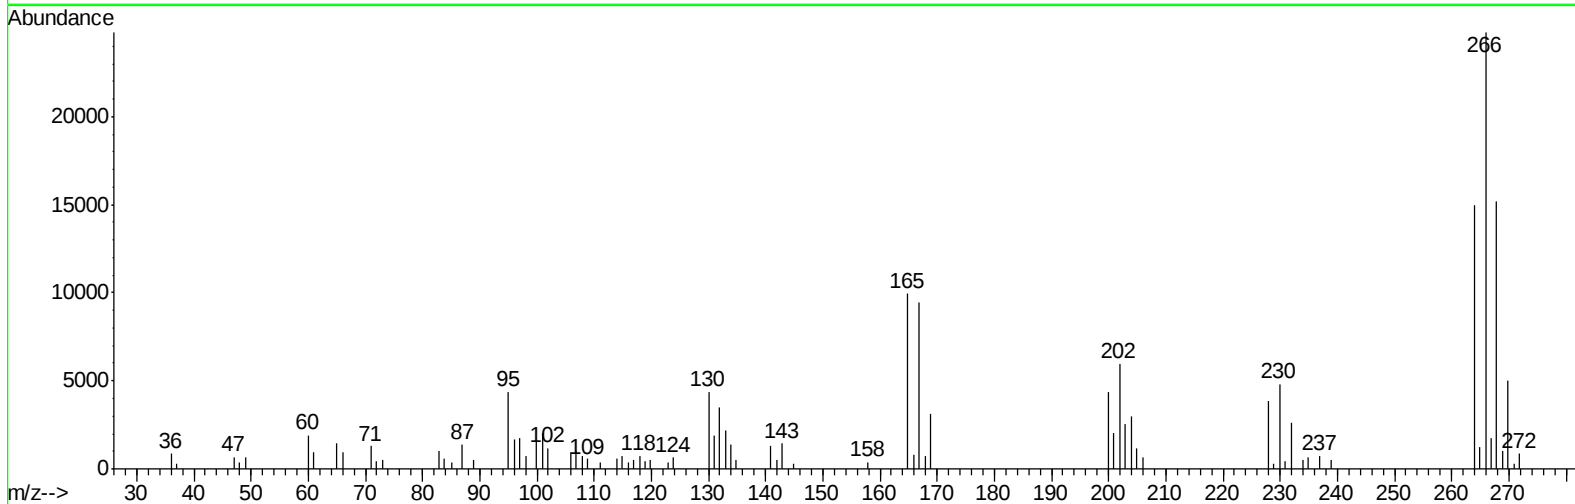


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040615\
Data File : BF078250.D
Acq On : 6 Apr 2015 11:57
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 08:13:12 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 04:11:17 2015
Response via : Initial Calibration

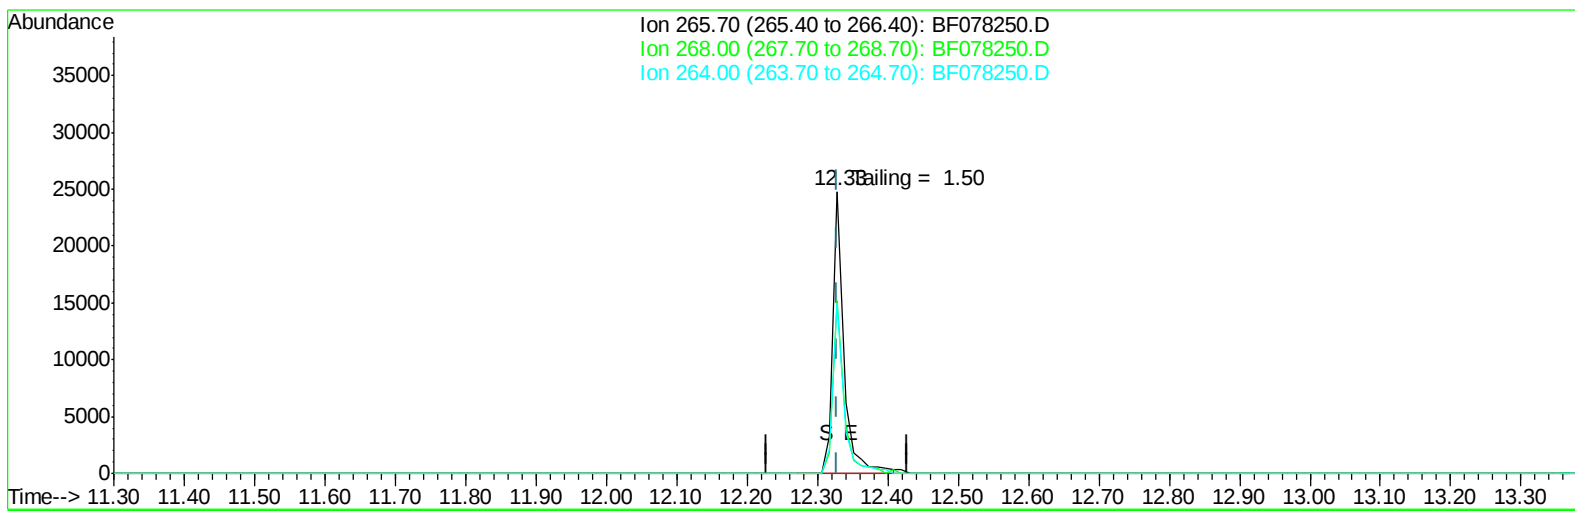

TIC: BF078250.D

(69) Pentachlorophenol (C)



12.328min (+0.000) 0.00ng

response 26313

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	61.23
264.00	62.50	60.35
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040615\
Data File : BF078250.D
Acq On : 6 Apr 2015 11:57
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 08:13:12 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 04:11:17 2015
Response via : Initial Calibration

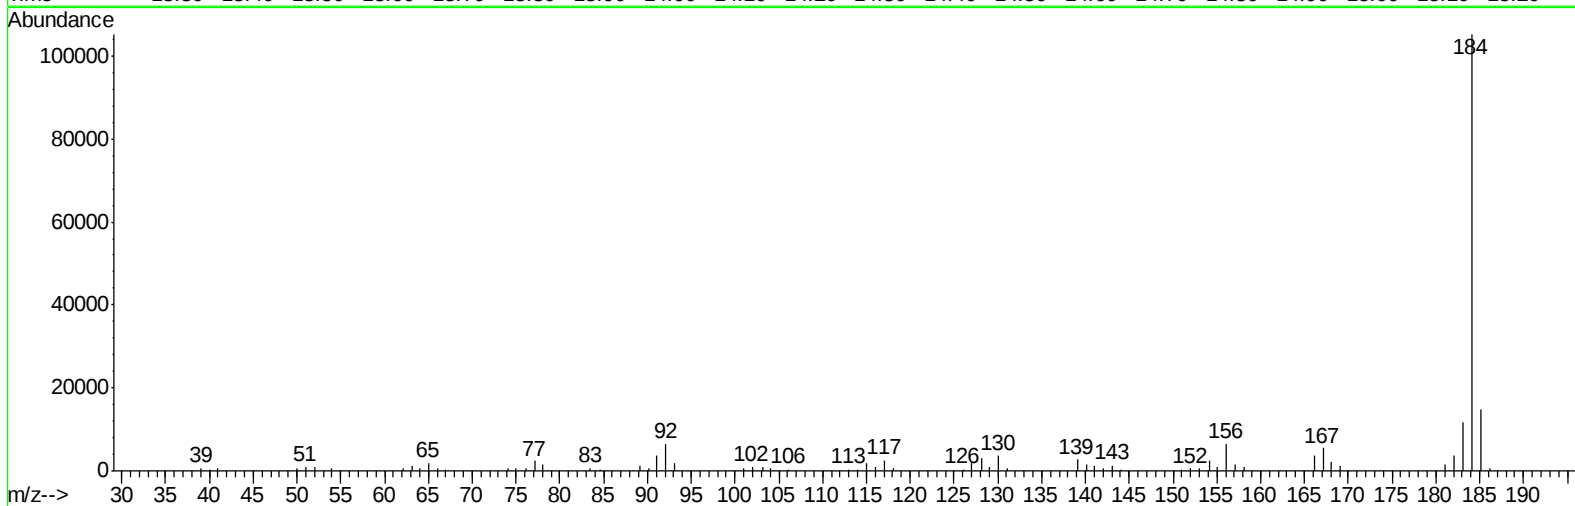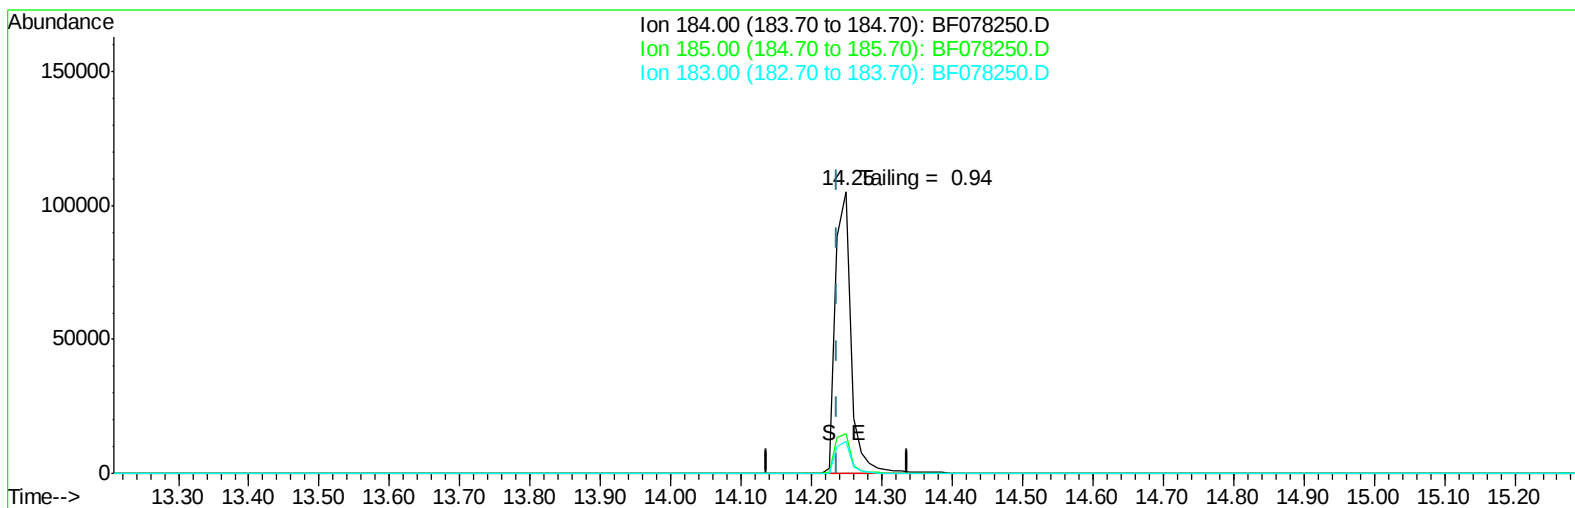

TIC: BF078250.D

(76) Benzidine

14.248min (+0.011) 0.00ng

response 157118

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	13.97
183.00	11.90	11.29
0.00	0.00	0.00