
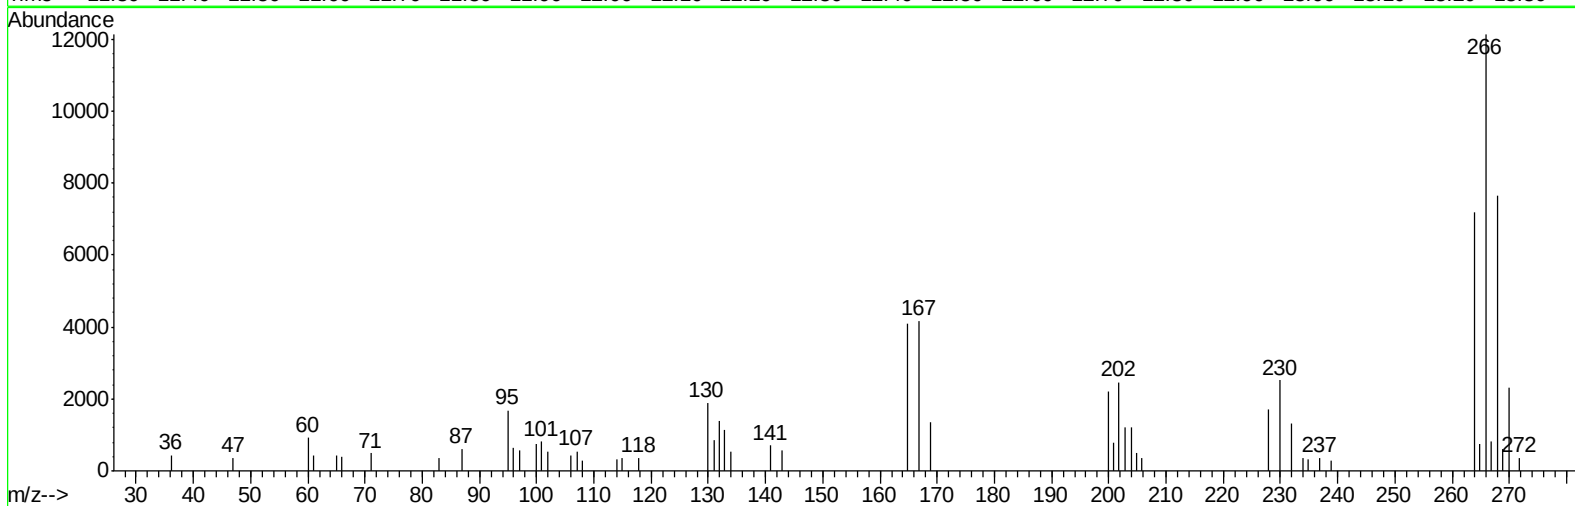


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF040615\  
Data File : BF078272.D  
Acq On : 6 Apr 2015 23:22  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 08:14:09 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF040115.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Apr 07 04:11:17 2015  
Response via : Initial Calibration

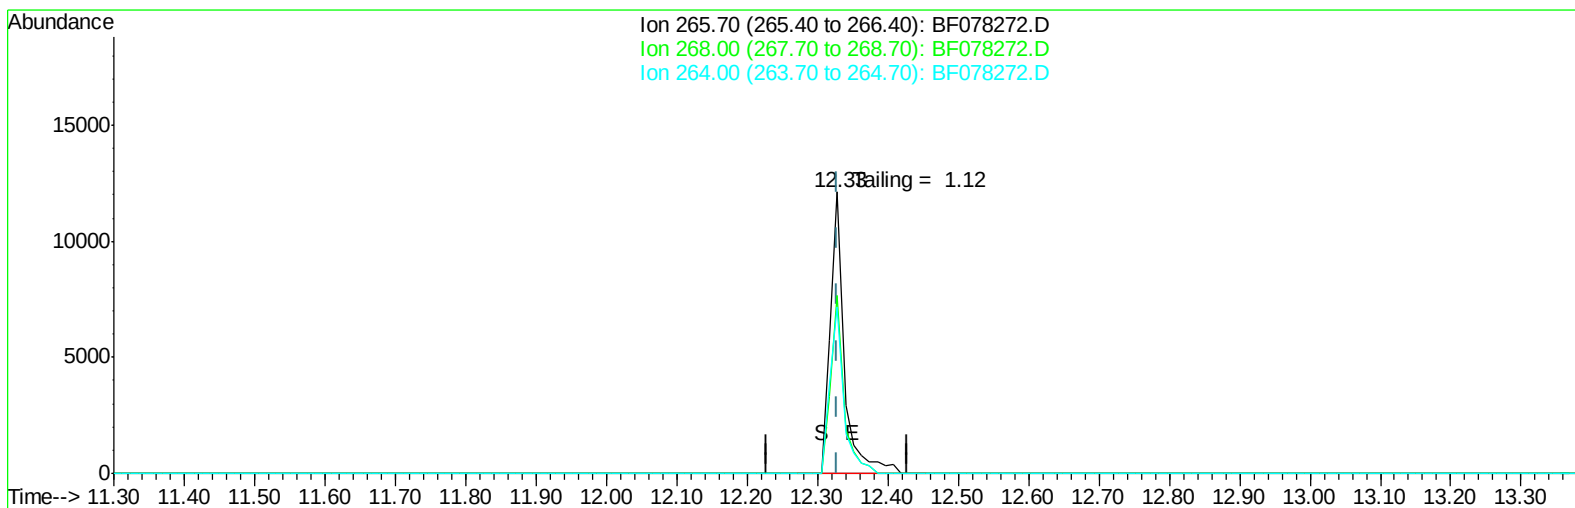

TIC: BF078272.D

(69) Pentachlorophenol (C)



12.328min (-0.000) 0.00ng

response 16289

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 62.60 | 63.13 |
| 264.00 | 62.50 | 59.27 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF040615\  
Data File : BF078272.D  
Acq On : 6 Apr 2015 23:22  
Operator : TP/IZ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 08:14:09 2015  
Quant Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF040115.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Apr 07 04:11:17 2015  
Response via : Initial Calibration

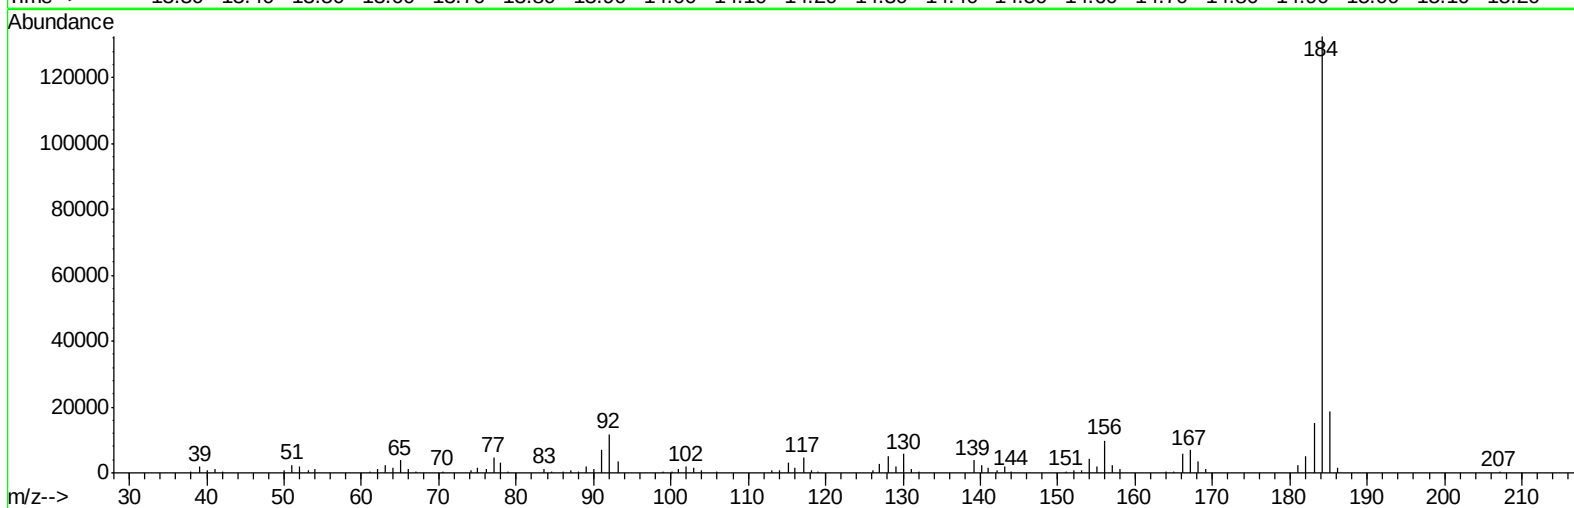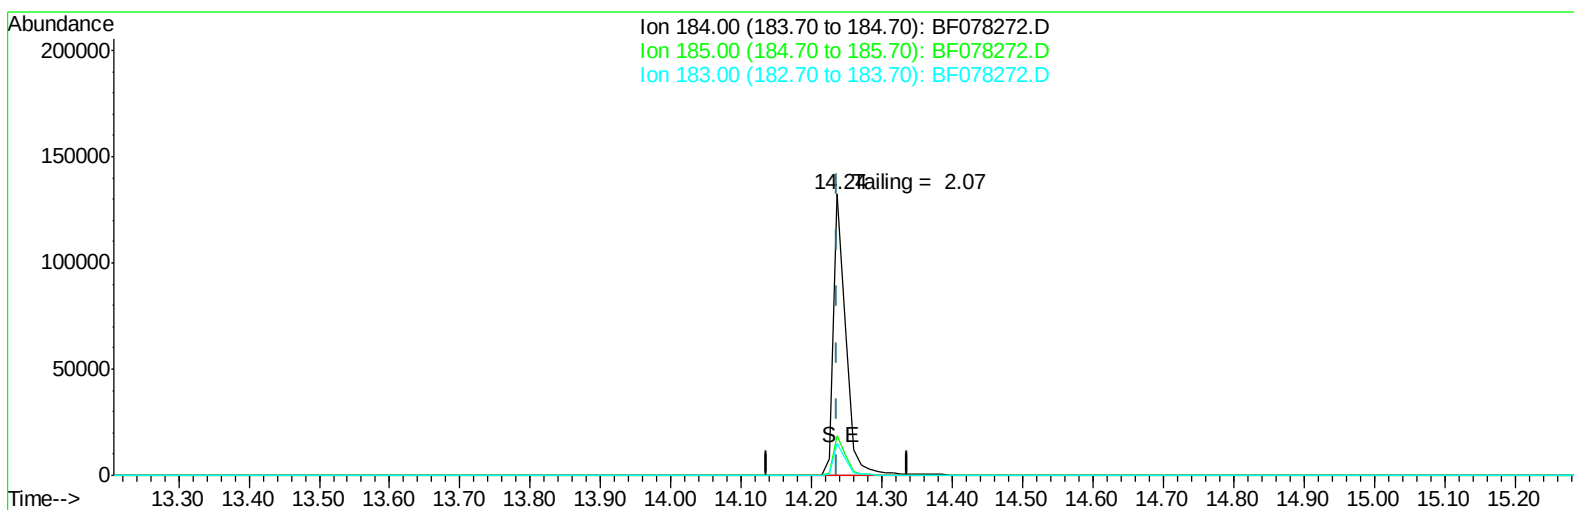

TIC: BF078272.D

(76) Benzidine

14.237min (-0.000) 0.00ng

response 156169

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.20 | 14.14 |
| 183.00 | 11.90 | 11.52 |
| 0.00   | 0.00  | 0.00  |