

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040615\
 Data File : BF078268.D
 Acq On : 6 Apr 2015 20:36
 Operator : TP/IZ
 Sample : G1755-06
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-04

Quant Time: Apr 07 02:15:39 2015
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 07 02:08:45 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.98	152	40548	20.00	ng	0.00
21) Naphthalene-d8	8.56	136	162267	20.00	ng	0.00
38) Acenaphthene-d10	10.72	164	84003	20.00	ng	0.00
63) Phenanthrene-d10	12.55	188	160911	20.00	ng	-0.01
75) Chrysene-d12	15.84	240	167527	20.00	ng	-0.01
86) Perylene-d12	17.64	264	156881	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.26	112	127460	51.83	ng	0.00
7) Phenol-d6	6.58	99	97289	31.57	ng	0.00
23) Nitrobenzene-d5	7.68	82	230887	86.25	ng	0.00
41) 2,4,6-Tribromophenol	11.70	330	100395	144.10	ng	0.00
44) 2-Fluorobiphenyl	9.90	172	526506	89.59	ng	0.00
78) Terphenyl-d14	14.55	244	594257	80.16	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040615\
Data File : BF078268.D
Acq On : 6 Apr 2015 20:36
Operator : TP/IZ
Sample : G1755-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-04

Quant Time: Apr 07 02:15:39 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 07 02:08:45 2015
Response via : Initial Calibration

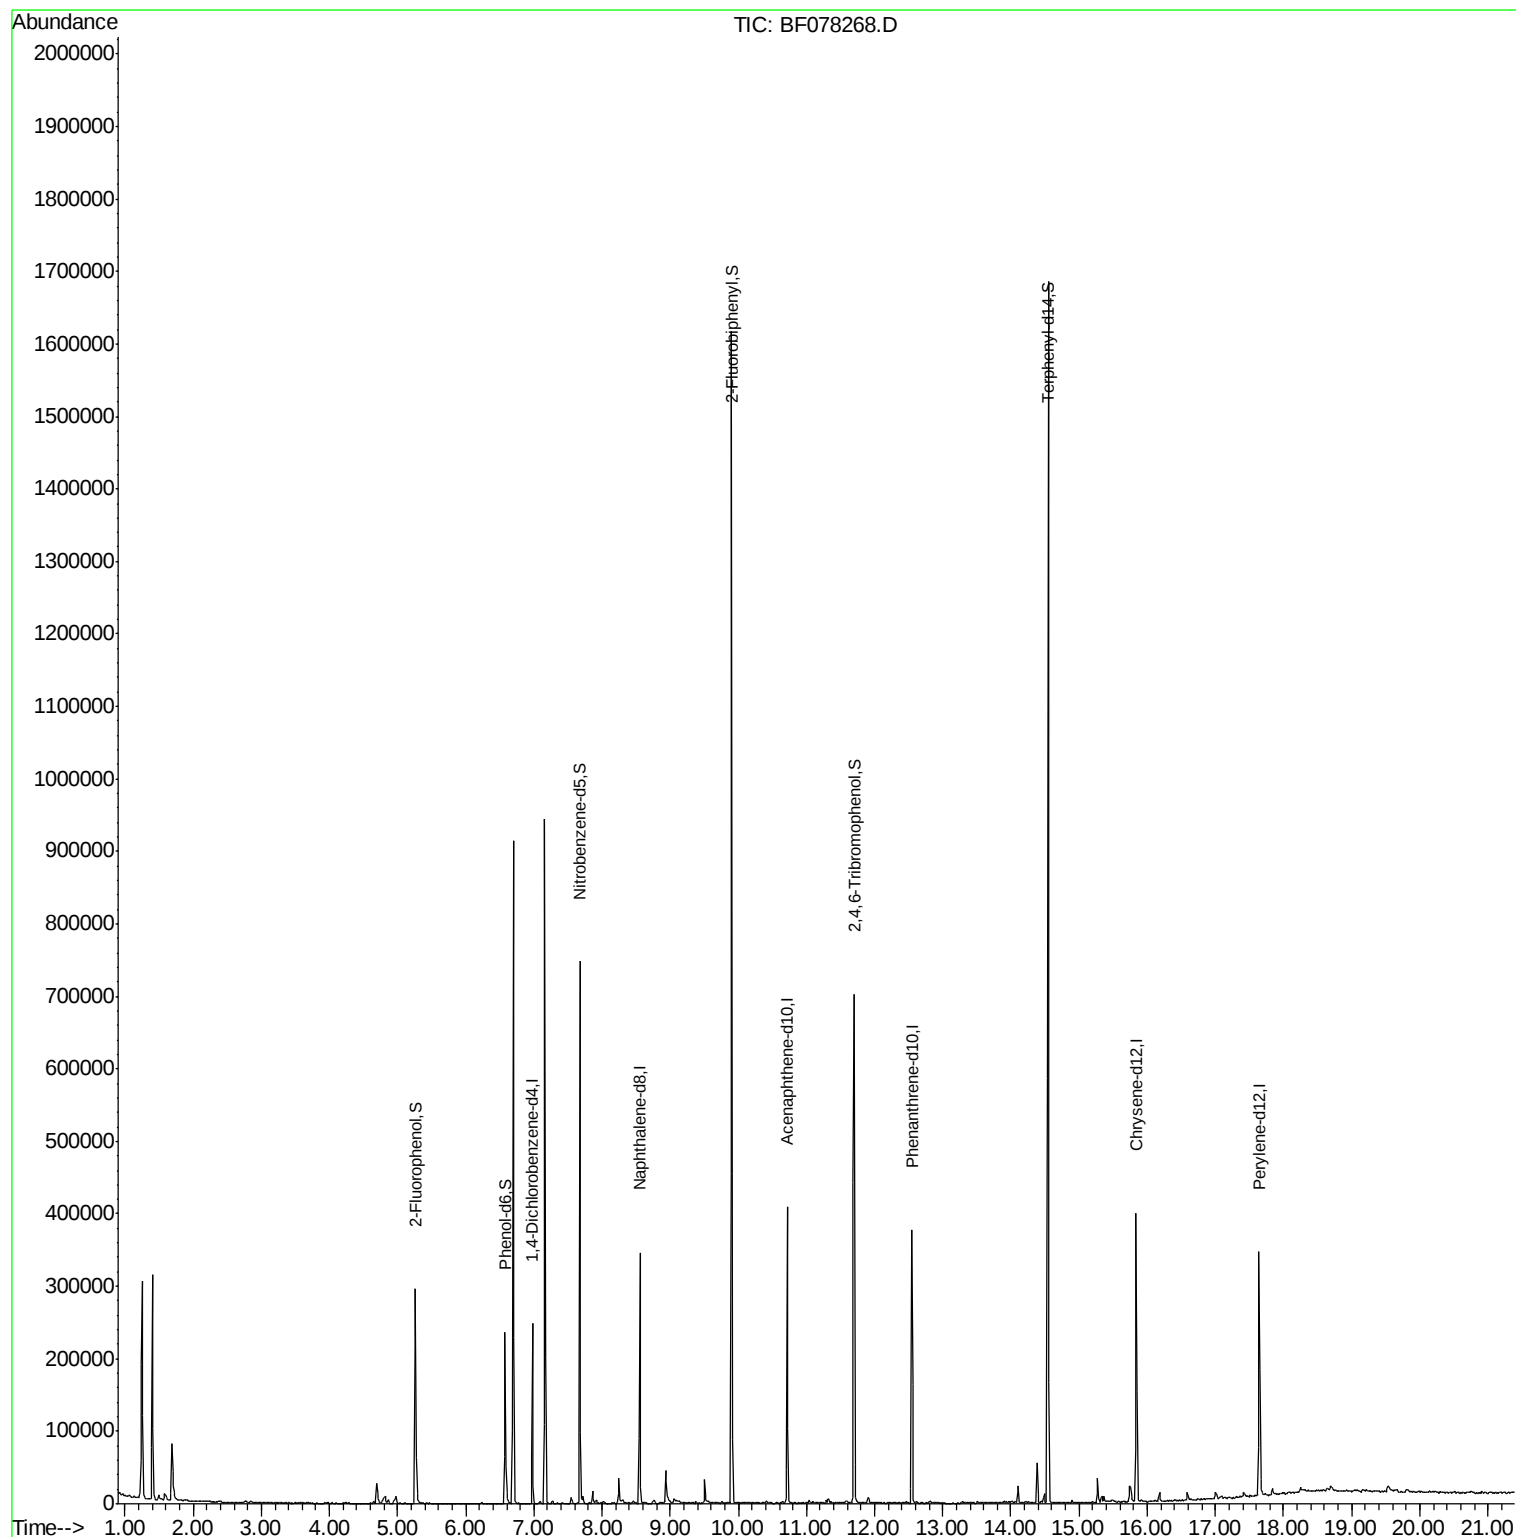

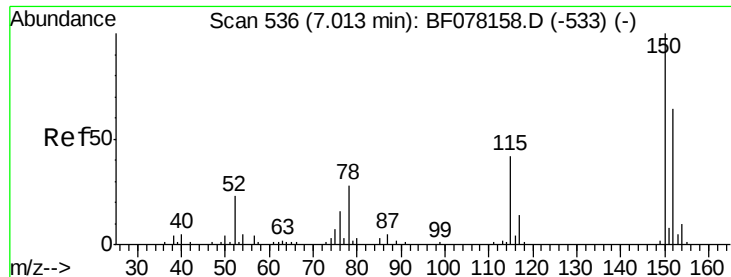


#1




1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.98 min Scan# 533
Delta R.T. -0.00 min
Lab File: BF078268.D
Acq: 6 Apr 2015 20:36

Instrument :
BNA_F
ClientSampleId :
MW-04

Tot Ion:152 Resp: 40548
Ion Ratio Lower Upper
152 100
150 156.9 125.9 188.9
115 58.6 52.7 79.1

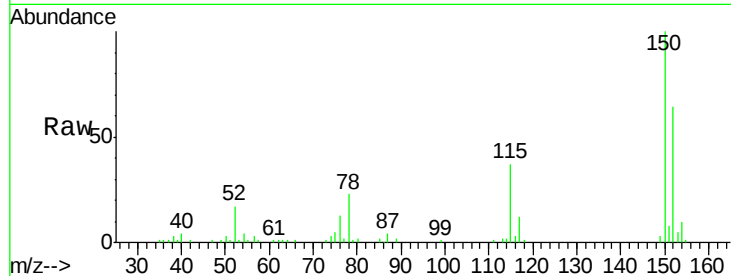


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

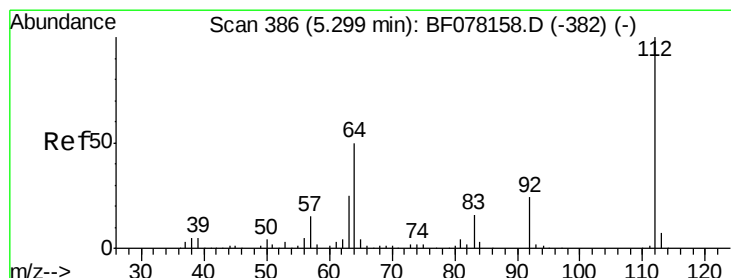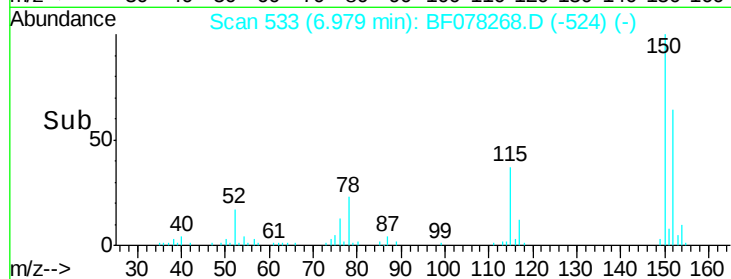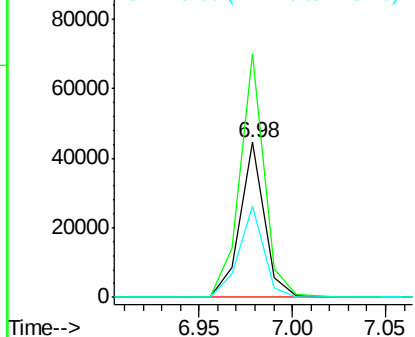



#5


2-Fluorophenol
Concen: 51.83 ng
RT: 5.26 min Scan# 383
Delta R.T. -0.00 min
Lab File: BF078268.D
Acq: 6 Apr 2015 20:36

Tgt Ion:112 Resp: 127460
Ion Ratio Lower Upper
112 100
64 50.8 39.9 59.9
63 26.4 20.2 30.4

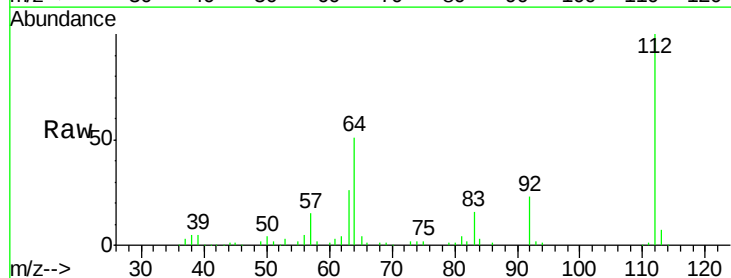

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF0
Ion 63.00 (62.70 to 63.70): BF0

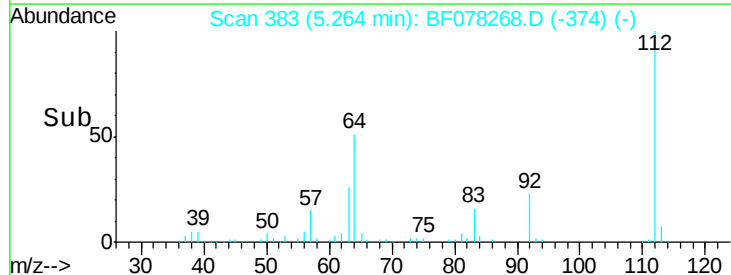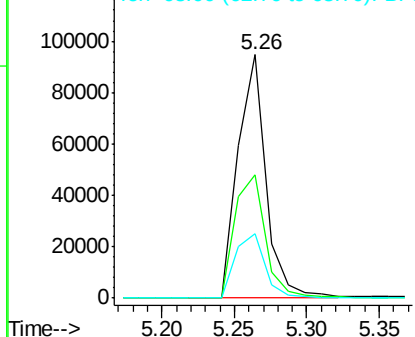

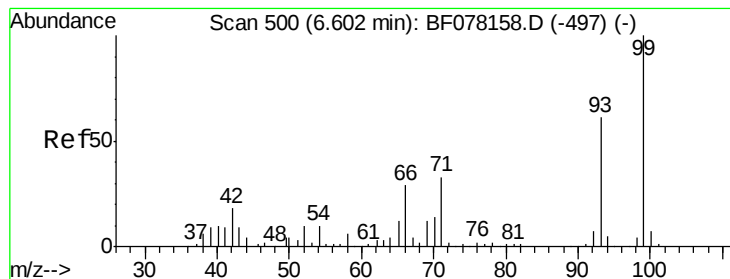

#7

Phenol-d6

Concen: 31.57 ng

RT: 6.58 min Scan# 498

Delta R.T. -0.00 min

Lab File: BF078268.D

Acq: 6 Apr 2015 20:36

Instrument :

BNA_F

ClientSampleId :

MW-04


Tot Ion: 99 Resp: 97289

Ion Ratio Lower Upper




99 100

42 15.0 14.8 22.2

71 30.3 26.6 39.8

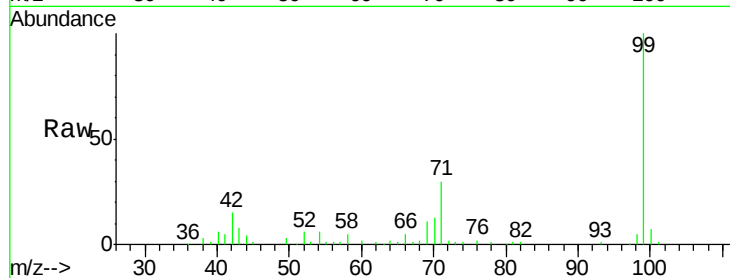

Abundance Ion 99.00 (98.70 to 99.70): BF0
Ion 42.00 (41.70 to 42.70): BF0
Ion 71.00 (70.70 to 71.70): BF0

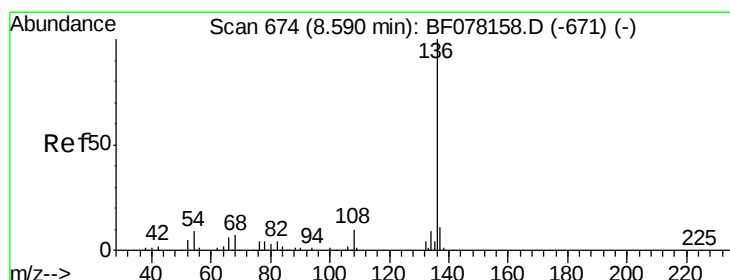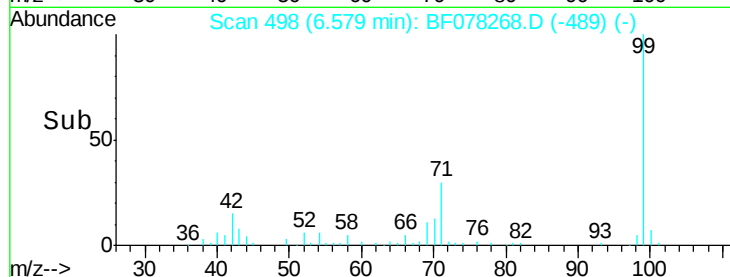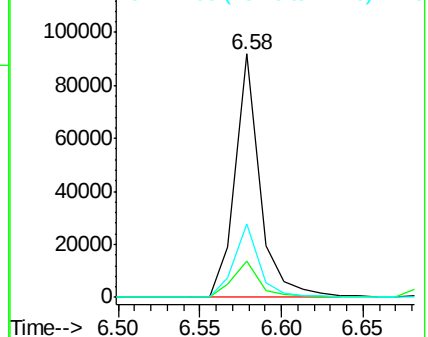

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.56 min Scan# 671

Delta R.T. -0.00 min

Lab File: BF078268.D

Acq: 6 Apr 2015 20:36

Tgt Ion: 136 Resp: 162267


Ion Ratio Lower Upper

136 100



137 10.5 9.0 13.4

54 6.4 7.0 10.6#

68 5.3 5.4 8.2#

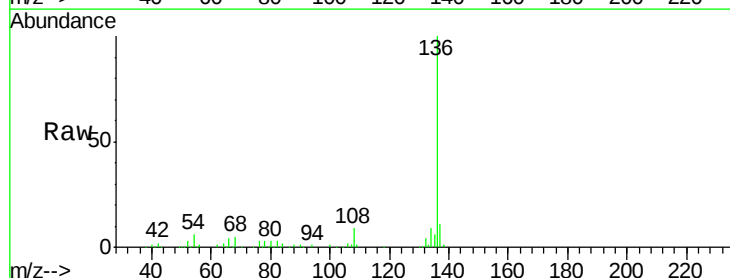

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF0
Ion 68.00 (67.70 to 68.70): BF0

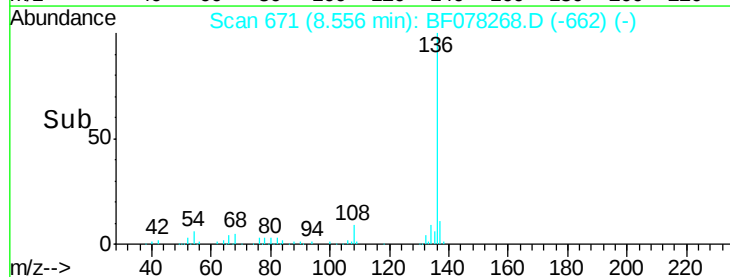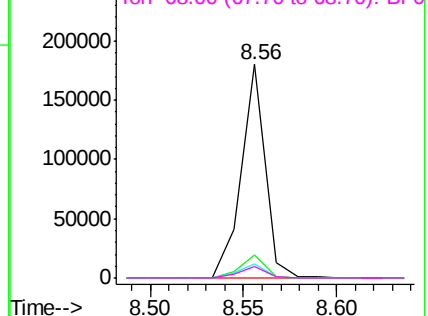



#23

Nitrobenzene-d5

Concen: 86.25 ng

RT: 7.68 min Scan# 594

Delta R.T. -0.00 min

Lab File: BF078268.D

Acq: 6 Apr 2015 20:36

Instrument :

BNA_F

ClientSampleId :

MW-04


Tot Ion: 82 Resp: 230887

Ion Ratio Lower Upper




82 100

128 43.7 31.8 47.8

54 48.7 41.5 62.3

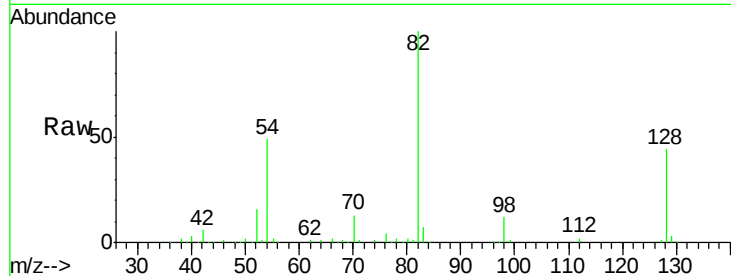

Abundance Ion 82.00 (81.70 to 82.70): BF0
Ion 128.00 (127.70 to 128.70): B
Ion 54.00 (53.70 to 54.70): BF0

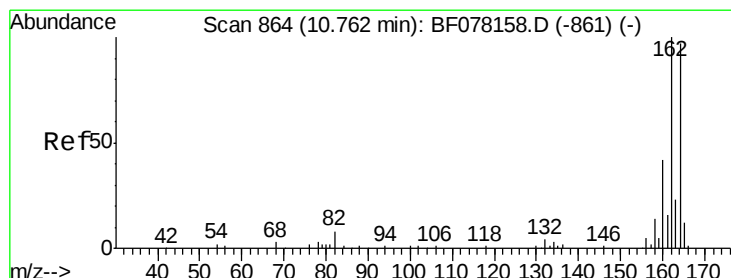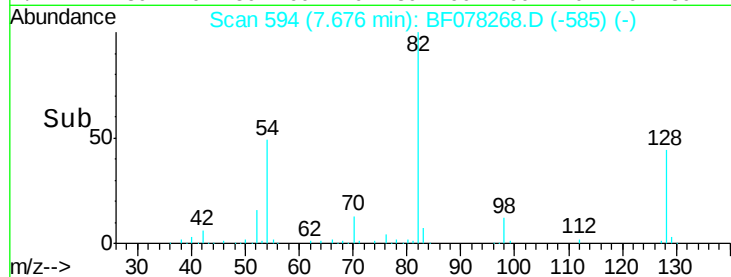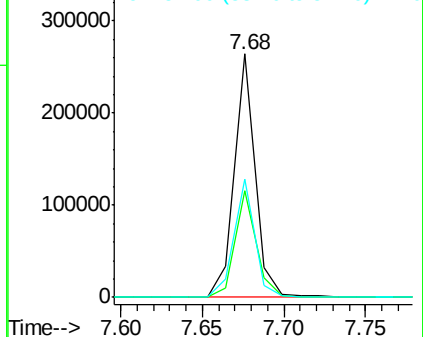

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 10.72 min Scan# 860

Delta R.T. -0.00 min

Lab File: BF078268.D

Acq: 6 Apr 2015 20:36


Tgt Ion:164 Resp: 84003

Ion Ratio Lower Upper



164 100

162 102.7 82.2 123.2

160 43.3 34.7 52.1

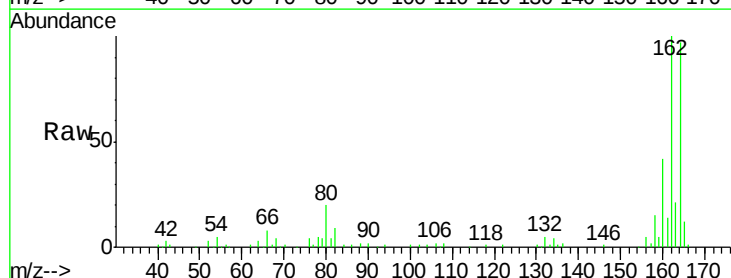

Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

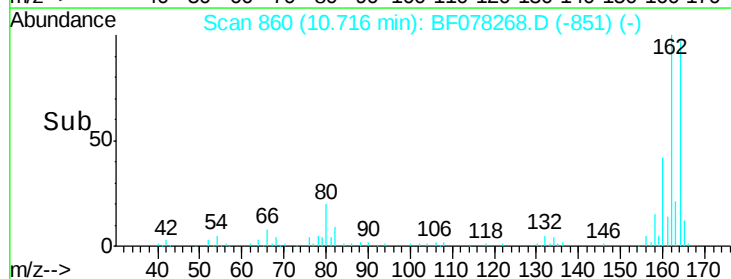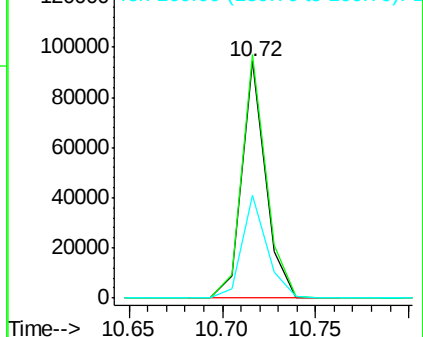







#41
 2,4,6-Tribromophenol
 Concen: 144.10 ng
 RT: 11.70 min Scan# 946
 Delta R.T. -0.00 min
 Lab File: BF078268.D
 Acq: 6 Apr 2015 20:36

Instrument :
 BNA_F
 ClientSampled :
 MW-04

Tot Ion	Ratio	Lower	Upper
330	100		
332	97.2	78.6	117.8
141	38.3	31.2	46.8

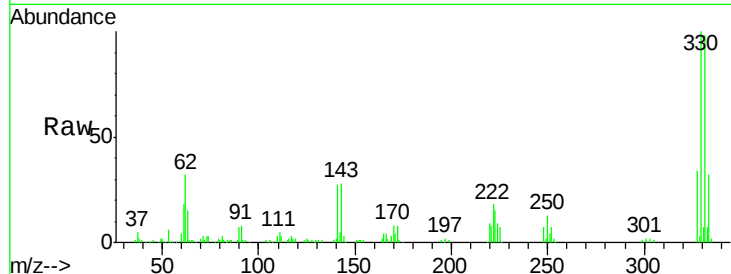


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

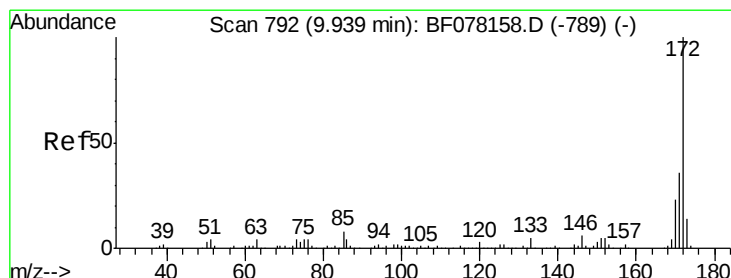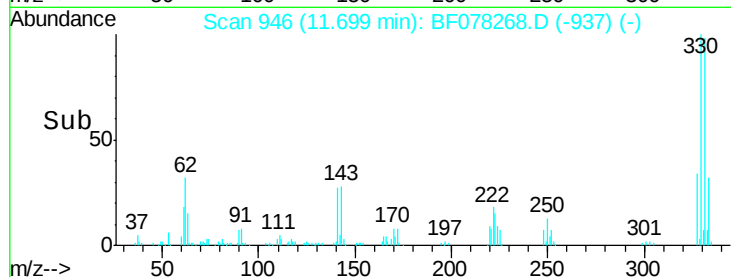
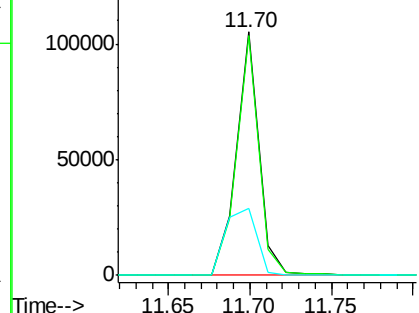



#44
 2-Fluorobiphenyl
 Concen: 89.59 ng
 RT: 9.90 min Scan# 789
 Delta R.T. -0.00 min
 Lab File: BF078268.D
 Acq: 6 Apr 2015 20:36

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.7	28.6	42.8
170	23.2	18.5	27.7

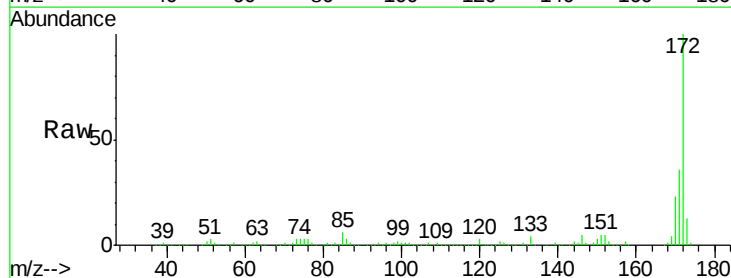

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

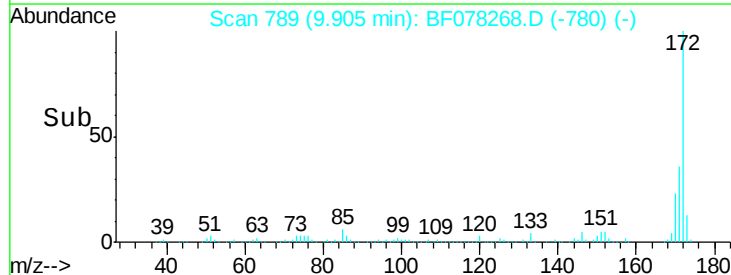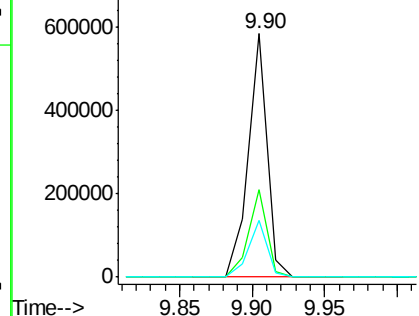


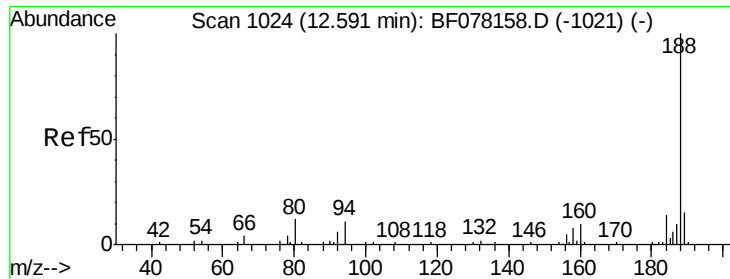




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.55 min Scan# 1020
Delta R.T. -0.01 min
Lab File: BF078268.D
Acq: 6 Apr 2015 20:36

Instrument :
BNA_F
ClientSampleId :
MW-04

Tot Ion	Ratio	Lower	Upper
188	100		
94	11.1	9.0	13.4
80	12.4	9.5	14.3

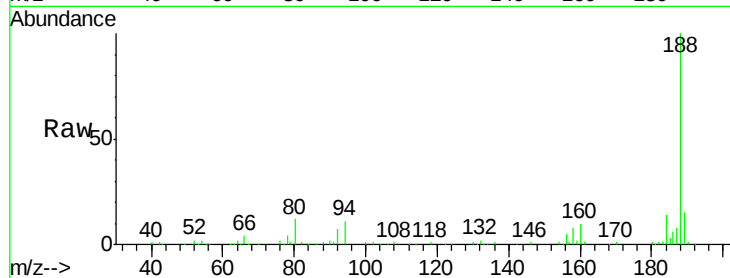


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

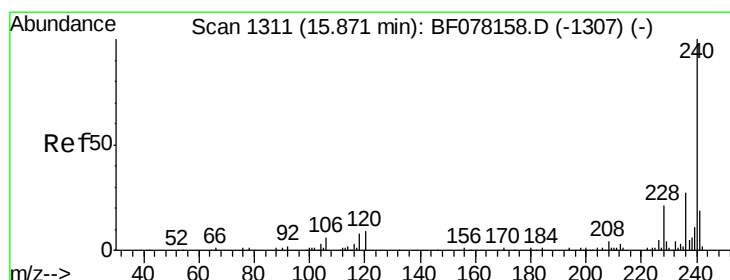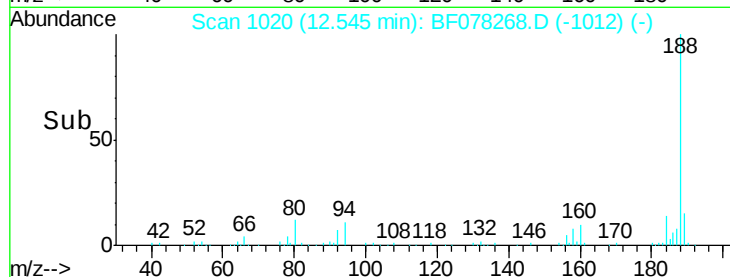
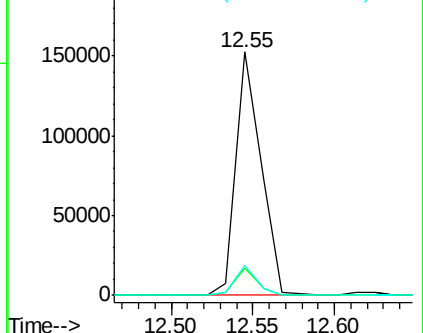



#75
Chrysene-d12
Concen: 20.00 ng
RT: 15.84 min Scan# 1308
Delta R.T. -0.01 min
Lab File: BF078268.D
Acq: 6 Apr 2015 20:36

Tgt Ion	Ratio	Lower	Upper
240	100		
120	12.3	7.1	10.7#
236	24.5	21.4	32.2

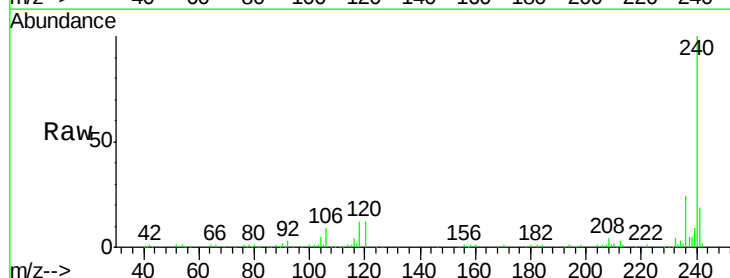

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



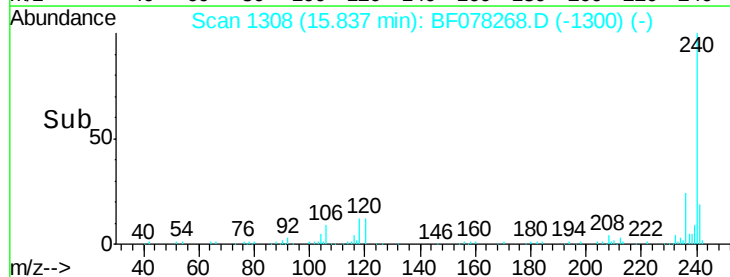
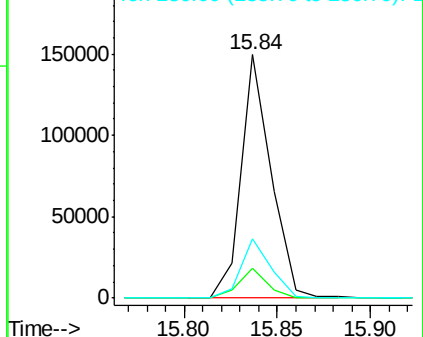


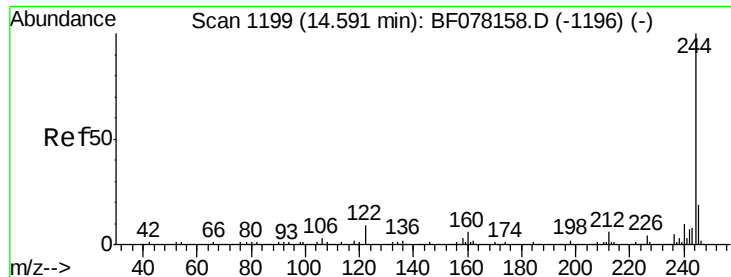

#78
 Terphenyl-d14
 Concen: 80.16 ng
 RT: 14.55 min Scan# 1195
 Delta R.T. -0.00 min
 Lab File: BF078268.D
 Acq: 6 Apr 2015 20:36

Instrument :
 BNA_F
 ClientSampleId :
 MW-04

Tot Ion:244 Resp: 594257
 Ion Ratio Lower Upper
 244 100
 212 6.7 5.0 7.4
 122 11.3 7.1 10.7#

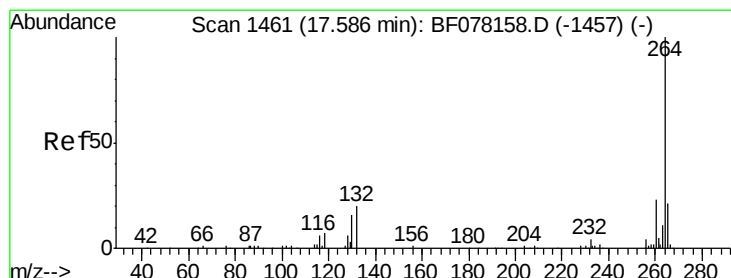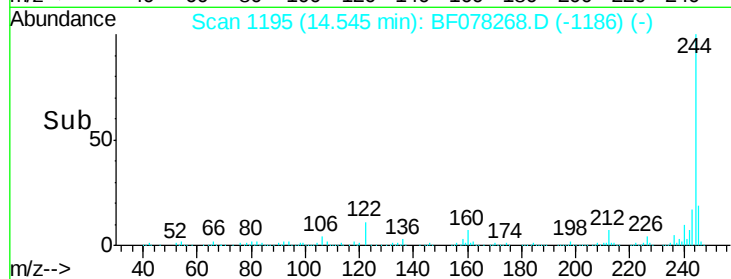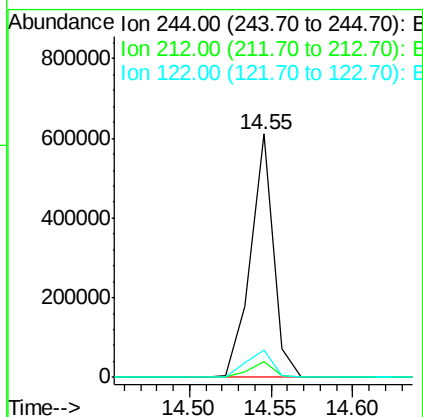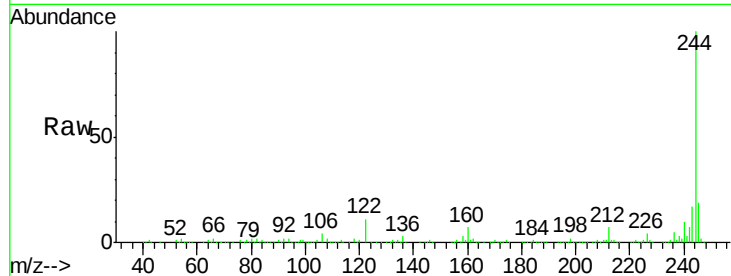

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 17.64 min Scan# 1466
 Delta R.T. -0.00 min
 Lab File: BF078268.D
 Acq: 6 Apr 2015 20:36

Tgt Ion:264 Resp: 156881
 Ion Ratio Lower Upper
 264 100
 260 23.0 18.6 27.8
 265 22.4 17.0 25.6

