


Data Path : Z:\HPCHEM1\BNA F\Data\BF040615\
 Data File : BF078250.D
 Acq On : 6 Apr 2015 11:57
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 03 14:42:25 2015

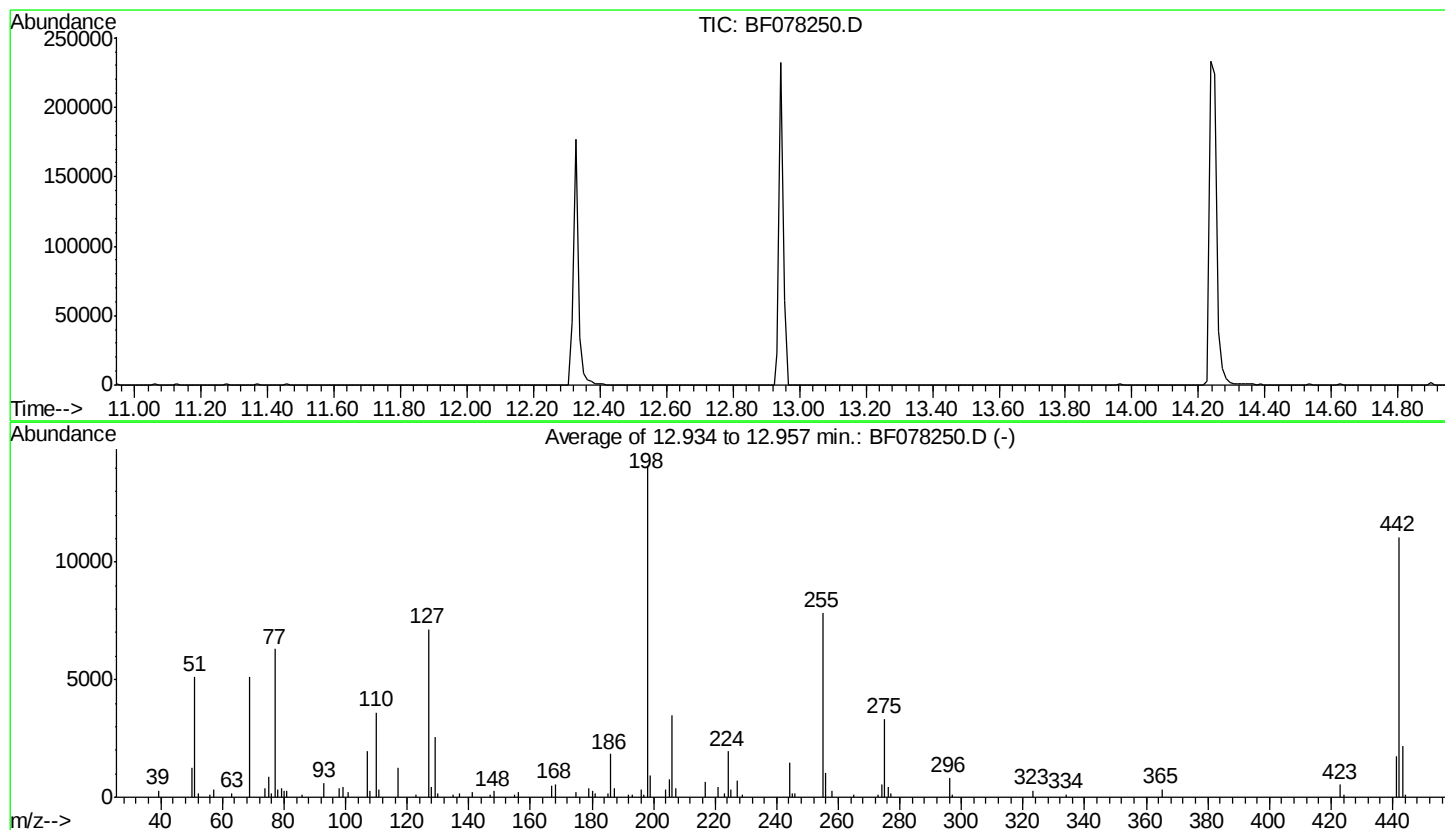

AutoFind: Scans 1054, 1055, 1056; Background Corrected with Scan 1051

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	5134	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.4	5129	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.7	7144	PASS
197	198	0.00	2	0.9	128	PASS
198	198	100	100	100.0	14104	PASS
199	198	5	9	6.5	916	PASS
275	198	10	60	23.7	3345	PASS
365	198	1	100	2.4	340	PASS
441	442	0.01	24	15.9	1763	PASS
442	198	50	100	78.5	11074	PASS
443	442	15	24	19.8	2194	PASS