

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040616\
 Data File : BF086117.D
 Acq On : 7 Apr 2016 00:21
 Operator : UM/SJ
 Sample : H2087-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TILCON-MH-SF-002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.556	214	216	219	rVV2	56116	126449	5.32%	0.320%
2	4.624	219	222	228	rVV2	47876	175533	7.39%	0.444%
3	4.876	242	244	246	rVV2	53259	74780	3.15%	0.189%
4	4.921	246	248	254	rVV	116219	224498	9.45%	0.568%
5	5.059	258	260	263	rVB2	88517	86990	3.66%	0.220%
6	5.344	282	285	287	rBV	2095485	2288333	96.30%	5.786%
7	5.401	289	290	292	rVB	164224	182845	7.69%	0.462%
8	5.470	292	296	297	rBV3	630696	1411258	59.39%	3.568%
9	5.664	311	313	316	rVV2	59213	112292	4.73%	0.284%
10	6.076	346	349	351	rVB2	59686	120651	5.08%	0.305%
11	6.396	374	377	379	rBV	2191771	2376204	100.00%	6.008%
12	6.510	385	387	390	rBV	2034811	2165743	91.14%	5.476%
13	6.613	392	396	397	rBV3	64609	133693	5.63%	0.338%
14	6.739	406	407	410	rBV	583845	672587	28.31%	1.701%
15	6.899	419	421	423	rBV	2078984	1857929	78.19%	4.698%
16	7.219	444	449	451	rBV2	49331	99594	4.19%	0.252%
17	7.310	455	457	461	rBV	1330830	1380604	58.10%	3.491%
18	7.447	466	469	472	rVB2	78899	142448	5.99%	0.360%
19	8.030	518	520	522	rBV	981425	834648	35.13%	2.110%
20	8.179	531	533	538	rBV4	73804	202319	8.51%	0.512%
21	8.499	558	561	564	rBB3	115701	185286	7.80%	0.468%
22	8.567	564	567	569	rBV3	149675	316680	13.33%	0.801%
23	8.602	569	570	572	rVV	93240	82538	3.47%	0.209%
24	8.716	579	580	583	rBV3	58110	86221	3.63%	0.218%
25	8.853	588	592	594	rVV4	112006	272707	11.48%	0.690%
26	8.956	597	601	602	rVV3	81169	120877	5.09%	0.306%
27	8.979	602	603	607	rVV3	115897	187784	7.90%	0.475%
28	9.036	607	608	612	rVB2	73959	102701	4.32%	0.260%
29	9.105	612	614	617	rBV	2443368	2207745	92.91%	5.582%
30	9.505	647	649	651	rBV	248290	201114	8.46%	0.509%
31	9.688	661	665	666	rBV2	85712	153218	6.45%	0.387%
32	9.779	671	673	676	rVV	821632	860433	36.21%	2.176%
33	9.848	677	679	682	rVB3	89337	192519	8.10%	0.487%
34	9.893	682	683	684	rBV	83640	71564	3.01%	0.181%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040616\
 Data File : BF086117.D
 Acq On : 7 Apr 2016 00:21
 Operator : UM/SJ
 Sample : H2087-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TILCON-MH-SF-002

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	10.110	700	702	710	rBV2	50608	216098	9.09%	0.546%
36	10.259	712	715	718	rBV4	28975	71148	2.99%	0.180%
37	10.350	721	723	726	rBV3	123886	194292	8.18%	0.491%
38	10.442	730	731	734	rBV3	51291	81521	3.43%	0.206%
39	10.568	740	742	745	rBV2	998077	1127564	47.45%	2.851%
40	10.682	751	752	754	rBV	76797	93193	3.92%	0.236%
41	10.739	754	757	760	rVB4	52021	103512	4.36%	0.262%
42	10.808	760	763	768	rBV6	51312	164481	6.92%	0.416%
43	10.899	768	771	774	rBV4	34532	93958	3.95%	0.238%
44	10.979	774	778	779	rVV4	88880	200778	8.45%	0.508%
45	11.025	779	782	786	rVV5	49680	124407	5.24%	0.315%
46	11.105	786	789	790	rVV3	34139	74184	3.12%	0.188%
47	11.196	795	797	801	rVB4	65514	100334	4.22%	0.254%
48	11.265	801	803	805	rBV	726059	636661	26.79%	1.610%
49	11.368	809	812	815	rVB2	43885	95507	4.02%	0.241%
50	11.425	815	817	818	rBV	70462	73821	3.11%	0.187%
51	11.493	821	823	826	rVV3	60771	129028	5.43%	0.326%
52	11.562	826	829	831	rVV	46568	79401	3.34%	0.201%
53	11.665	835	838	843	rVV7	79996	241974	10.18%	0.612%
54	11.802	848	850	855	rVV2	91980	209316	8.81%	0.529%
55	12.088	872	875	878	rBV5	47021	99577	4.19%	0.252%
56	12.294	890	893	897	rBV4	95942	236037	9.93%	0.597%
57	12.465	905	908	911	rBV4	62849	126189	5.31%	0.319%
58	12.522	911	913	916	rVB2	156003	176442	7.43%	0.446%
59	12.648	923	924	926	rBV2	95074	135693	5.71%	0.343%
60	12.808	934	938	939	rBV3	163425	270542	11.39%	0.684%
61	12.854	939	942	944	rVV	1556634	2305409	97.02%	5.829%
62	12.968	951	952	954	rVB2	60156	72241	3.04%	0.183%
63	13.025	954	957	959	rBV3	48114	73540	3.09%	0.186%
64	13.105	960	964	965	rBV2	229945	338607	14.25%	0.856%
65	13.128	965	966	972	rVB4	148487	238415	10.03%	0.603%
66	13.219	972	974	977	rBV3	218024	416194	17.52%	1.052%
67	13.288	977	980	986	rVB8	95652	389313	16.38%	0.984%
68	13.425	986	992	996	rBV5	226566	761451	32.04%	1.925%
69	13.539	1000	1002	1003	rBV2	68087	79729	3.36%	0.202%
70	13.631	1007	1010	1014	rBV6	274597	781778	32.90%	1.977%
71	13.745	1017	1020	1023	rBV	390156	619253	26.06%	1.566%

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040616\
 Data File : BF086117.D
 Acq On : 7 Apr 2016 00:21
 Operator : UM/SJ
 Sample : H2087-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 TILCON-MH-SF-002

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	13.791	1023	1024	1025	rVV	133258	133755	5.63%	0.338%
73	13.825	1025	1027	1028	rVV2	142493	177625	7.48%	0.449%
74	13.871	1028	1031	1032	rVV3	204672	532632	22.42%	1.347%
75	13.894	1032	1033	1038	rVB	683338	1200267	50.51%	3.035%
76	13.997	1038	1042	1043	rBV2	86118	165080	6.95%	0.417%
77	14.145	1050	1055	1058	rVB7	102536	367969	15.49%	0.930%
78	14.202	1058	1060	1062	rVB3	111799	123825	5.21%	0.313%
79	14.339	1070	1072	1073	rBV2	88851	88324	3.72%	0.223%
80	14.397	1075	1077	1078	rVV	85485	100339	4.22%	0.254%
81	14.477	1081	1084	1087	rVB3	96484	210387	8.85%	0.532%
82	14.534	1087	1089	1092	rBV3	207073	414943	17.46%	1.049%
83	14.579	1092	1093	1095	rVV2	231152	267165	11.24%	0.676%
84	14.659	1098	1100	1101	rVV2	96754	156376	6.58%	0.395%
85	14.728	1103	1106	1108	rVB3	337903	527684	22.21%	1.334%
86	15.117	1136	1140	1142	rBV3	141004	215507	9.07%	0.545%
87	15.151	1142	1143	1144	rVV	64631	81088	3.41%	0.205%
88	15.185	1144	1146	1148	rVV2	261297	371732	15.64%	0.940%
89	15.231	1148	1150	1151	rVV2	79436	94257	3.97%	0.238%
90	15.265	1151	1153	1154	rVV2	67917	124054	5.22%	0.314%
91	15.300	1154	1156	1160	rVV	467023	663188	27.91%	1.677%
92	15.380	1160	1163	1166	rVB5	90309	167241	7.04%	0.423%
93	15.494	1171	1173	1177	rVB5	154231	367255	15.46%	0.929%
94	15.562	1177	1179	1184	rVB6	191105	450414	18.96%	1.139%
95	15.642	1184	1186	1187	rBV2	87595	137337	5.78%	0.347%
96	15.677	1187	1189	1192	rVB4	115280	246723	10.38%	0.624%
97	15.802	1197	1200	1202	rVV4	106495	318206	13.39%	0.805%
98	15.860	1202	1205	1208	rVV4	175782	412113	17.34%	1.042%
99	15.928	1209	1211	1214	rVV4	113912	239628	10.08%	0.606%
100	15.974	1214	1215	1221	rVV5	89475	252711	10.64%	0.639%


Sum of corrected areas: 39550198

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040616\
Data File : BF086117.D
Acq On : 7 Apr 2016 00:21
Operator : UM/SJ
Sample : H2087-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TILCON-MH-SF-002

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

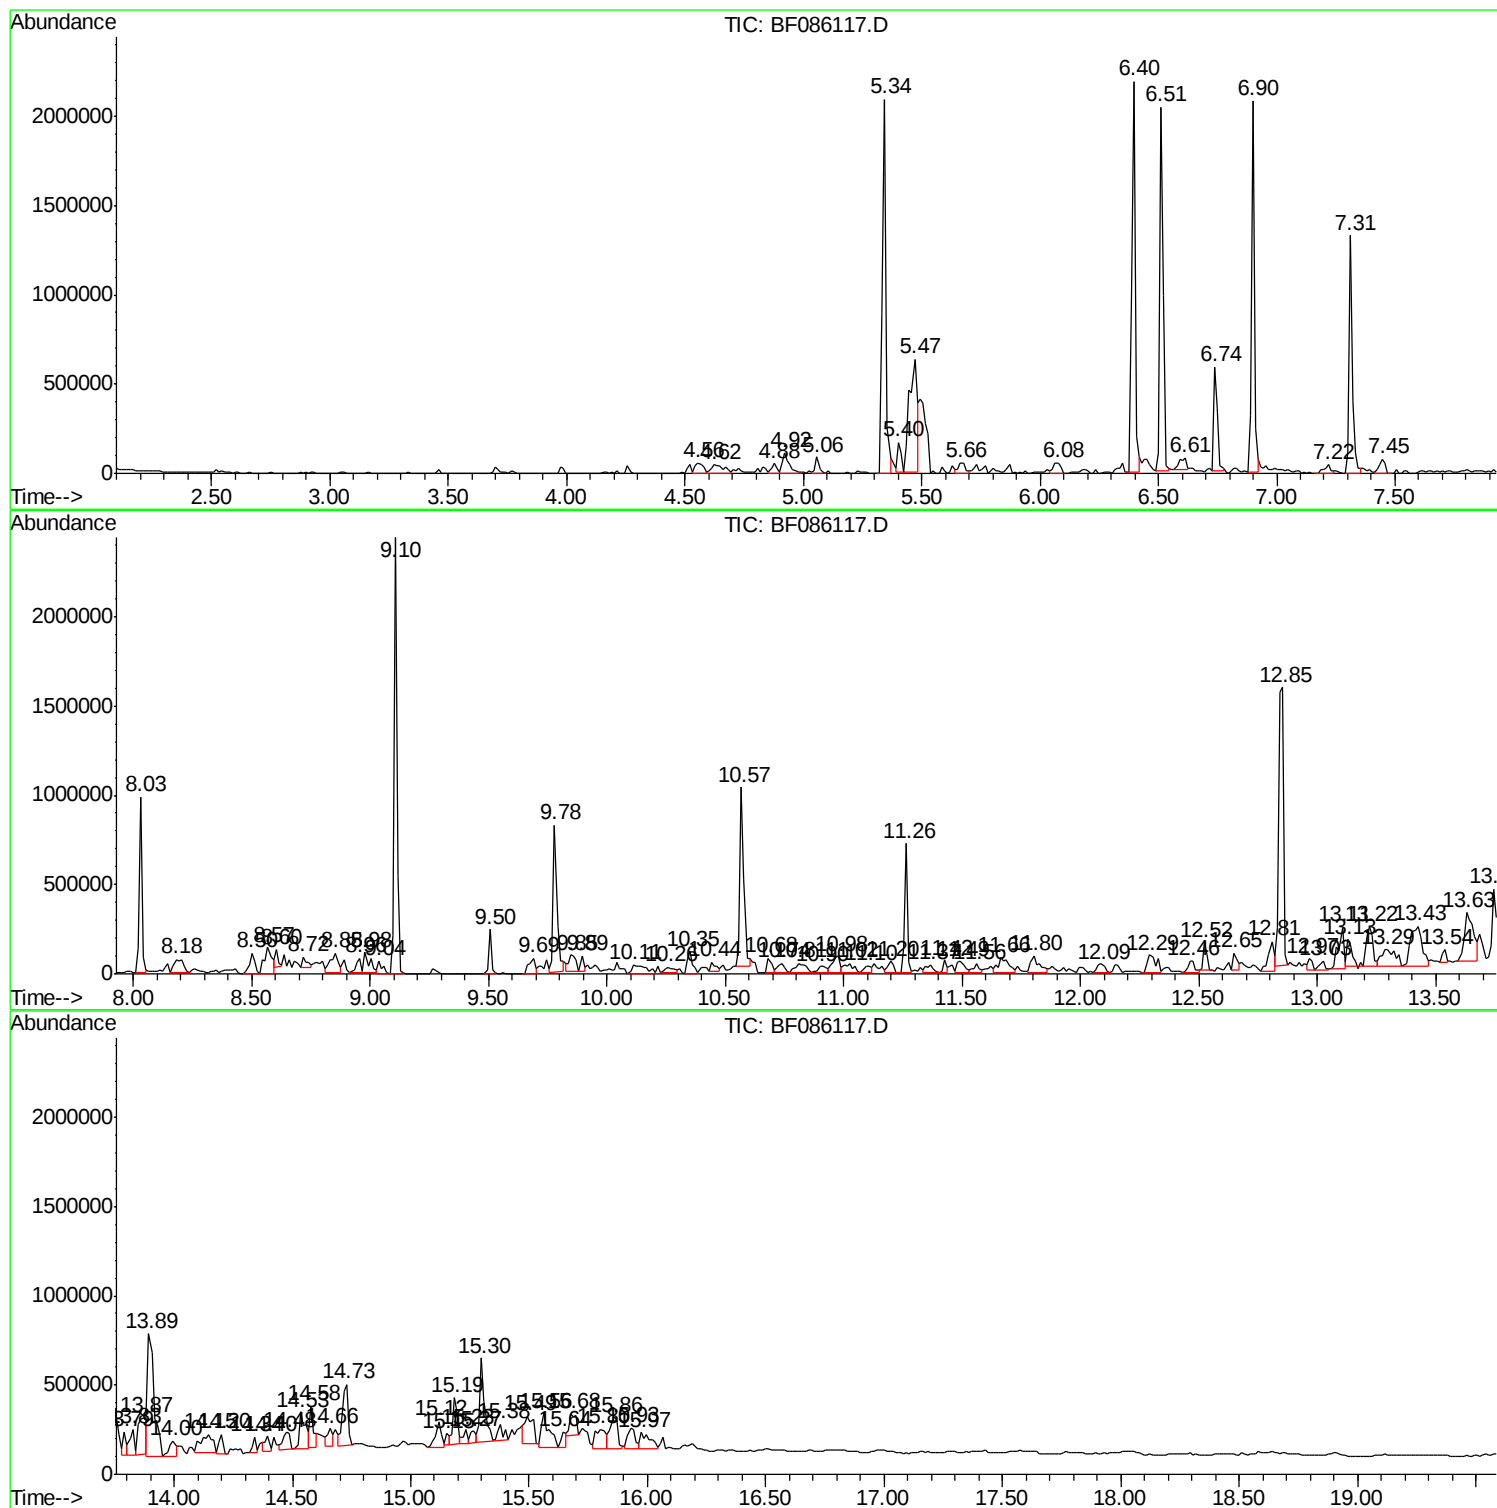

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040616\
Data File : BF086117.D
Acq On : 7 Apr 2016 00:21
Operator : UM/SJ
Sample : H2087-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TILCON-MH-SF-002









Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.47 Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.47	41.97 ng	1411260	1,4-Dichlorobenzene-d4	6.74

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	2	Benzenamine, 4-trifluoromethoxyv-...	544	C23H15BrF6N2O2	284495-96-1	38
2		Vanadium, oxo[2,7,12,17-tetraeth...	543	C32H36N4OV	014055-20-0	9

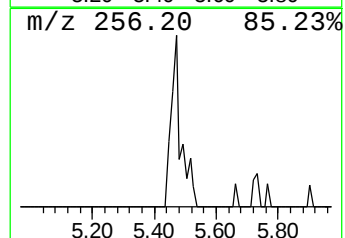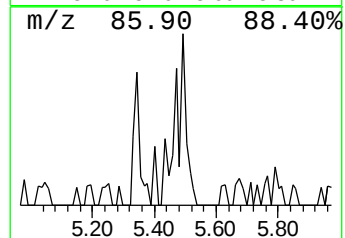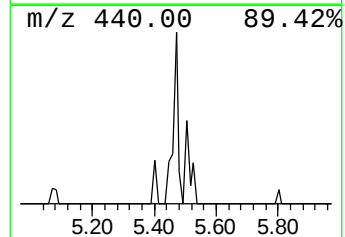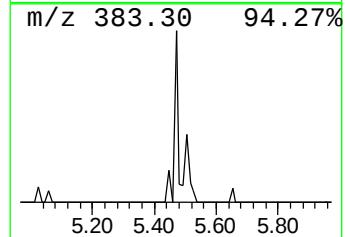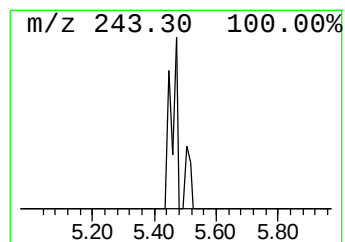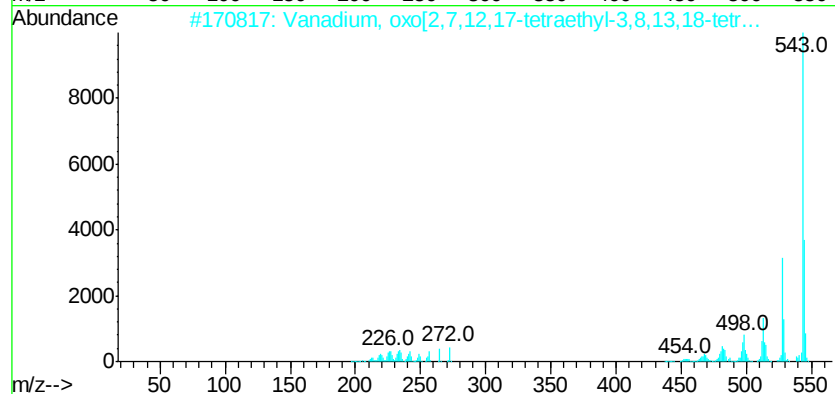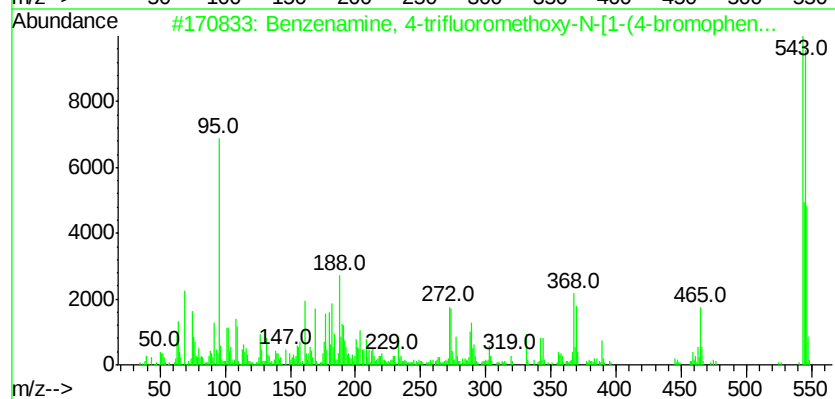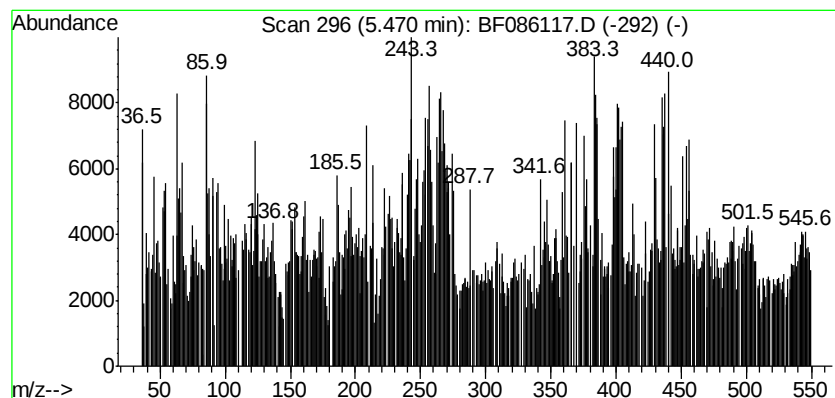

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040616\
Data File : BF086117.D
Acq On : 7 Apr 2016 00:21
Operator : UM/SJ
Sample : H2087-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TILCON-MH-SF-002










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.51 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.51	64.40 ng	2165740	1,4-Dichlorobenzene-d4	6.74

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		Tranylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
3		5-Aminoindole	132	C8H8N2	005192-03-0	9
4		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

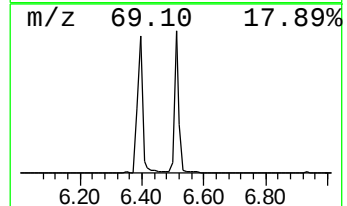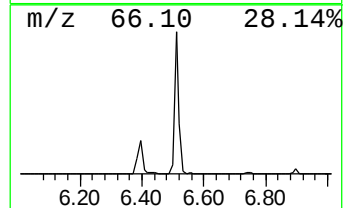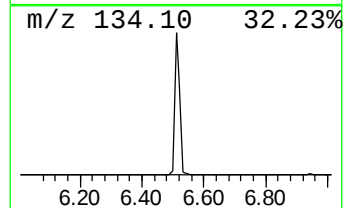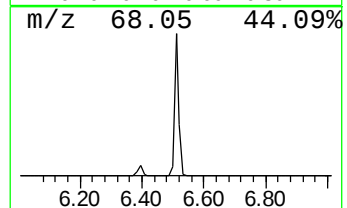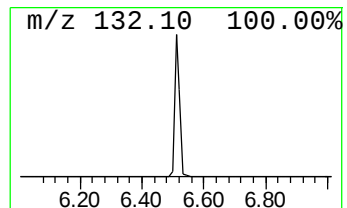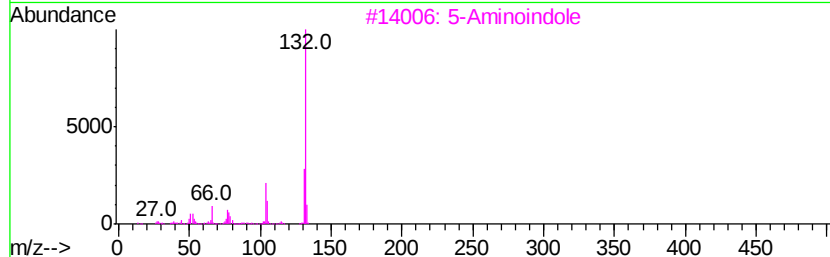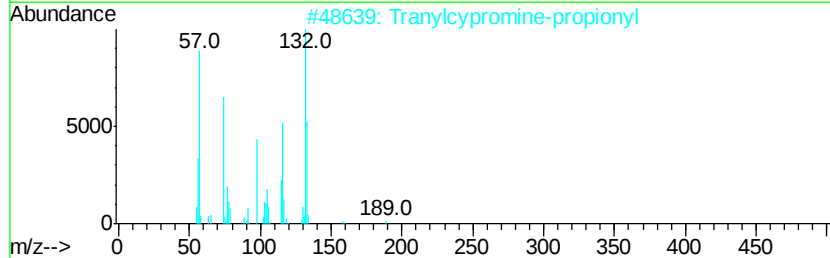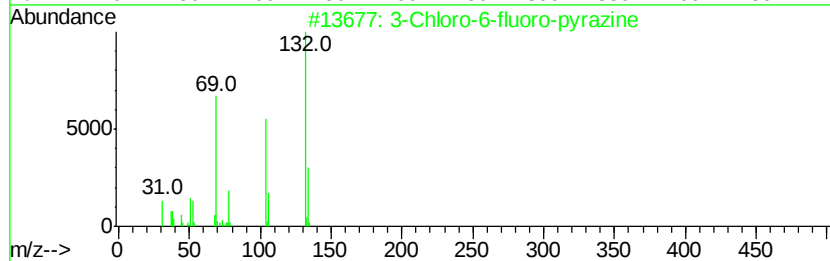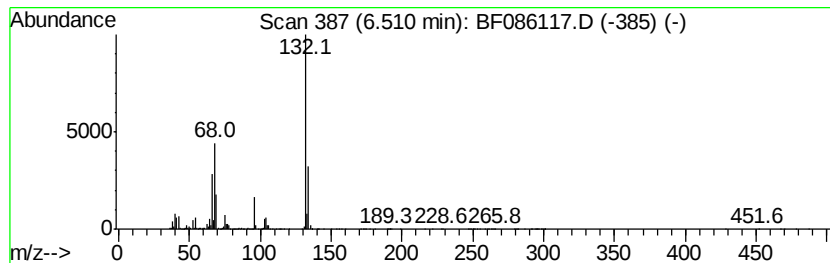

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040616\
Data File : BF086117.D
Acq On : 7 Apr 2016 00:21
Operator : UM/SJ
Sample : H2087-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TILCON-MH-SF-002










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Iminobis[[bis(trimethylsilyl... Concentration Rank 15

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.57	7.59 ng	316680	Naphthalene-d8	8.03

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Iminobis[[bis(trimethylsilyl)ami...	533	C18H57B2N5Si6	113678-60-7	55
2			Crypto dioxmine diacetate	544	C31H48N2O6	1000128-11-7	11
3			1,3,5-Triazine, 2,4-bis(2,2,2-tr...	518	C16H10F12N4O2	302602-86-4	9
4			Stannane, tributyl[(1-oxooctadec...	574	C30H62O2Sn	004027-13-8	7
5			Osmium methyl, (.eta.-5-cyclopen...	548	C22H30O5P2	1000158-92-4	4

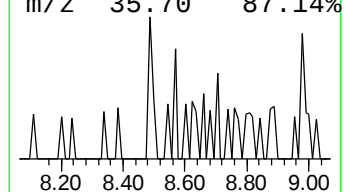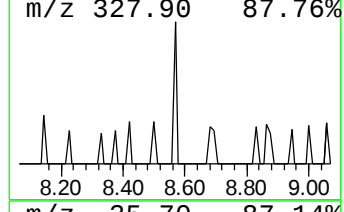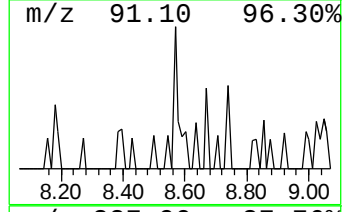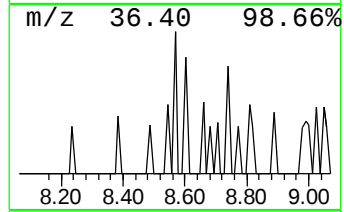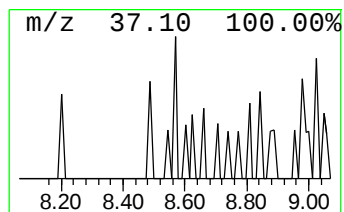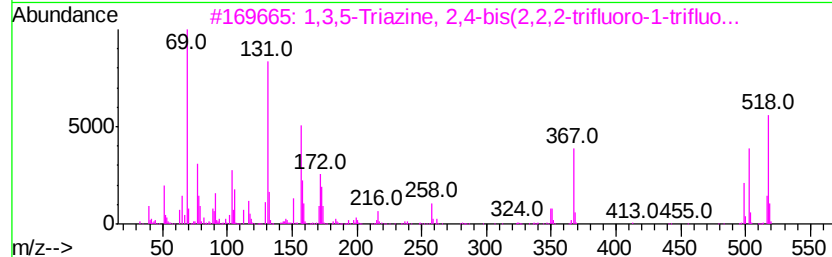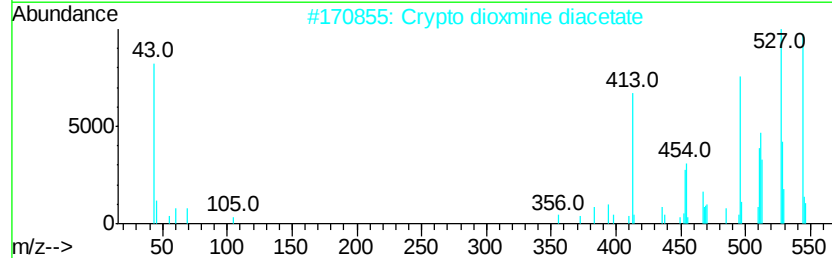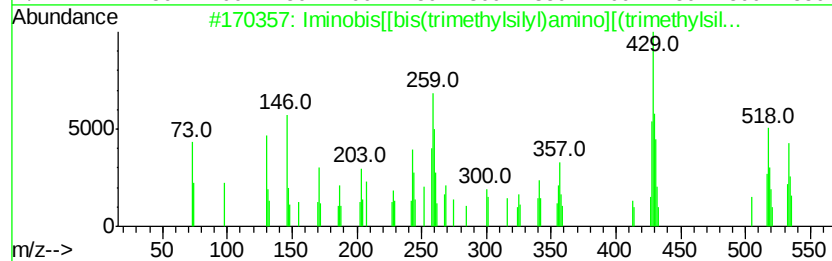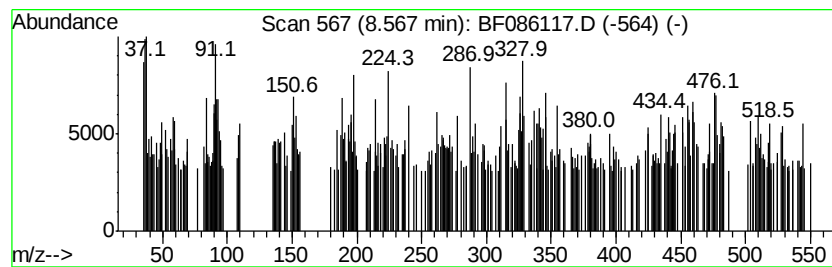

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040616\
Data File : BF086117.D
Acq On : 7 Apr 2016 00:21
Operator : UM/SJ
Sample : H2087-01
Misc :
ALS Vial : 28 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
TILCON-MH-SF-002

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 unknown11.66 Concentration Rank 14

R.T.	EstConc	Area	Relative to ISTD		R.T.		
11.66	7.60 ng	241974	Phenanthrene-d10		11.26		
Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2,4,6-Trioxabicyclo[3.3.0]octane...	248	C10H16O7	076110-72-0	44		
2	.beta.-Chlordene	336	C10H6Cl6	056534-03-3	35		
3	o-Veratramide	181	C9H11NO3	001521-39-7	18		
4	Acetamide, 2-chloro-N-(4-chlorod...	269	C9H7Cl2F2N02	1000276-46-6	14		
5	1-Propene, 1,3-dichloro-	110	C3H4Cl2	000542-75-6	14		

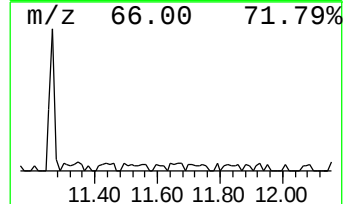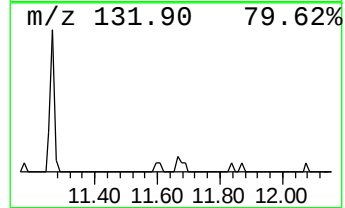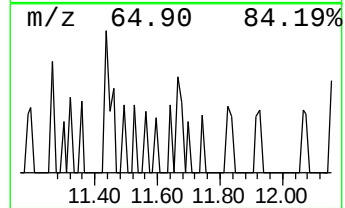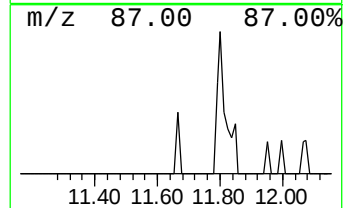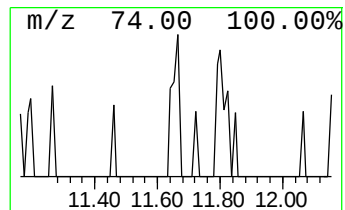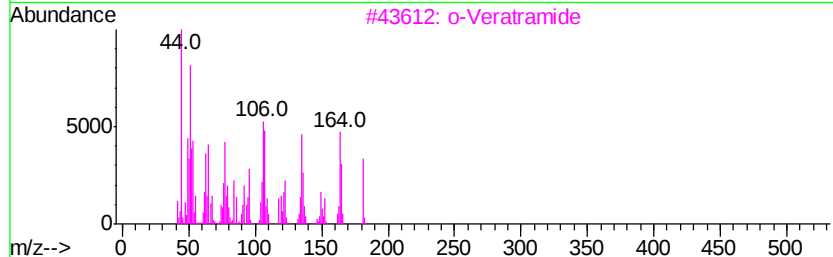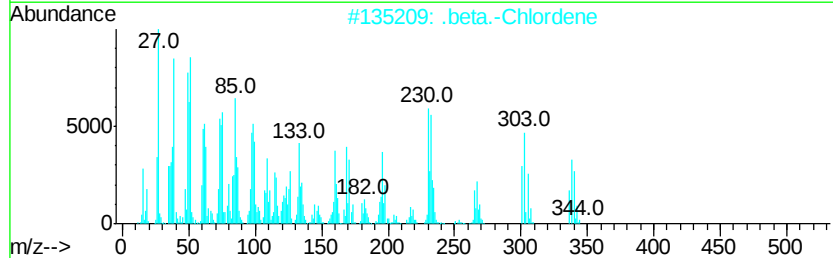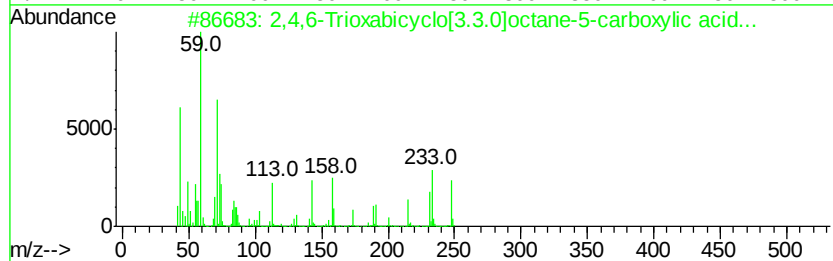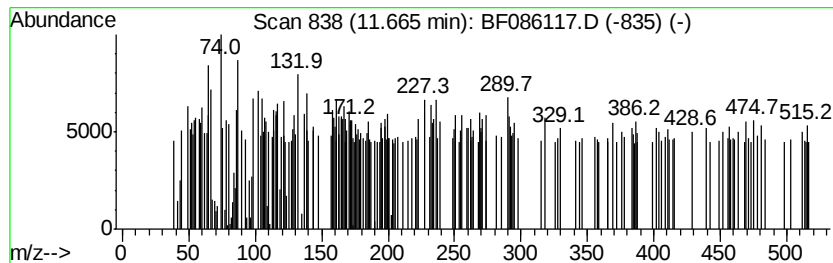

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040616\
Data File : BF086117.D
Acq On : 7 Apr 2016 00:21
Operator : UM/SJ
Sample : H2087-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TILCON-MH-SF-002










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 10 Heptafluorobutanoic acid, h... Concentration Rank 11

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.75	10.32 ng	619253	Chrysene-d12	13.91

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Heptafluorobutanoic acid, heptad...	452	C21H35F7O2	1000282-97-3	94
2		Heptafluorobutyric acid, n-octad...	466	C22H37F7O2	000400-57-7	91
3		Trifluoroacetic acid, n-octadecv...	366	C20H37F3O2	079392-43-1	91
4		Heptafluorobutyric acid, n-penta...	424	C19H31F7O2	1000216-79-3	91
5		3-Eicosene, (E)-	280	C20H40	074685-33-9	91

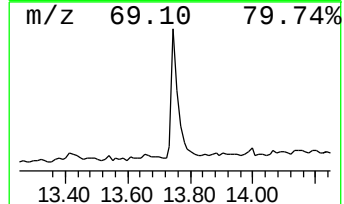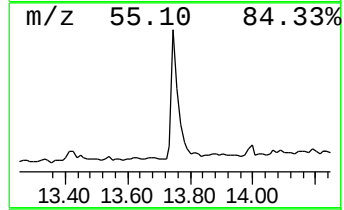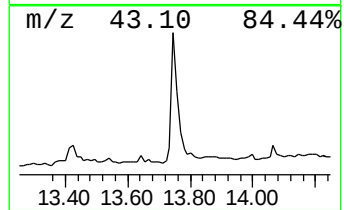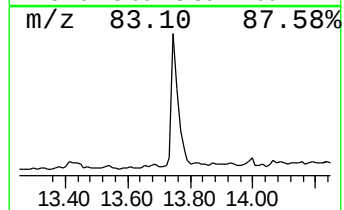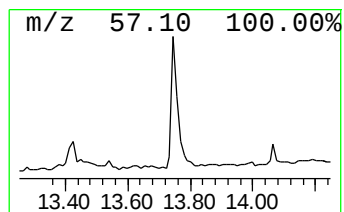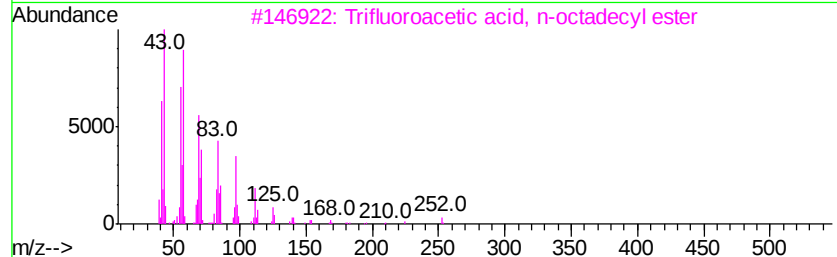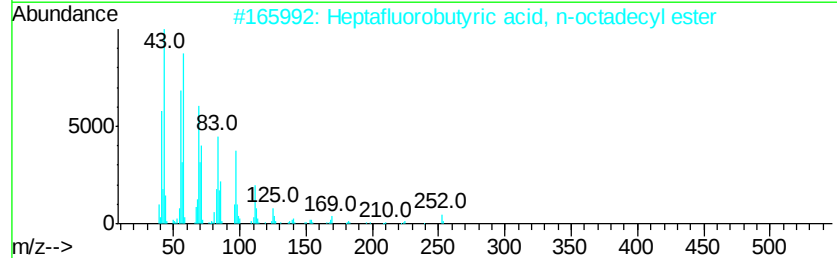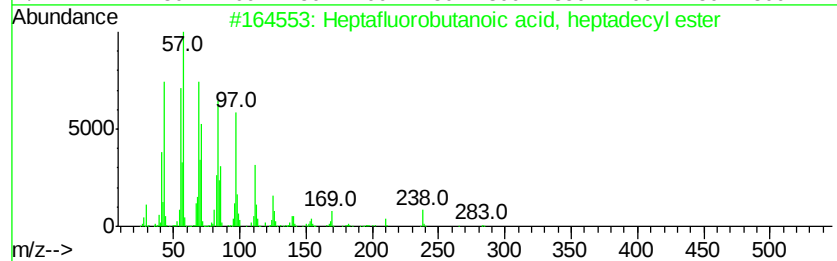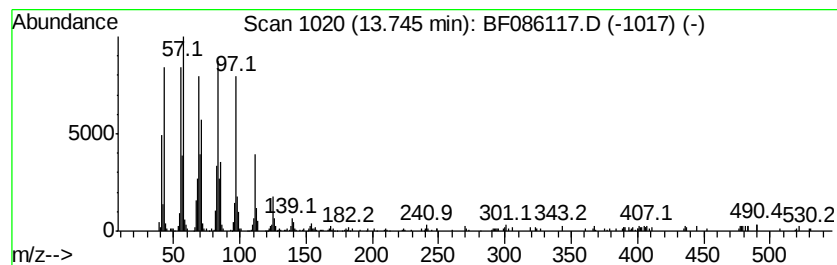

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040616\
Data File : BF086117.D
Acq On : 7 Apr 2016 00:21
Operator : UM/SJ
Sample : H2087-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TILCON-MH-SF-002










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 17 unknown15.80 Concentration Rank 12

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.80	9.60 ng	318206	Perylene-d12	15.30

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	4-(2-Chloroethoxy)-N-isopropyl-6...	262	C9H15ClN4OS	073775-70-9	44
2		2(1H)-Pyrimidinone, 4-(4-methylp...	262	C17H14N2O	024030-10-2	35
3		Furazano[3,4-E]indole, 8-acetyl-...	261	C12H11N3O4	257869-88-8	25
4		(1'R,2S,3R)-1',3-Dimethyl-2,2'-s...	262	C19H18O	1000099-36-1	25
5		5-hydroxy-6,7-dehydromatrine	262	C15H22N2O2	040444-76-6	25

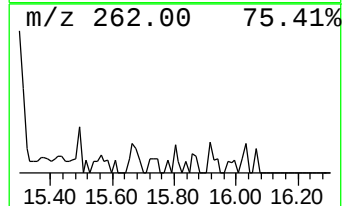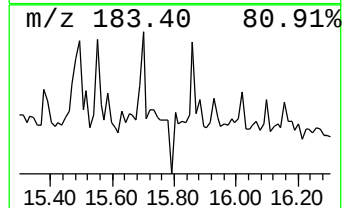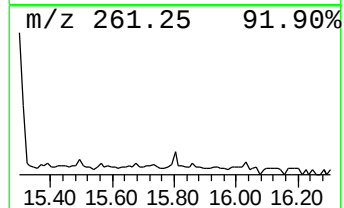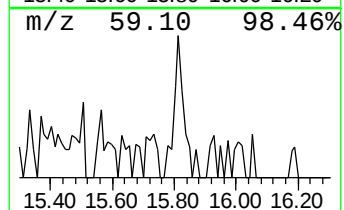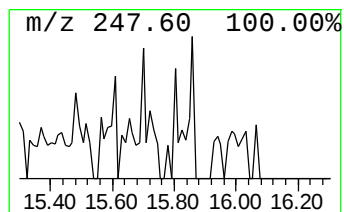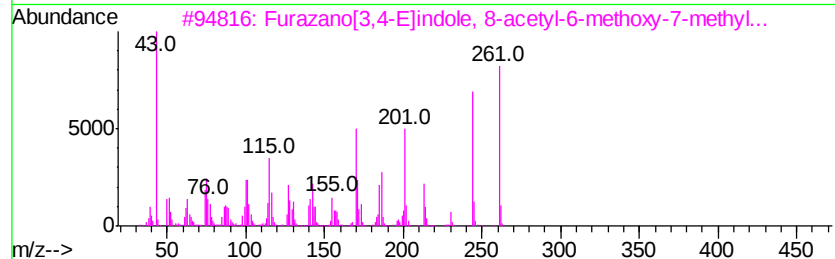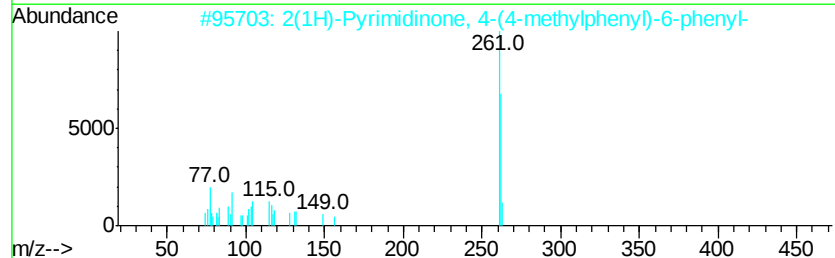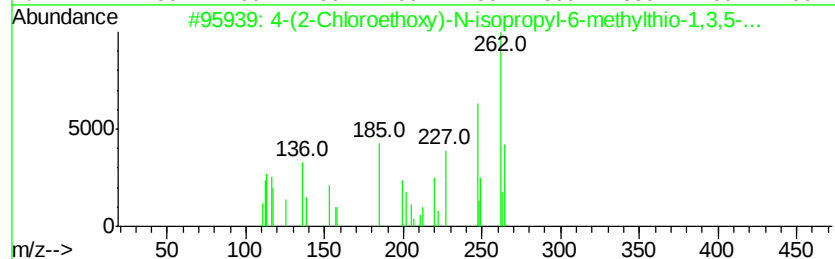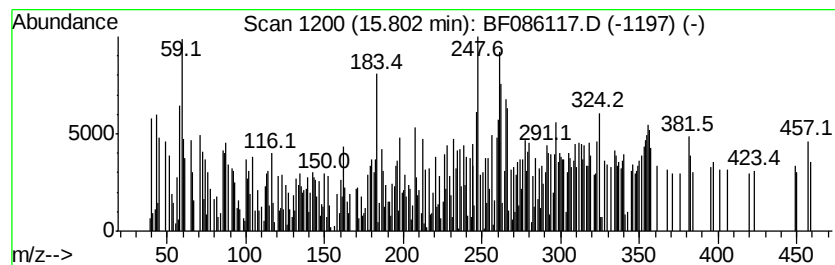

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040616\
Data File : BF086117.D
Acq On : 7 Apr 2016 00:21
Operator : UM/SJ
Sample : H2087-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TILCON-MH-SF-002










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 19 Coumarin-6-ol, 5,7-dibromo-... Concentration Rank 18

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.93	7.23 ng	239628	Perylene-d12	15.30

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Coumarin-6-ol, 5,7-dibromo-3,4-d...	348	C11H10Br2O3	040662-32-6	56
2		1,2-Dihydro-11-oxo-prednisolone,...	501	C26H31NO7S	1000128-12-9	9
3		1,2,4,5-Benzenetetracarboxylic 1...	504	C22H8Cl4N2O4	031663-86-2	9
4		D:C-Friedo-B':A'-neogammacer-9(1...	486	C31H50O4	038242-20-5	9
5		7-Bromo-5-(2-chlorophenyl)-2,3-d...	348	C15H10BrClN2O	051753-57-2	9

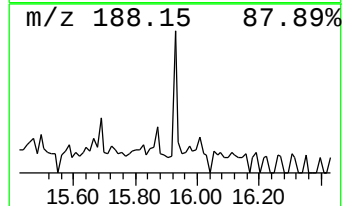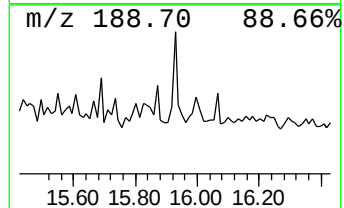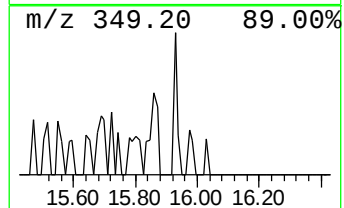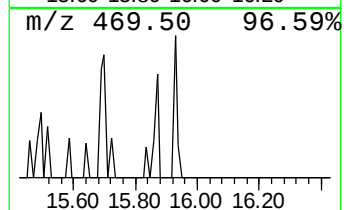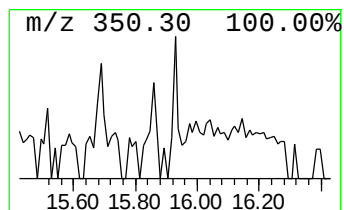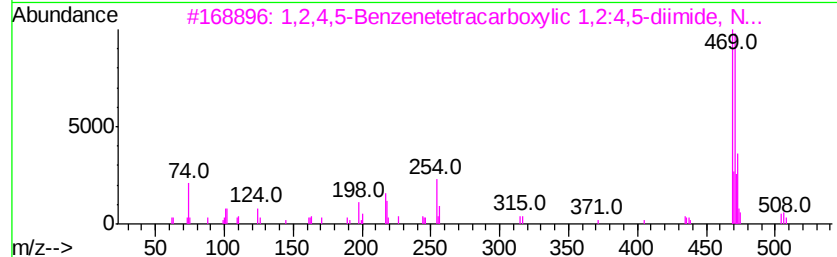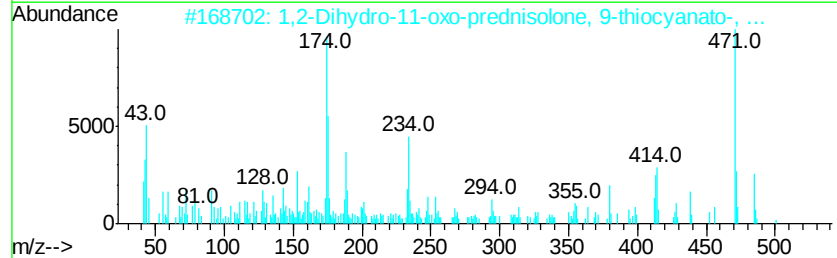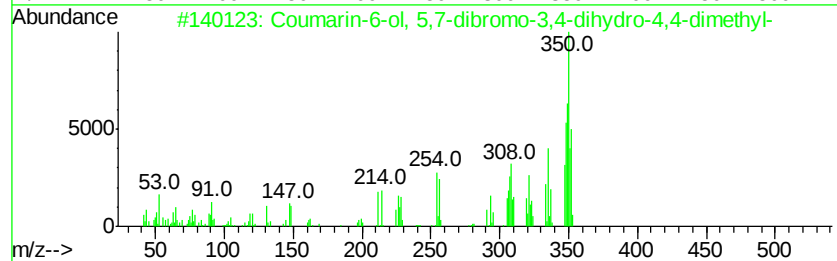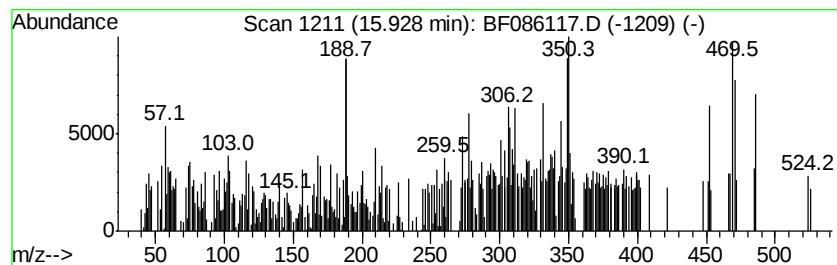

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040616\
Data File : BF086117.D
Acq On : 7 Apr 2016 00:21
Operator : UM/SJ
Sample : H2087-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
TILCON-MH-SF-002

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.47	5.47	42.0	ng	1411260	1	6.74	672587	20.0
unknown6.51	6.51	64.4	ng	2165740	1	6.74	672587	20.0
Iminobis[[bis(tri...	8.57	7.6	ng	316680	2	8.03	834648	20.0
unknown11.66	11.66	7.6	ng	241974	4	11.26	636661	20.0
unknown13.63	13.63	13.0	ng	781778	5	13.91	1200270	20.0
Heptafluorobutano...	13.75	10.3	ng	619253	5	13.91	1200270	20.0
unknown15.80	15.80	9.6	ng	318206	6	15.30	663188	20.0
Coumarin-6-ol, 5,...	15.93	7.2	ng	239628	6	15.30	663188	20.0