


Data Path : Z:\HPCHEM1\BNA F\DATA\BF040616\
 Data File : BF086099.D
 Acq On : 6 Apr 2016 15:30
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 01 23:17:06 2016

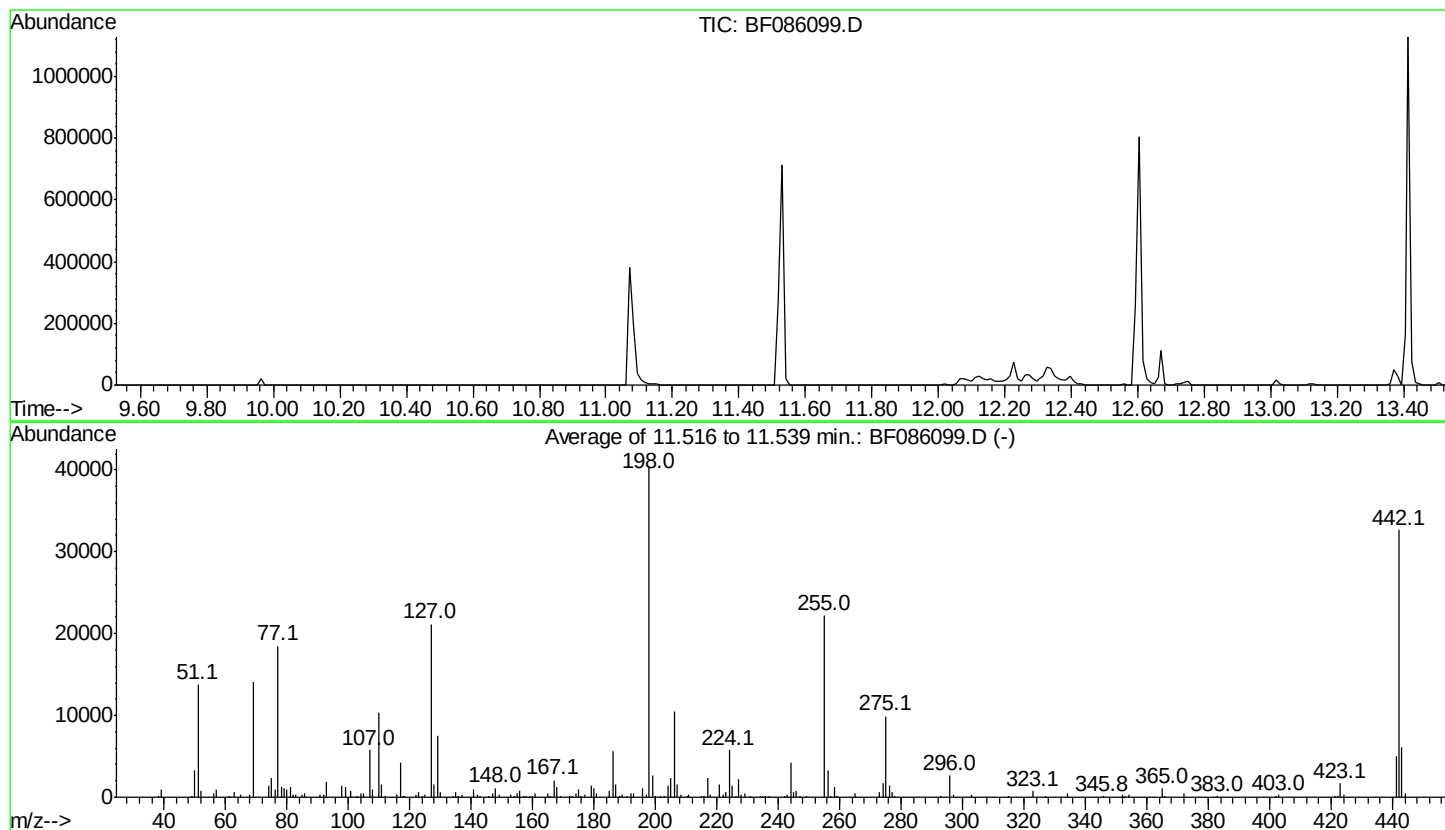

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.9	13730	PASS
68	69	0.00	2	1.9	261	PASS
69	198	0.00	100	34.6	14010	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	52.1	21127	PASS
197	198	0.00	2	0.6	254	PASS
198	198	100	100	100.0	40525	PASS
199	198	5	9	6.5	2651	PASS
275	198	10	60	24.5	9922	PASS
365	198	1	100	2.6	1053	PASS
441	442	0.01	24	15.4	5030	PASS
442	198	50	100	80.6	32669	PASS
443	442	15	24	18.5	6049	PASS