
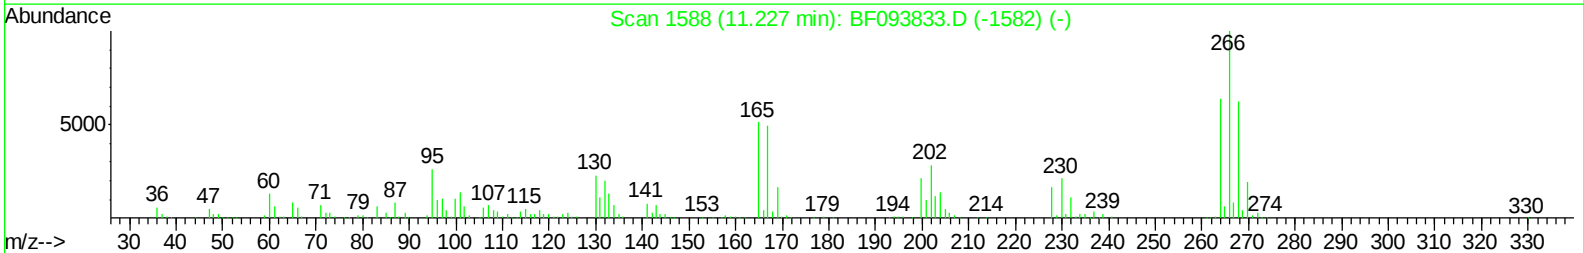
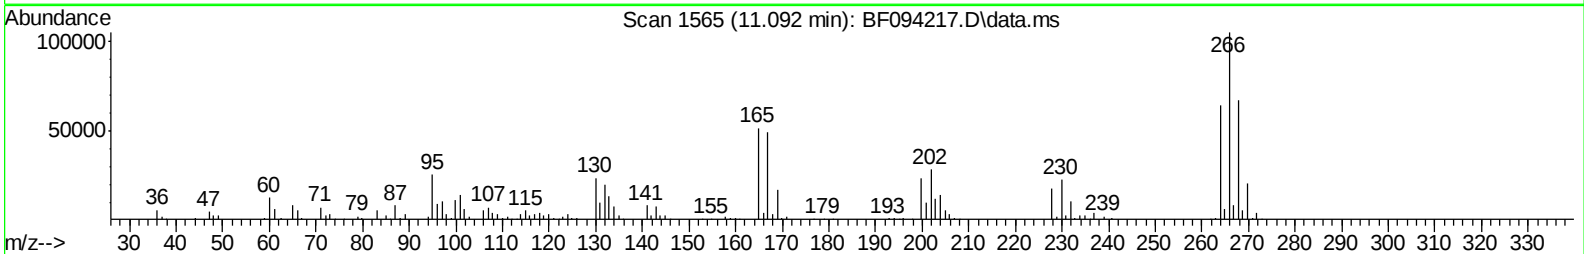


```
Data Path : Z:\HPCHEM1\BNA F\Data\BF040617\  
Data File : BF094217.D  
Acq On    : 6 Apr 2017    9:53  
Operator  : SJ/MA  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Apr 06 19:04:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 13:20:29 2017
Response via : Initial Calibration

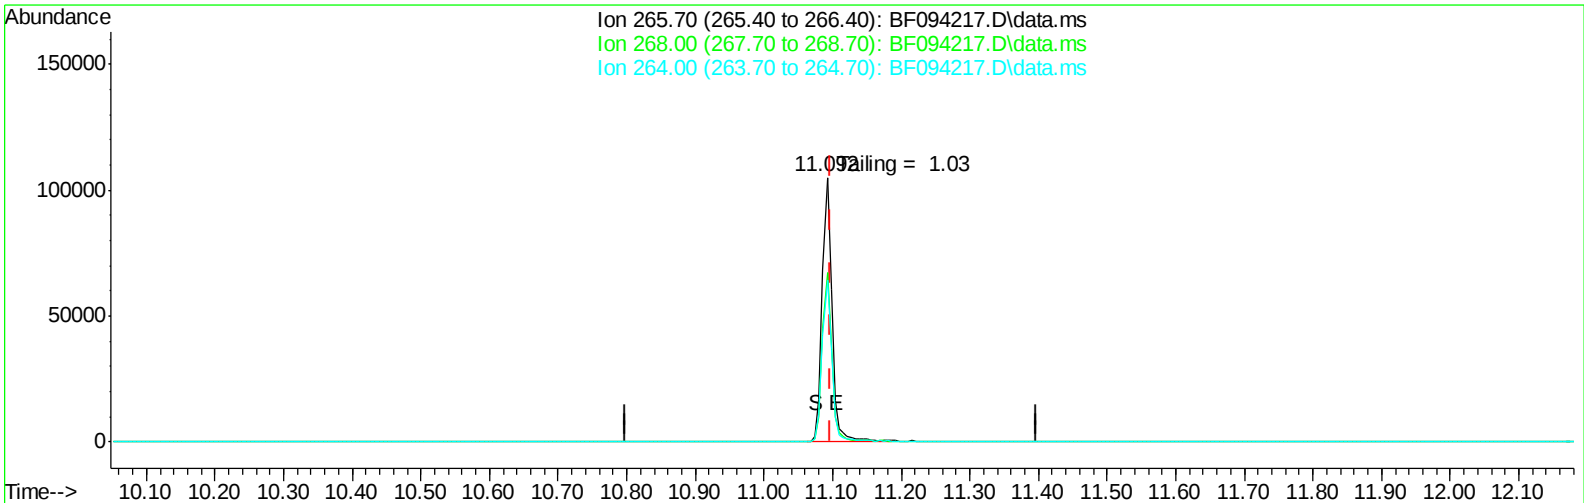

TIC: BF094217.D\data.ms

(69) Pentachlorophenol (C)




11.092min (-0.006) 35300.74ng

```
response 102158
```

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	63.97
264.00	64.60	61.11
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF040617\
Data File : BF094217.D
Acq On : 6 Apr 2017 9:53
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 19:04:51 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 13:20:29 2017
Response via : Initial Calibration

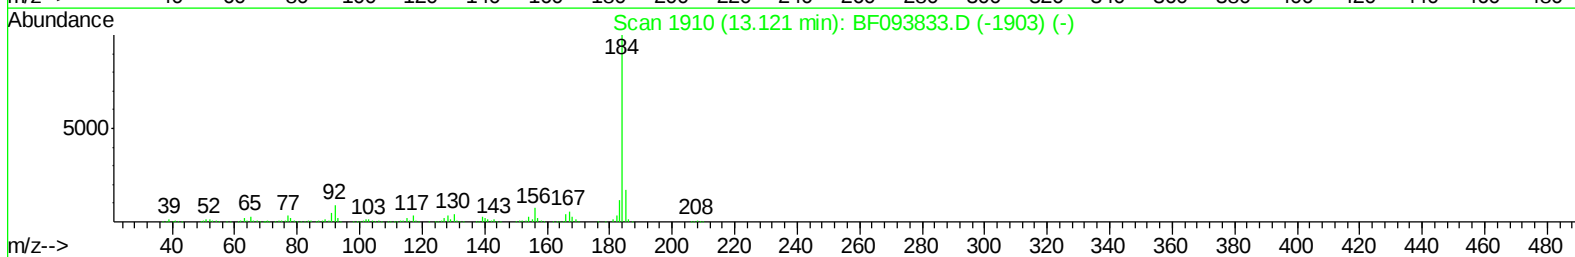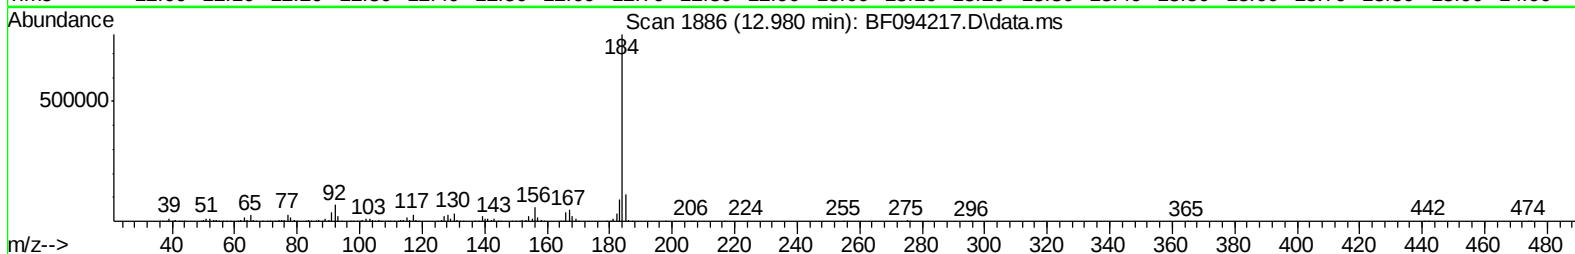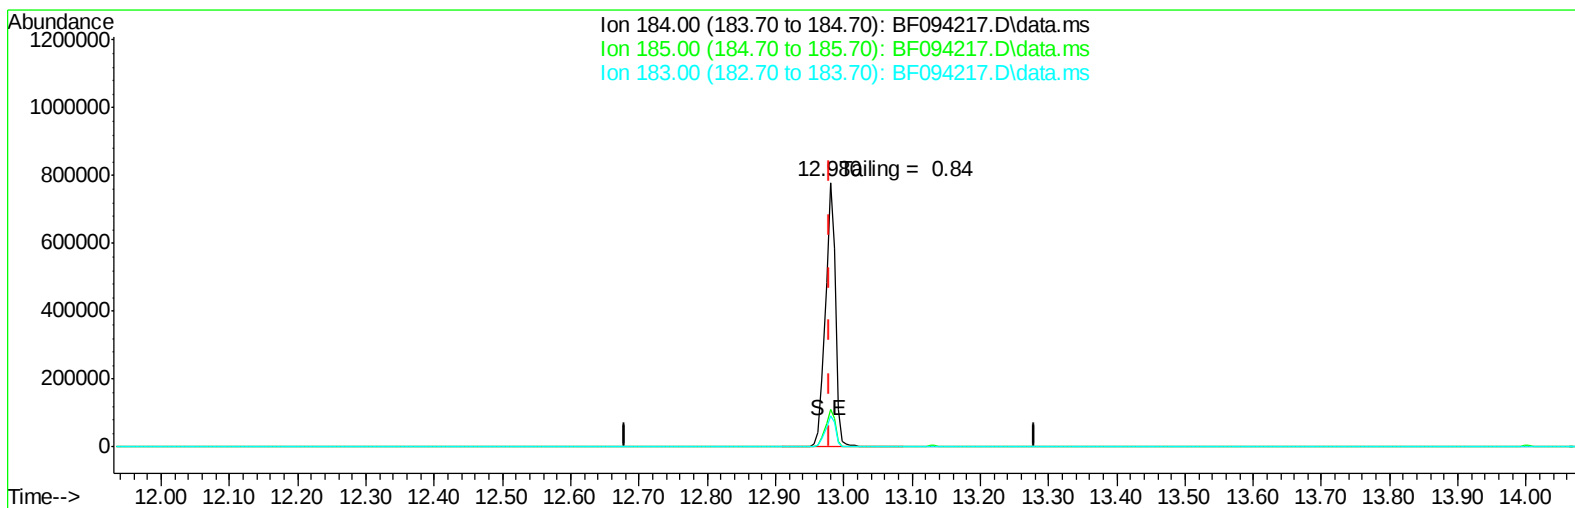

TIC: BF094217.D\data.ms

(76) Benzidine

12.980min (-0.000) 43225.83ng m

response 798945

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.21#
183.00	12.20	11.94
0.00	0.00	0.00