
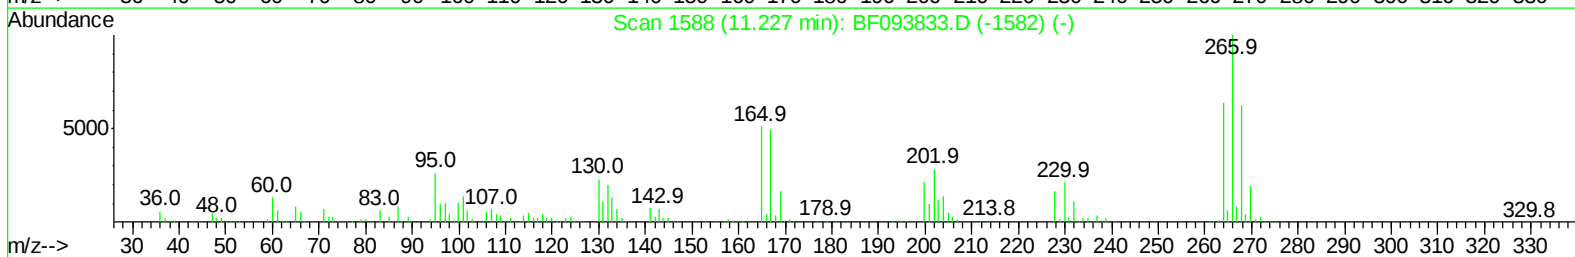
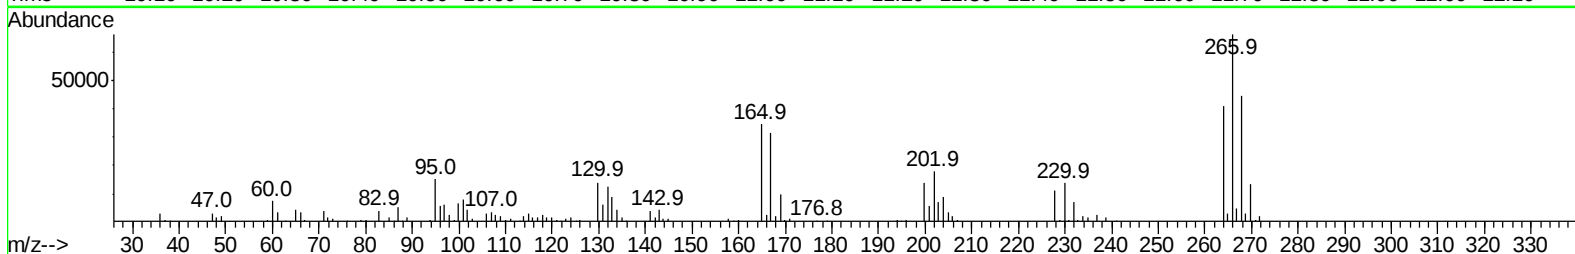


Data Path : Z:\HPCHEM1\BNA F\DATA\BF040617\
 Data File : BF094243.D
 Acq On : 7 Apr 2017 00:00
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 04:24:30 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 13:20:29 2017
 Response via : Initial Calibration

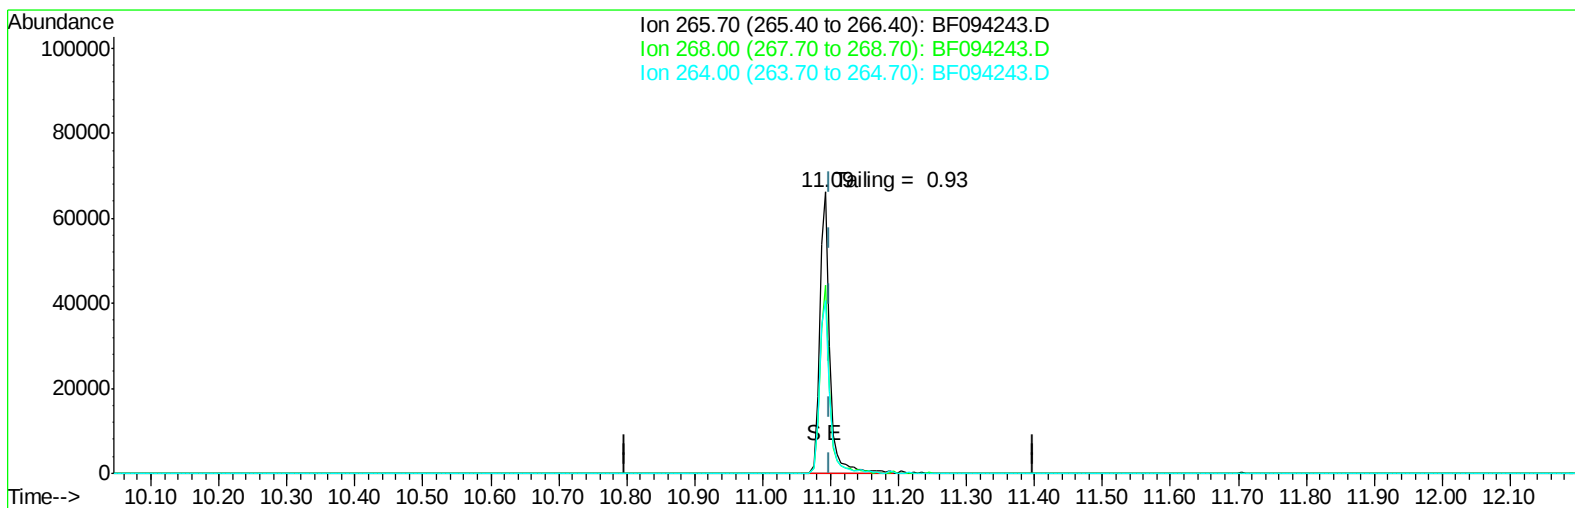

TIC: BF094243.D

(69) Pentachlorophenol (C)




11.092min (-0.006) 0.00ng

response 69534

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.97
264.00	64.60	61.52
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040617\
 Data File : BF094243.D
 Acq On : 7 Apr 2017 00:00
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 07 04:24:30 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Apr 06 13:20:29 2017
 Response via : Initial Calibration

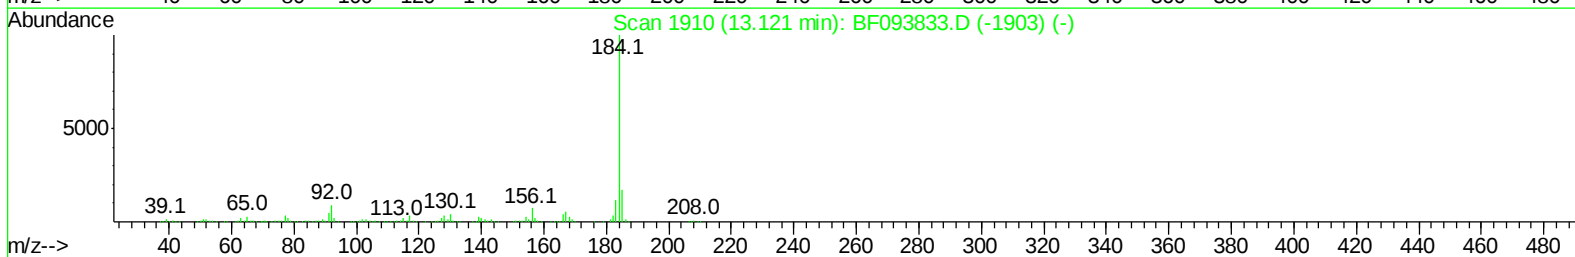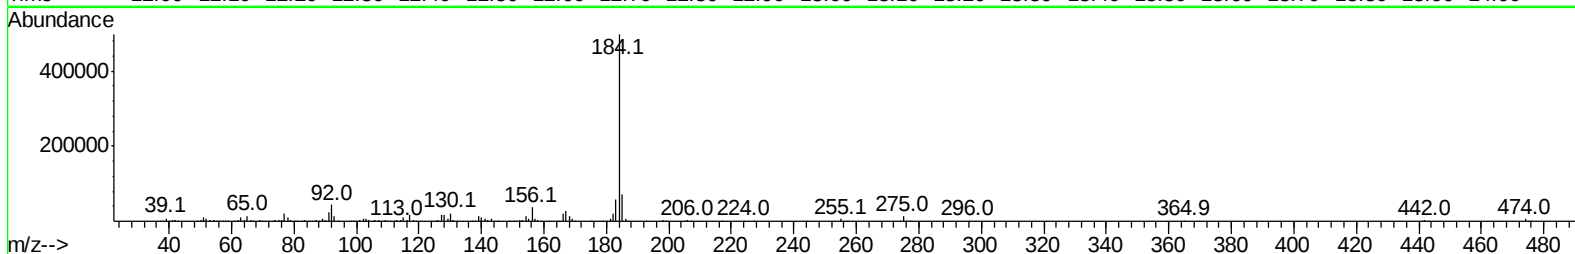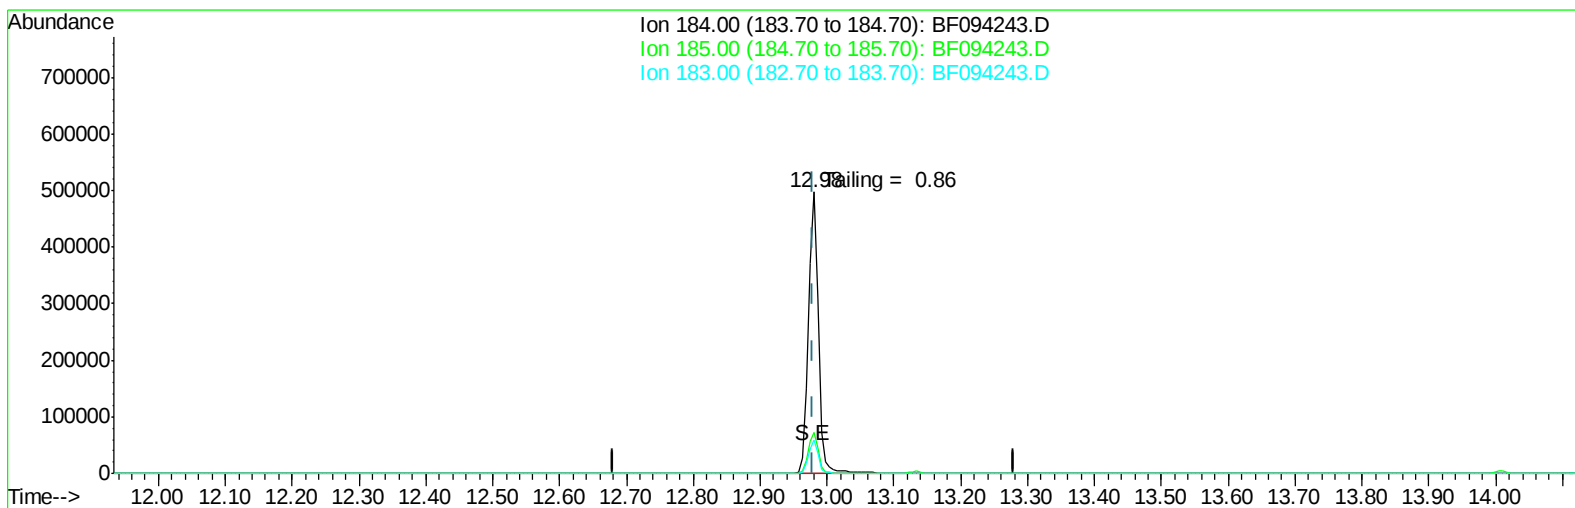

TIC: BF094243.D

(76) Benzidine

12.980min (-0.000) 0.00ng

response 530792

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.48#
183.00	12.20	11.99
0.00	0.00	0.00