


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040617\
 Data File : BF094217.D
 Acq On : 6 Apr 2017 9:53
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Apr 06 13:20:29 2017

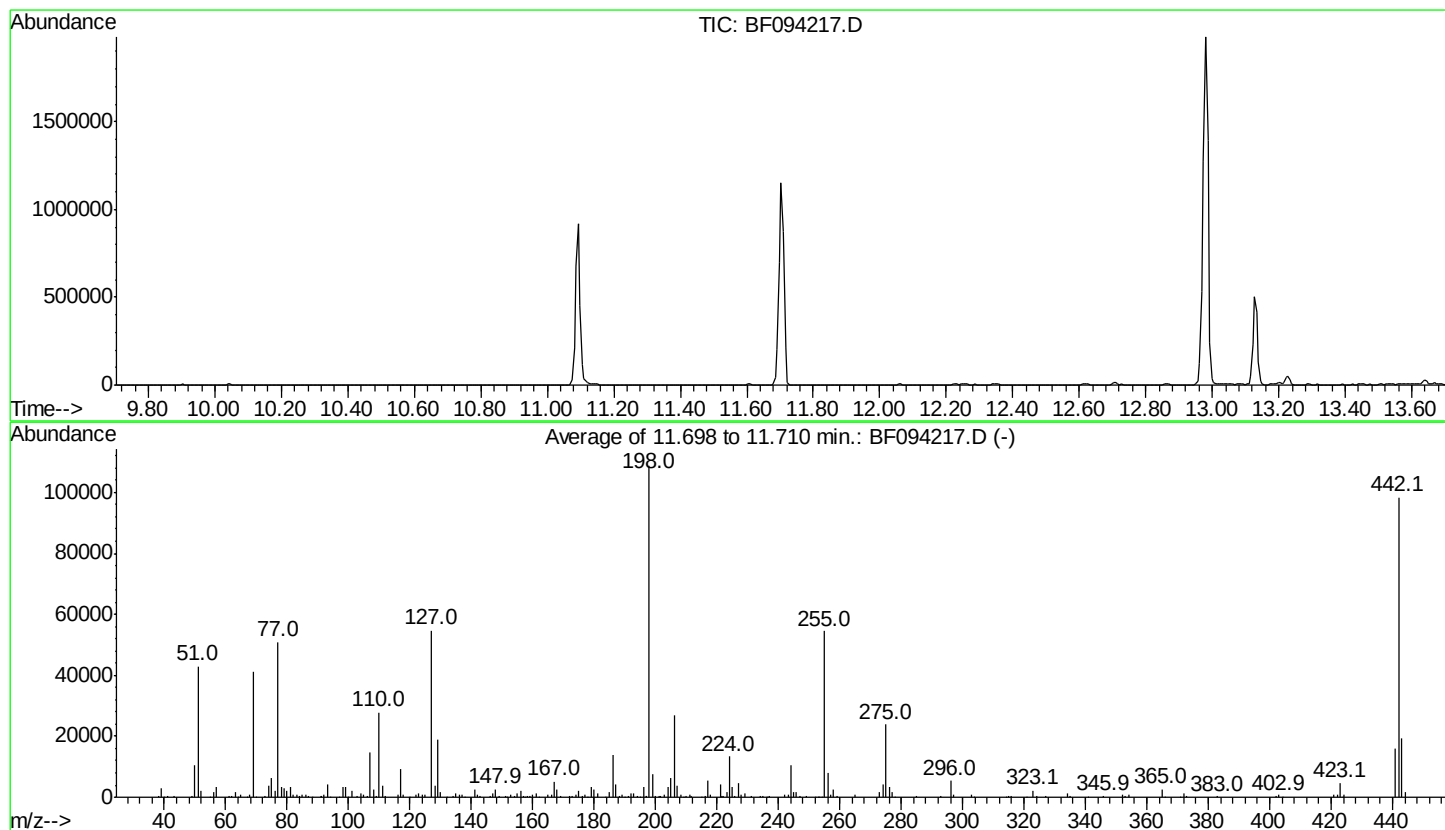

AutoFind: Scans 1668, 1669, 1670; Background Corrected with Scan 1661

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	42906	PASS
68	69	0.00	2	1.8	746	PASS
69	198	0.00	100	37.7	40981	PASS
70	69	0.00	2	0.4	146	PASS
127	198	10	80	50.4	54794	PASS
197	198	0.00	2	0.5	496	PASS
198	198	100	100	100.0	108770	PASS
199	198	5	9	6.8	7371	PASS
275	198	10	60	21.9	23857	PASS
365	198	1	100	2.5	2714	PASS
441	442	0.01	24	16.3	16003	PASS
442	198	50	100	90.5	98405	PASS
443	442	15	24	19.4	19125	PASS