


Data Path : Z:\HPCHEM1\BNA\_F\DATA\BF040617\  
 Data File : BF094243.D  
 Acq On : 7 Apr 2017 00:00  
 Operator : SJ/MA  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF032217.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Thu Apr 06 13:20:29 2017

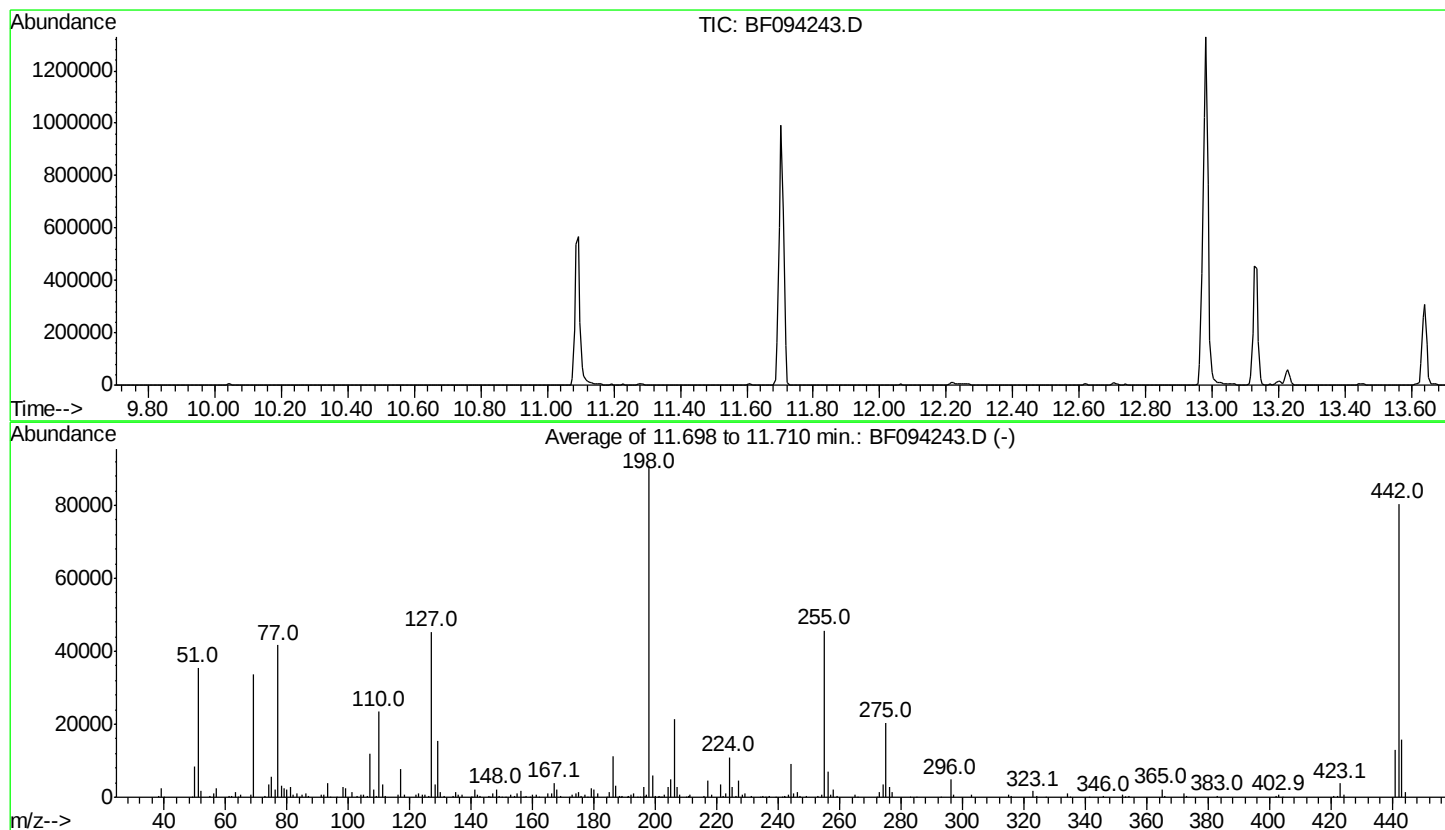

AutoFind: Scans 1668, 1669, 1670; Background Corrected with Scan 1663

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 39.1      | 35528   | PASS             |
| 68          | 69           | 0.00         | 2            | 2.0       | 686     | PASS             |
| 69          | 198          | 0.00         | 100          | 36.9      | 33541   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.0       | 0       | PASS             |
| 127         | 198          | 10           | 80           | 49.9      | 45384   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.8       | 719     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 90869   | PASS             |
| 199         | 198          | 5            | 9            | 6.6       | 6015    | PASS             |
| 275         | 198          | 10           | 60           | 22.5      | 20476   | PASS             |
| 365         | 198          | 1            | 100          | 2.4       | 2176    | PASS             |
| 441         | 442          | 0.01         | 24           | 16.2      | 13066   | PASS             |
| 442         | 198          | 50           | 100          | 88.6      | 80488   | PASS             |
| 443         | 442          | 15           | 24           | 19.8      | 15939   | PASS             |