



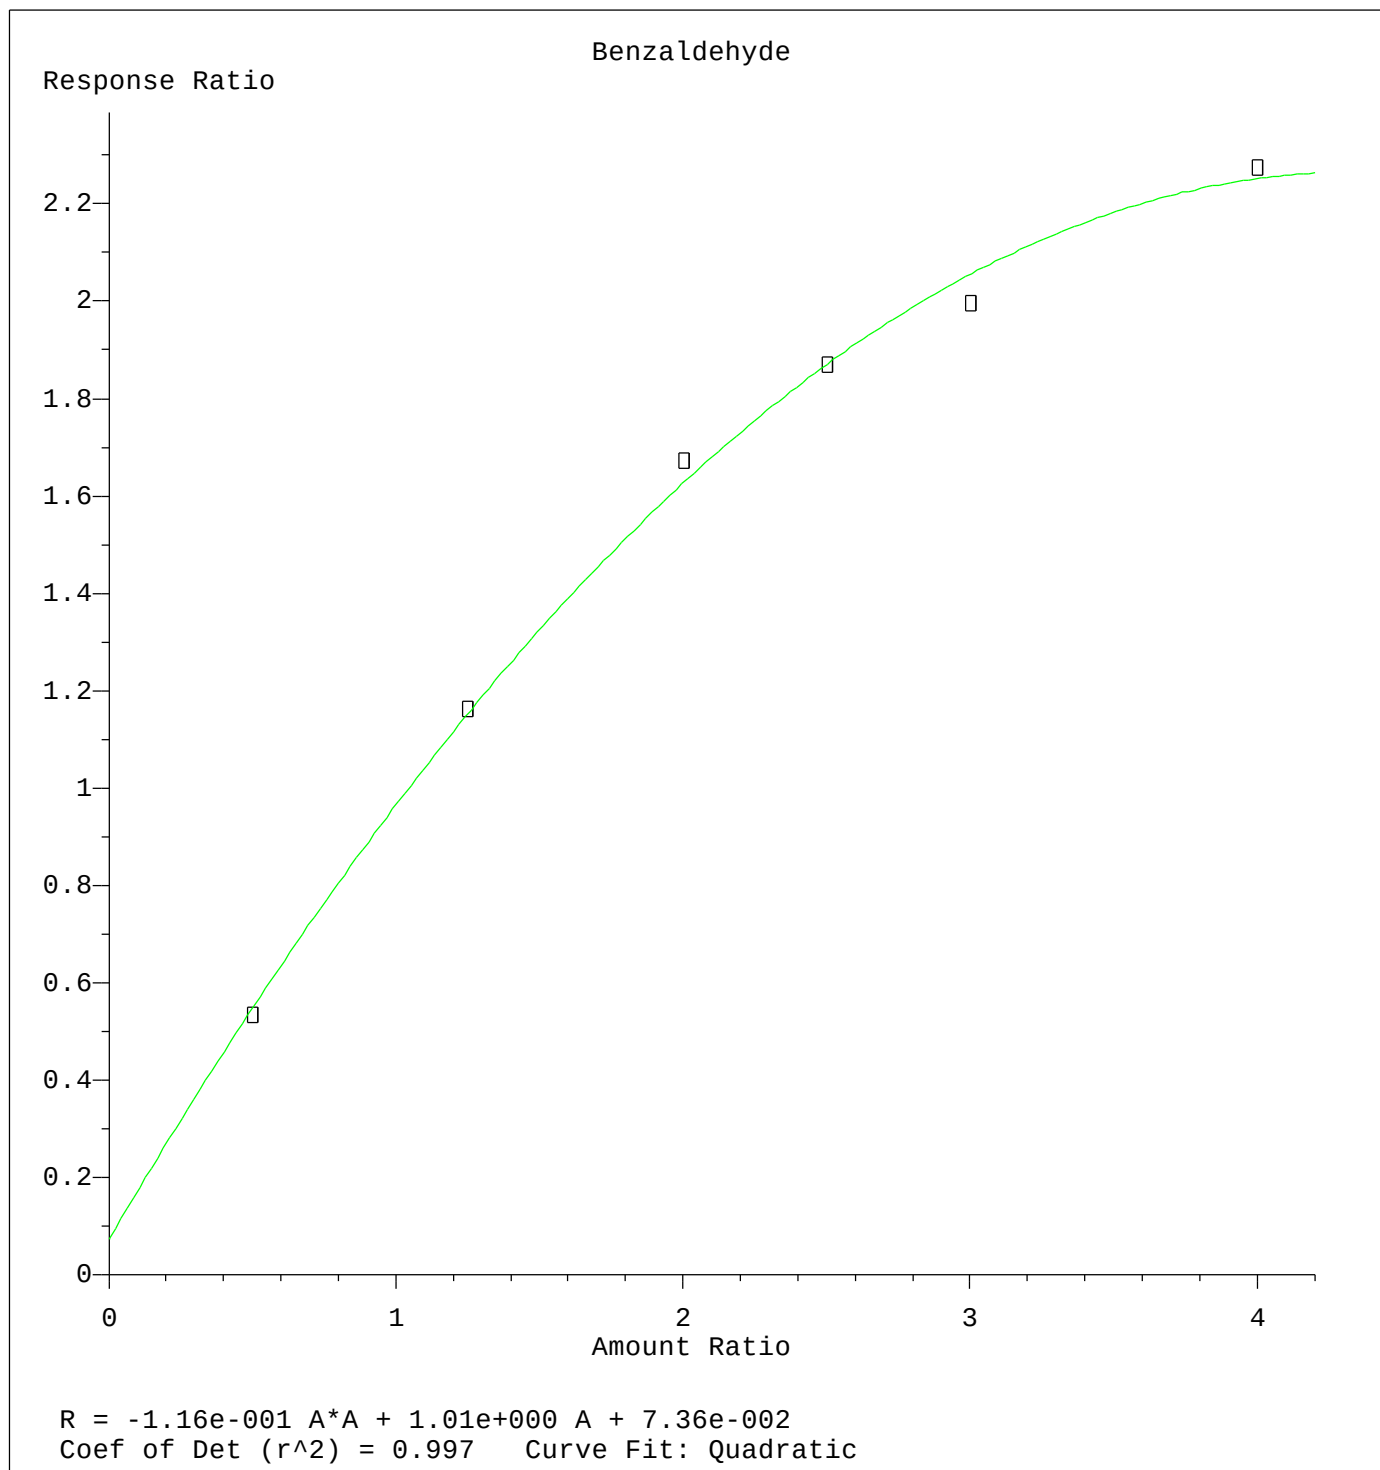


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
Calibration Table Last Updated: Fri Apr 06 16:44:53 2018

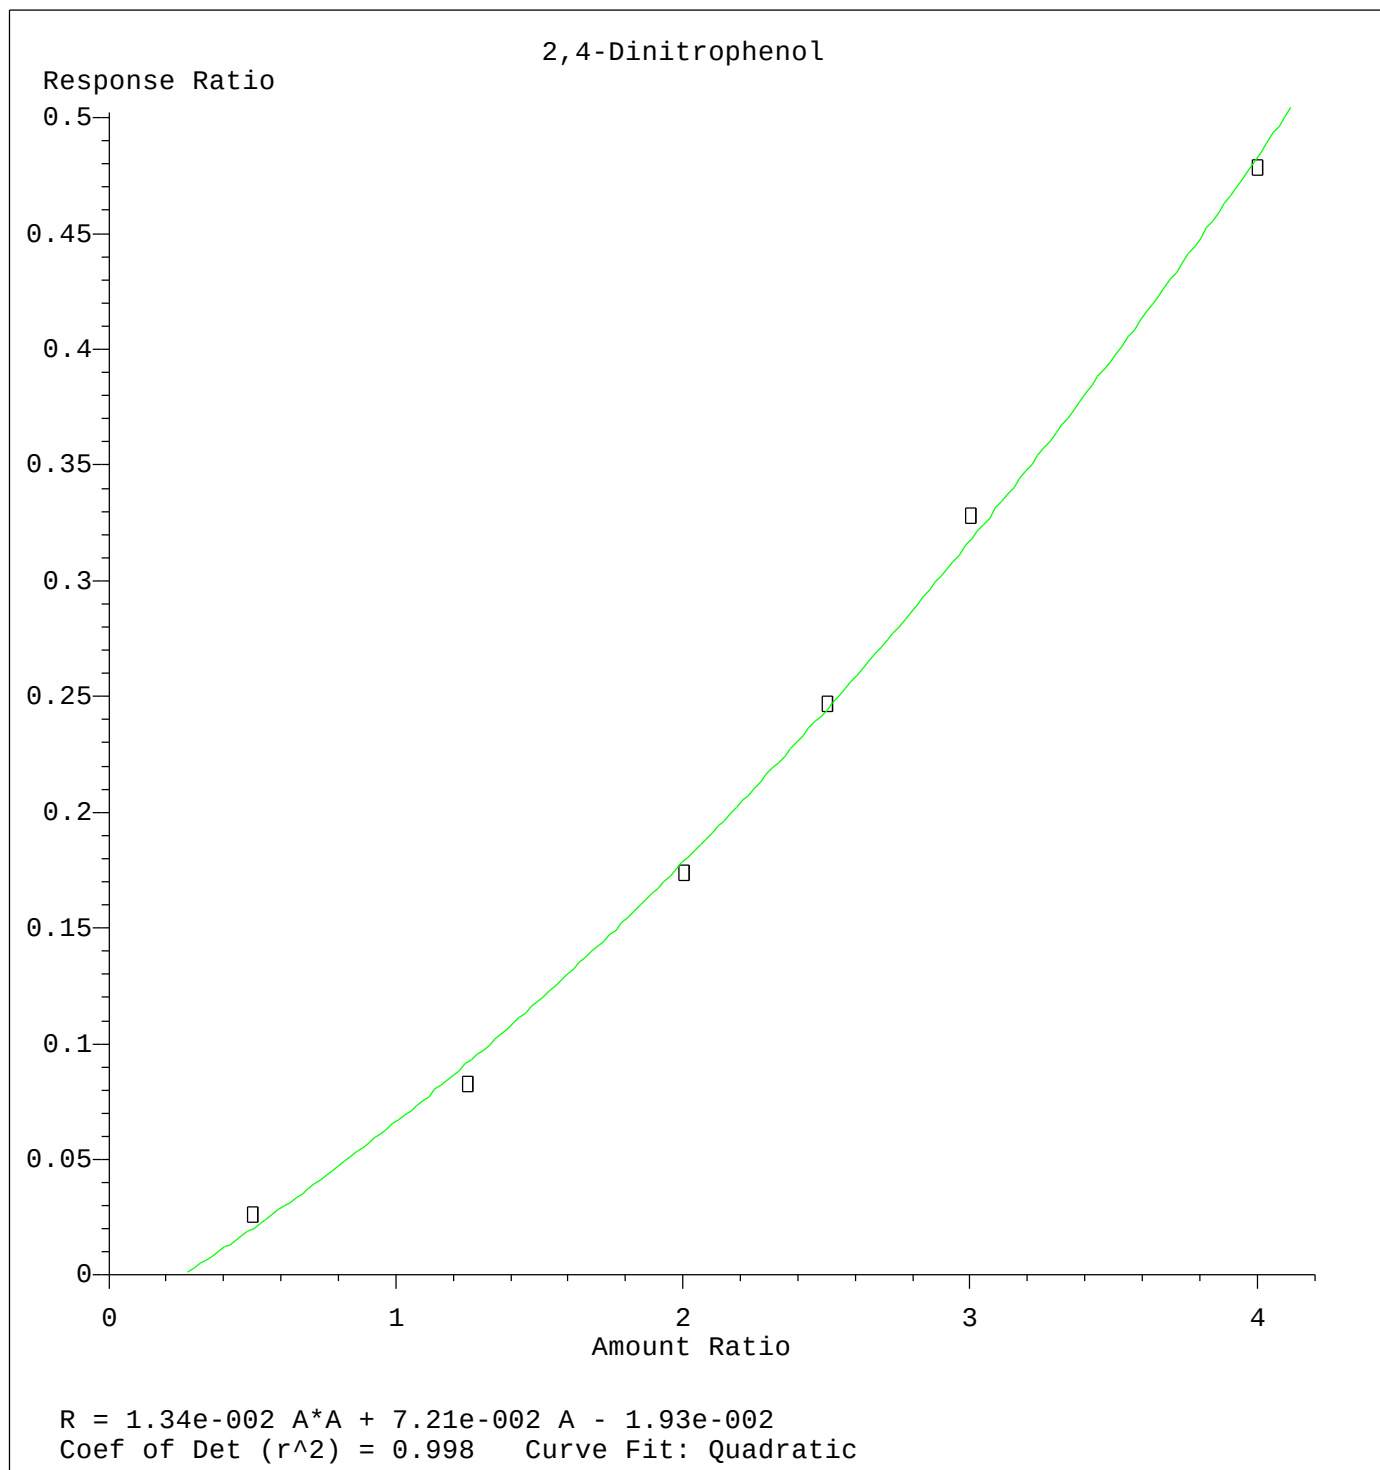


Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
Calibration Table Last Updated: Fri Apr 06 16:44:53 2018

4,6-Dinitro-2-methylphenol

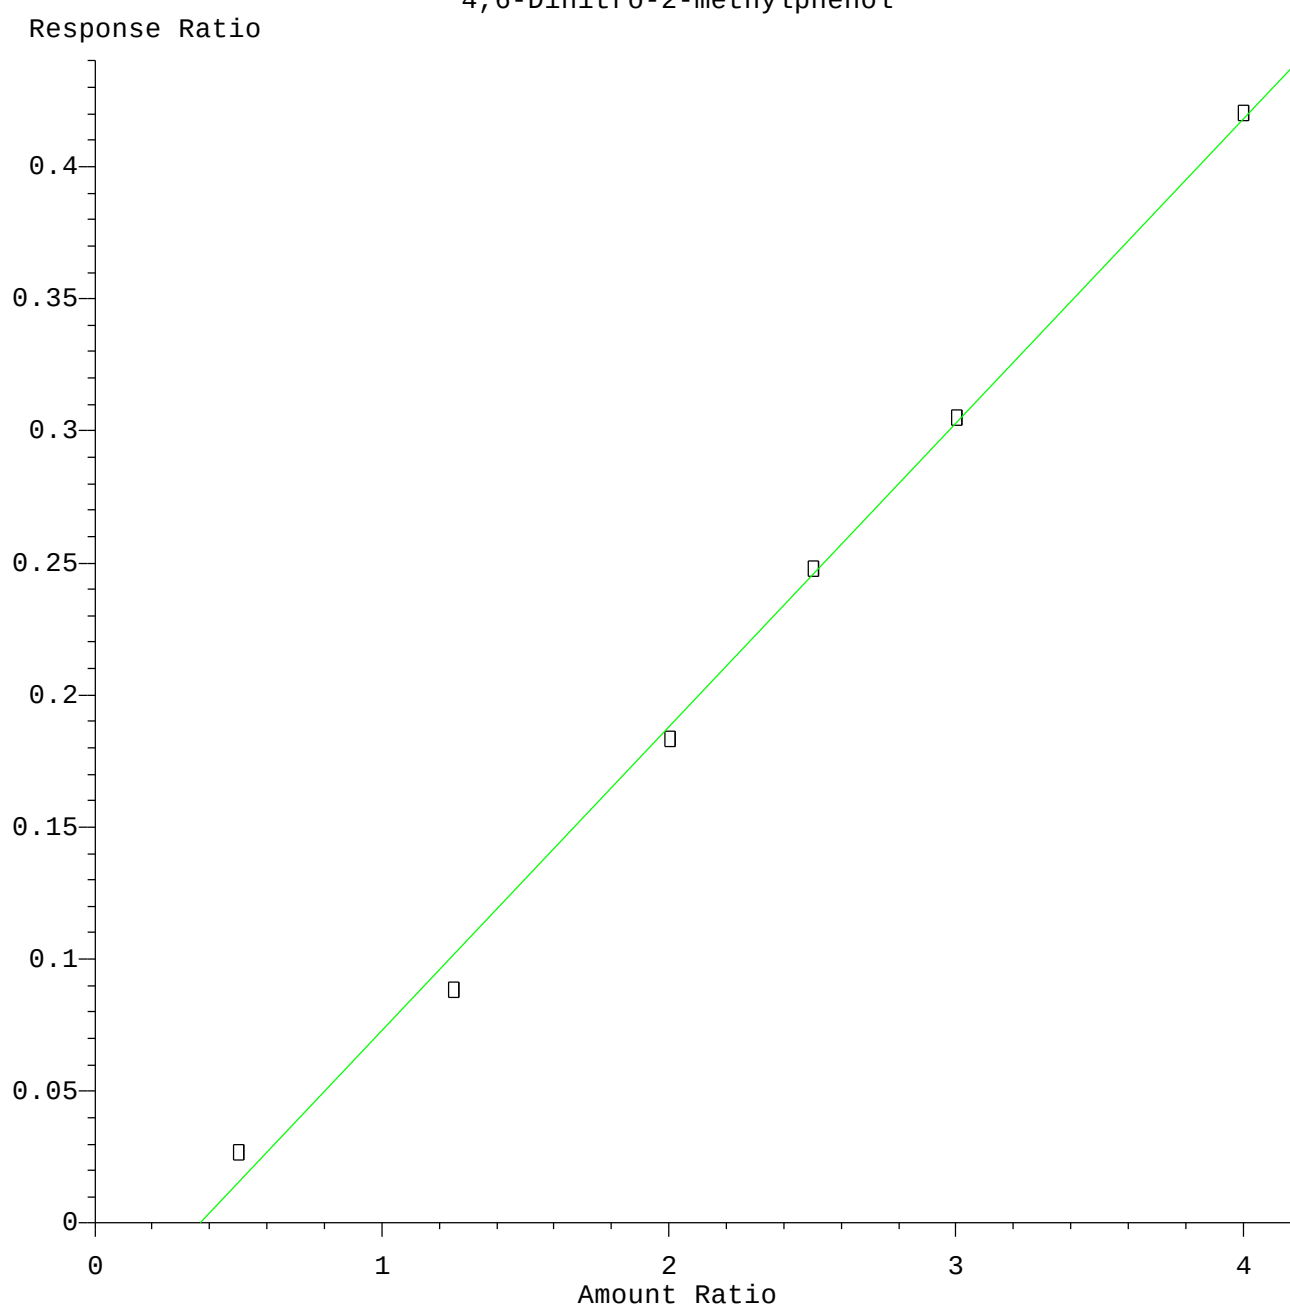

Resp Ratio = $1.15 \times 10^{-1} \times \text{Amt} - 4.22 \times 10^{-2}$
Coef of Det (r^2) = 0.997 Curve Fit: Linear

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
Calibration Table Last Updated: Fri Apr 06 16:44:53 2018

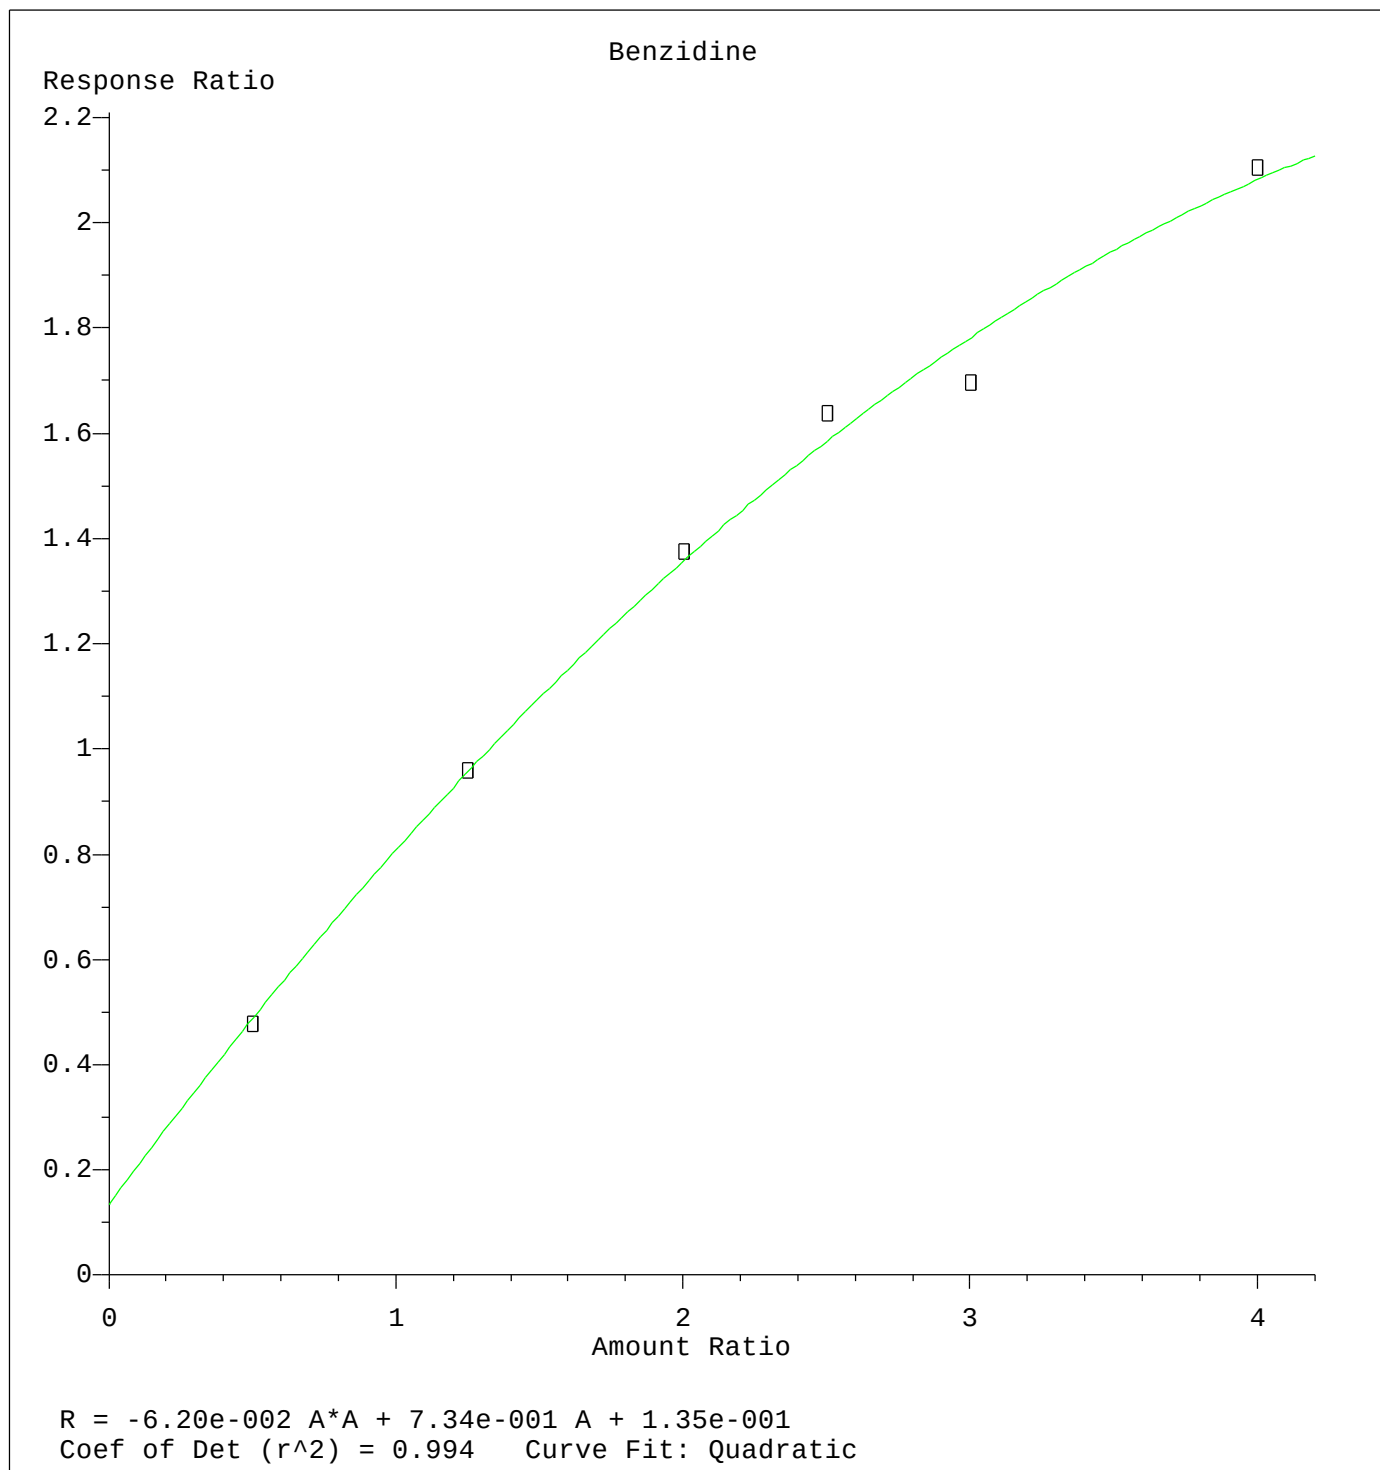

Method Name: Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
Calibration Table Last Updated: Fri Apr 06 16:44:53 2018