
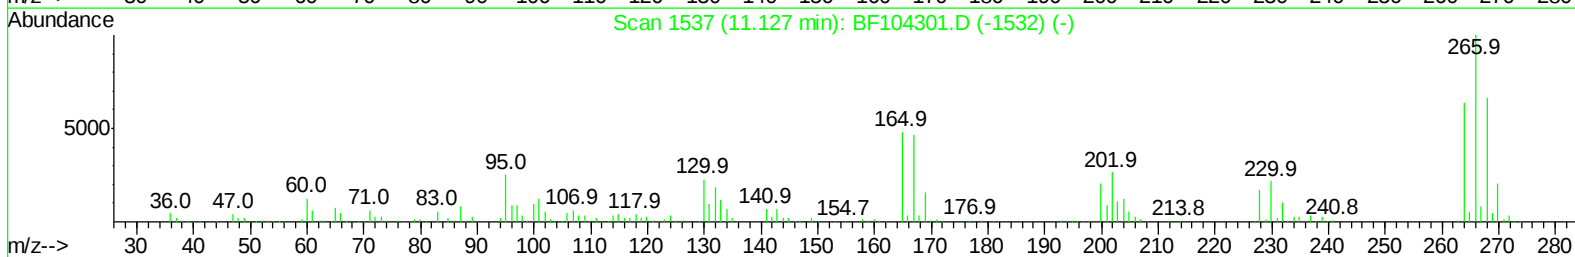
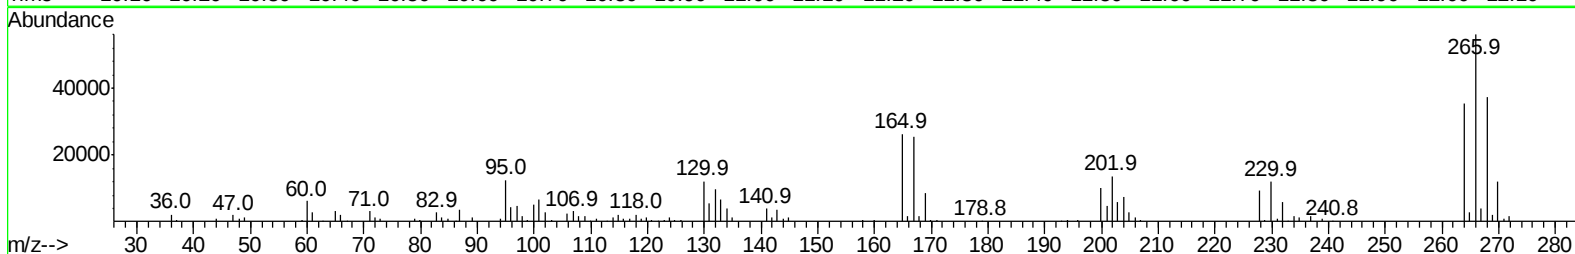


Data Path : Z:\HPCHEM1\BNA F\DATA\BF040618\
Data File : BF104332.D
Acq On : 7 Apr 2018 3:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 01:43:54 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 06 16:44:53 2018
Response via : Initial Calibration

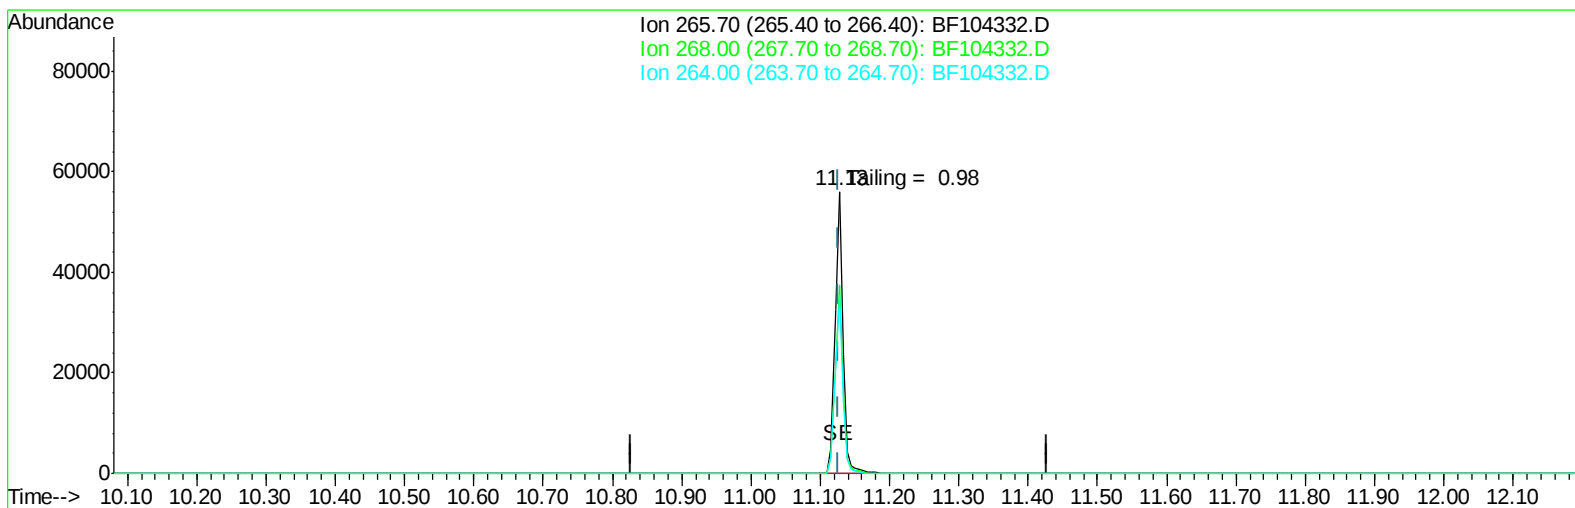

TIC: BF104332.D

(69) Pentachlorophenol (C)




11.127min (-0.000) 34203.36ng

response 44573

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	66.67
264.00	61.90	63.25
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040618\
Data File : BF104332.D
Acq On : 7 Apr 2018 3:14
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 09 01:43:54 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 06 16:44:53 2018
Response via : Initial Calibration

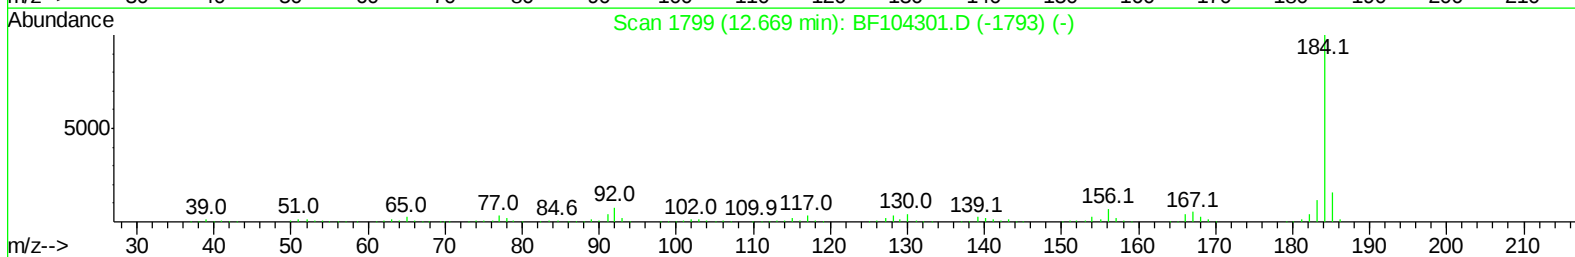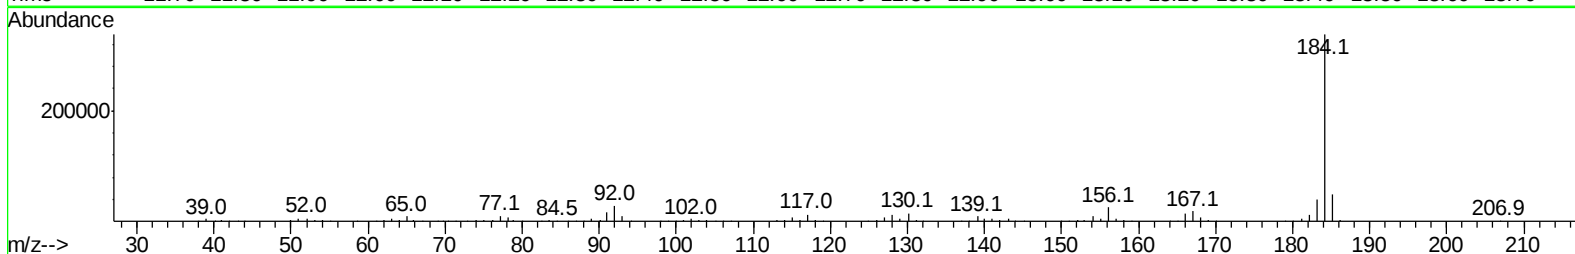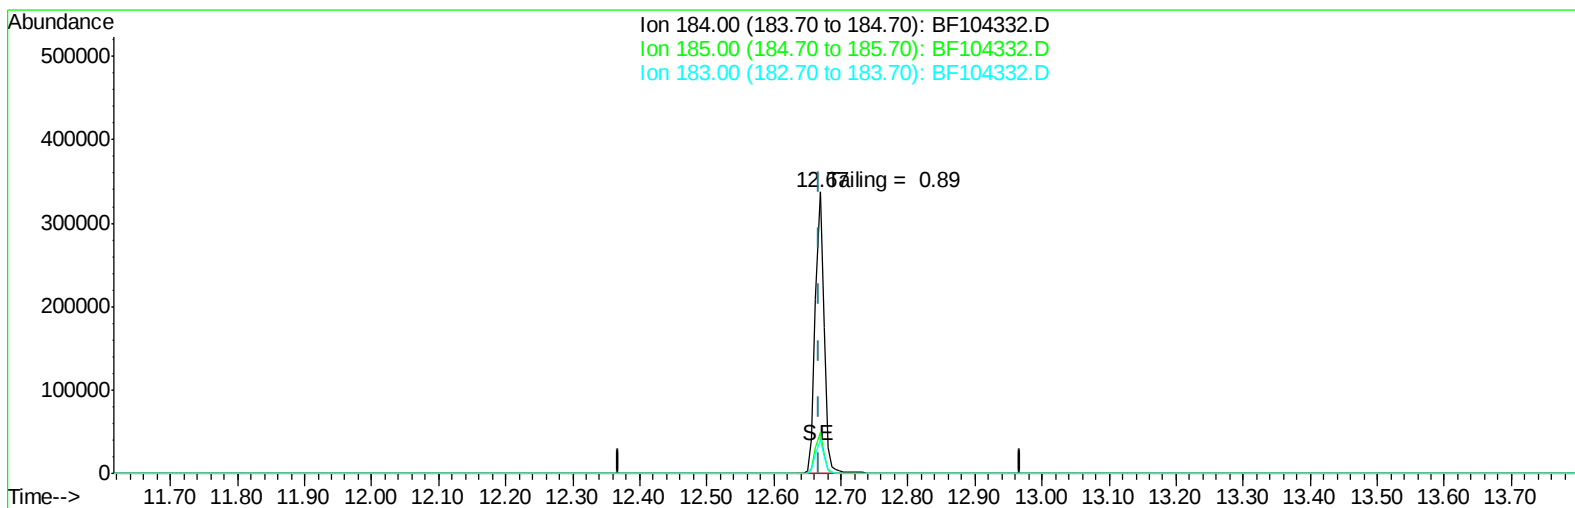

TIC: BF104332.D

(76) Benzidine

12.668min (+0.000) -20.00ng

response 291533

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.60
183.00	11.60	12.05
0.00	0.00	0.00