

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040618\
 Data File : BF104352.D
 Acq On : 7 Apr 2018 12:02
 Operator : JU/SJ
 Sample : J2255-07
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 040418-DBRI-E-D-B

Quant Time: Apr 09 01:21:15 2018
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 06 16:44:53 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.80	152	137976	20.00	ng	0.00
21) Naphthalene-d8	8.09	136	540182	20.00	ng	0.00
38) Acenaphthene-d10	9.84	164	234784	20.00	ng	0.00
63) Phenanthrene-d10	11.33	188	349779	20.00	ng	0.00
75) Chrysene-d12	13.97	240	268796	20.00	ng	0.00
86) Perylene-d12	15.43	264	252017	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.40	112	345773	38.32	ng	0.00
7) Phenol-d6	6.42	99	257730	23.25	ng	-0.01
23) Nitrobenzene-d5	7.37	82	802114	96.96	ng	0.00
41) 2,4,6-Tribromophenol	10.63	330	188751	77.50	ng	0.00
44) 2-Fluorobiphenyl	9.16	172	1366546	91.95	ng	0.00
78) Terphenyl-d14	12.92	244	948188	80.42	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040618\
Data File : BF104352.D
Acq On : 7 Apr 2018 12:02
Operator : JU/SJ
Sample : J2255-07
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
040418-DBRI-E-D-B

Quant Time: Apr 09 01:21:15 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 06 16:44:53 2018
Response via : Initial Calibration

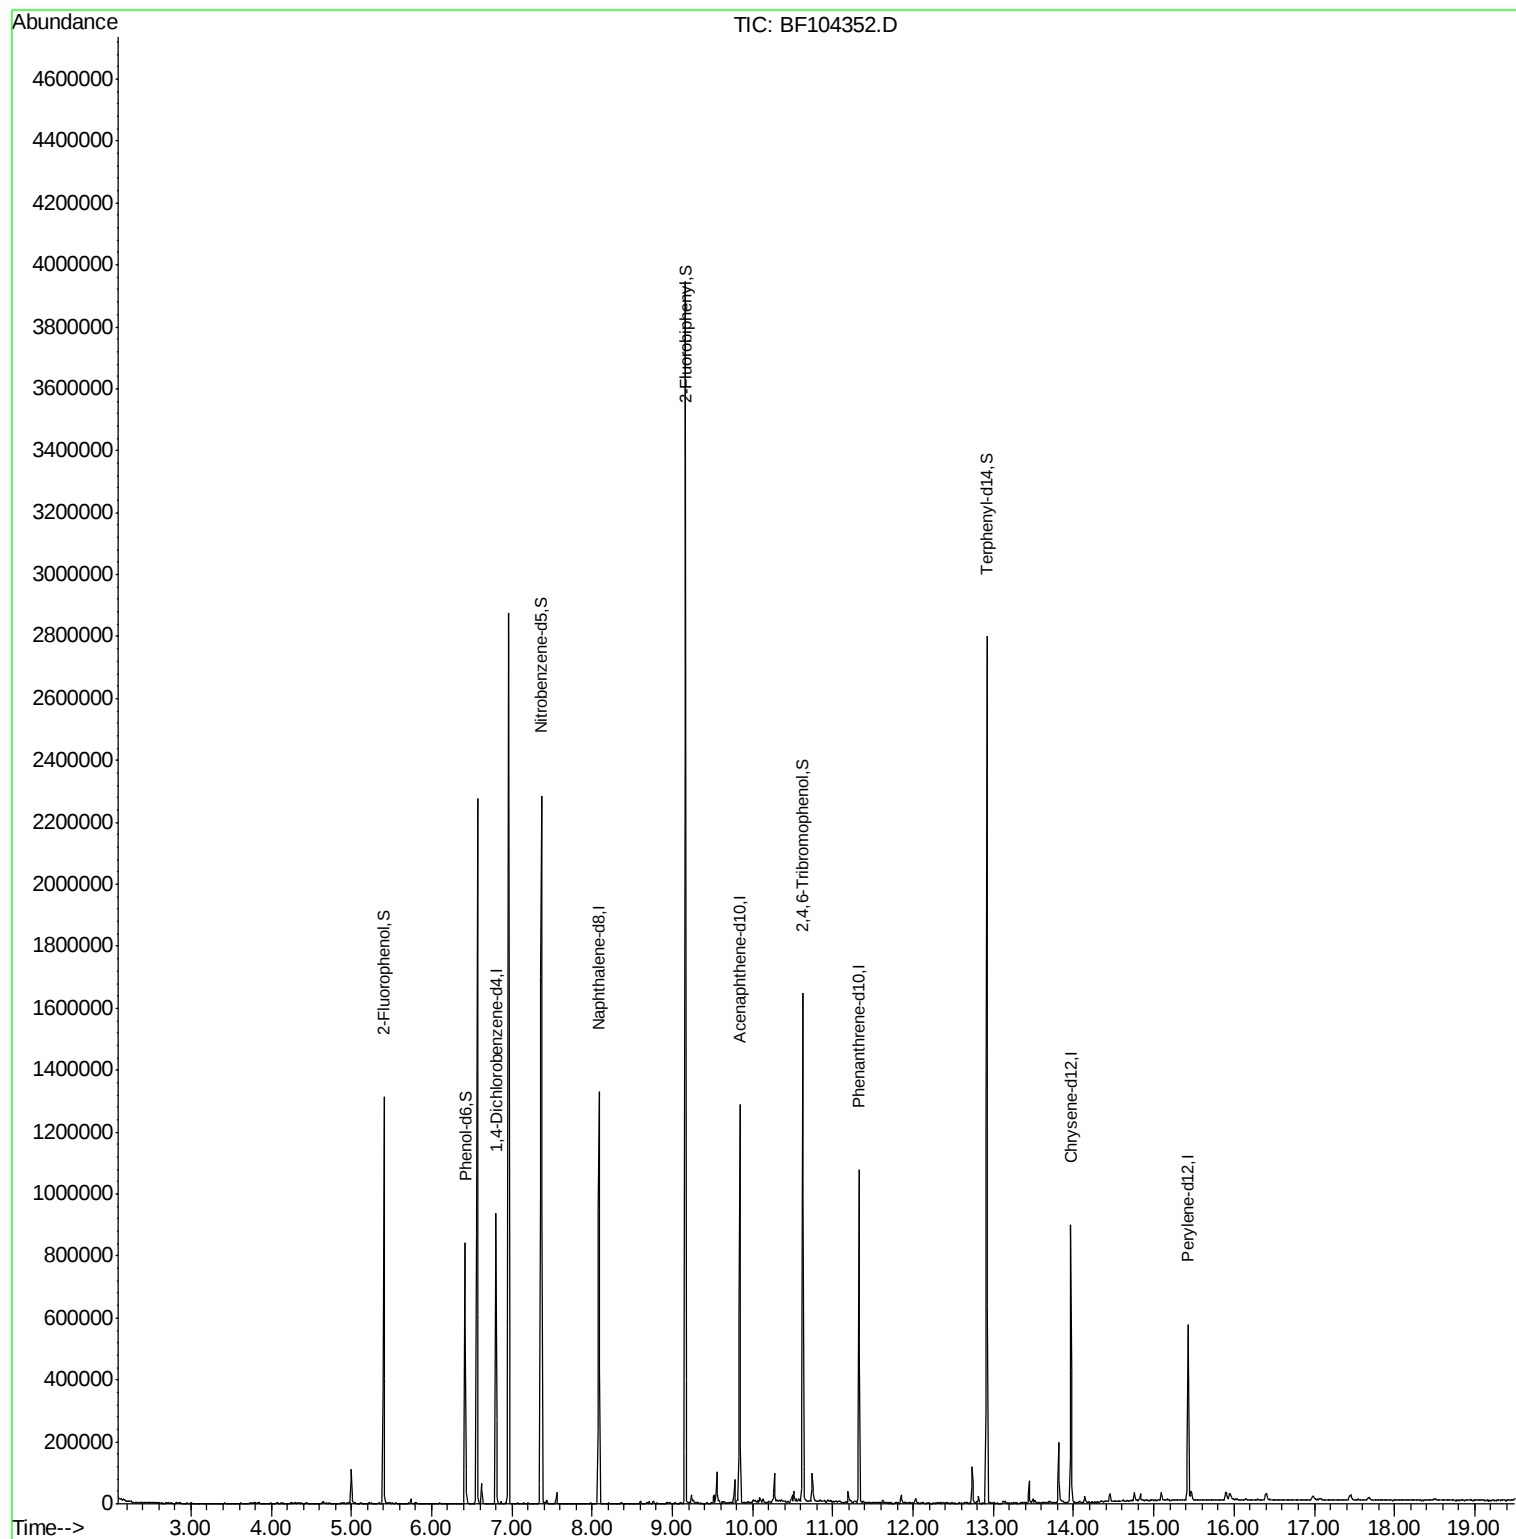

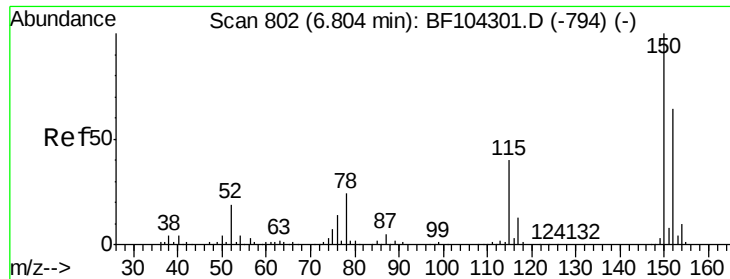


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.80 min Scan# 802
Delta R.T. -0.00 min
Lab File: BF104352.D
Acq: 7 Apr 2018 12:02

Instrument :
BNA_F
ClientSampleId :
040418-DBRI-E-D-B

Tot Ion:152 Resp: 137976
Ion Ratio Lower Upper
152 100
150 154.1 124.6 186.8
115 60.8 50.1 75.1

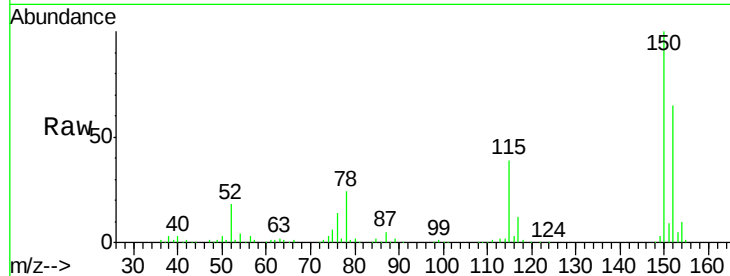


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

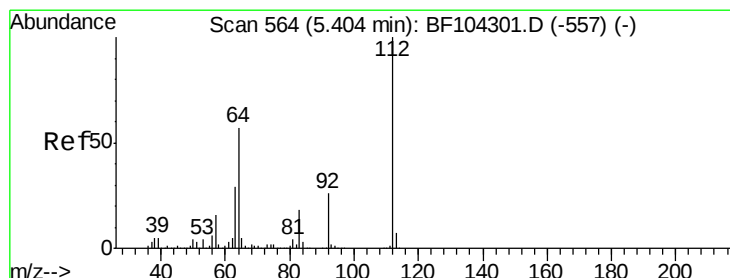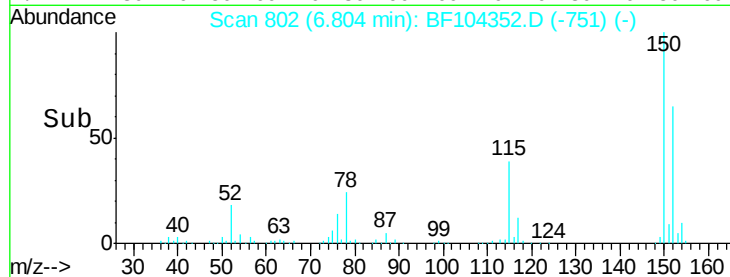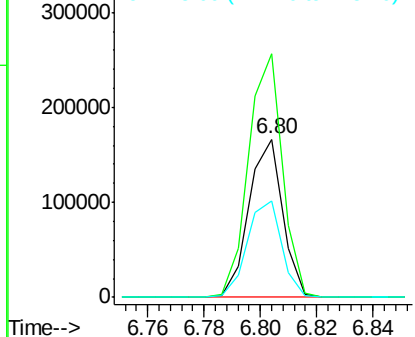



#5

2-Fluorophenol
Concen: 38.319 ng
RT: 5.40 min Scan# 564
Delta R.T. -0.00 min
Lab File: BF104352.D
Acq: 7 Apr 2018 12:02

Tgt Ion:112 Resp: 345773
Ion Ratio Lower Upper
112 100
64 53.9 47.9 71.9
63 27.3 23.7 35.5

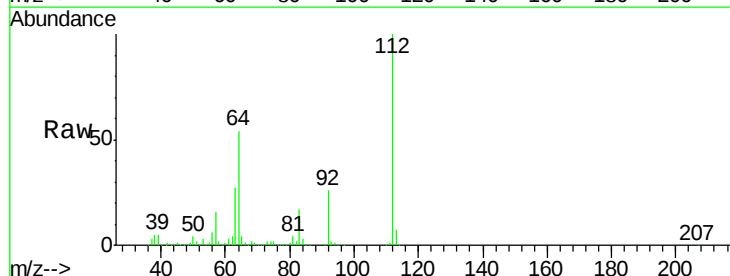

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

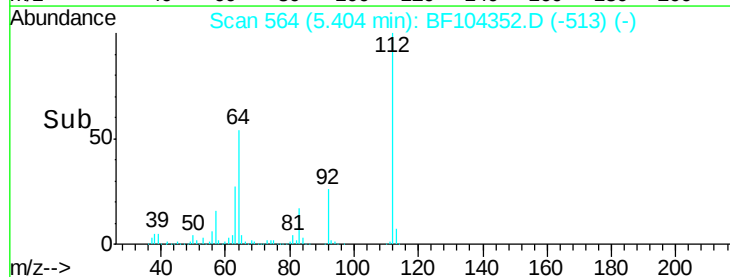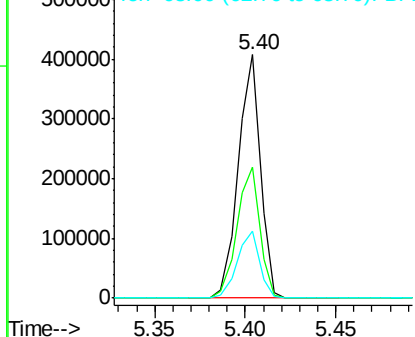



#7

Phenol-d6

Concen: 23.246 ng

RT: 6.42 min Scan# 736

Delta R.T. -0.01 min

Lab File: BF104352.D

Acq: 7 Apr 2018 12:02

Instrument :

BNA_F

ClientSampleId :

040418-DBRI-E-D-B





Tot Ion: 99 Resp: 257730

Ion Ratio Lower Upper

99 100

42 15.8 14.5 21.7

71 31.4 25.4 38.0

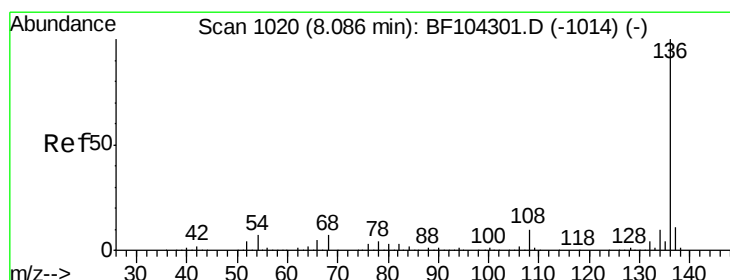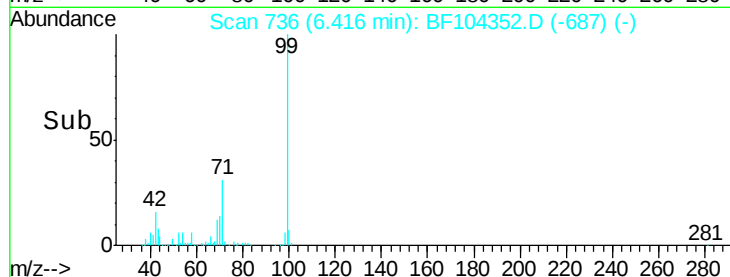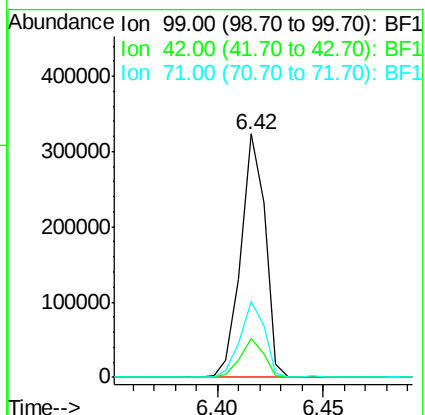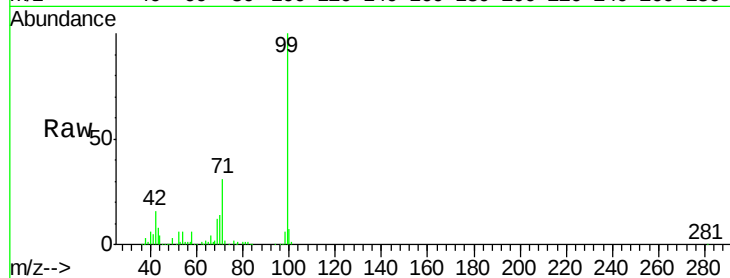

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.09 min Scan# 1020

Delta R.T. -0.00 min

Lab File: BF104352.D

Acq: 7 Apr 2018 12:02

Tgt Ion: 136 Resp: 540182




Ion Ratio Lower Upper

136 100

137 11.0 8.9 13.3

54 6.9 6.6 9.8

68 6.0 5.0 7.4


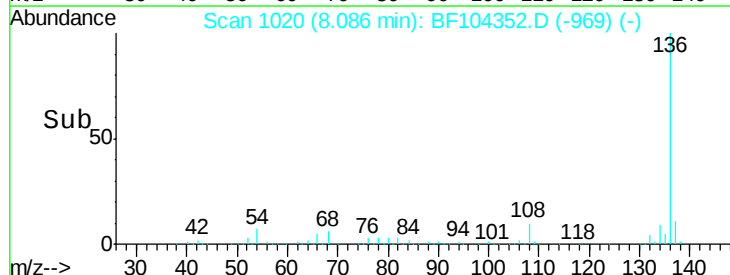
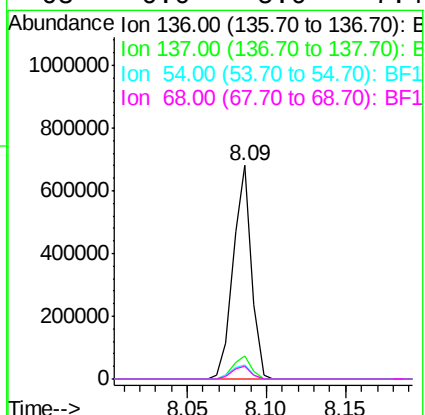
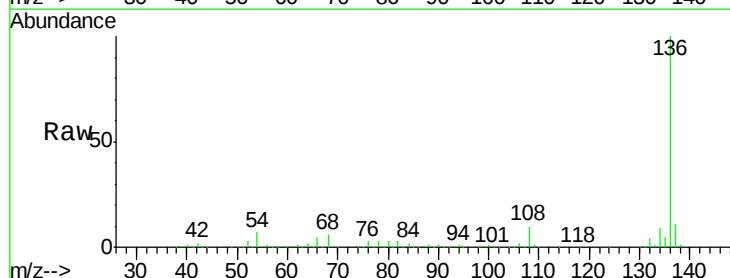




#23
 Nitrobenzene-d5
 Concen: 96.961 ng
 RT: 7.37 min Scan# 898
 Delta R.T. -0.00 min
 Lab File: BF104352.D
 Acq: 7 Apr 2018 12:02




Instrument :
 BNA_F
 ClientSampleId :
 040418-DBRI-E-D-B


Tot Ion: 82 Resp: 802114
 Ion Ratio Lower Upper
 82 100
 128 45.8 36.1 54.1
 54 45.5 41.4 62.2

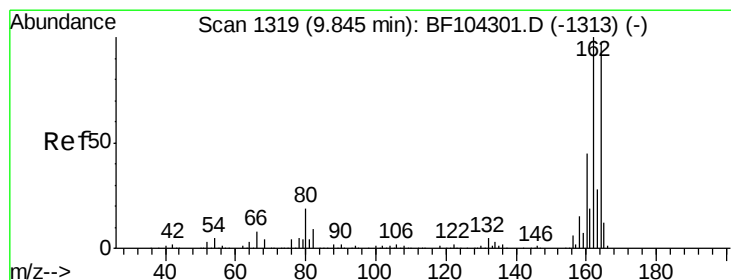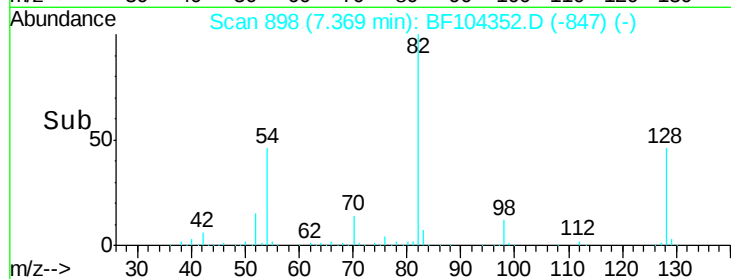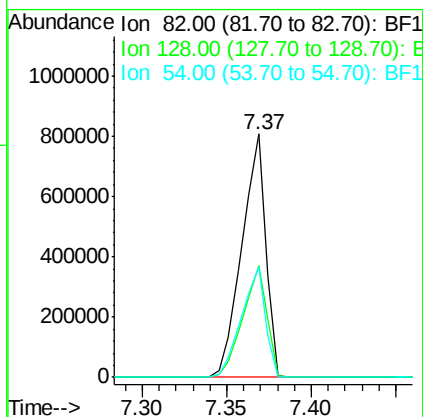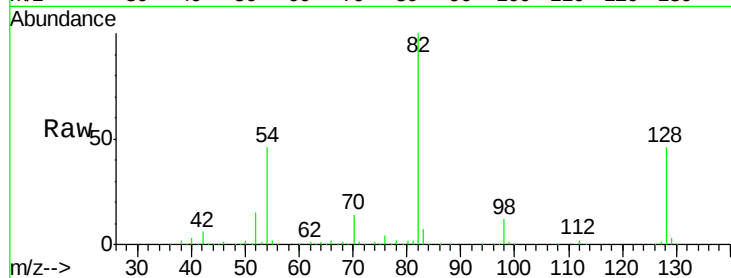

#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.84 min Scan# 1318
 Delta R.T. -0.01 min
 Lab File: BF104352.D
 Acq: 7 Apr 2018 12:02

Tgt Ion:164 Resp: 234784
 Ion Ratio Lower Upper
 164 100
 162 105.0 86.1 129.1
 160 46.6 38.3 57.5

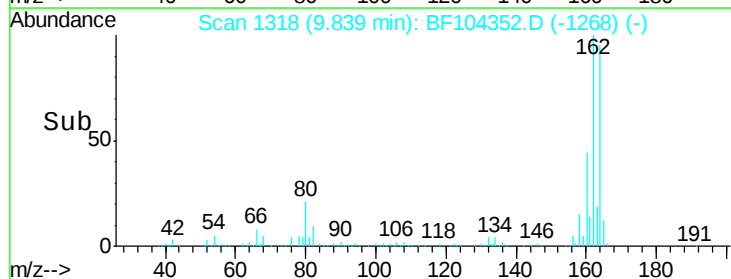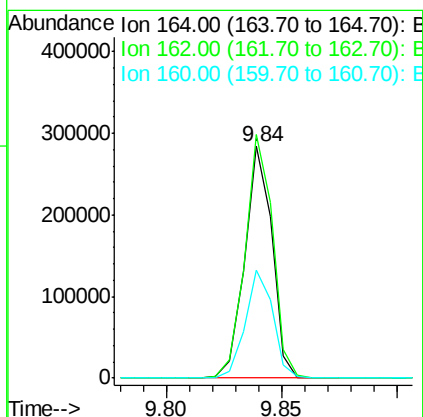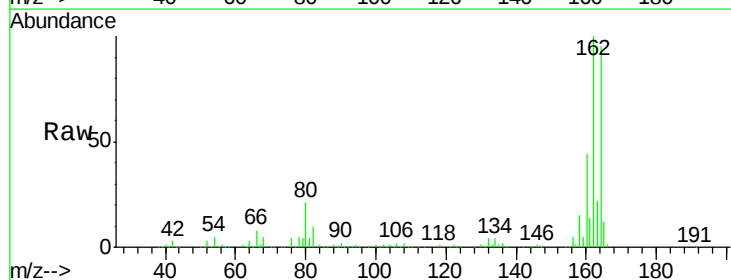

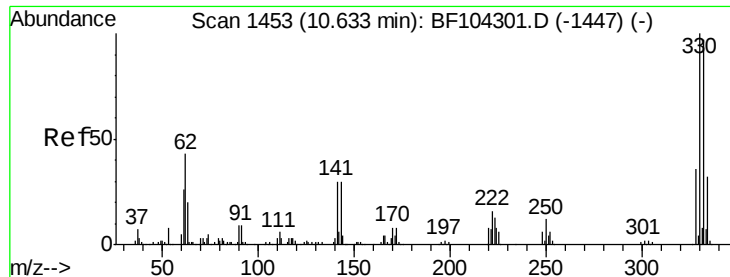

#41

2,4,6-Tribromophenol

Concen: 77.501 ng

RT: 10.63 min Scan# 1452

Delta R.T. -0.01 min

Lab File: BF104352.D

Acq: 7 Apr 2018 12:02

Instrument :

BNA_F

ClientSampleId :

040418-DBRI-E-D-B


Tot Ion:330 Resp: 188751

Ion Ratio Lower Upper

330 100

332 95.3 77.0 115.6




141 35.1 29.9 44.9

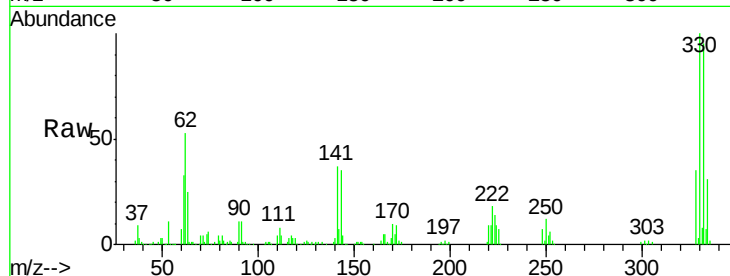

Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

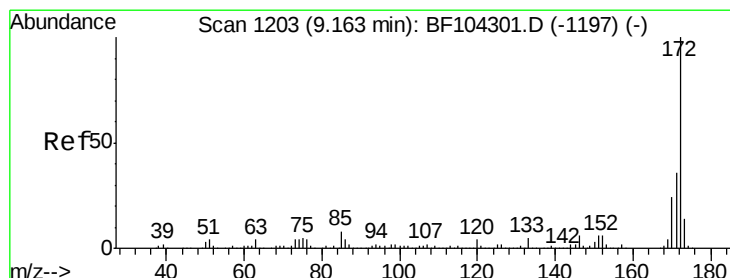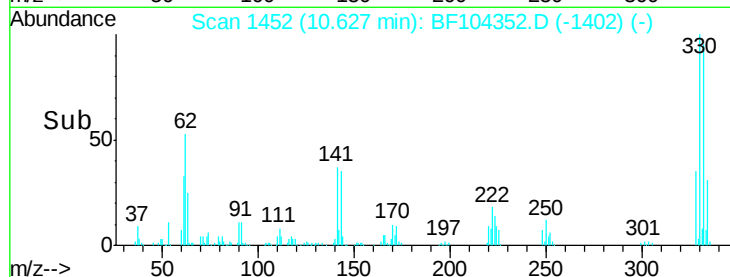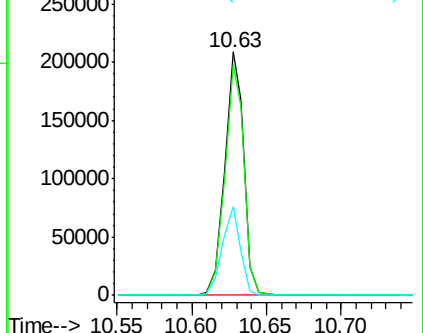

#44

2-Fluorobiphenyl

Concen: 91.948 ng

RT: 9.16 min Scan# 1203

Delta R.T. 0.00 min

Lab File: BF104352.D

Acq: 7 Apr 2018 12:02


Tgt Ion:172 Resp: 1366546

Ion Ratio Lower Upper

172 100

171 36.2 29.7 44.5



170 24.1 19.6 29.4

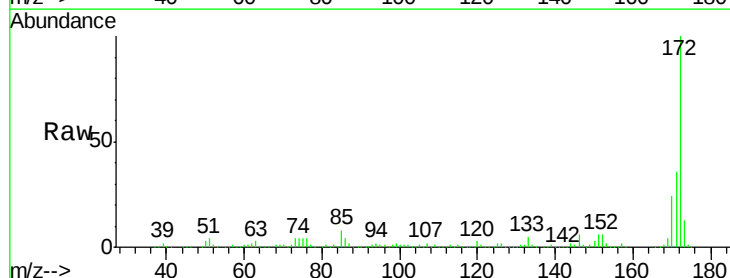


Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

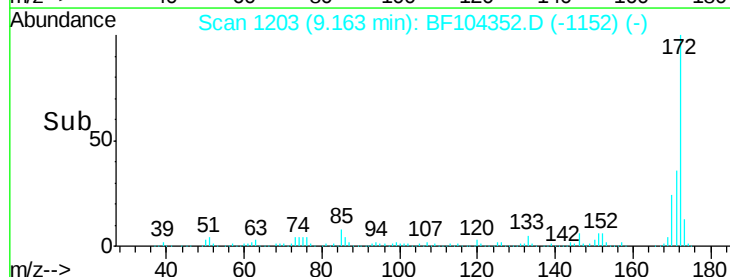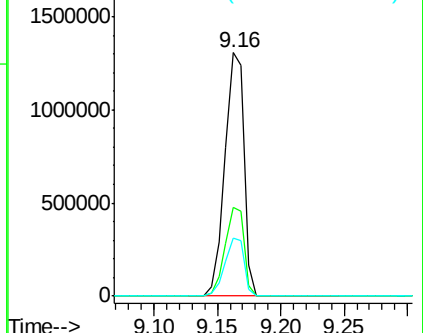


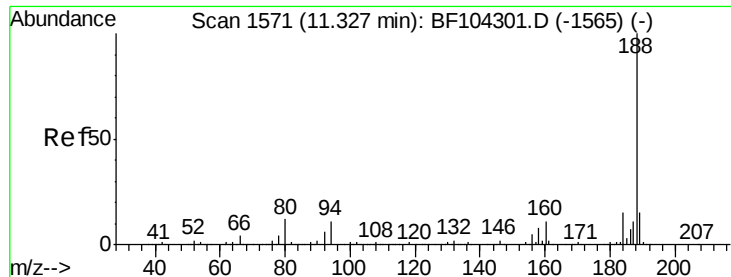




#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.33 min Scan# 1571
Delta R.T. -0.00 min
Lab File: BF104352.D
Acq: 7 Apr 2018 12:02

Instrument :
BNA_F
ClientSampleId :
040418-DBRI-E-D-B

Tot Ion:188 Resp: 349779
Ion Ratio Lower Upper
188 100
94 10.6 8.5 12.7
80 11.6 9.2 13.8

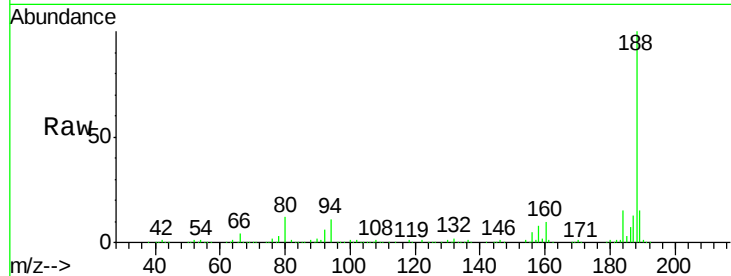


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

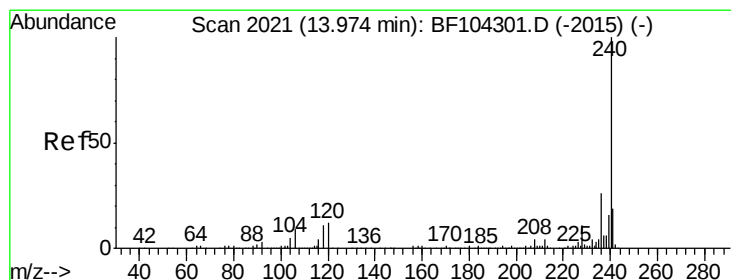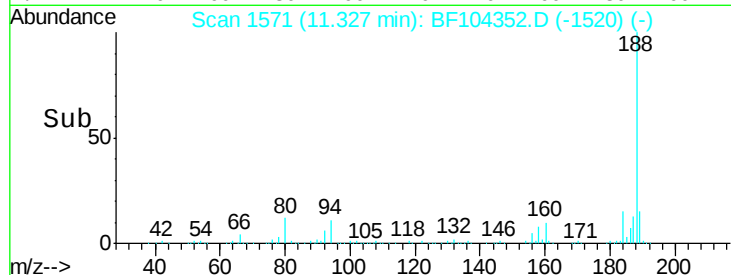
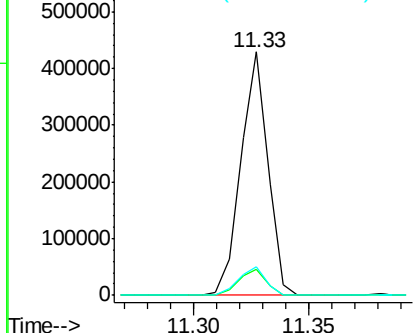



#75
Chrysene-d12
Concen: 20.000 ng
RT: 13.97 min Scan# 2020
Delta R.T. -0.01 min
Lab File: BF104352.D
Acq: 7 Apr 2018 12:02

Tgt Ion:240 Resp: 268796
Ion Ratio Lower Upper
240 100
120 12.8 9.5 14.3
236 25.7 20.7 31.1

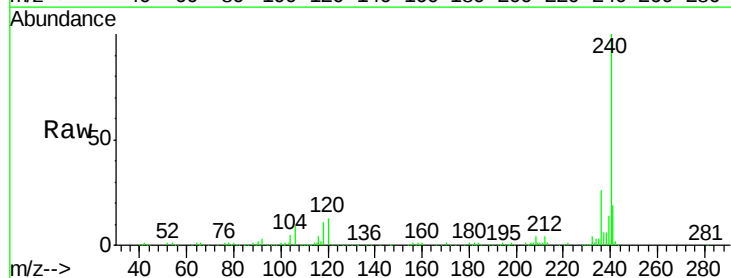

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

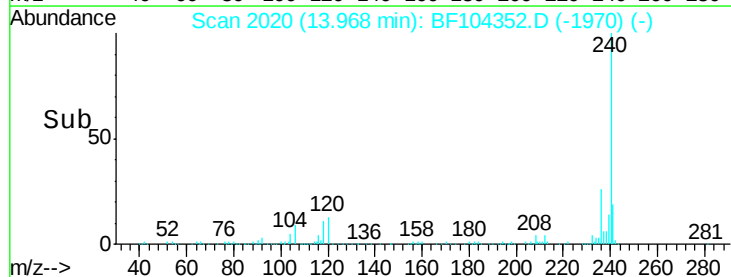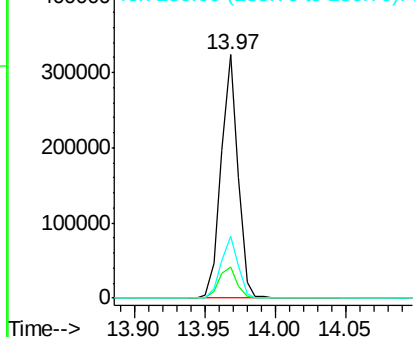

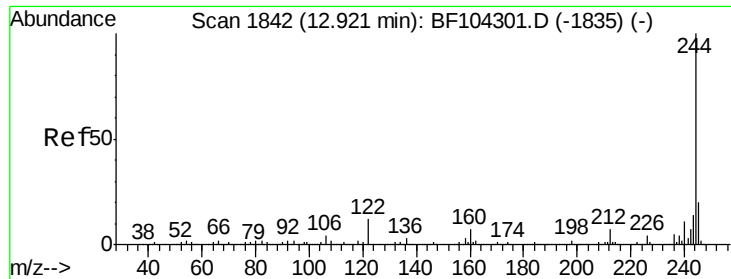

#78

Terphenyl-d14

Concen: 80.422 ng

RT: 12.92 min Scan# 1842

Delta R.T. -0.00 min

Lab File: BF104352.D

Acq: 7 Apr 2018 12:02

Instrument :

BNA_F

ClientSampleId :

040418-DBRI-E-D-B


Tot Ion:244 Resp: 948188

Ion Ratio Lower Upper

244 100

212 7.0 5.4 8.0




122 11.7 11.0 16.4

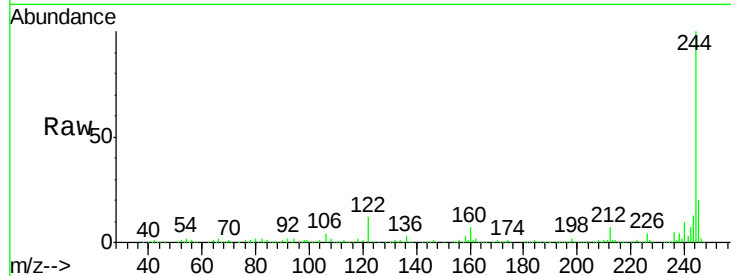

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

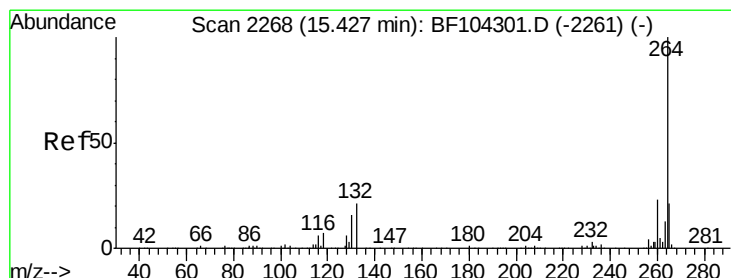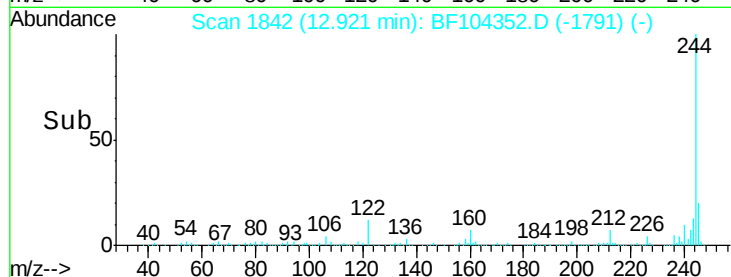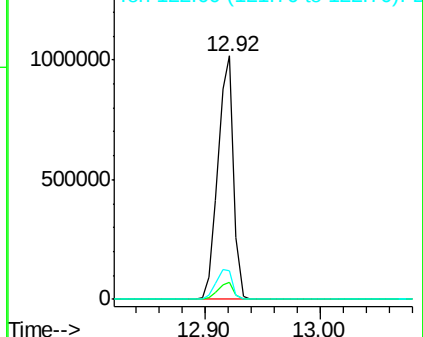

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.43 min Scan# 2268

Delta R.T. -0.00 min

Lab File: BF104352.D

Acq: 7 Apr 2018 12:02


Tgt Ion:264 Resp: 252017

Ion Ratio Lower Upper

264 100

260 23.8 19.2 28.8

265 21.2 17.5 26.3

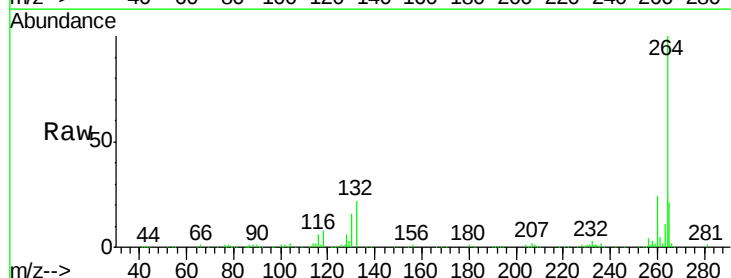

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

