

Data Path : Z:\HPCHEM1\BNA F\Data\BF040618\
 Data File : BF104313.D
 Acq On : 6 Apr 2018 18:51
 Operator : JU/SJ
 Sample : J2153-01 5X
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 HR-06-040418-A

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.993	491	494	500	rBV2	32796	37304	3.44%	0.362%
2	5.393	558	562	566	rVB	700575	650777	60.09%	6.317%
3	6.410	731	735	740	rVB	713085	631802	58.34%	6.133%
4	6.563	757	761	764	rBV	817941	678764	62.67%	6.589%
5	6.798	798	801	805	rVB	956811	804299	74.27%	7.807%
6	6.957	824	828	831	rVB	611227	528700	48.82%	5.132%
7	7.357	893	896	899	rBV	472060	354542	32.74%	3.442%
8	7.398	899	903	906	rVB2	12908	12952	1.20%	0.126%
9	8.081	1013	1019	1023	rBV	1169705	1072274	99.01%	10.409%
10	9.157	1198	1202	1205	rBV	951681	717542	66.25%	6.965%
11	9.239	1212	1216	1219	rBV	17884	15624	1.44%	0.152%
12	9.551	1265	1269	1273	rBV	54418	48091	4.44%	0.467%
13	9.769	1304	1306	1309	rVB	27953	19515	1.80%	0.189%
14	9.839	1314	1318	1321	rVB	1276028	1083011	100.00%	10.513%
15	10.269	1389	1391	1394	rVB	33035	25023	2.31%	0.243%
16	10.492	1424	1429	1431	rBV	13898	15096	1.39%	0.147%
17	10.622	1447	1451	1455	rBV	431070	344344	31.80%	3.343%
18	10.745	1469	1472	1480	rBV	27990	36507	3.37%	0.354%
19	11.192	1546	1548	1551	rBV3	16293	16270	1.50%	0.158%
20	11.322	1566	1570	1574	rBV	1012485	875288	80.82%	8.497%
21	11.851	1656	1660	1663	rBV	21875	22807	2.11%	0.221%
22	12.910	1836	1840	1844	rBV	602097	482907	44.59%	4.688%
23	13.357	1912	1916	1918	rBV4	9500	13297	1.23%	0.129%
24	13.810	1990	1993	1996	rBV3	45498	47647	4.40%	0.463%
25	13.839	1996	1998	2001	rVB	19782	17257	1.59%	0.168%
26	13.963	2015	2019	2023	rBV	875004	815172	75.27%	7.913%
27	14.445	2099	2101	2104	rBV3	14237	13319	1.23%	0.129%
28	14.827	2163	2166	2169	rBV3	23195	23431	2.16%	0.227%
29	15.086	2208	2210	2218	rVB6	20702	25185	2.33%	0.244%
30	15.421	2262	2267	2272	rBV	695099	848203	78.32%	8.234%
31	15.574	2290	2293	2297	rVB6	21301	24740	2.28%	0.240%


Sum of corrected areas: 10301690

Data Path : Z:\HPCHEM1\BNA_F\Data\BF040618\
Data File : BF104313.D
Acq On : 6 Apr 2018 18:51
Operator : JU/SJ
Sample : J2153-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-040418-A

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

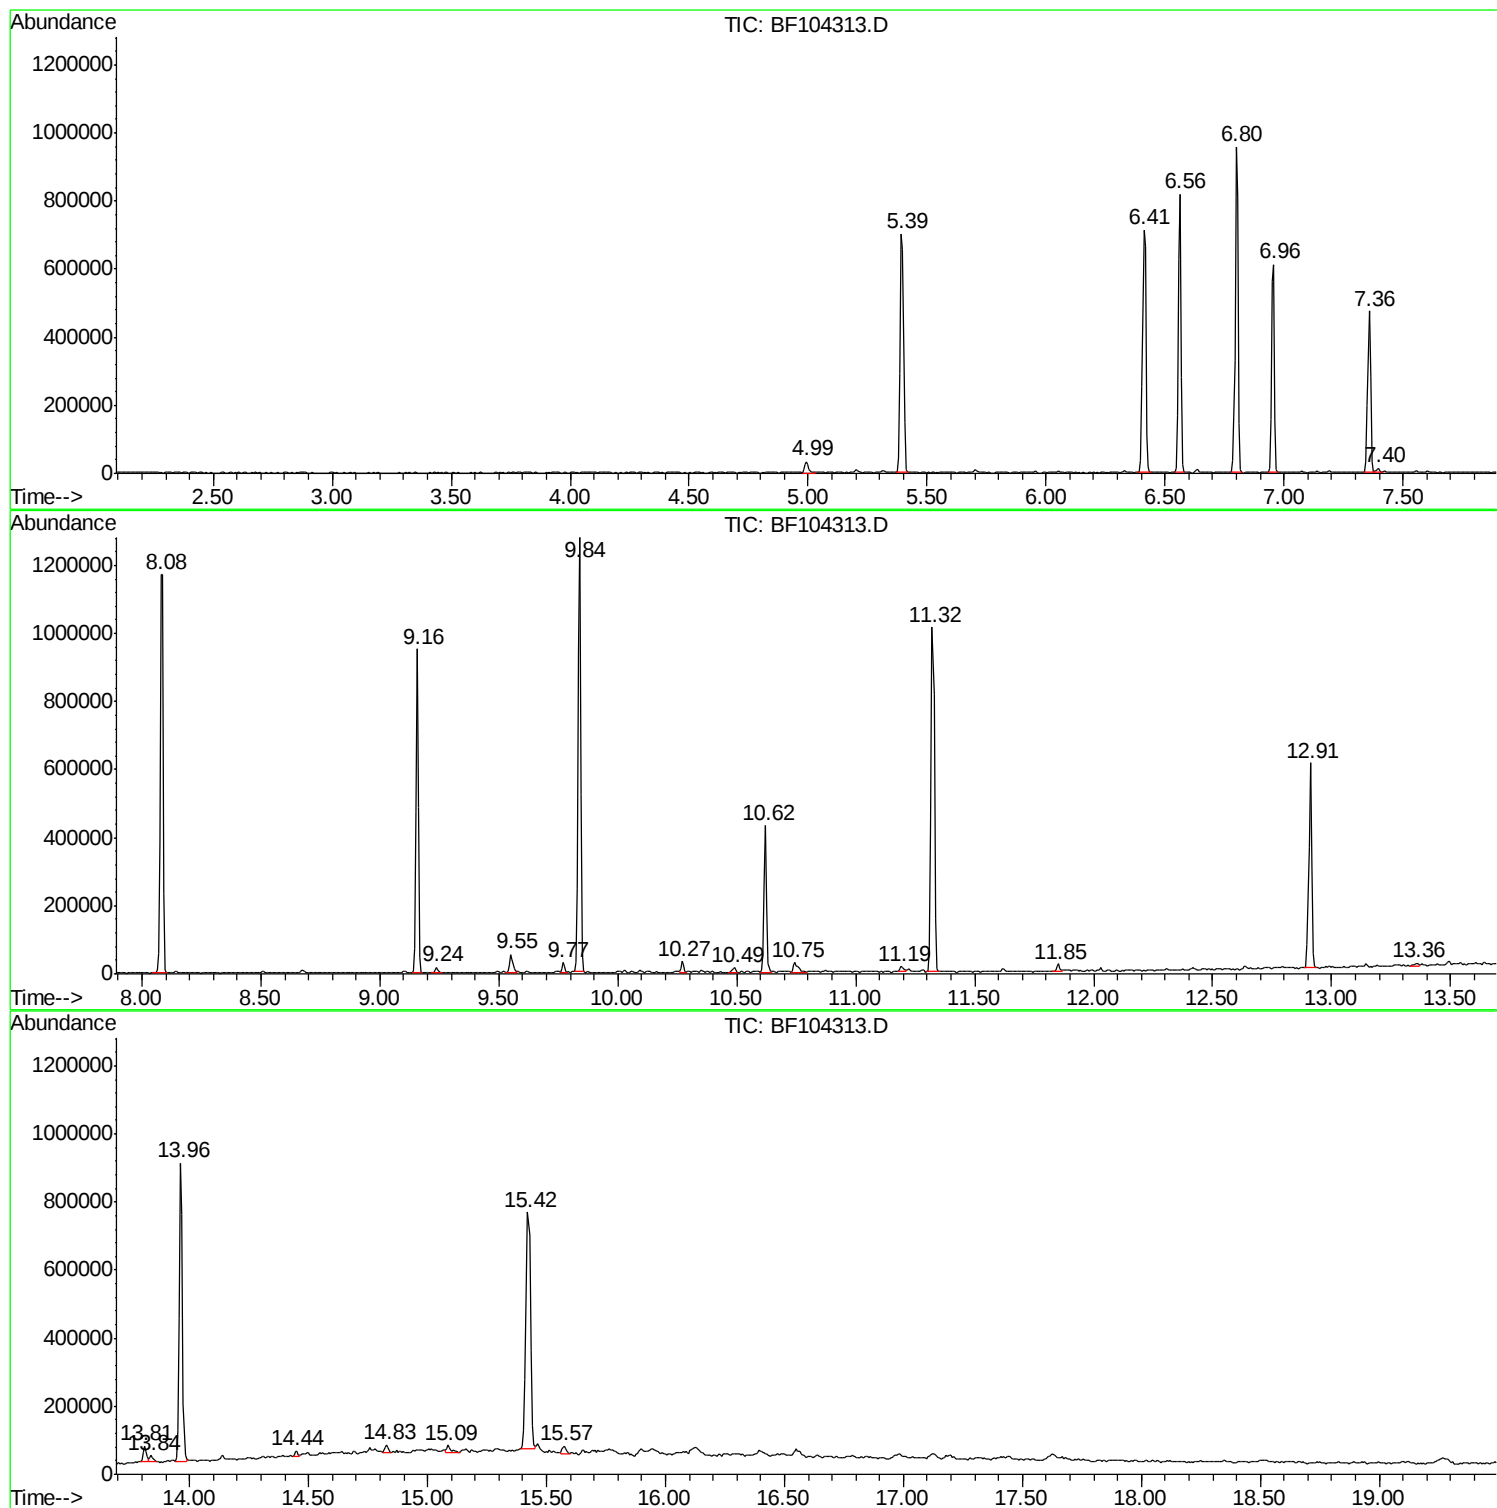

Data Path : Z:\HPCHEM1\BNA F\Data\BF040618\
Data File : BF104313.D
Acq On : 6 Apr 2018 18:51
Operator : JU/SJ
Sample : J2153-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-040418-A









Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.56 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.56	16.88 ng	678764	1,4-Dichlorobenzene-d4	6.80

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	27
2		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
3		Tranvlcypropine-propionyl	189	C12H15NO	1000123-86-3	10
4		5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9
5		1-Aminoindan	133	C9H11N	034698-41-4	9

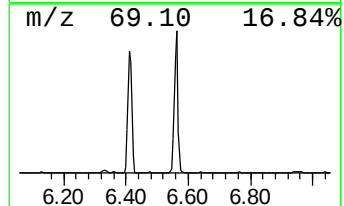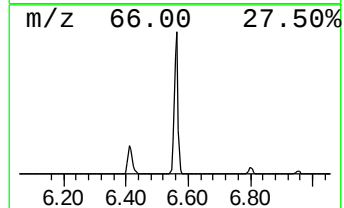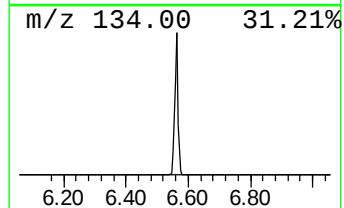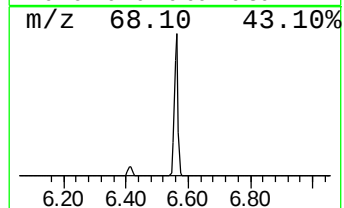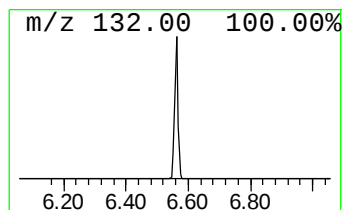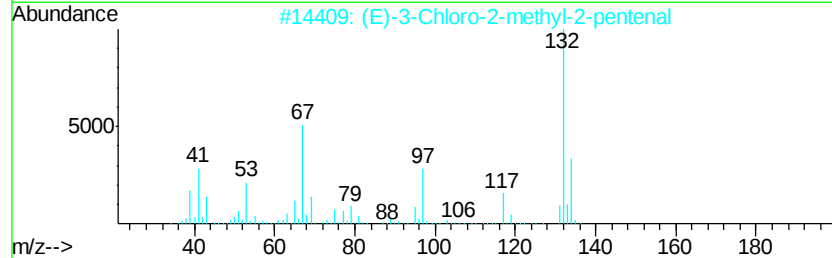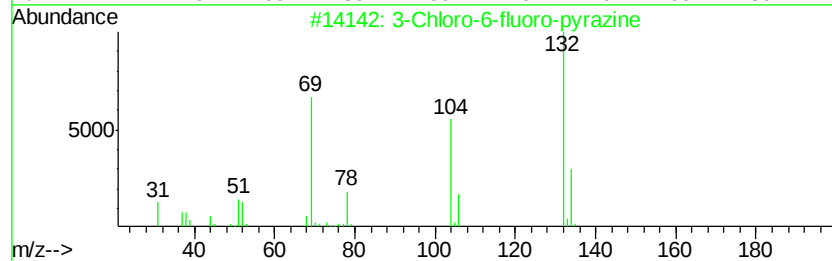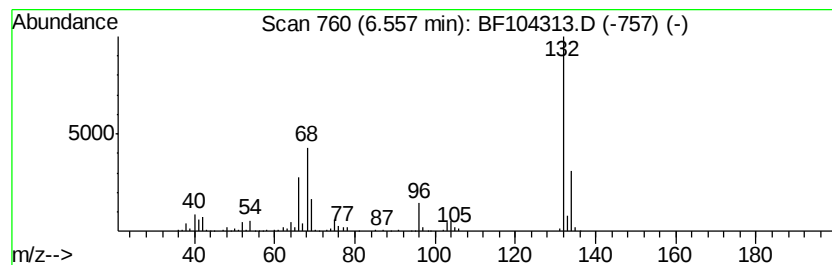

Data Path : Z:\HPCHEM1\BNA_F\Data\BF040618\
Data File : BF104313.D
Acq On : 6 Apr 2018 18:51
Operator : JU/SJ
Sample : J2153-01 5X
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
HR-06-040418-A

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.56	6.56	16.9	ng	678764	1	6.80	804299	20.0