

Data Path : Z:\HPCHEM1\BNA F\Data\BF040618\
 Data File : BF104327.D
 Acq On : 7 Apr 2018 1:01
 Operator : JU/SJ
 Sample : J2257-01 10X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 LP-OILY-STONE

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.992	491	494	498	rBV	17655	17538	1.63%	0.217%
2	5.398	559	563	566	rVB	467208	397985	36.90%	4.928%
3	6.416	732	736	743	rBV	532361	426846	39.58%	5.285%
4	6.563	757	761	764	rBV	546575	421342	39.07%	5.217%
5	6.804	798	802	805	rVB	1001837	790494	73.30%	9.788%
6	6.957	824	828	831	rVB	410862	313083	29.03%	3.877%
7	7.363	893	897	900	rVB	259581	216874	20.11%	2.685%
8	8.086	1016	1020	1023	rBV	1373743	1056812	98.00%	13.086%
9	9.163	1199	1203	1206	rBV	494689	418250	38.78%	5.179%
10	9.504	1258	1261	1267	rBV	19457	15187	1.41%	0.188%
11	9.557	1267	1270	1273	rVB	33602	27324	2.53%	0.338%
12	9.845	1315	1319	1322	rVB	1151501	1078416	100.00%	13.353%
13	10.627	1448	1452	1455	rBV	248637	211731	19.63%	2.622%
14	11.198	1545	1549	1550	rBV3	14714	15462	1.43%	0.191%
15	11.327	1567	1571	1574	rBV	1069680	859563	79.71%	10.643%
16	11.786	1646	1649	1654	rBV5	12949	20982	1.95%	0.260%
17	11.892	1664	1667	1670	rBV	25579	20367	1.89%	0.252%
18	12.316	1736	1739	1741	rBV3	15251	14323	1.33%	0.177%
19	12.421	1755	1757	1760	rBV4	13248	14474	1.34%	0.179%
20	12.539	1773	1777	1779	rBV	42012	44693	4.14%	0.553%
21	12.768	1814	1816	1818	rBV	33541	23023	2.13%	0.285%
22	12.915	1837	1841	1847	rBV	333772	326354	30.26%	4.041%
23	13.968	2017	2020	2024	rVB	749912	723398	67.08%	8.957%
24	15.427	2264	2268	2272	rBV	513959	621478	57.63%	7.695%


Sum of corrected areas: 8075999

Data Path : Z:\HPCHEM1\BNA_F\Data\BF040618\
Data File : BF104327.D
Acq On : 7 Apr 2018 1:01
Operator : JU/SJ
Sample : J2257-01 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LP-OILY-STONE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

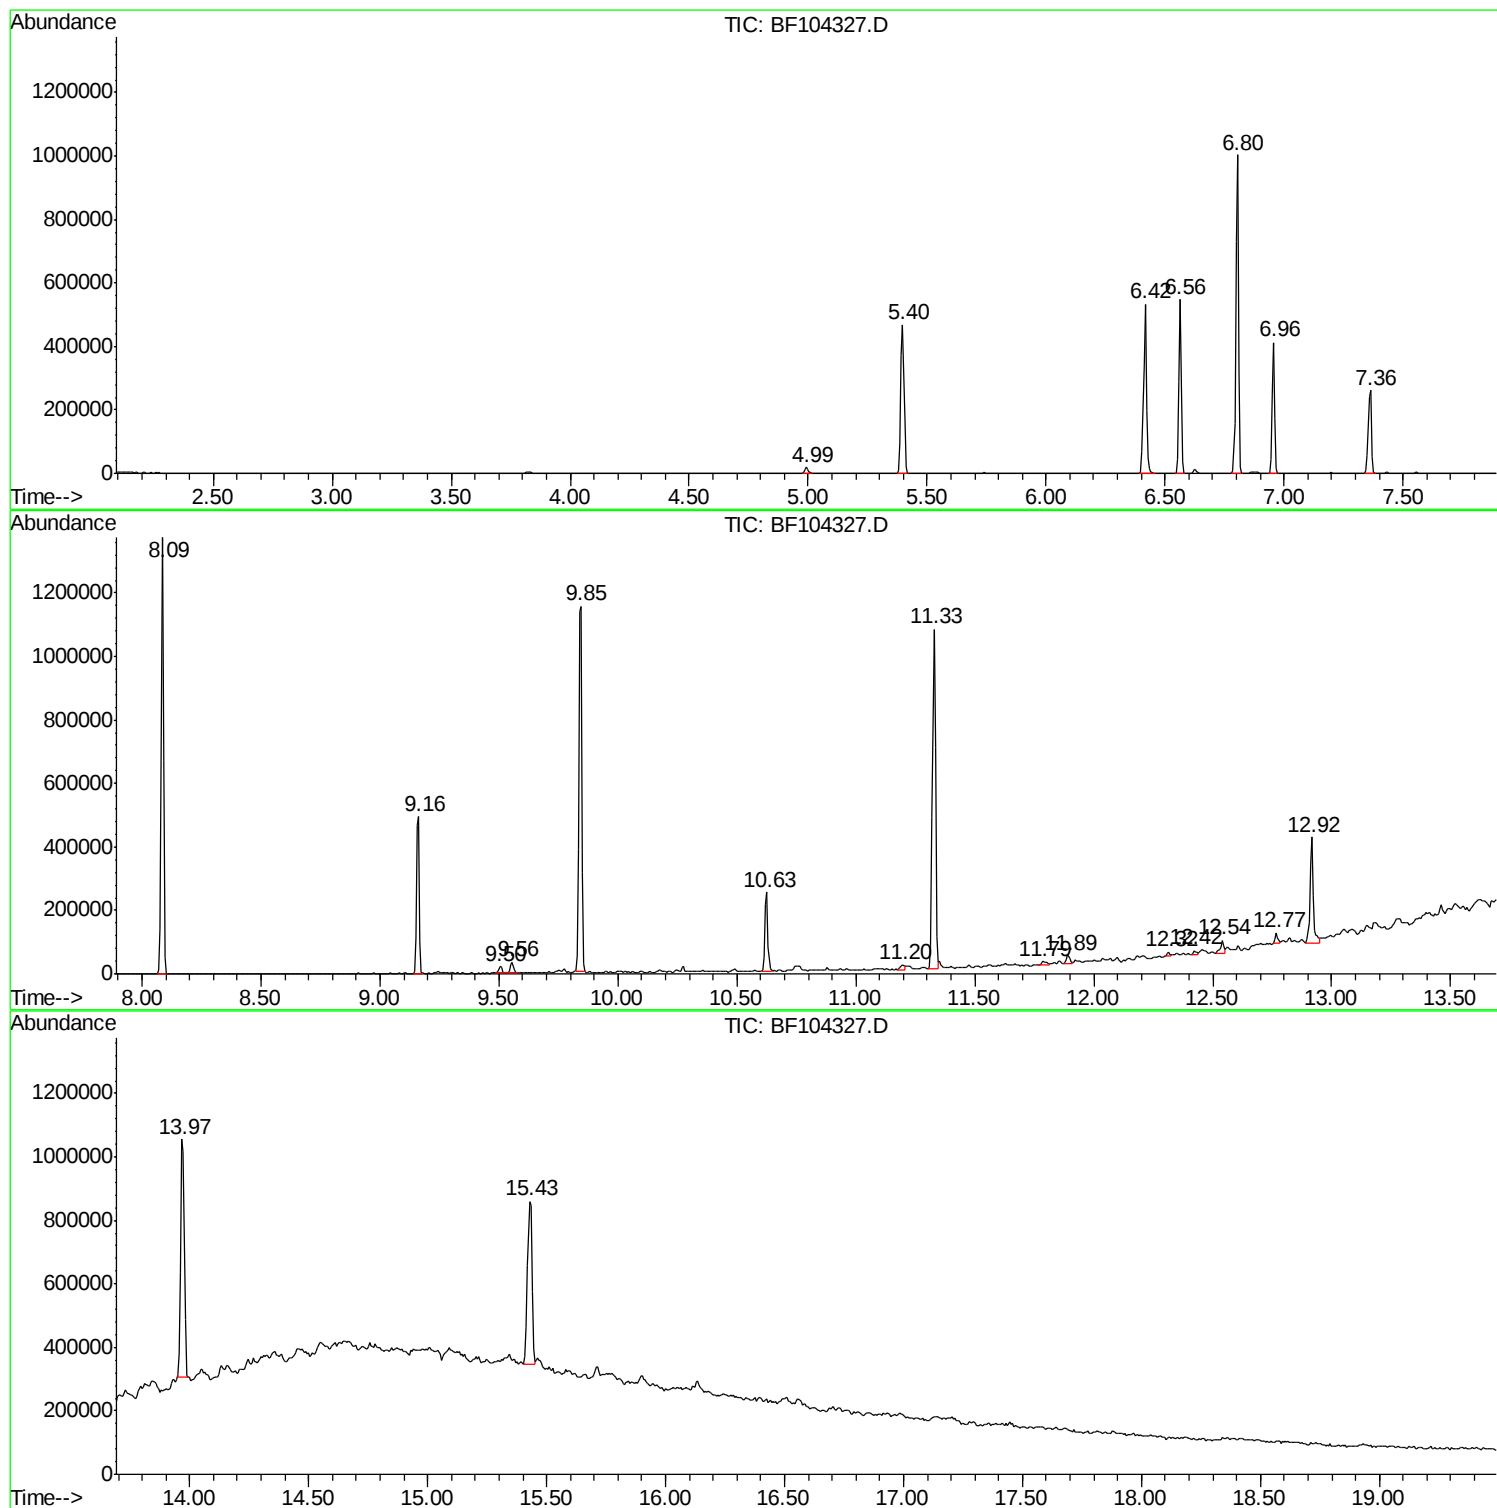

Data Path : Z:\HPCHEM1\BNA F\Data\BF040618\
Data File : BF104327.D
Acq On : 7 Apr 2018 1:01
Operator : JU/SJ
Sample : J2257-01 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LP-OILY-STONE










Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.56 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.56	10.66 ng	421342	1,4-Dichlorobenzene-d4	6.80

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	17
2		3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
3		5-Aminoindole	132	C8H8N2	005192-03-0	12
4		2H-Cyclopenta[d]pyridazine, 2-me...	132	C8H8N2	022291-85-6	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

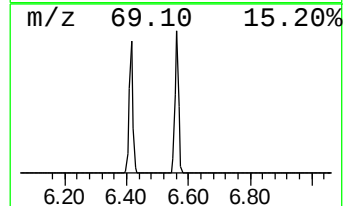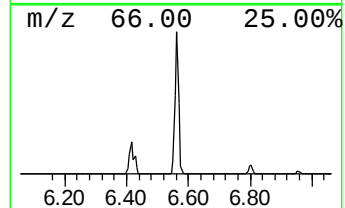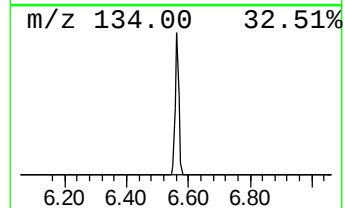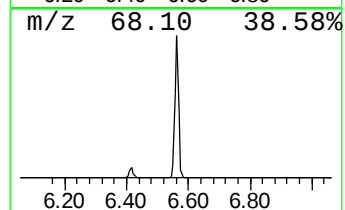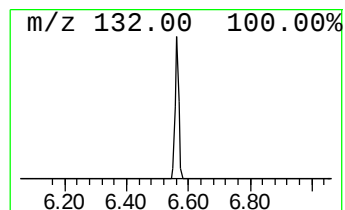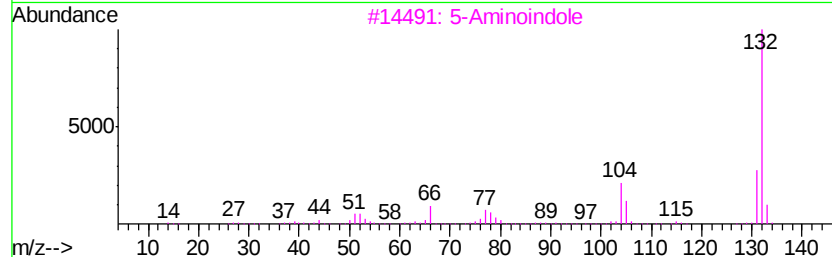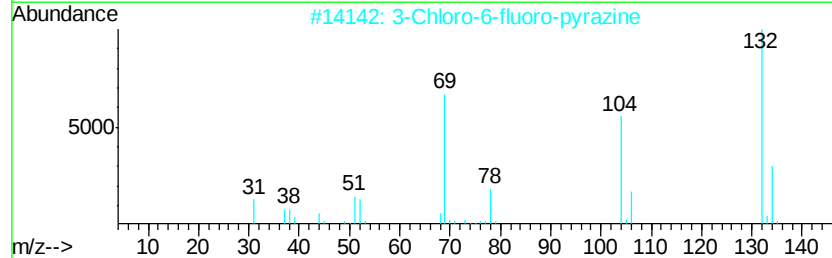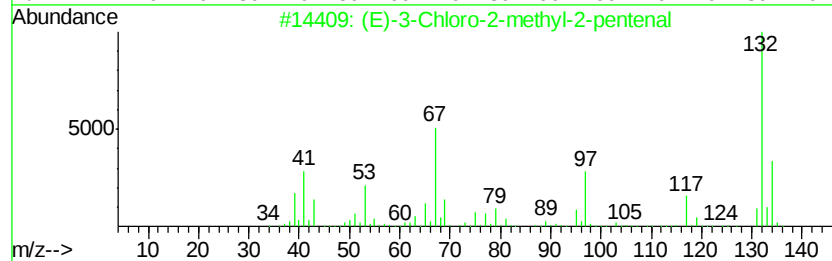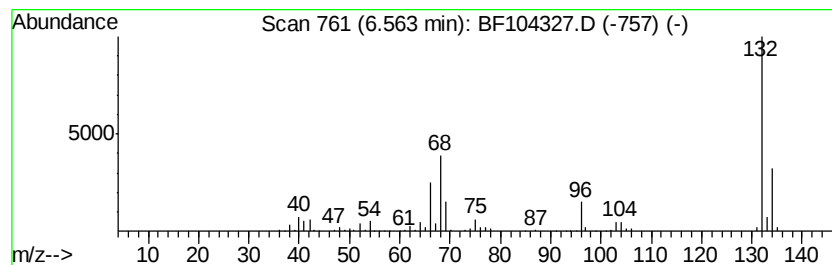

Data Path : Z:\HPCHEM1\BNA_F\Data\BF040618\
Data File : BF104327.D
Acq On : 7 Apr 2018 1:01
Operator : JU/SJ
Sample : J2257-01 10X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
LP-OILY-STONE

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown6.56	6.56	10.7	ng	421342	1	6.80	790494	20.0