


Data Path : Z:\HPCHEM1\BNA F\Data\BF040618\
 Data File : BF104297.D
 Acq On : 6 Apr 2018 11:08
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040618.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 06 16:44:53 2018

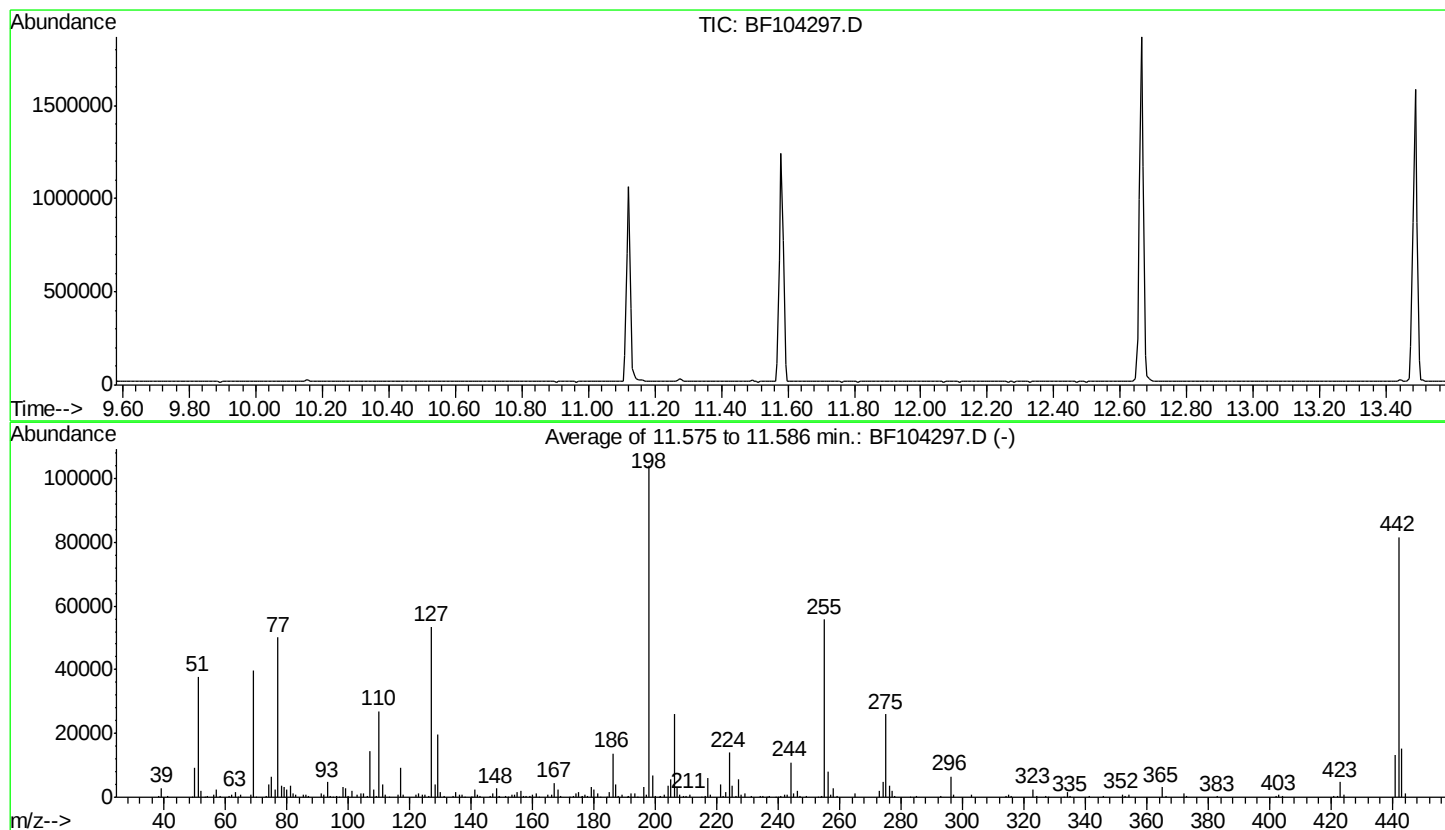

AutoFind: Scans 1613, 1614, 1615; Background Corrected with Scan 1608

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	36.4	37861	PASS
68	69	0.00	2	1.6	651	PASS
69	198	0.00	100	38.4	39919	PASS
70	69	0.00	2	0.4	165	PASS
127	198	10	80	51.3	53405	PASS
197	198	0.00	2	0.8	838	PASS
198	198	100	100	100.0	104010	PASS
199	198	5	9	6.5	6717	PASS
275	198	10	60	25.1	26085	PASS
365	198	1	100	3.0	3159	PASS
441	443	0.01	100	86.3	13313	PASS
442	198	50	100	78.5	81677	PASS
443	442	15	24	18.9	15433	PASS