
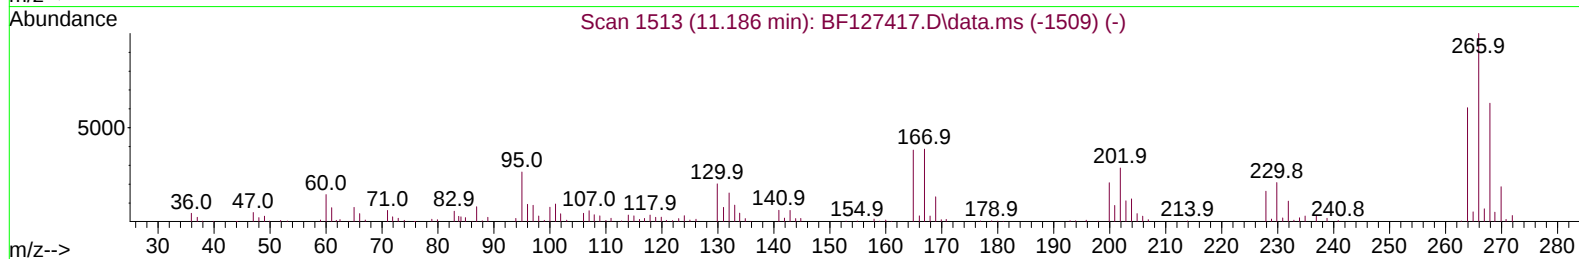
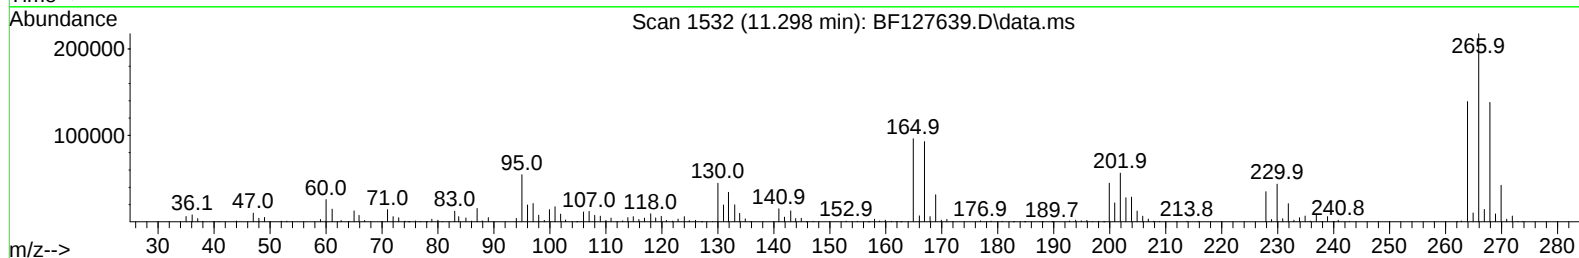


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF040622\  
Data File : BF127639.D  
Acq On : 06 Apr 2022 09:43  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 13:06:50 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 06 13:06:44 2022  
Response via : Initial Calibration

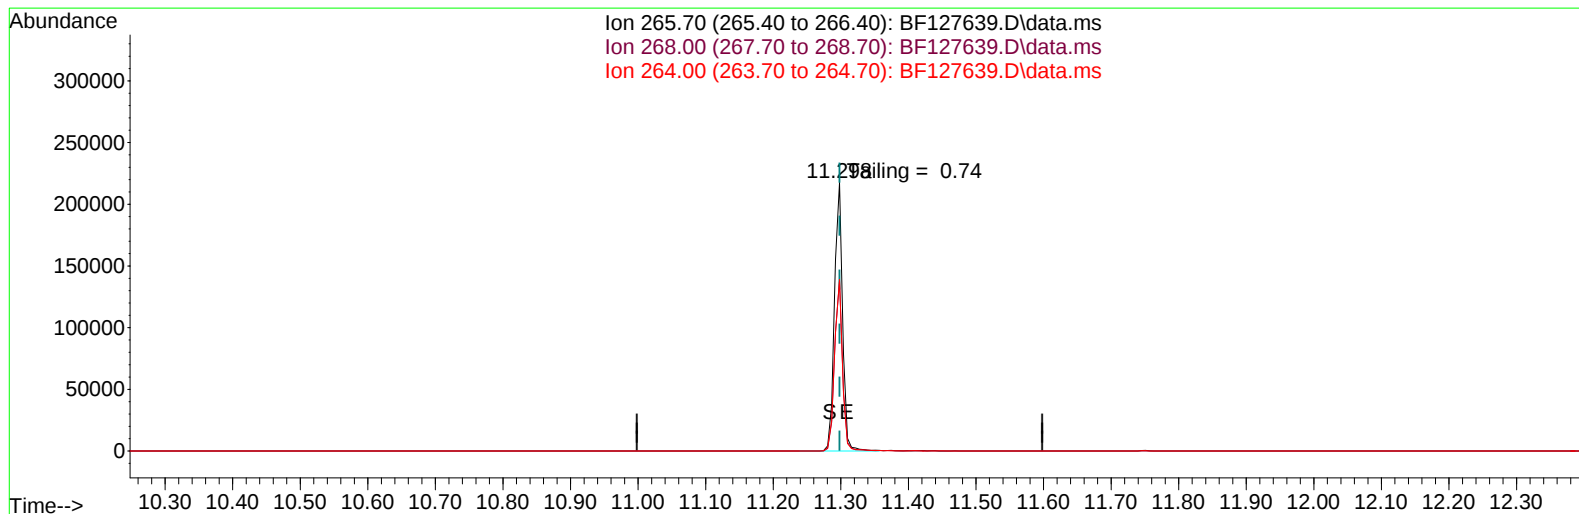

TIC: BF127639.D\data.ms

**(70) Pentachlorophenol (C)**




11.298min ( 0.000) 377428.56 ng

response 182284

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.00  | 63.52  |
| 264.00 | 60.60  | 63.93  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF040622\  
Data File : BF127639.D  
Acq On : 06 Apr 2022 09:43  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 13:56:14 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF040622.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Apr 06 13:55:27 2022  
Response via : Initial Calibration

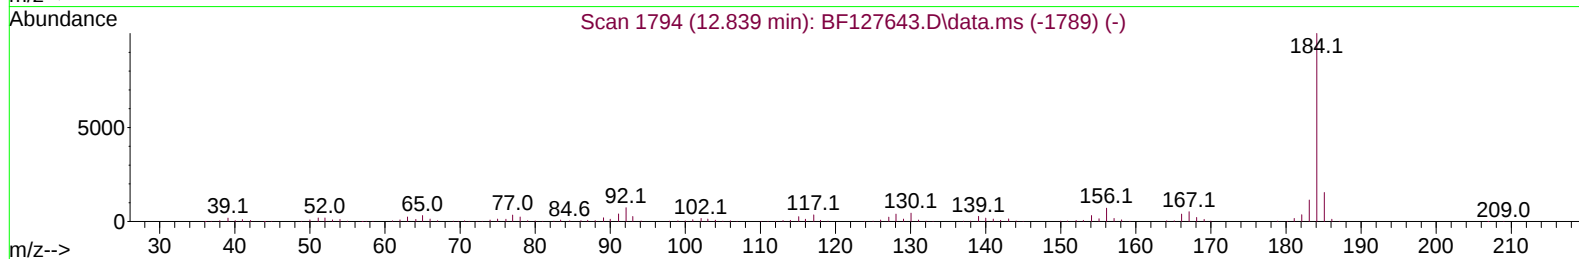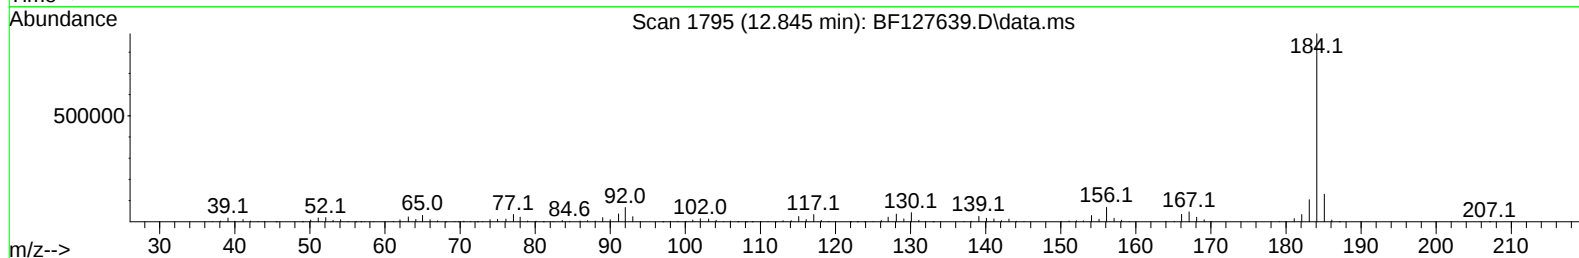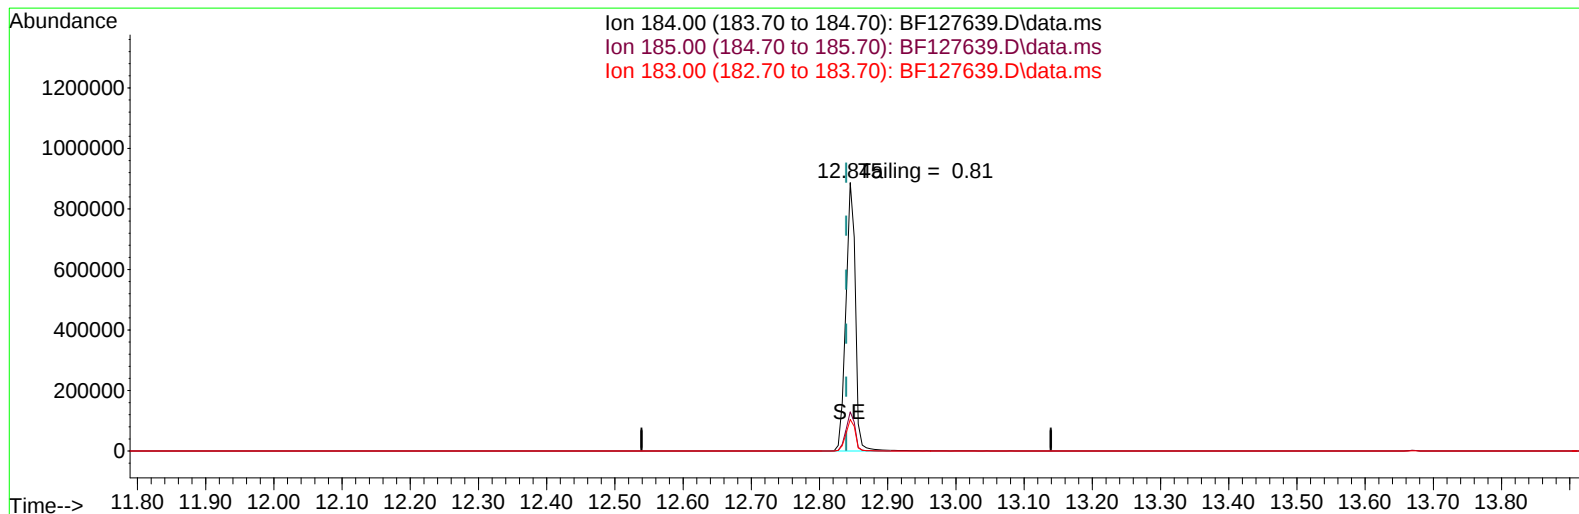

TIC: BF127639.D\data.ms

**(77) Benzidine**

12.845min (+ 0.006) 5638.61 ng m

response 856981

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 15.20  | 14.63  |
| 183.00 | 11.70  | 11.77  |
| 0.00   | 0.00   | 0.00   |