
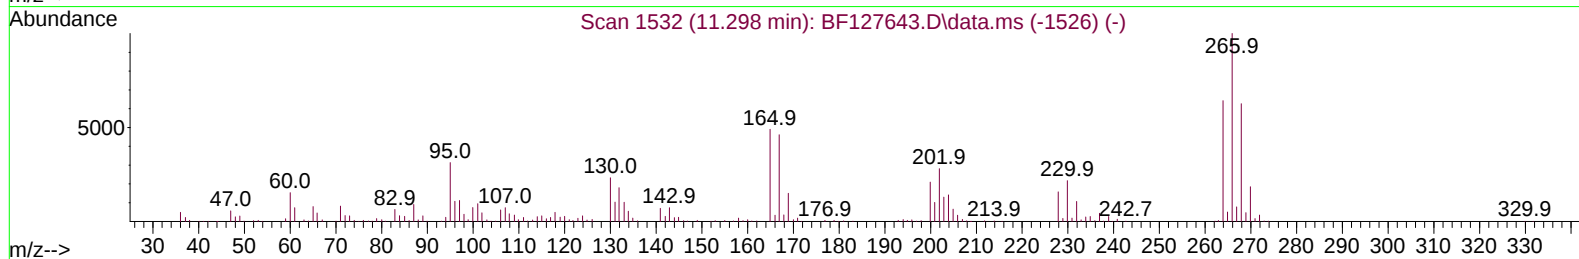
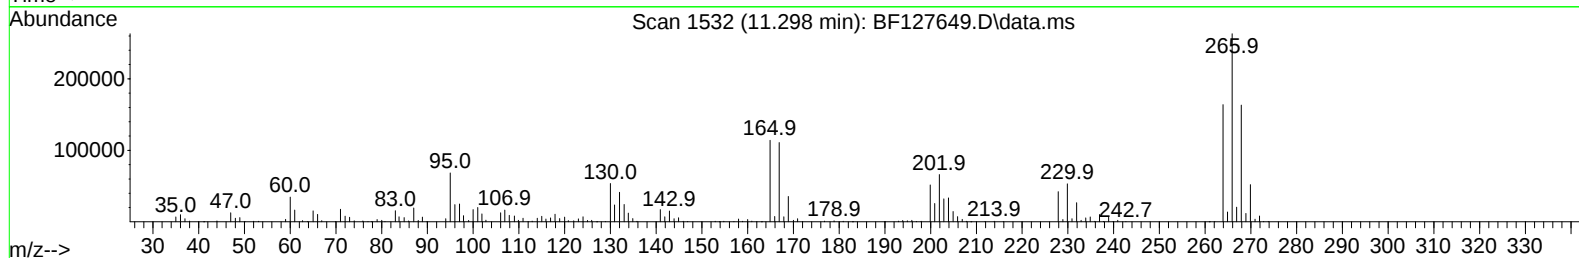


Quant Time: Apr 06 17:03:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 06 13:55:27 2022
Response via : Initial Calibration

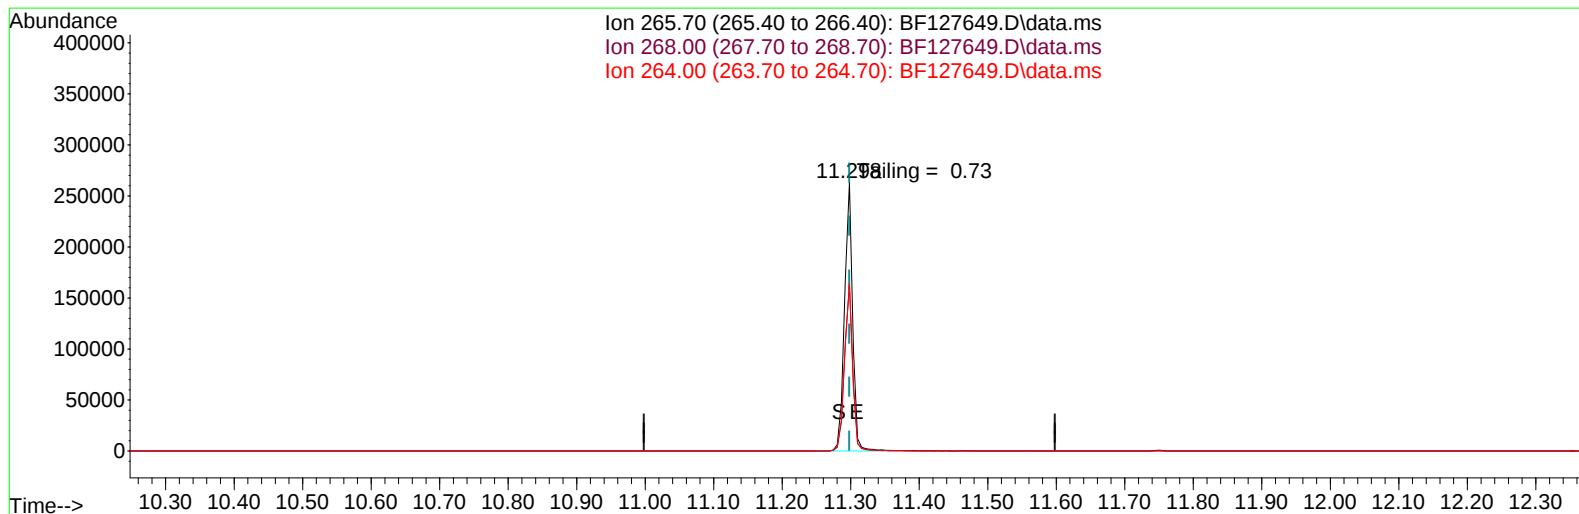

TIC: BF127649.D\data.ms

(70) Pentachlorophenol (C)




11.298min (+ 0.000) 472269.49 ng

response **217043**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	62.07
264.00	60.60	62.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040622\
Data File : BF127649.D
Acq On : 06 Apr 2022 15:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 06 17:03:54 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 06 13:55:27 2022
Response via : Initial Calibration

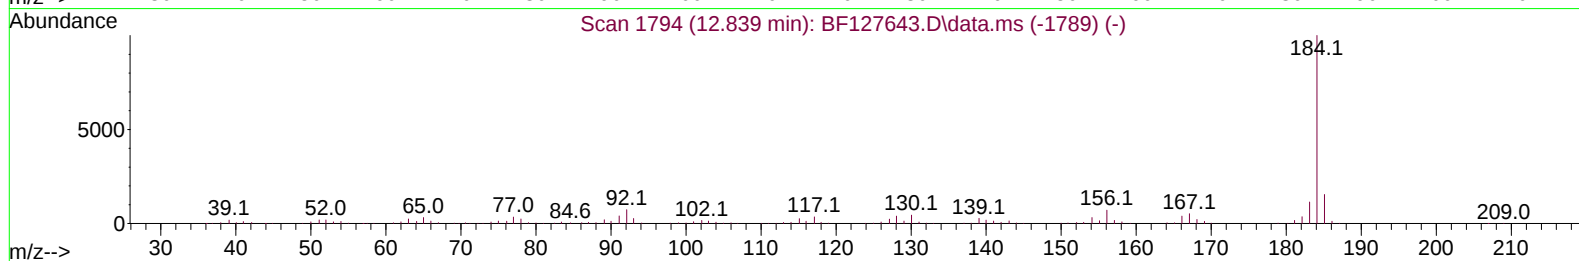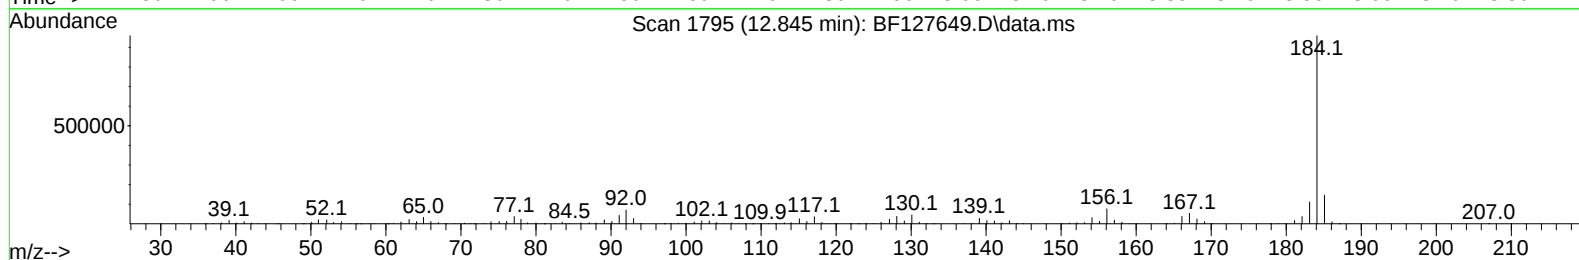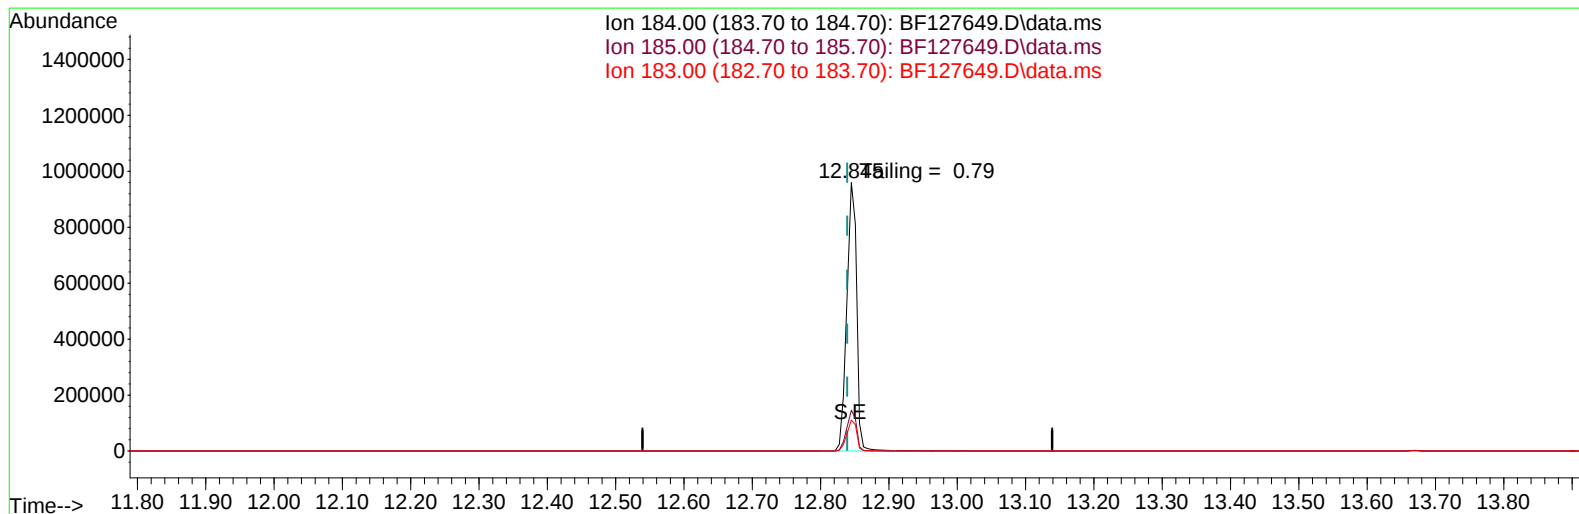

TIC: BF127649.D\data.ms

(77) Benzidine

12.845min (+ 0.006) 5151.18 ng m

response 957951

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	15.21
183.00	11.70	11.59
0.00	0.00	0.00