

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040622\
 Data File : BF127651.D
 Acq On : 06 Apr 2022 16:39
 Operator : CG\JU
 Sample : PB143833BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB143833BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127651.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.599	556	563	566	rBV	4082386	4744056	74.39%	12.451%
2	6.581	723	730	733	rBV	3720393	4976588	78.04%	13.061%
3	6.963	791	795	798	rBV	1199831	990742	15.54%	2.600%
4	7.528	884	891	894	rBV	2871089	3351612	52.55%	8.796%
5	8.245	1008	1013	1017	rVB	1278297	1292904	20.27%	3.393%
6	9.328	1190	1197	1200	rBV	5306221	6065874	95.12%	15.920%
7	10.010	1306	1313	1316	rBV	1578725	1534095	24.06%	4.026%
8	10.804	1440	1448	1451	rBV	3759254	4002867	62.77%	10.506%
9	11.504	1560	1567	1570	rBV	1742279	1616721	25.35%	4.243%
10	12.904	1802	1805	1809	rBV	164049	135120	2.12%	0.355%
11	13.098	1832	1838	1841	rBV	5660183	6377365	100.00%	16.738%
12	13.616	1923	1926	1930	rBV	123738	96729	1.52%	0.254%
13	14.151	2012	2017	2020	rBV	1505340	1326890	20.81%	3.482%
14	14.245	2026	2033	2041	rBV	208319	255474	4.01%	0.671%
15	15.304	2209	2213	2219	rBV	67163	78595	1.23%	0.206%
16	15.674	2270	2276	2280	rBV	760885	992193	15.56%	2.604%
17	15.716	2280	2283	2291	rVB	75756	102592	1.61%	0.269%
18	16.186	2358	2363	2371	rVB2	53135	81604	1.28%	0.214%
19	16.739	2450	2457	2463	rBV2	41518	79739	1.25%	0.209%

Sum of corrected areas: 38101760

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040622\
Data File : BF127651.D
Acq On : 06 Apr 2022 16:39
Operator : CG\JU
Sample : PB143833BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143833BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Hexadecanoic acid, butyl ester Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.904	2.04 ng	135120	Chrysene-d12	14.151

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexadecanoic acid, butyl ester	312	C20H40O2	000111-06-8	91
2			Hexadecanoic acid, 1,1-dimethyle...	312	C20H40O2	031158-91-5	83
3			Hexadecanoic acid, 2-methylpropy...	312	C20H40O2	000110-34-9	47
4			Cyclohexanol, 4-amino-, trans-	115	C6H13NO	027489-62-9	38
5			Cyclobutane, 1,1-dimethyl-2-octyl-	196	C14H28	062338-30-1	38

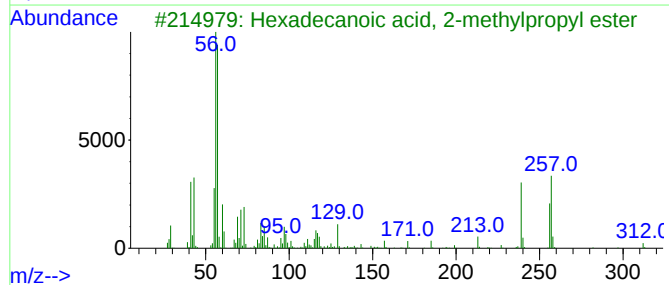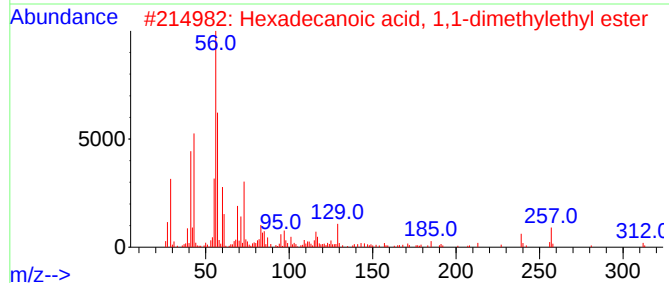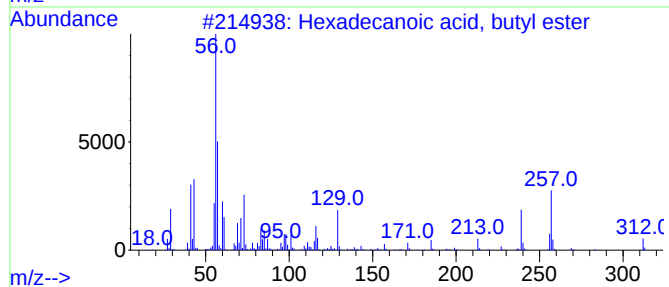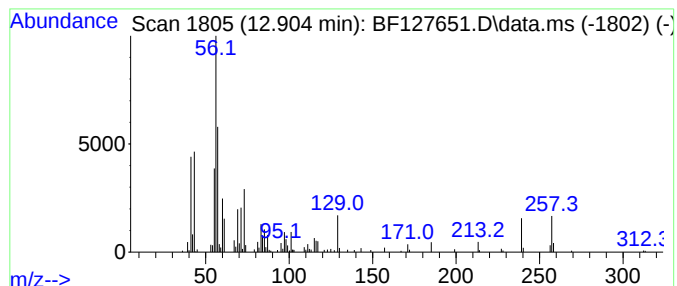

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040622\
Data File : BF127651.D
Acq On : 06 Apr 2022 16:39
Operator : CG\JU
Sample : PB143833BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143833BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Triphenylphosphine oxide Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.245	3.85 ng	255474	Chrysene-d12	14.151

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Triphenylphosphine oxide	278	C18H15OP	000791-28-6	93
2			(E)-7-Benzylidene-1-azabicyclo[3...]	293	C15H19NO3S	1000483-83-4	70
3			Formaldehyde, (triphenylphosphor...	304	C19H17N2P	015990-54-2	45
4			Carbazol-1-one, 1,2,3,4-tetrahyd...	277	C18H15NO2	299962-12-2	38
5			Cobalt,(.eta.<5>-2,4-cyclopentad...	277	C16H15BCo	036682-12-9	35

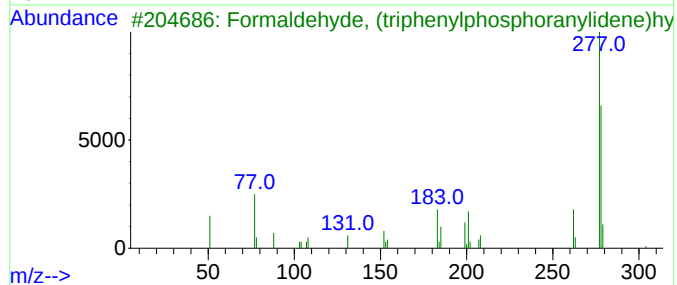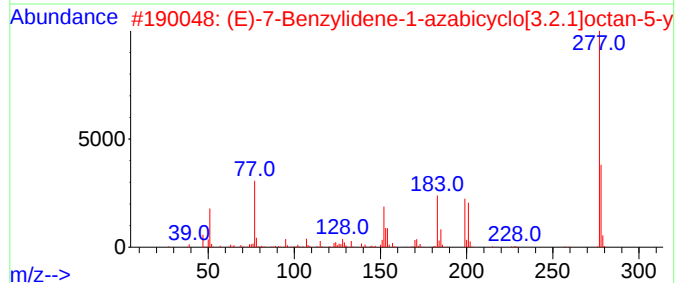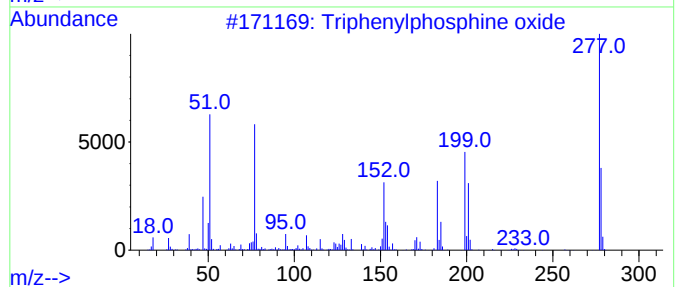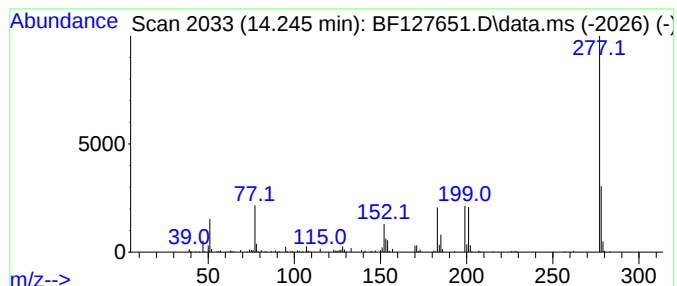

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040622\
Data File : BF127651.D
Acq On : 06 Apr 2022 16:39
Operator : CG\JU
Sample : PB143833BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB143833BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Hexadecanoic ac...	12.904	2.0	ng	135120	5	14.151	1326890	20.0
Triphenylphosph...	14.245	3.9	ng	255474	5	14.151	1326890	20.0