


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040622\
 Data File : BF127639.D
 Acq On : 06 Apr 2022 09:43
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Apr 06 13:55:27 2022

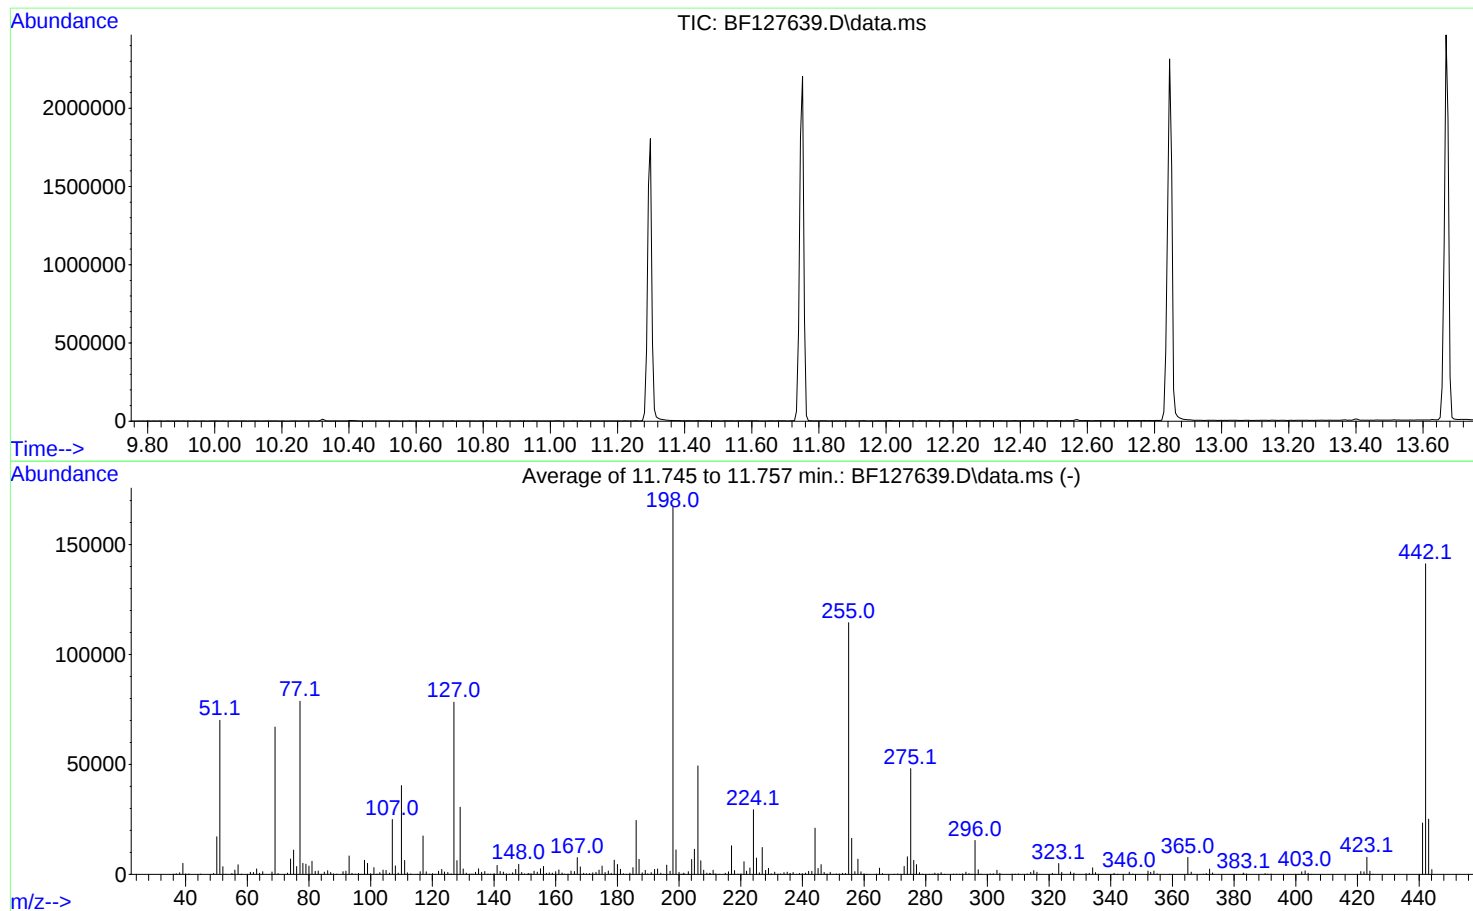




AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.9	70058	PASS
68	69	0.00	2	1.6	1096	PASS
69	198	0.00	100	40.1	67013	PASS
70	69	0.00	2	0.5	362	PASS
127	198	10	80	46.8	78291	PASS
197	198	0.00	2	0.9	1426	PASS
198	198	100	100	100.0	167299	PASS
199	198	5	9	6.7	11136	PASS
275	198	10	60	28.7	48080	PASS
365	198	1	100	4.6	7709	PASS
441	198	0.01	100	14.0	23392	PASS
442	442	50	100	100.0	141229	PASS
443	442	15	24	17.8	25091	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040622\
Data File : BF127639.D
Acq On : 06 Apr 2022 09:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 06 13:06:50 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 06 13:06:44 2022
Response via : Initial Calibration

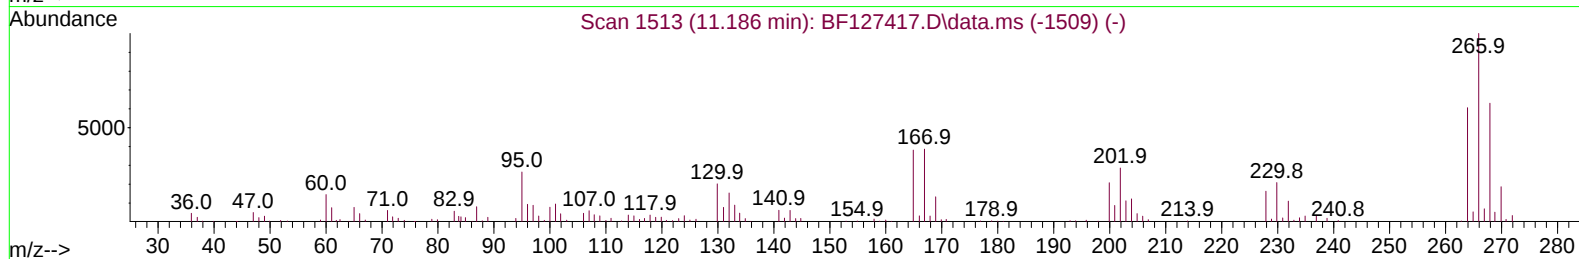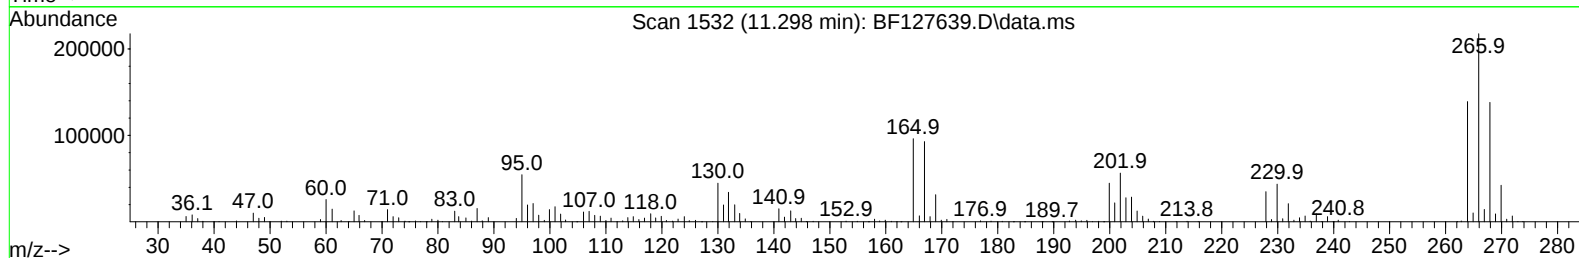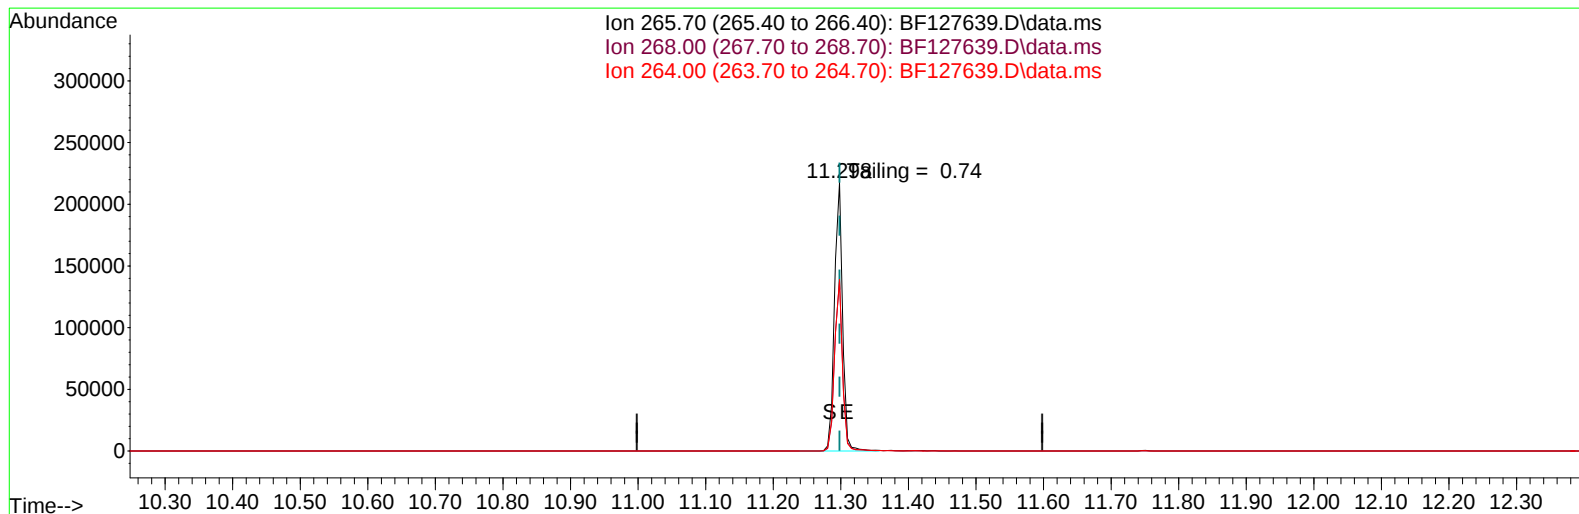

TIC: BF127639.D\data.ms

(70) Pentachlorophenol (C)

11.298min (0.000) 377428.56 ng




response 182284

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.00	63.52
264.00	60.60	63.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF040622\
Data File : BF127639.D
Acq On : 06 Apr 2022 09:43
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Apr 06 13:56:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF040622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Apr 06 13:55:27 2022
Response via : Initial Calibration

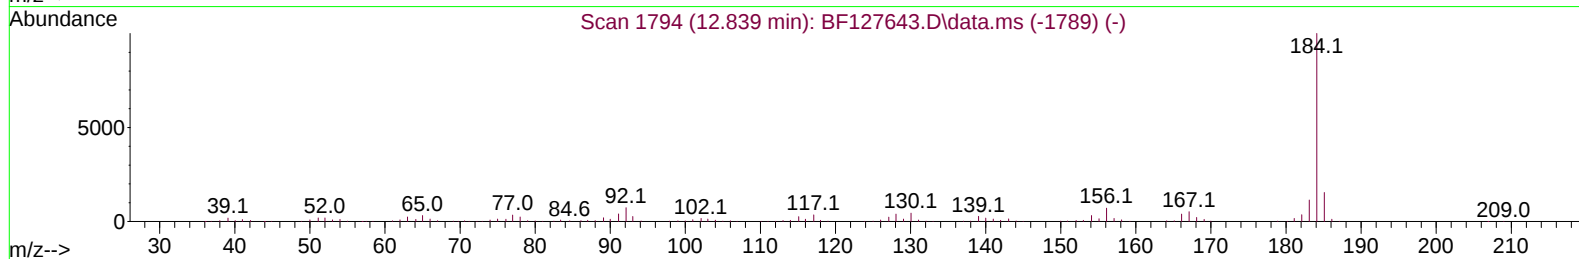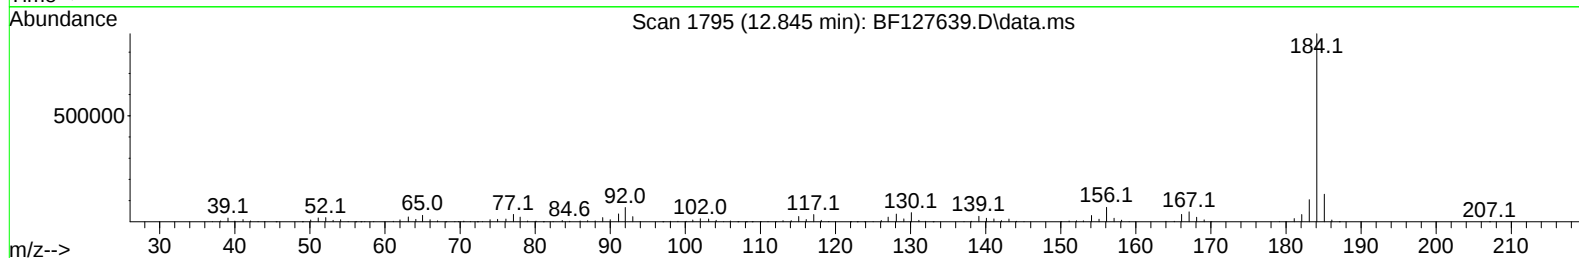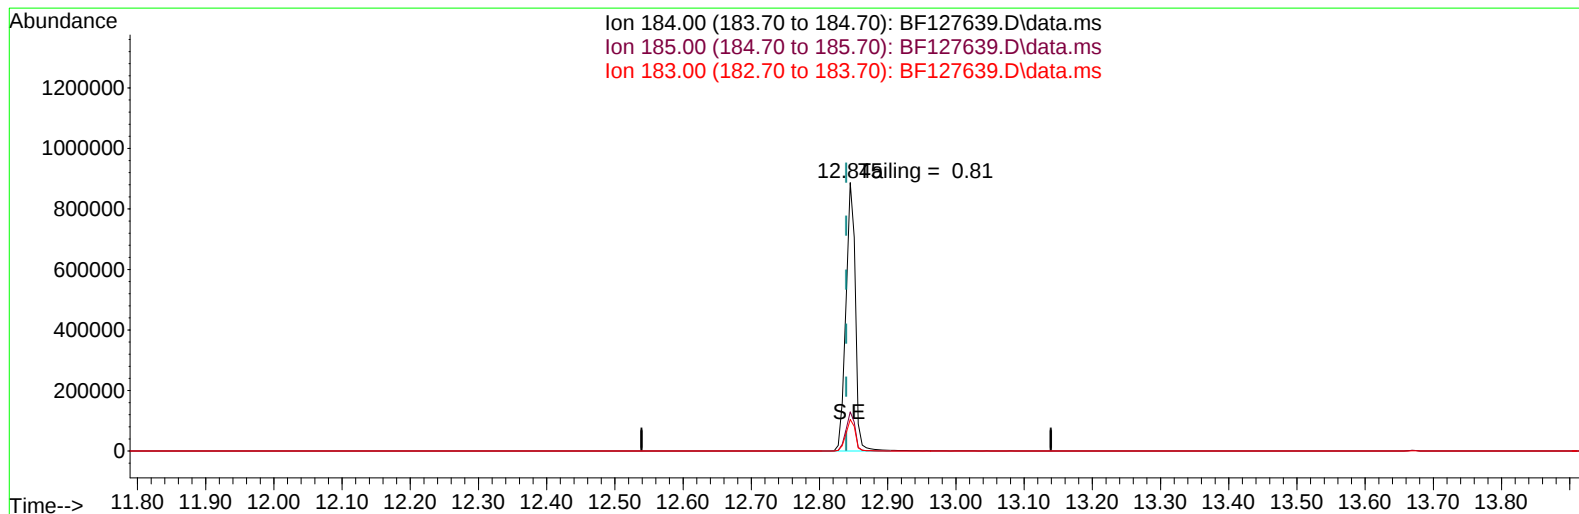

TIC: BF127639.D\data.ms

(77) Benzidine

12.845min (+ 0.006) 5638.61 ng m

response 856981

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.63
183.00	11.70	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
4/6/2022	BNA_F	<u>BF127639.D</u>
Compound Name	Response	Retention Time
DDT	394233	13.66
DDD	594	13.36
DDE	0	13.02
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
594	394827	0.15

Instrument :
BNA_F
ClientSampleId :
DFTPP