
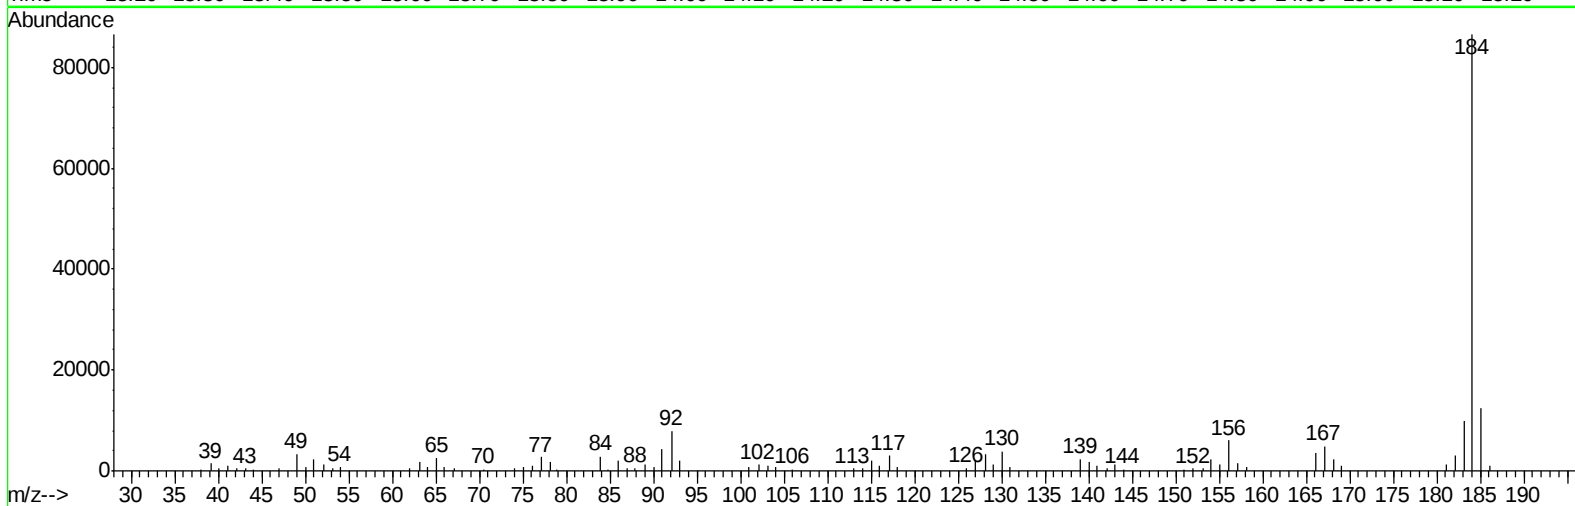


Data Path : Z:\HPCHEM1\BNA F\Data\BF040715\
Data File : BF078295.D
Acq On : 7 Apr 2015 12:33
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 07:11:39 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 03 14:42:25 2015
Response via : Initial Calibration

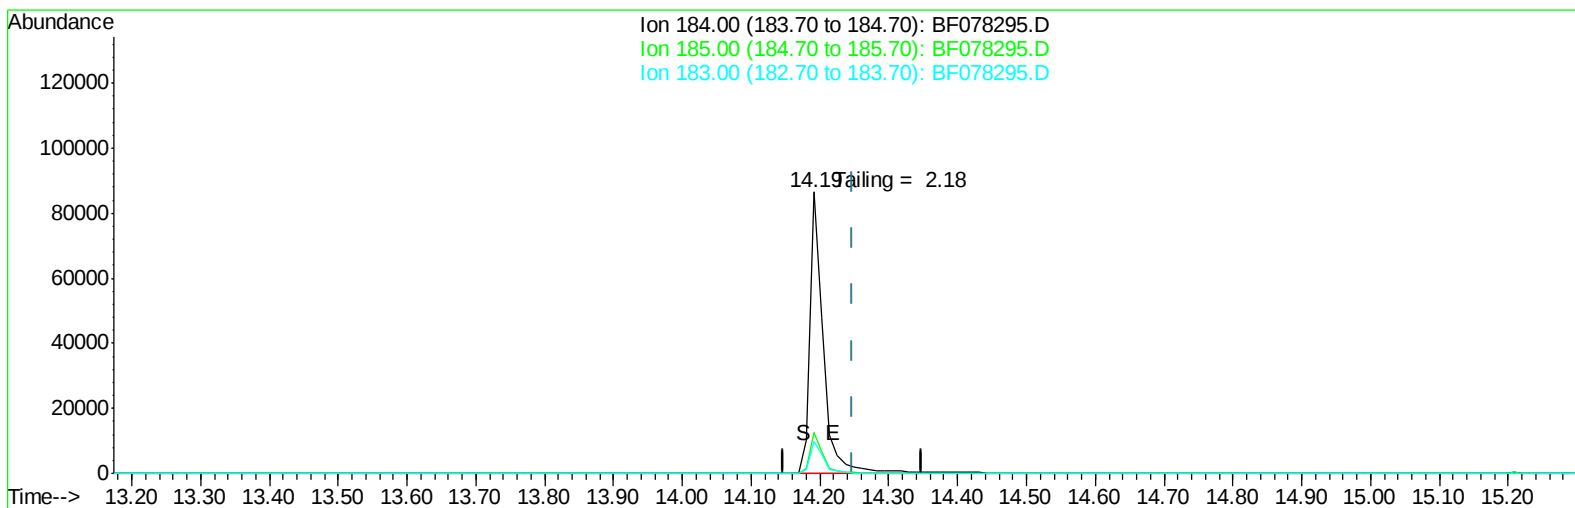

TIC: BF078295.D

(76) Benzidine



14.191min (-0.057) 0.00ng

response 117782

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.34
183.00	11.90	11.41
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF040715\
Data File : BF078295.D
Acq On : 7 Apr 2015 12:33
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 07:11:39 2015
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 03 14:42:25 2015
Response via : Initial Calibration

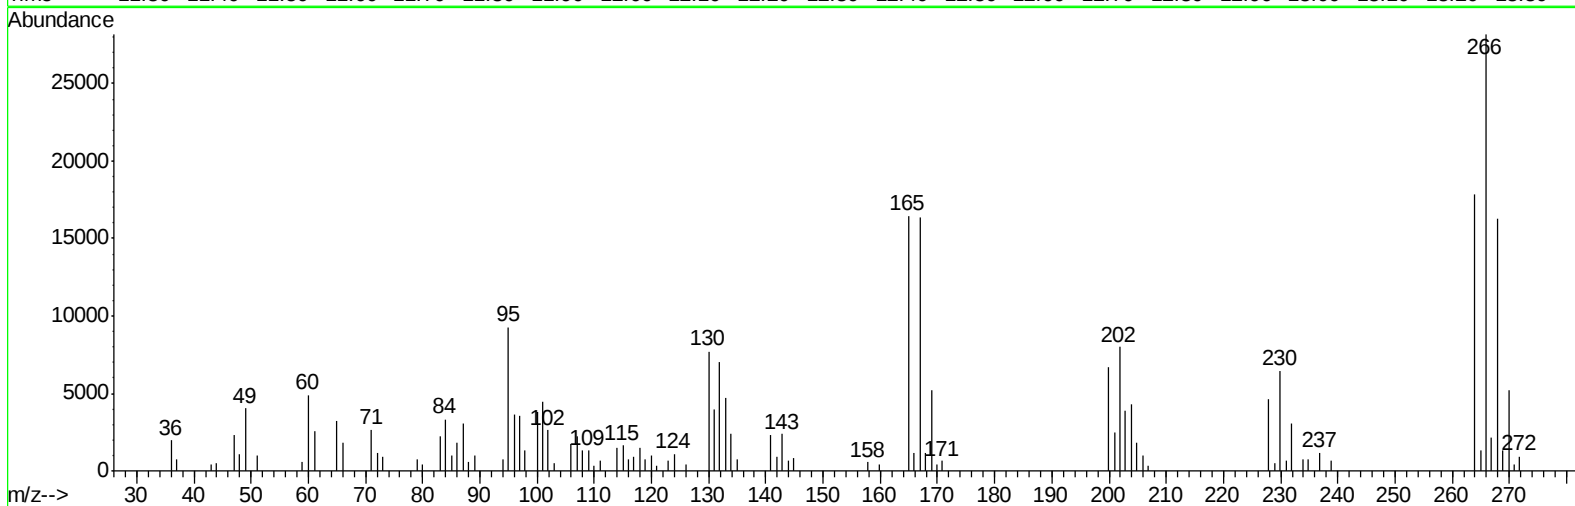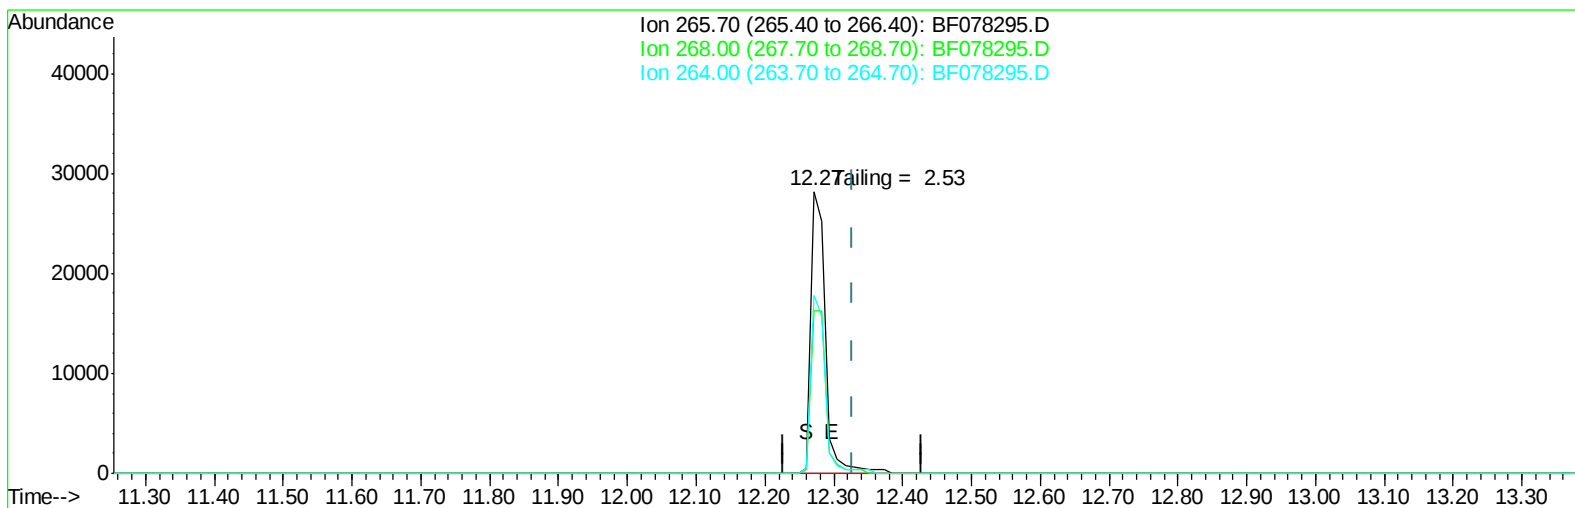

TIC: BF078295.D

(69) Pentachlorophenol (C)

12.271min (-0.057) 0.00ng

response 42454

Ion	Exp%	Act%
265.70	100	100
268.00	62.60	57.88
264.00	62.50	63.34
0.00	0.00	0.00