

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040715\
 Data File : BF078299.D
 Acq On : 7 Apr 2015 15:43
 Operator : TP/IZ
 Sample : G1784-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SVOC-GPC-BLANK

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.081	16	17	21	rVB3	5059	7723	2.04%	0.345%
2	1.207	25	28	30	rVB	48578	66583	17.62%	2.974%
3	1.344	39	40	45	rVB3	4383	4988	1.32%	0.223%
4	1.561	57	59	65	rVB3	2367	4562	1.21%	0.204%
5	1.664	65	68	83	rBV	160418	283878	75.13%	12.679%
6	6.933	526	529	531	rBV	173475	186431	49.34%	8.326%
7	8.510	664	667	669	rBV	269289	264096	69.90%	11.795%
8	10.614	849	851	854	rBV	6038	9936	2.63%	0.444%
9	10.671	854	856	859	rVB	341716	312719	82.77%	13.967%
10	12.499	1013	1016	1019	rBV	367523	332324	87.96%	14.842%
11	15.757	1299	1301	1304	rBV	259036	375043	99.26%	16.750%
12	16.306	1340	1349	1350	rBV4	873	3786	1.00%	0.169%
13	17.460	1447	1450	1453	rBV	275860	377827	100.00%	16.875%
14	17.860	1483	1485	1488	rBV4	1837	4424	1.17%	0.198%
15	19.586	1633	1636	1638	rBV3	2342	4709	1.25%	0.210%


Sum of corrected areas: 2239029

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040715\
Data File : BF078299.D
Acq On : 7 Apr 2015 15:43
Operator : TP/IZ
Sample : G1784-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

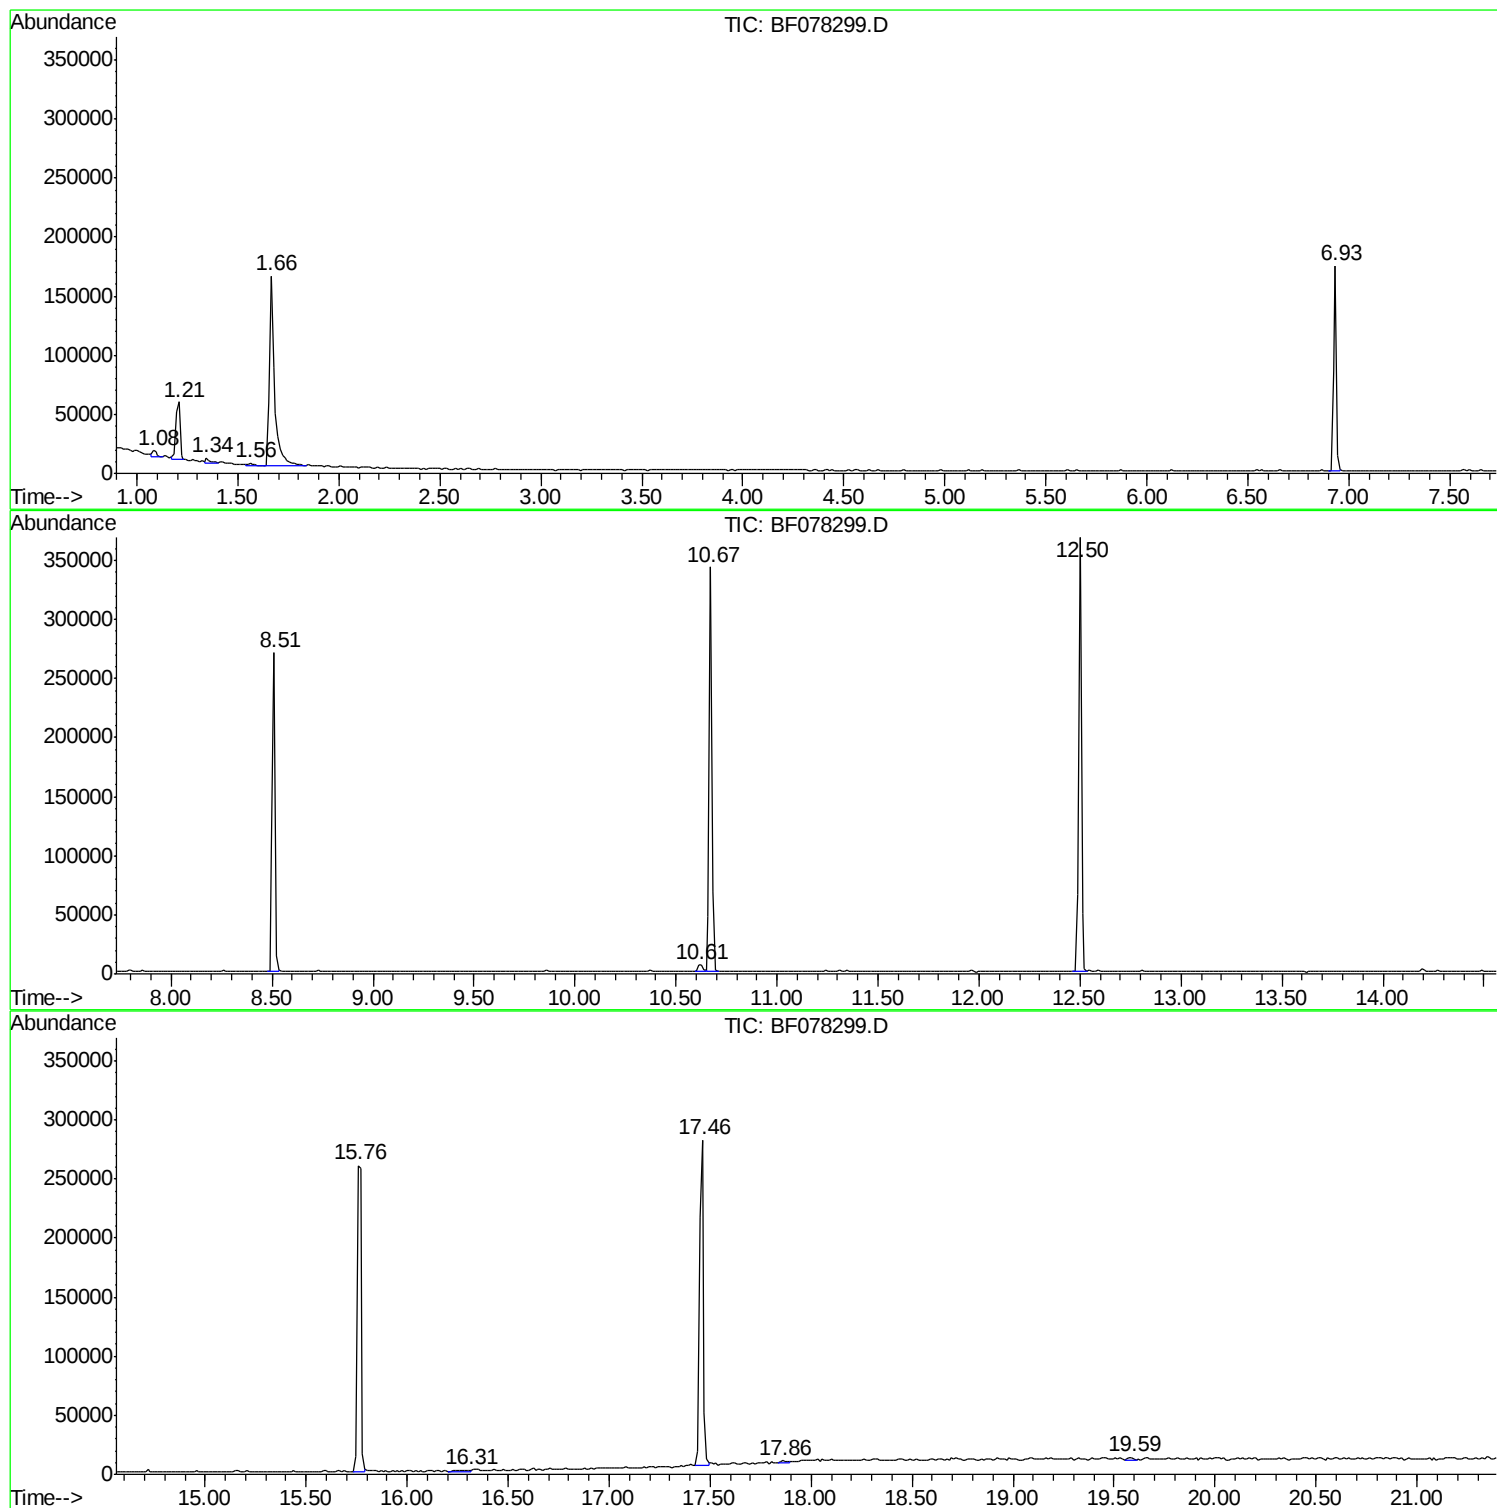

Data_Path : Z:\HPCHEM1\BNA_F\DATA\BF040715\
Data_File : BF078299.D
Acq_On : 7 Apr 2015 15:433
Operator : TP/IZZ
Sample : G1784-055
Misc :
ALS_Vial : 5 Sample_Multiplier: 11

Instrument :
BNA_F
ClientSampleId :
SVOC-GPC-BLANK

Quant_Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.MM
Quant_Title : ASP_BNA_STANDARDS_FOR_5_POINT_CALIBRATION.NN

TIC_Library : C:\DATABASE\NIST02.LL
TIC_Integration_Parameters: LSCINT.PP

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------

No Library Search Compounds Detected
