


Data Path : Z:\HPCHEM1\BNA F\Data\BF040715\
 Data File : BF078295.D
 Acq On : 7 Apr 2015 12:33
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 03 14:42:25 2015

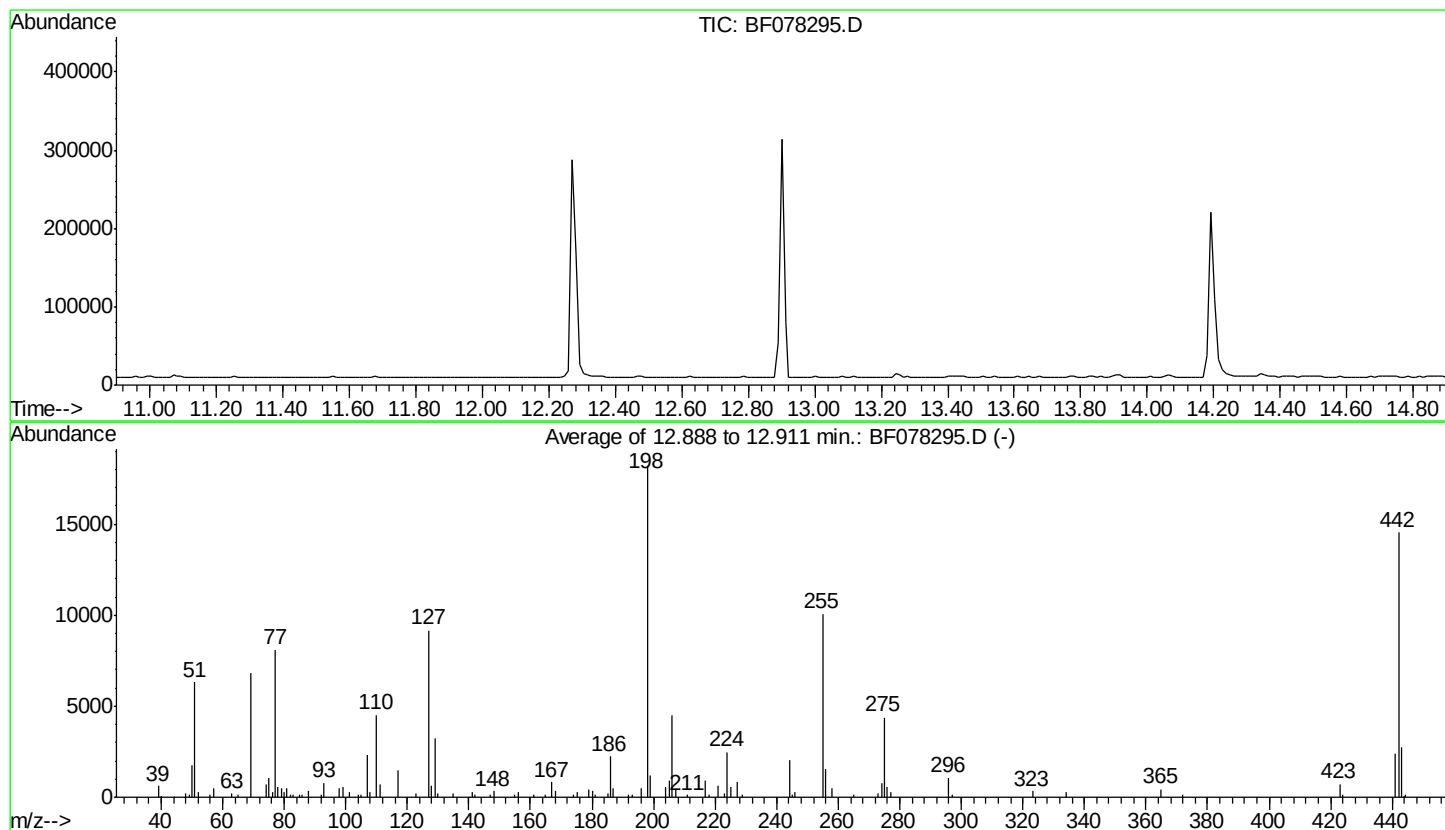

AutoFind: Scans 1050, 1051, 1052; Background Corrected with Scan 1047

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.6	6303	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.5	6828	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.2	9138	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	18209	PASS
199	198	5	9	6.5	1181	PASS
275	198	10	60	24.1	4391	PASS
365	198	1	100	2.3	425	PASS
441	442	0.01	24	16.6	2406	PASS
442	198	50	100	79.8	14537	PASS
443	442	15	24	19.1	2777	PASS