


Data Path : Z:\HPCHEM1\BNA F\Data\BF040715\
Data File : BF078317.D
Acq On : 8 Apr 2015 2:14
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040115.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Apr 03 14:42:25 2015

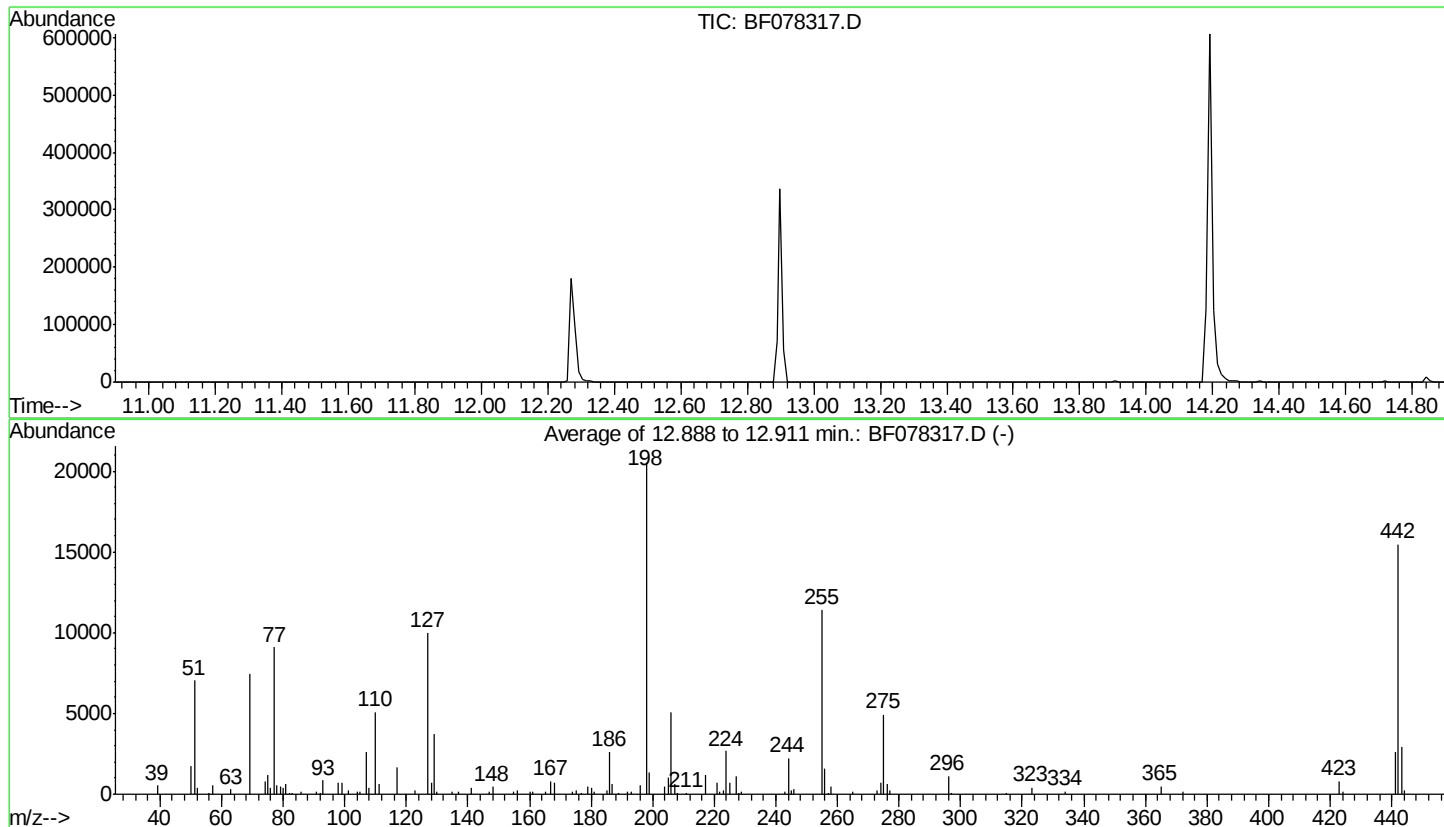

AutoFind: Scans 1050, 1051, 1052; Background Corrected with Scan 1047

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	7045	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	36.2	7422	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.8	10009	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	20525	PASS
199	198	5	9	6.6	1345	PASS
275	198	10	60	24.1	4946	PASS
365	198	1	100	2.4	487	PASS
441	442	0.01	24	17.1	2655	PASS
442	198	50	100	75.4	15485	PASS
443	442	15	24	19.1	2958	PASS