

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040716\
 Data File : BF086143.D
 Acq On : 7 Apr 2016 21:31
 Operator : UM/SJ
 Sample : H2230-11
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 RW-3-040116

Quant Time: Apr 08 01:43:23 2016
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 01 23:17:06 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	100610	20.00	ng	-0.03
21) Naphthalene-d8	8.02	136	410455	20.00	ng	-0.05
38) Acenaphthene-d10	9.77	164	186062	20.00	ng	-0.05
63) Phenanthrene-d10	11.25	188	369709	20.00	ng	-0.05
75) Chrysene-d12	13.89	240	276816	20.00	ng	-0.03
86) Perylene-d12	15.29	264	186440	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	364985	62.01	ng	-0.03
7) Phenol-d6	6.38	99	278048	37.19	ng	-0.03
23) Nitrobenzene-d5	7.31	82	691193	99.31	ng	-0.03
41) 2,4,6-Tribromophenol	10.57	330	282061	161.51	ng	-0.03
44) 2-Fluorobiphenyl	9.10	172	1142193	102.07	ng	-0.03
78) Terphenyl-d14	12.84	244	1079668	91.68	ng	-0.03
Target Compounds						
9) Benzaldehyde	6.50	77	13903	3.46	ng	# 78
15) Benzyl Alcohol	6.89	79	9783	2.02	ng	# 50
18) Hexachloroethane	7.30	117	44835	15.90	ng	# 1
19) n-Nitroso-di-n-propylamine	7.31	70	91432	19.73	ng	# 75
25) Isophorone	7.31	82	682174	49.65	ng	# 68
50) 2,6-Dinitrotoluene	9.77	165	25453	8.72	ng	# 22
53) 2,4-Dinitrophenol	9.93	184	410	2.32	ng	# 1
66) 4-Bromophenyl-phenylether	10.57	248	18617	4.93	ng	# 1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040716\
Data File : BF086143.D
Acq On : 7 Apr 2016 21:31
Operator : UM/SJ
Sample : H2230-11
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
RW-3-040116

Quant Time: Apr 08 01:43:23 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

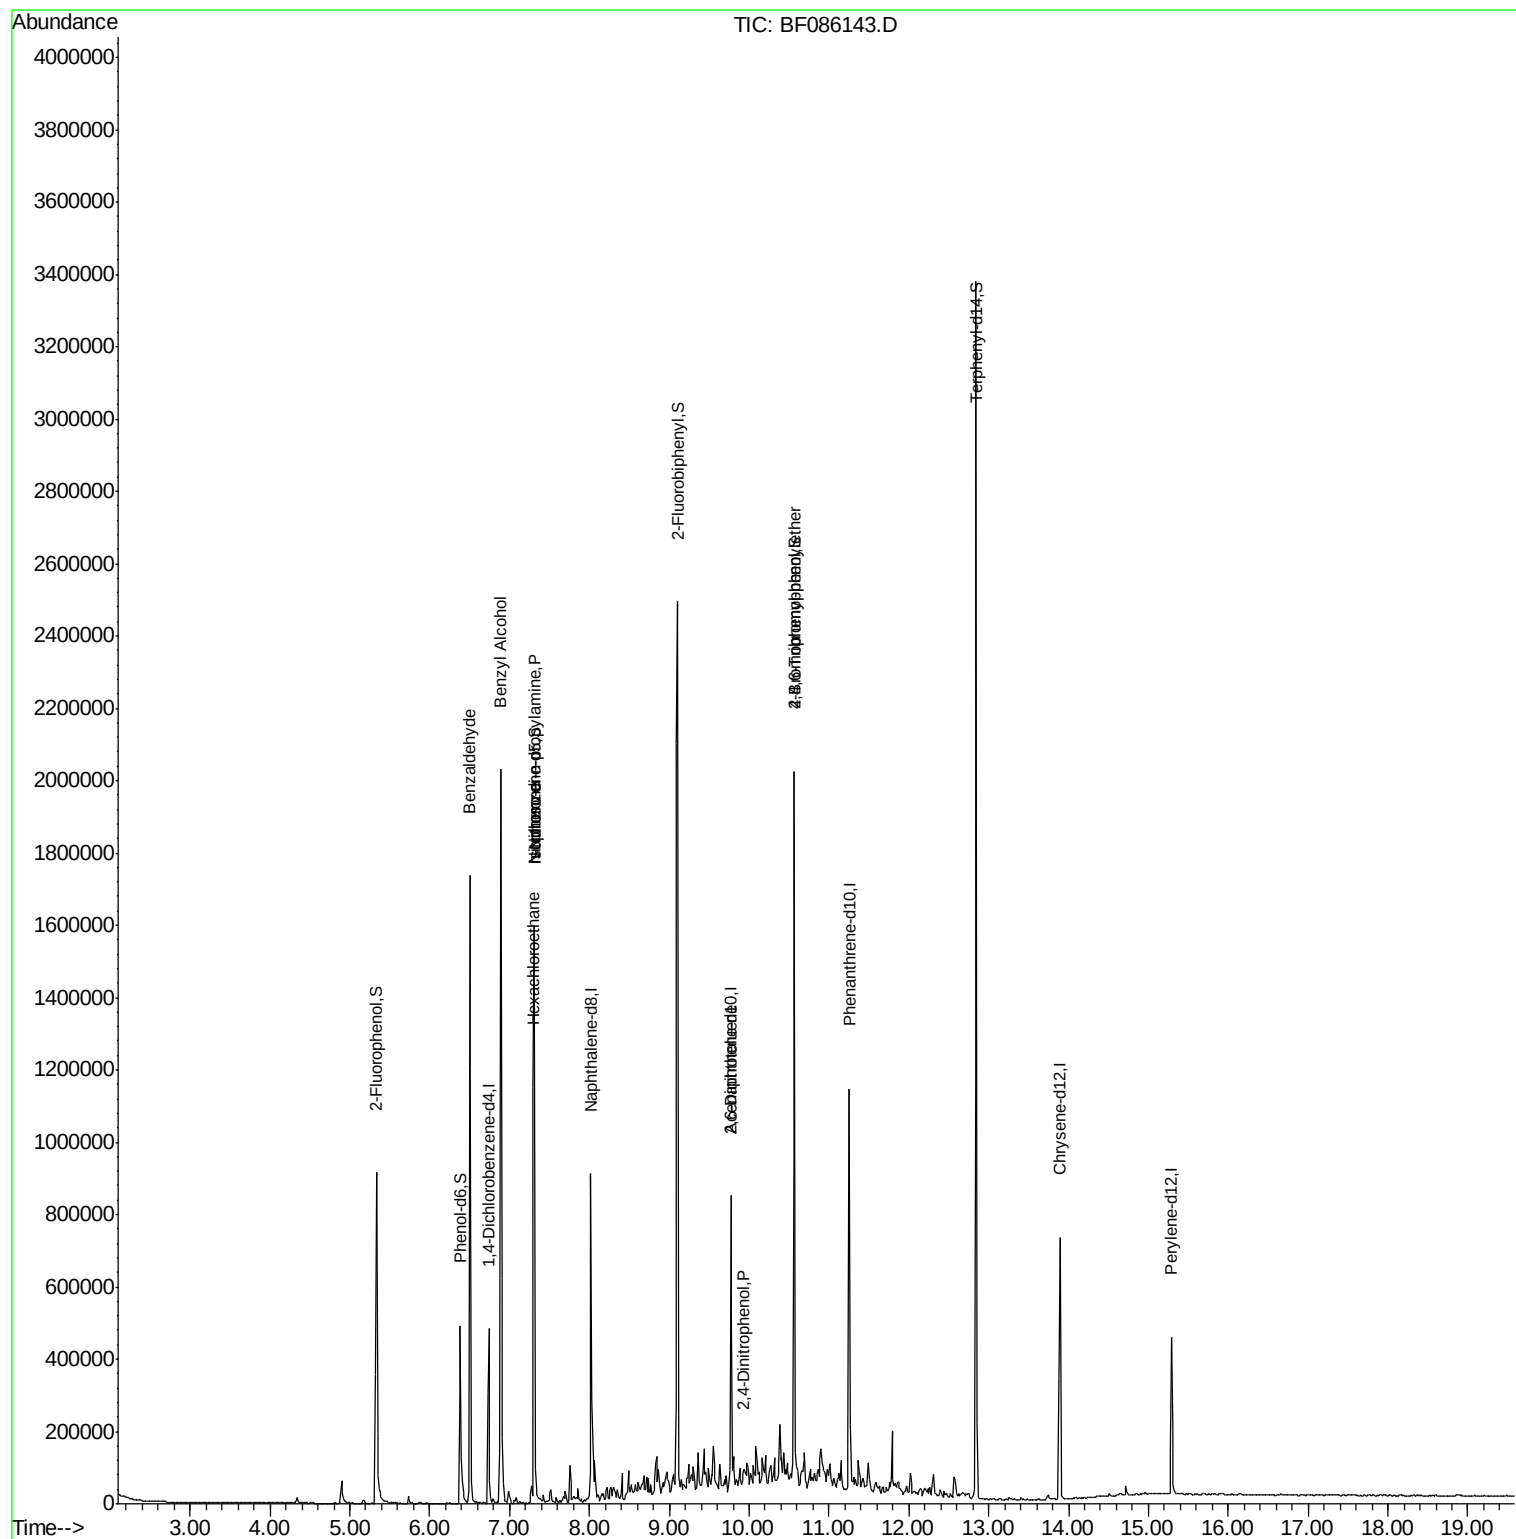







#1

1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.74 min Scan# 407
Delta R.T. -0.03 min
Lab File: BF086143.D
Acq: 7 Apr 2016 21:31

Instrument :
BNA_F
ClientSampleId :
RW-3-040116




Tgt Ion:152 Resp: 100610
Ion Ratio Lower Upper
152 100
150 151.4 124.2 186.2
115 56.2 47.0 70.6

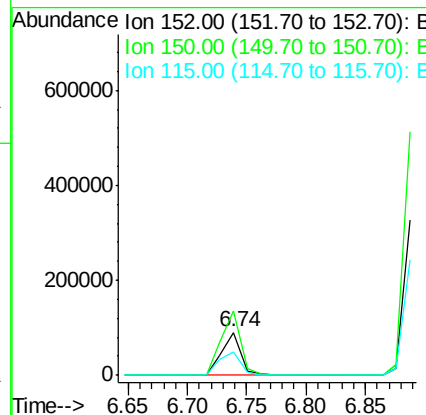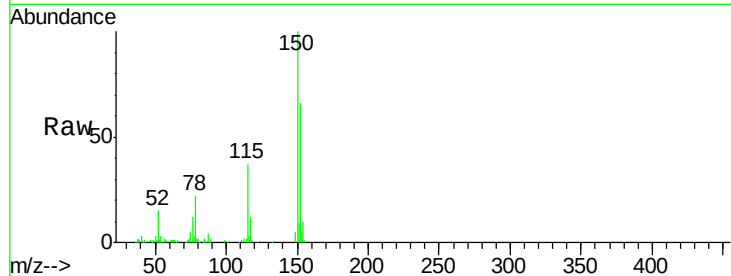


#5

2-Fluorophenol
Concen: 62.01 ng
RT: 5.33 min Scan# 284
Delta R.T. -0.03 min
Lab File: BF086143.D
Acq: 7 Apr 2016 21:31

Tgt Ion:112 Resp: 364985
Ion Ratio Lower Upper
112 100
64 48.9 39.9 59.9
63 24.8 20.2 30.2

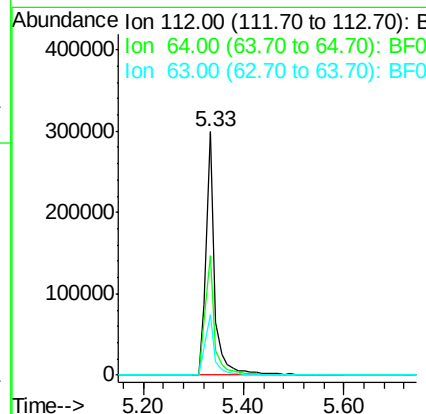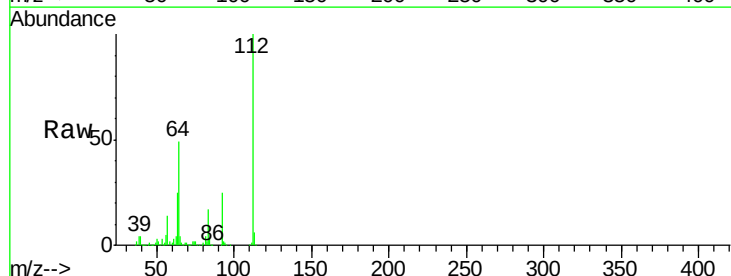

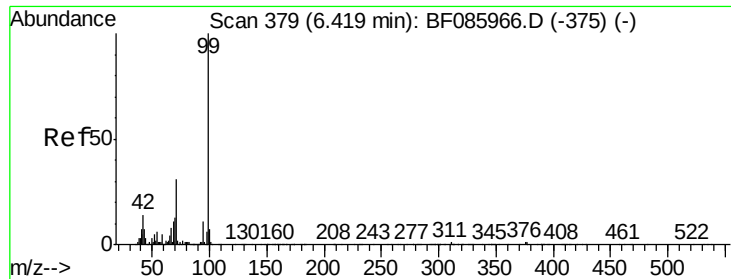

#7

Phenol-d6

Concen: 37.19 ng

RT: 6.38 min Scan# 376

Delta R.T. -0.03 min

Lab File: BF086143.D

Acq: 7 Apr 2016 21:31

Instrument :

BNA_F

ClientSampleId :

RW-3-040116


Tgt Ion: 99 Resp: 278048

Ion Ratio Lower Upper

99 100

42 12.7 11.1 16.7




71 28.8 24.9 37.3



Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

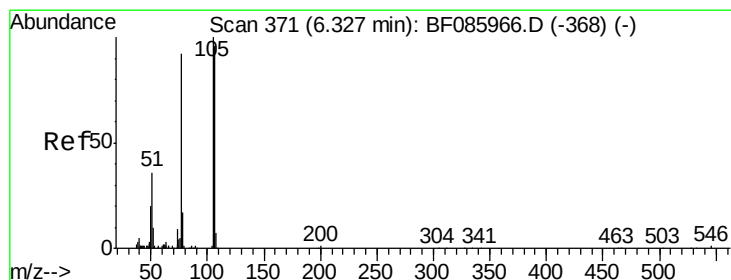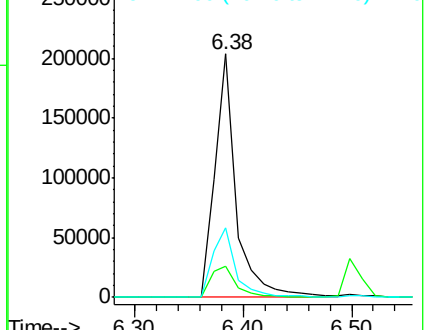

#9

Benzaldehyde

Concen: 3.46 ng

RT: 6.50 min Scan# 386

Delta R.T. 0.17 min

Lab File: BF086143.D

Acq: 7 Apr 2016 21:31


Tgt Ion: 77 Resp: 13903

Ion Ratio Lower Upper

77 100

105 78.0 80.1 120.1#



106 74.4 75.0 115.0#

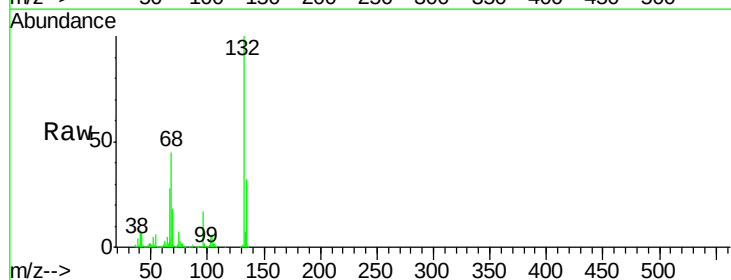


Abundance Ion 77.00 (76.70 to 77.70): BF0

Ion 105.00 (104.70 to 105.70): BF0

Ion 106.00 (105.70 to 106.70): BF0



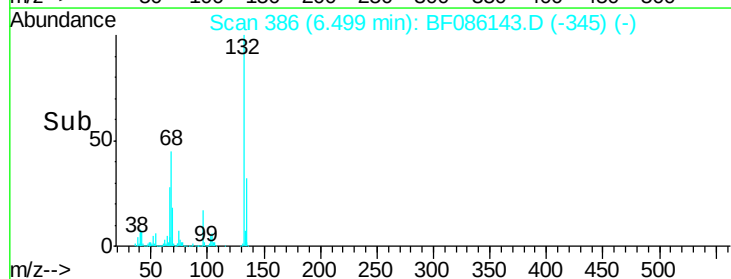
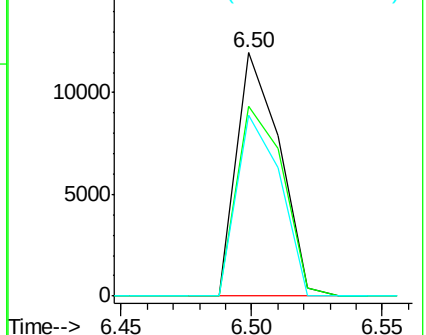


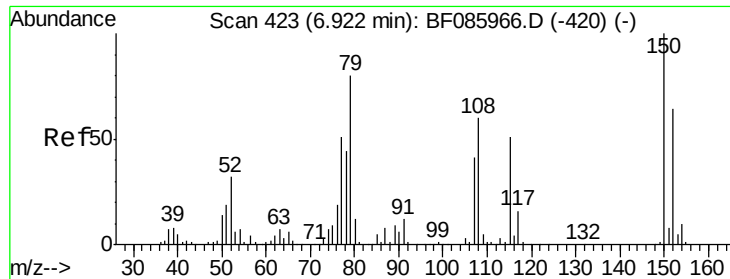

#15
Benzyl Alcohol
Concen: 2.02 ng
RT: 6.89 min Scan# 420
Delta R.T. -0.03 min
Lab File: BF086143.D
Acq: 7 Apr 2016 21:31




Instrument :
BNA_F
ClientSampleId :
RW-3-040116


Tgt Ion: 79 Resp: 9783
Ion Ratio Lower Upper
79 100
108 32.4 61.8 92.6#
77 98.0 49.6 74.4#

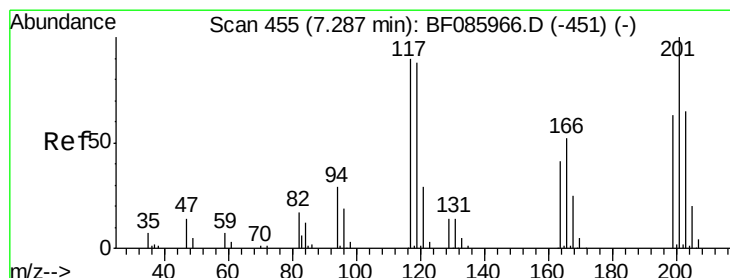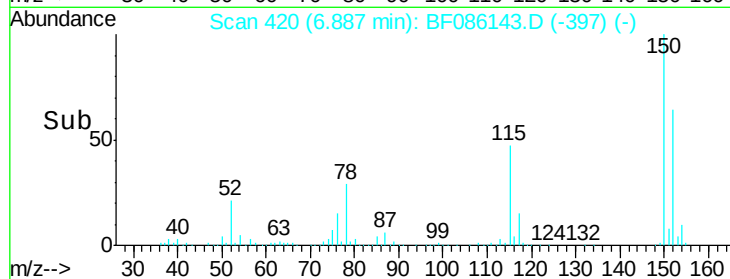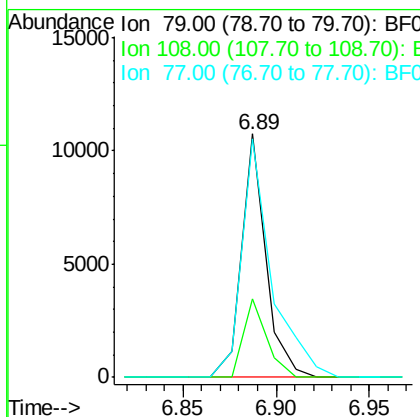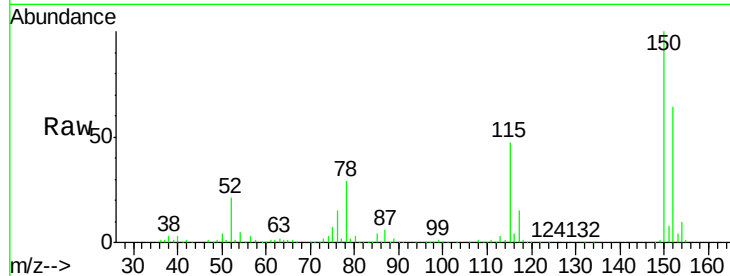

#18
Hexachloroethane
Concen: 15.90 ng
RT: 7.30 min Scan# 456
Delta R.T. 0.01 min
Lab File: BF086143.D
Acq: 7 Apr 2016 21:31

Tgt Ion: 117 Resp: 44835
Ion Ratio Lower Upper
117 100
119 1.0 76.7 115.1#
201 0.0 83.3 124.9#


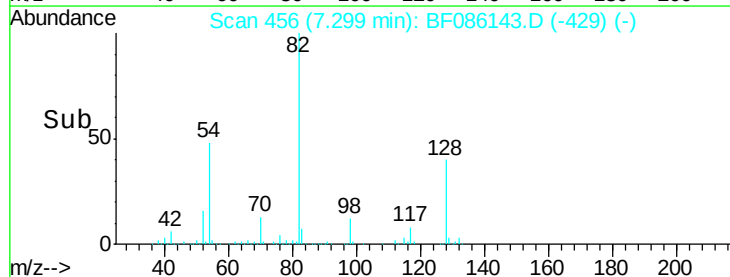
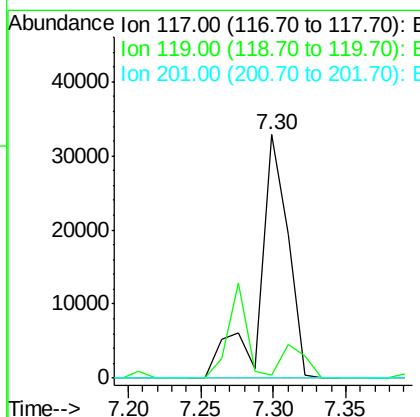
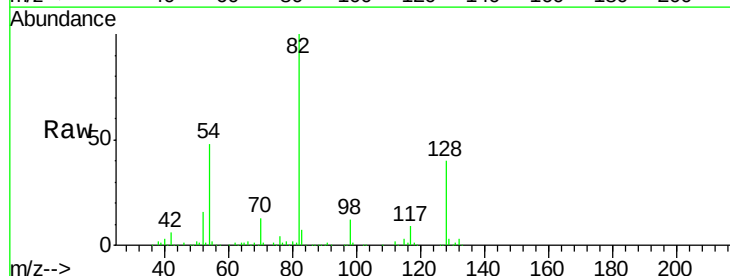




#19
 n-Nitroso-di-n-propylamine
 Concen: 19.73 ng
 RT: 7.31 min Scan# 457
 Delta R.T. 0.11 min
 Lab File: BF086143.D
 Acq: 7 Apr 2016 21:31




Instrument :
 BNA_F
 ClientSampleId :
 RW-3-040116


Tgt Ion: 70 Resp: 91432
 Ion Ratio Lower Upper
 70 100
 42 37.1 37.1 55.7#
 101 0.0 8.6 12.8#
 130 3.0 19.6 29.4#

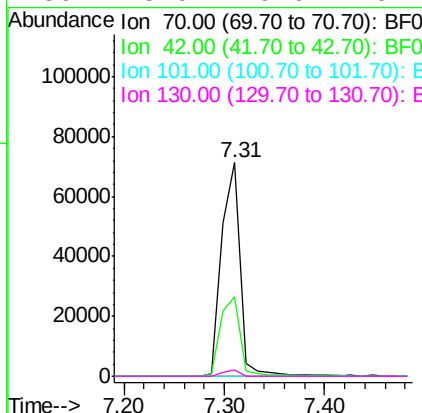

#21
 Naphthalene-d8
 Concen: 20.00 ng
 RT: 8.02 min Scan# 519
 Delta R.T. -0.05 min
 Lab File: BF086143.D
 Acq: 7 Apr 2016 21:31

Tgt Ion: 136 Resp: 410455
 Ion Ratio Lower Upper
 136 100
 137 10.9 9.1 13.7
 54 7.8 7.4 11.0
 68 6.6 5.8 8.8


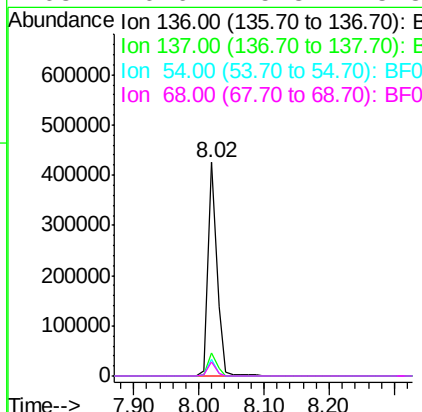




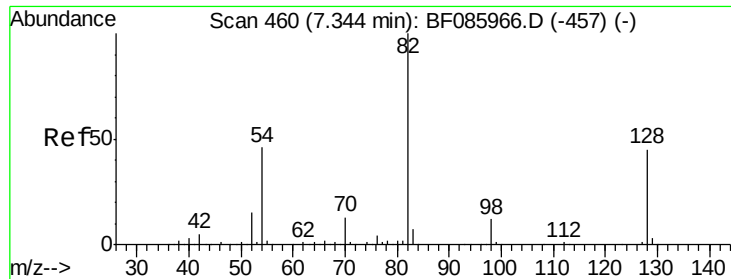

#23
 Nitrobenzene-d5
 Concen: 99.31 ng
 RT: 7.31 min Scan# 457
 Delta R.T. -0.03 min
 Lab File: BF086143.D
 Acq: 7 Apr 2016 21:31




Instrument :
 BNA_F
 ClientSampleId :
 RW-3-040116


Tgt Ion: 82 Resp: 691193
 Ion Ratio Lower Upper
 82 100
 128 51.1 41.8 62.8
 54 41.7 33.4 50.0

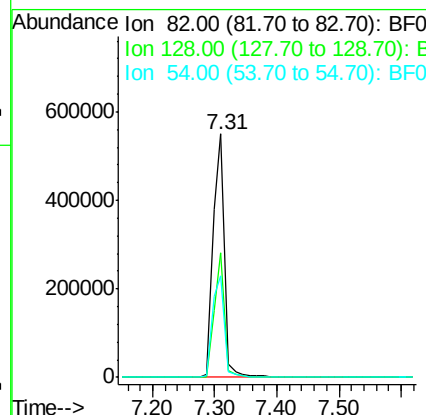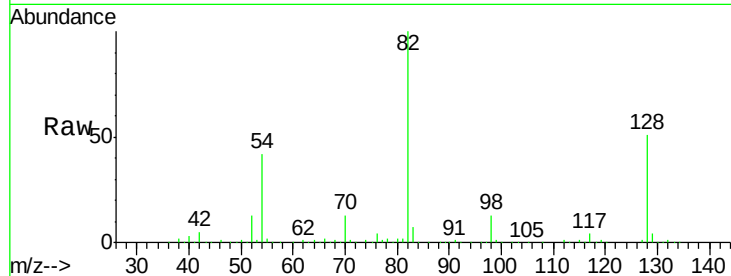

#25
 Isophorone
 Concen: 49.65 ng
 RT: 7.31 min Scan# 457
 Delta R.T. -0.30 min
 Lab File: BF086143.D
 Acq: 7 Apr 2016 21:31

Tgt Ion: 82 Resp: 682174
 Ion Ratio Lower Upper
 82 100
 95 0.0 5.4 8.2#
 138 0.0 12.9 19.3#

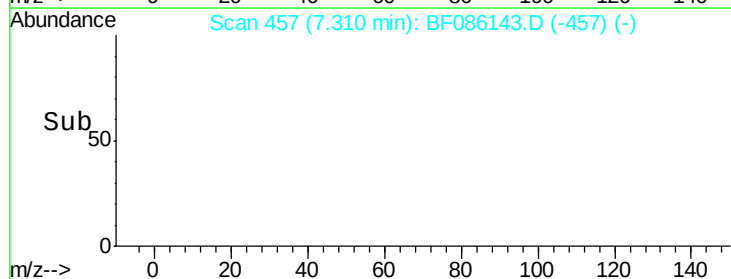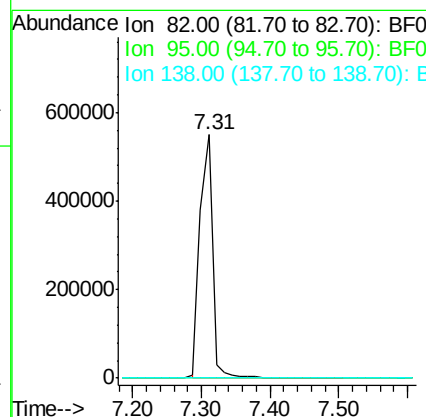

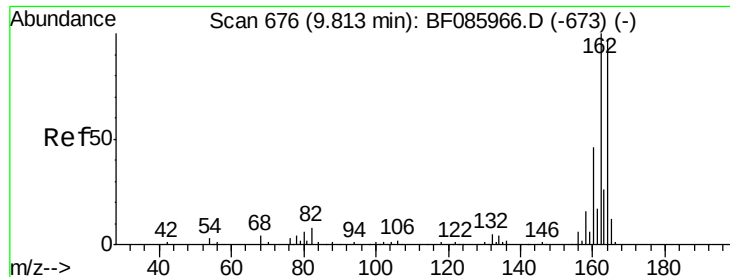

#38

Acenaphthene-d10

Concen: 20.00 ng

RT: 9.77 min Scan# 672

Delta R.T. -0.05 min

Lab File: BF086143.D

Acq: 7 Apr 2016 21:31

Instrument :

BNA_F

ClientSampleId :

RW-3-040116


Tgt Ion:164 Resp: 186062

Ion Ratio Lower Upper

164 100

162 100.9 82.1 123.1




160 47.3 37.4 56.2

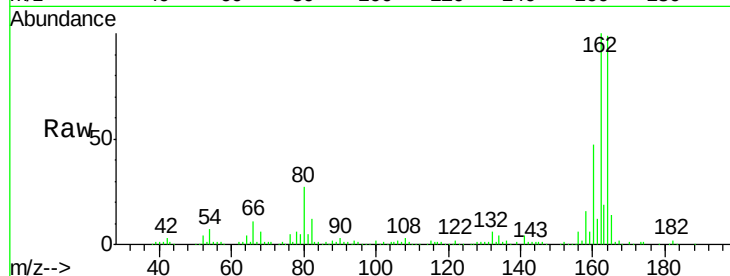

Abundance Ion 164.00 (163.70 to 164.70): E

Ion 162.00 (161.70 to 162.70): E

Ion 160.00 (159.70 to 160.70): E

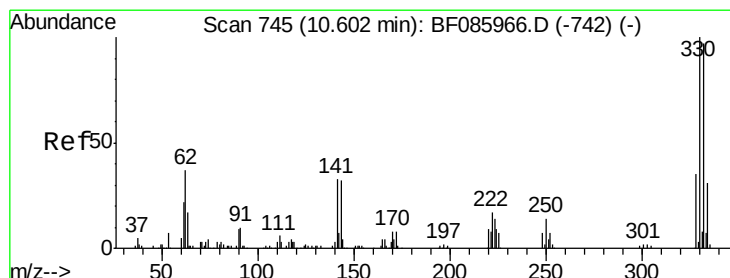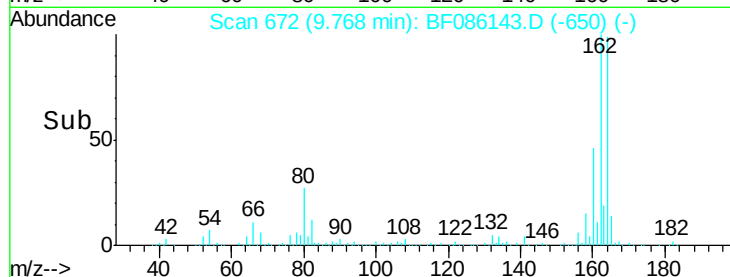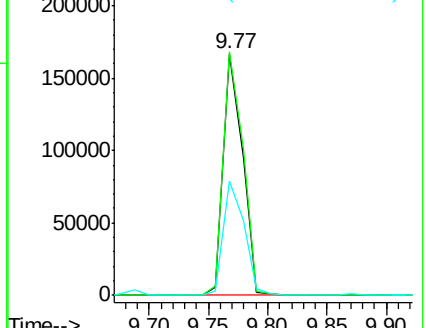

#41

2,4,6-Tribromophenol

Concen: 161.51 ng

RT: 10.57 min Scan# 742

Delta R.T. -0.03 min

Lab File: BF086143.D

Acq: 7 Apr 2016 21:31


Tgt Ion:330 Resp: 282061

Ion Ratio Lower Upper

330 100

332 95.0 78.2 117.2



141 33.2 31.5 47.3

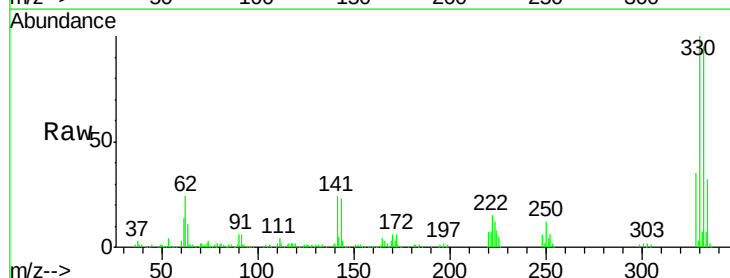


Abundance Ion 329.80 (329.50 to 330.50): E

Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

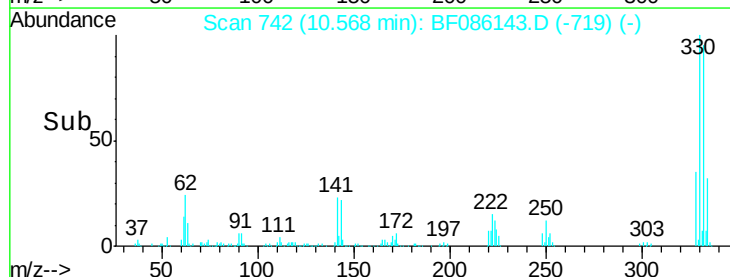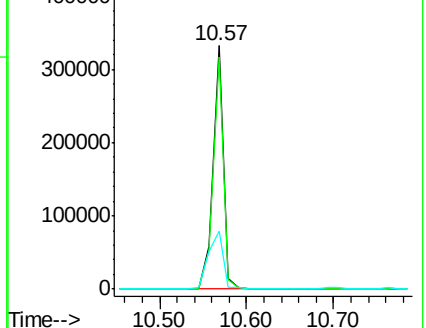

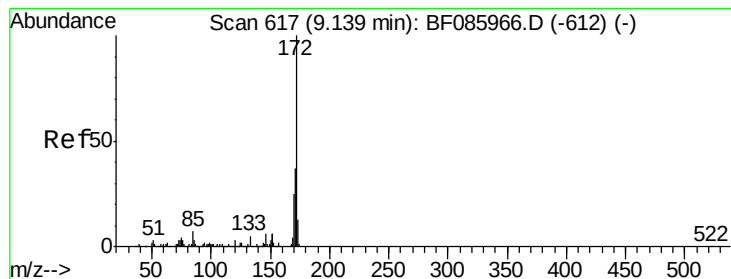

#44

2-Fluorobiphenyl

Concen: 102.07 ng

RT: 9.10 min Scan# 614

Delta R.T. -0.03 min

Lab File: BF086143.D

Acq: 7 Apr 2016 21:31

Instrument :

BNA_F

ClientSampleId :

RW-3-040116


Tgt Ion:172 Resp: 1142193

Ion Ratio Lower Upper

172 100

171 35.8 29.4 44.2




170 23.8 19.8 29.6



Abundance Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

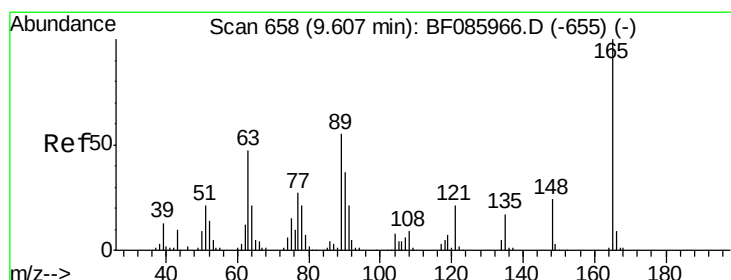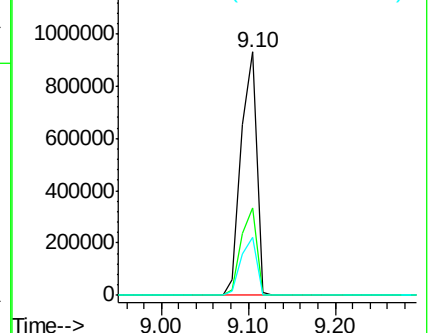

#50

2,6-Dinitrotoluene

Concen: 8.72 ng

RT: 9.77 min Scan# 672

Delta R.T. 0.16 min

Lab File: BF086143.D

Acq: 7 Apr 2016 21:31


Tgt Ion:165 Resp: 25453

Ion Ratio Lower Upper

165 100

63 4.1 51.8 77.8#



89 4.6 53.7 80.5#




Abundance Ion 165.00 (164.70 to 165.70): E

Ion 63.00 (62.70 to 63.70): BF0

Ion 89.00 (88.70 to 89.70): BF0



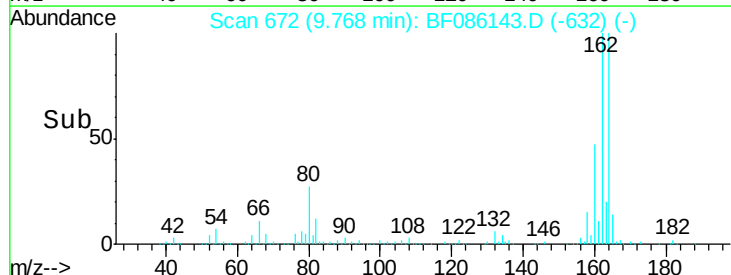
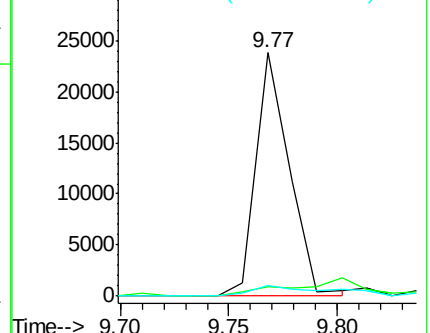


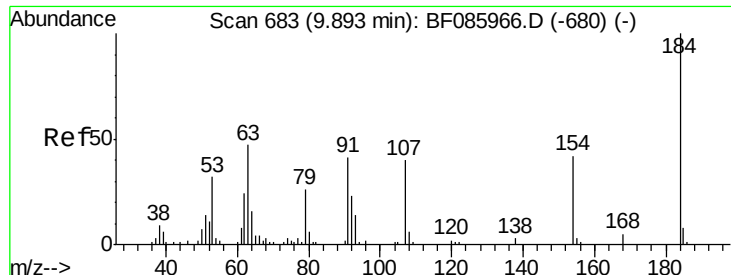

#53
 2,4-Dinitrophenol
 Concen: 2.32 ng
 RT: 9.93 min Scan# 686
 Delta R.T. 0.03 min
 Lab File: BF086143.D
 Acq: 7 Apr 2016 21:31




Instrument :
 BNA_F
 ClientSampleId :
 RW-3-040116


Tgt Ion:184 Resp: 410
 Ion Ratio Lower Upper
 184 100
 63 110.9 69.5 104.3#
 154 280.4 58.3 87.5#

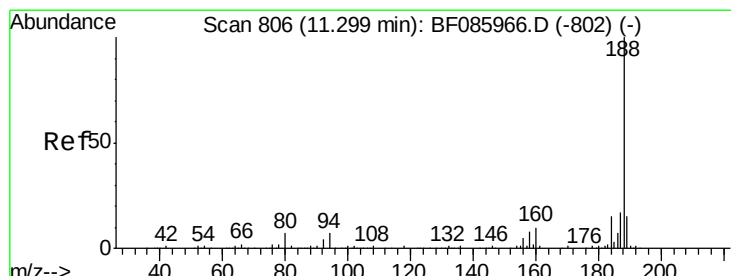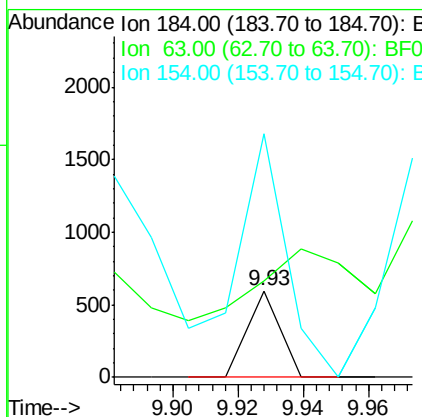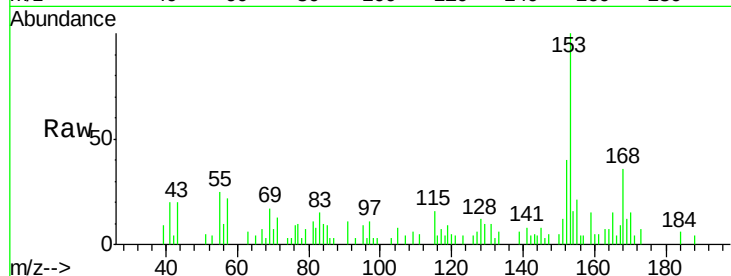

#63
 Phenanthrene-d10
 Concen: 20.00 ng
 RT: 11.25 min Scan# 802
 Delta R.T. -0.05 min
 Lab File: BF086143.D
 Acq: 7 Apr 2016 21:31

Tgt Ion:188 Resp: 369709
 Ion Ratio Lower Upper
 188 100
 94 10.8 5.4 8.0#
 80 11.3 5.5 8.3#

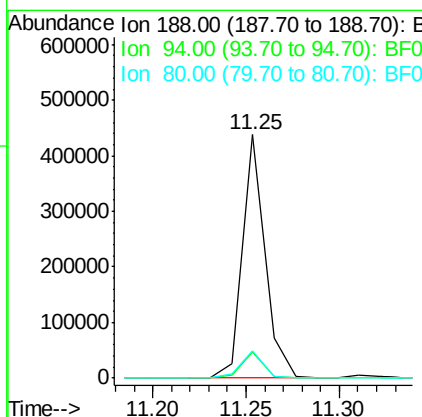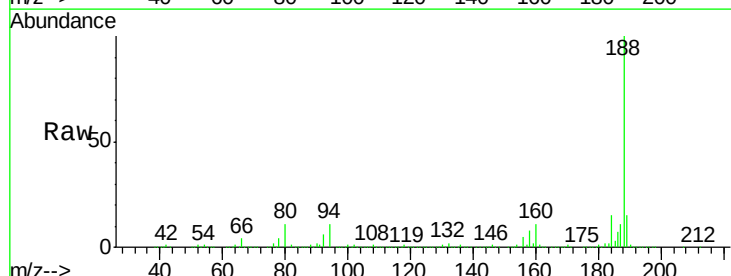


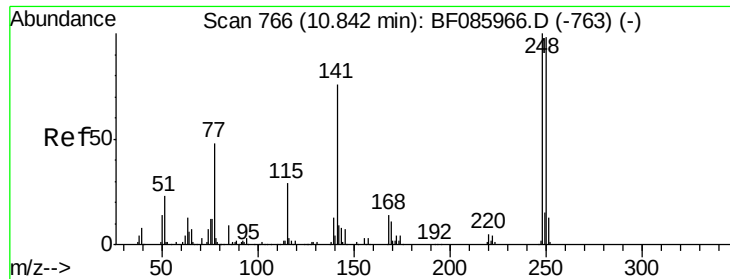




#66
4-Bromophenyl-phenylether
Concen: 4.93 ng
RT: 10.57 min Scan# 742
Delta R.T. -0.27 min
Lab File: BF086143.D
Acq: 7 Apr 2016 21:31

Instrument :
BNA_F
ClientSampleId :
RW-3-040116

Tgt Ion:248 Resp: 18617
Ion Ratio Lower Upper
248 100
250 200.4 77.4 116.0#
141 386.0 63.6 95.4#

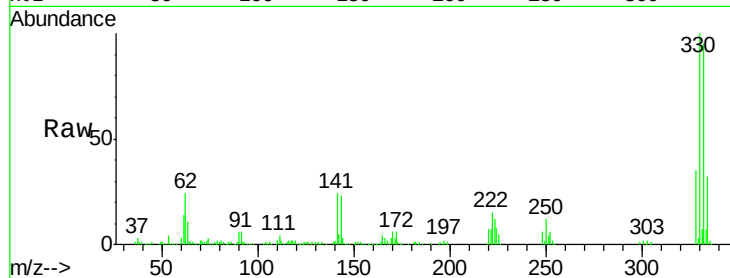


Abundance Ion 248.00 (247.70 to 248.70): E
Ion 250.00 (249.70 to 250.70): E
Ion 141.00 (140.70 to 141.70): E

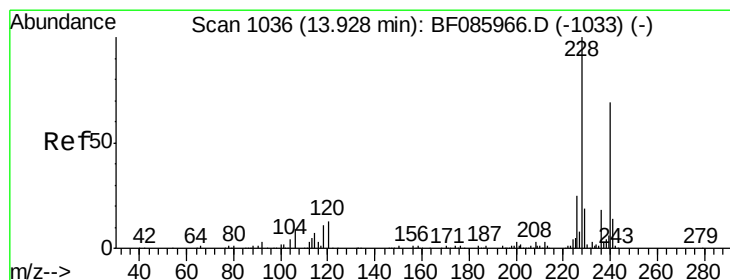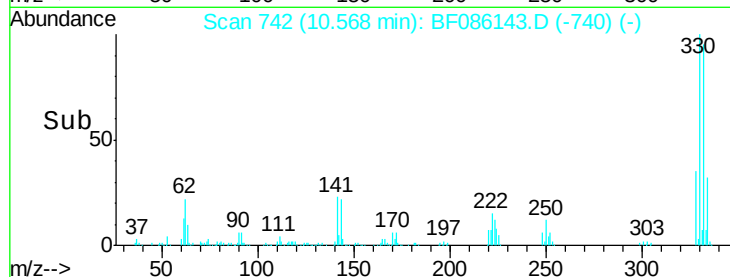
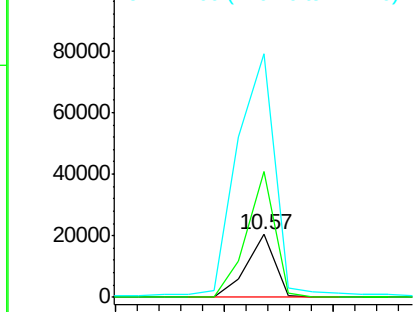



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.89 min Scan# 1033
Delta R.T. -0.03 min
Lab File: BF086143.D
Acq: 7 Apr 2016 21:31

Tgt Ion:240 Resp: 276816
Ion Ratio Lower Upper
240 100
120 8.9 13.8 20.8#
236 26.6 20.6 30.8

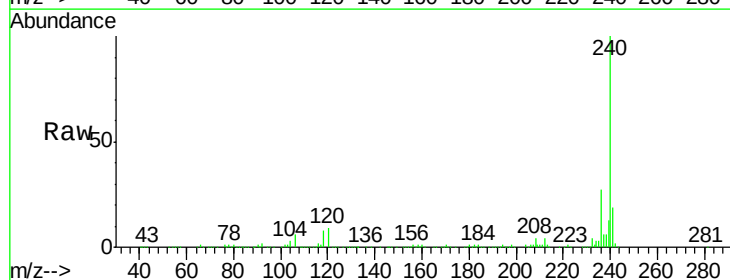

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E



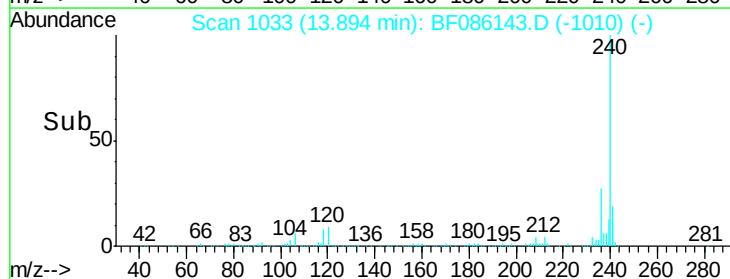
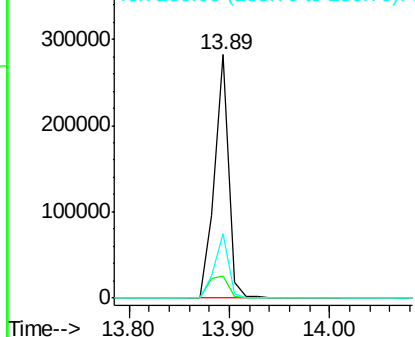




#78
 Terphenyl-d14
 Concen: 91.68 ng
 RT: 12.84 min Scan# 941
 Delta R.T. -0.03 min
 Lab File: BF086143.D
 Acq: 7 Apr 2016 21:31

Instrument :
 BNA_F
 ClientSampleId :
 RW-3-040116

Tgt Ion:244 Resp: 1079668
 Ion Ratio Lower Upper
 244 100
 212 7.2 6.1 9.1
 122 11.1 10.2 15.4

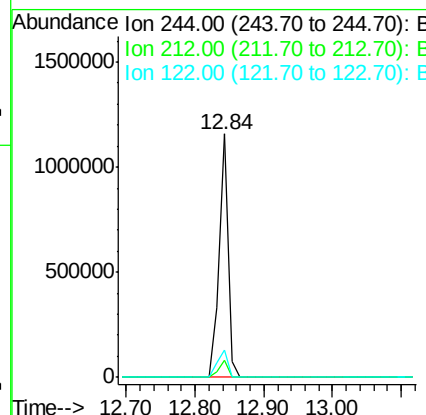

#86
 Perylene-d12
 Concen: 20.00 ng
 RT: 15.29 min Scan# 1155
 Delta R.T. -0.05 min
 Lab File: BF086143.D
 Acq: 7 Apr 2016 21:31

Tgt Ion:264 Resp: 186440
 Ion Ratio Lower Upper
 264 100
 260 24.7 19.4 29.2
 265 20.7 17.2 25.8

