
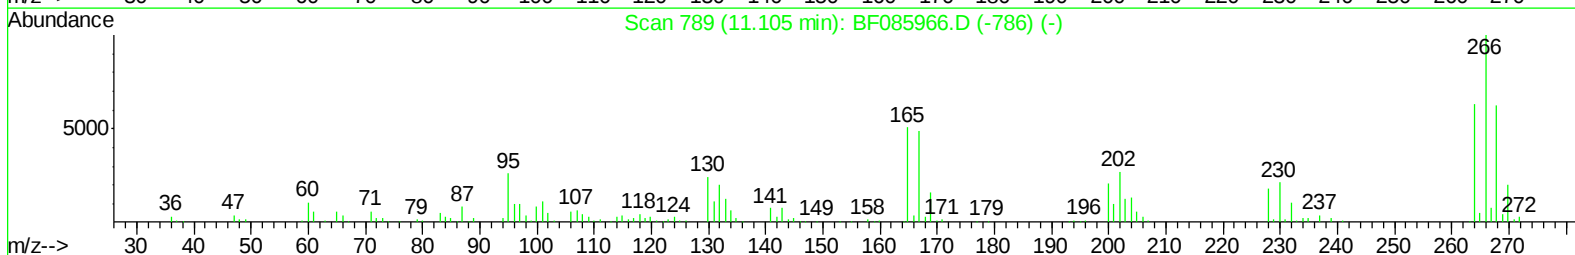
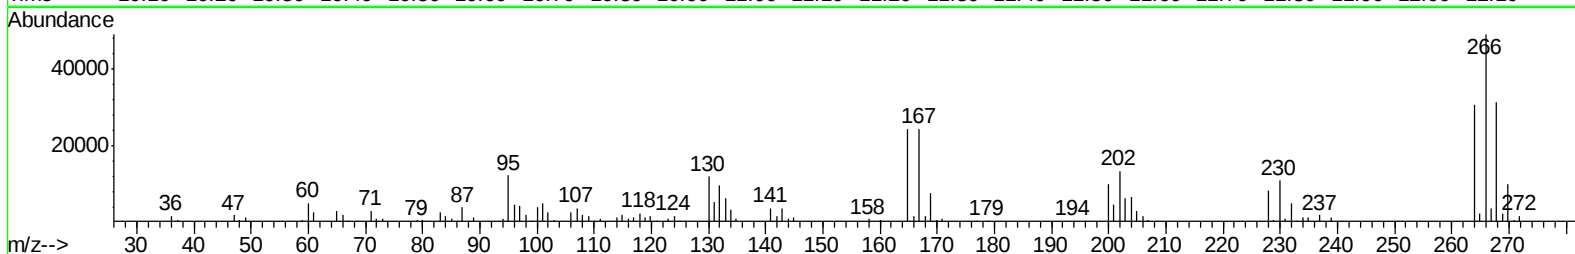


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040716\
Data File : BF086124.D
Acq On : 7 Apr 2016 11:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 07:25:26 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

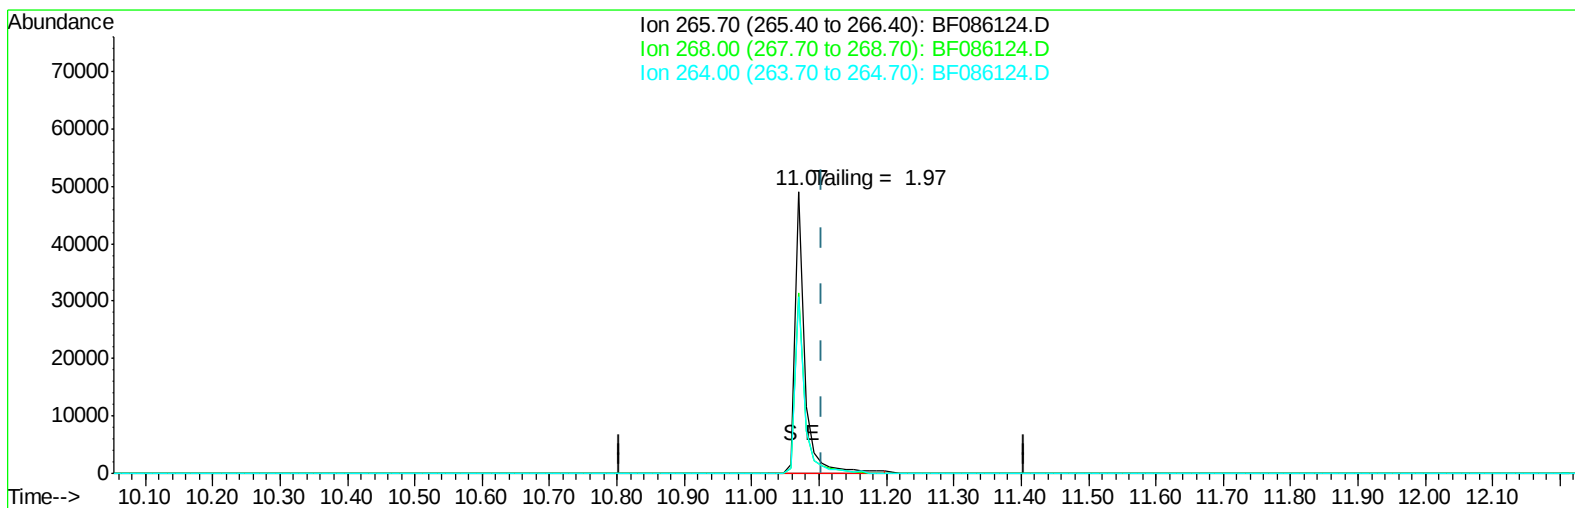

TIC: BF086124.D

(69) Pentachlorophenol (C)




11.070min (-0.034) 35456.82ng

response 50176

Ion	Exp%	Act%
265.70	100	100
268.00	64.40	64.07
264.00	63.30	62.83
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF040716\
Data File : BF086124.D
Acq On : 7 Apr 2016 11:27
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 08 07:25:26 2016
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

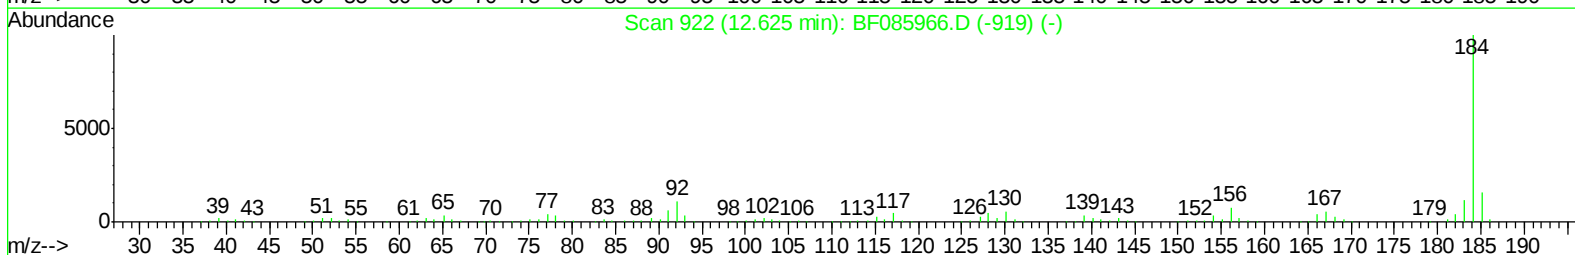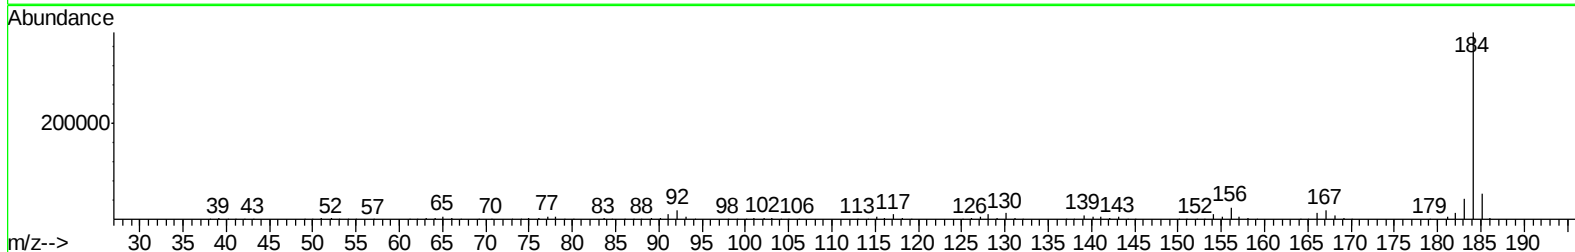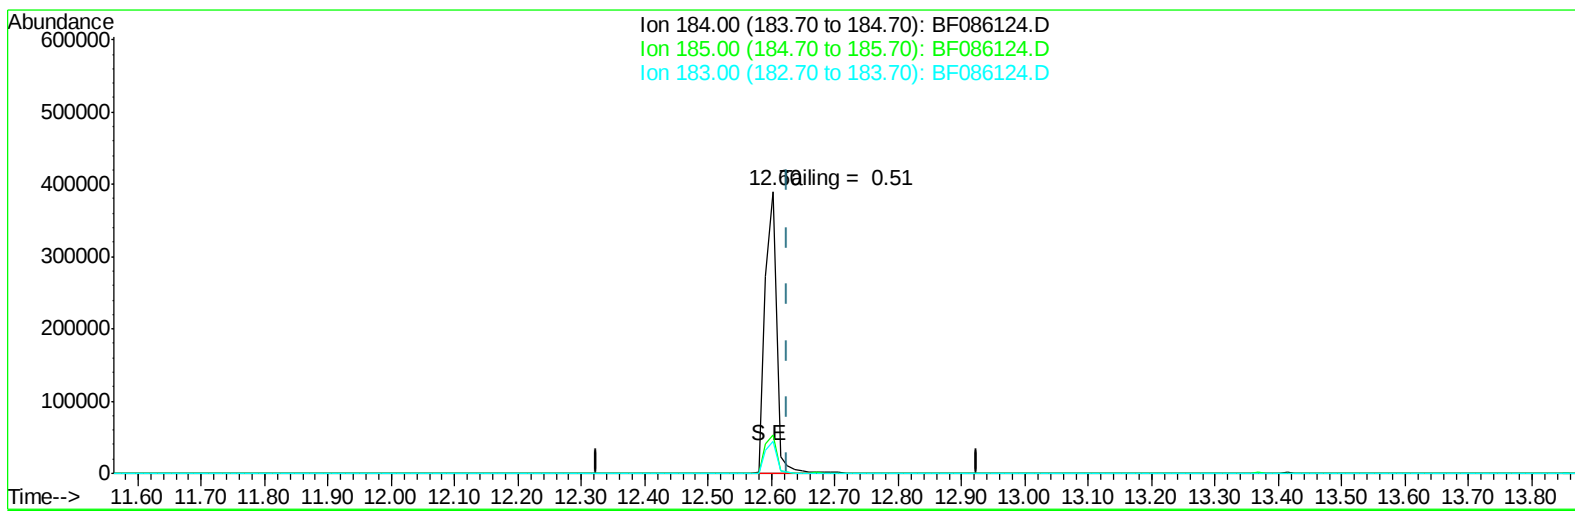

TIC: BF086124.D

(76) Benzidine

12.602min (-0.023) 0.00ng

response 496739

Ion	Exp%	Act%
184.00	100	100
185.00	15.50	13.59
183.00	11.80	11.39
0.00	0.00	0.00