

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040716\
 Data File : BF086131.D
 Acq On : 7 Apr 2016 14:48
 Operator : UM/SJ
 Sample : H2230-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-10-040116

Quant Time: Apr 08 02:20:06 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 01 23:17:06 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	96105	20.00	ng	-0.03
21) Naphthalene-d8	8.02	136	391615	20.00	ng	-0.05
38) Acenaphthene-d10	9.77	164	172715	20.00	ng	-0.05
63) Phenanthrene-d10	11.25	188	348209	20.00	ng	-0.05
75) Chrysene-d12	13.89	240	296029	20.00	ng	-0.03
86) Perylene-d12	15.29	264	205878	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	353078	62.80	ng	-0.03
7) Phenol-d6	6.37	99	270605	37.89	ng	-0.05
23) Nitrobenzene-d5	7.31	82	626321	94.32	ng	-0.03
41) 2,4,6-Tribromophenol	10.57	330	273151	168.50	ng	-0.03
44) 2-Fluorobiphenyl	9.10	172	1075002	103.49	ng	-0.03
78) Terphenyl-d14	12.84	244	974346	77.37	ng	-0.03


Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040716\
Data File : BF086131.D
Acq On : 7 Apr 2016 14:48
Operator : UM/SJ
Sample : H2230-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-10-040116

Quant Time: Apr 08 02:20:06 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

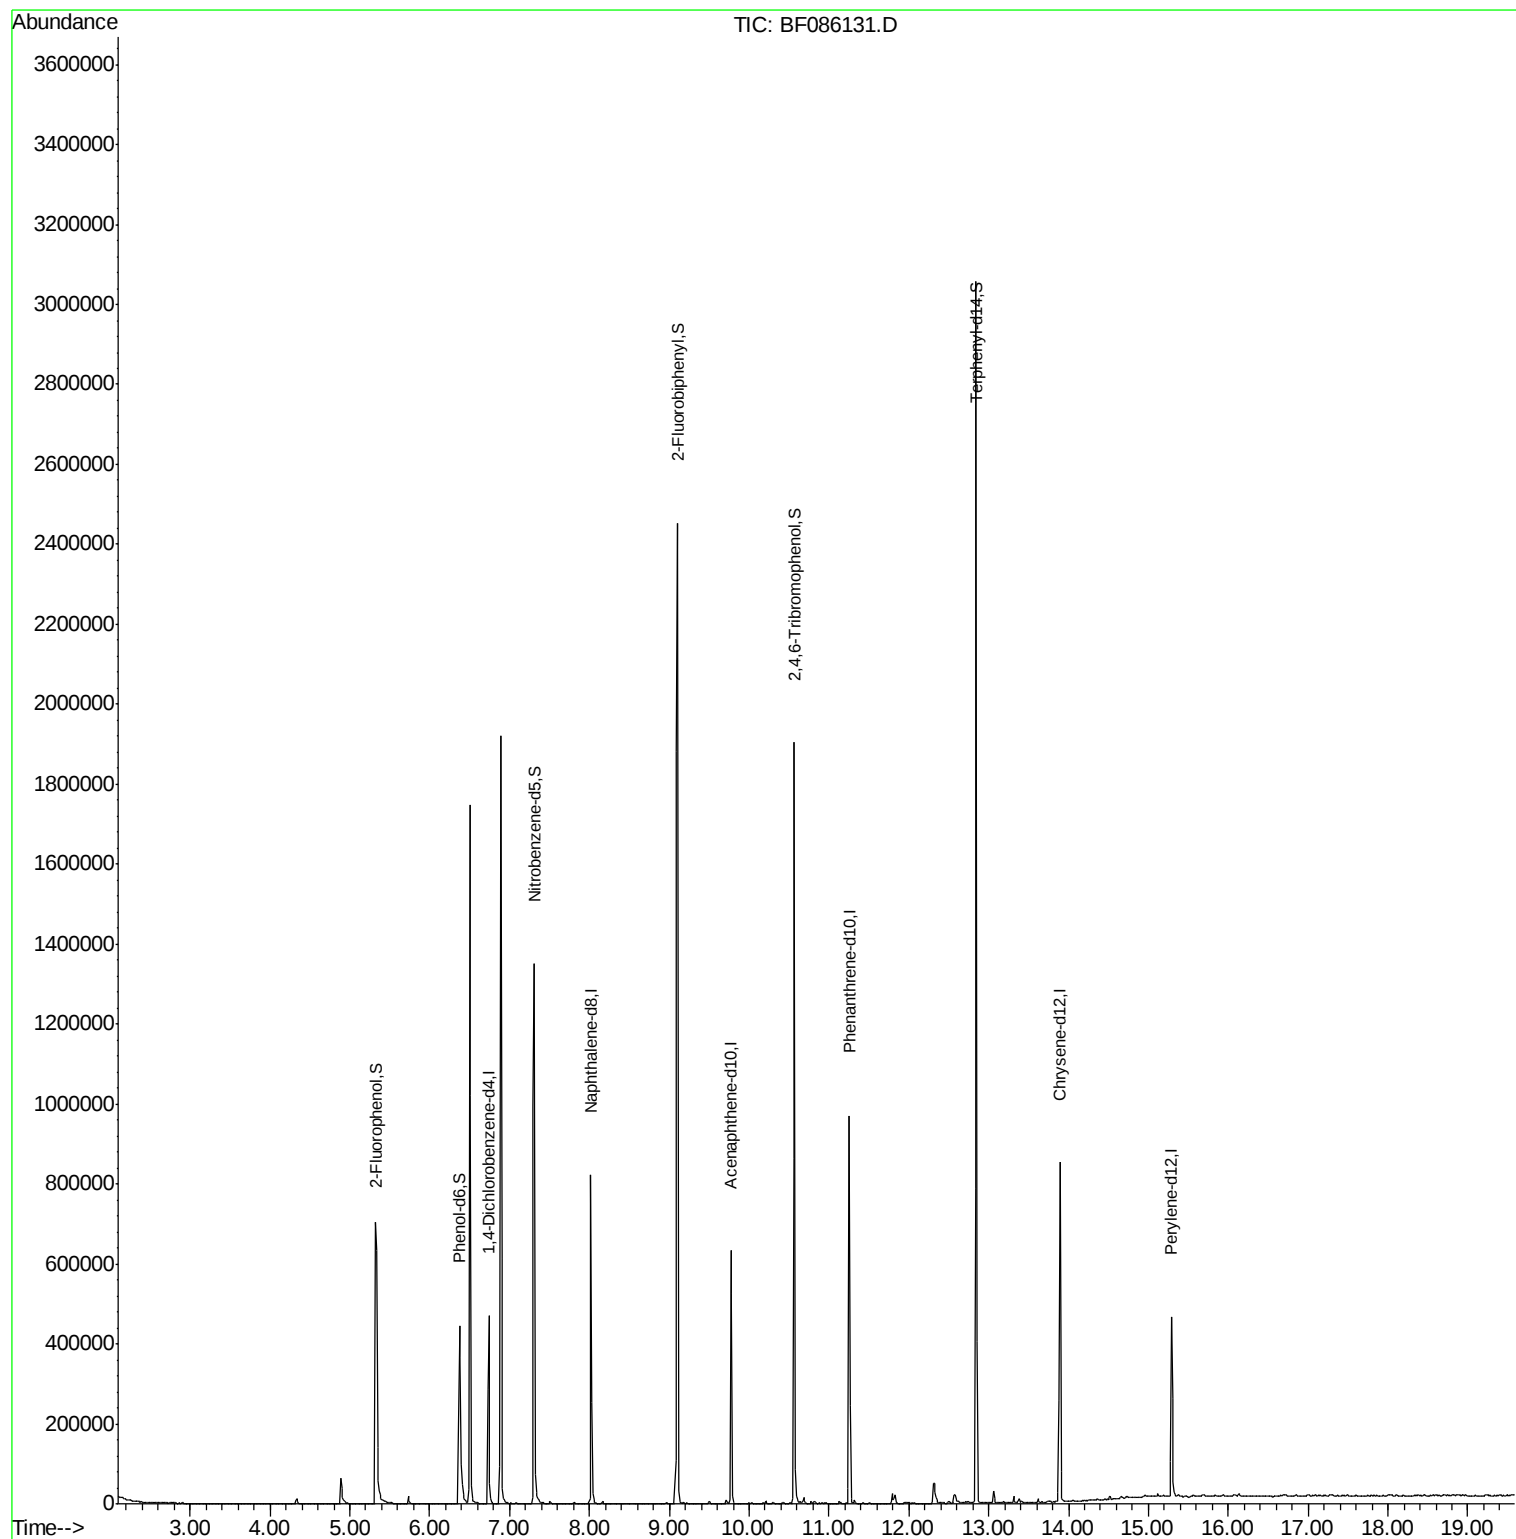



#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.74 min Scan# 407

Delta R.T. -0.03 min

Lab File: BF086131.D

Acq: 7 Apr 2016 14:48

Instrument :

BNA_F

ClientSampleId :

MW-10-040116


Tot Ion:152 Resp: 96105

Ion Ratio Lower Upper

152 100

150 152.5 124.2 186.2




115 55.7 47.0 70.6

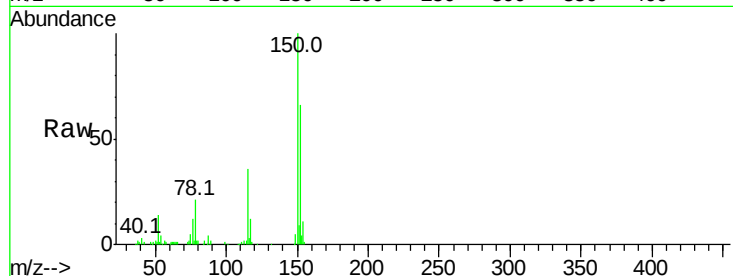

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 150.00 (149.70 to 150.70): E

Ion 115.00 (114.70 to 115.70): E

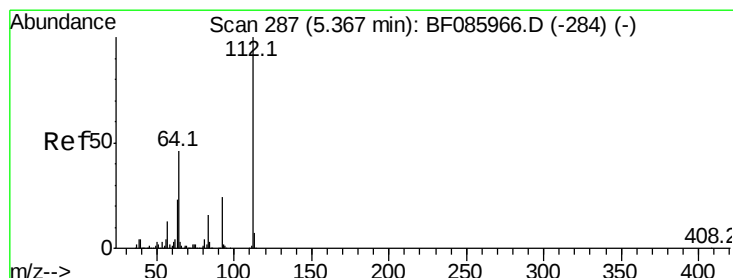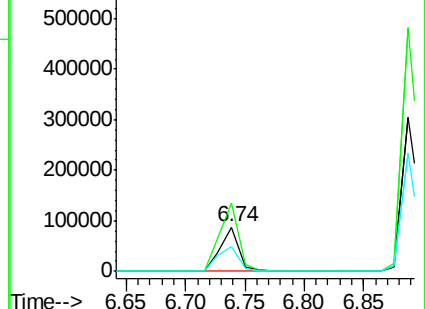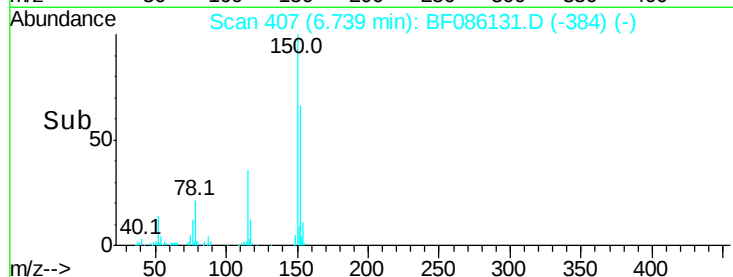

#5

2-Fluorophenol

Concen: 62.80 ng

RT: 5.33 min Scan# 284

Delta R.T. -0.03 min

Lab File: BF086131.D

Acq: 7 Apr 2016 14:48


Tgt Ion:112 Resp: 353078

Ion Ratio Lower Upper

112 100

64 48.3 39.9 59.9



63 24.5 20.2 30.2

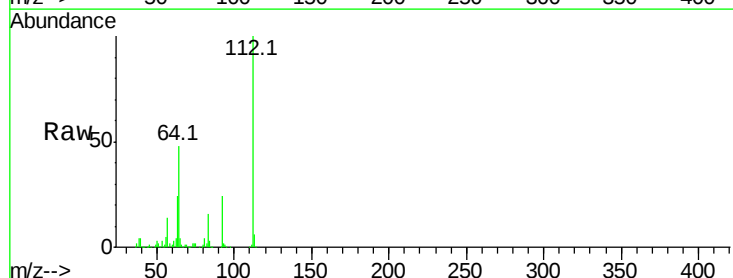

Abundance Ion 112.00 (111.70 to 112.70): E

Ion 64.00 (63.70 to 64.70): BF0

Ion 63.00 (62.70 to 63.70): BF0

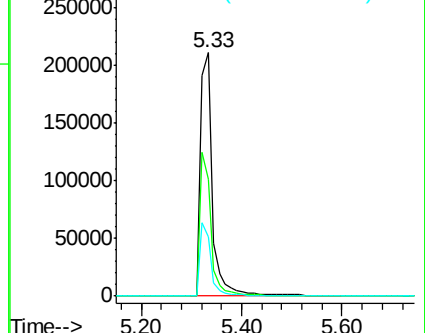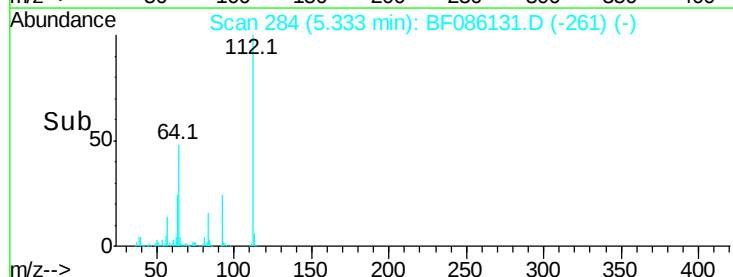



#7

Phenol-d6

Concen: 37.89 ng

RT: 6.37 min Scan# 375

Delta R.T. -0.05 min

Lab File: BF086131.D

Acq: 7 Apr 2016 14:48

Instrument :





BNA_F

ClientSampleId :

MW-10-040116

Tot Ion: 99 Resp: 270605

Ion	Ratio	Lower	Upper
99	100		
42	19.5	11.1	16.7#
71	35.1	24.9	37.3

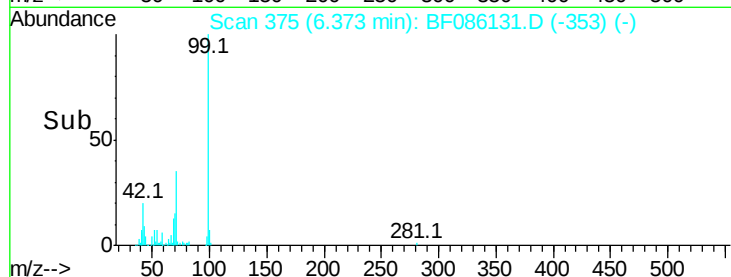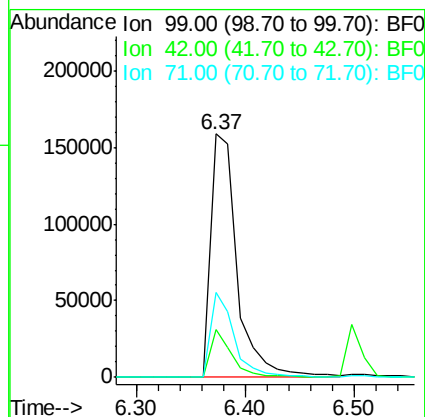

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.02 min Scan# 519




Delta R.T. -0.05 min

Lab File: BF086131.D

Acq: 7 Apr 2016 14:48

Tgt Ion: 136 Resp: 391615

Ion	Ratio	Lower	Upper
136	100		
137	11.2	9.1	13.7
54	8.1	7.4	11.0
68	6.8	5.8	8.8


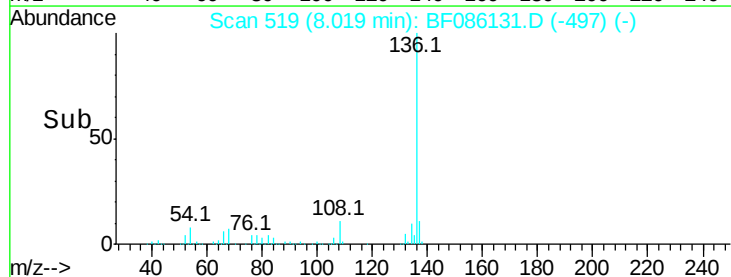
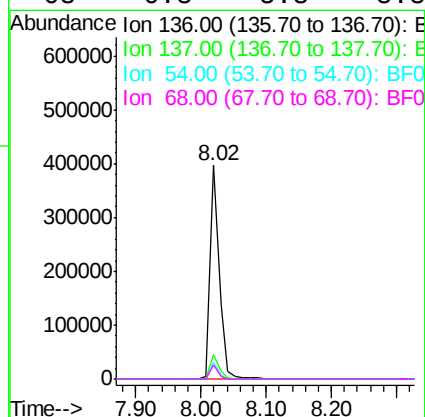





#23
 Nitrobenzene-d5
 Concen: 94.32 ng
 RT: 7.31 min Scan# 457
 Delta R.T. -0.03 min
 Lab File: BF086131.D
 Acq: 7 Apr 2016 14:48




Instrument :
 BNA_F
 ClientSampleId :
 MW-10-040116


Tot Ion: 82 Resp: 626321
 Ion Ratio Lower Upper
 82 100
 128 53.3 41.8 62.8
 54 40.4 33.4 50.0

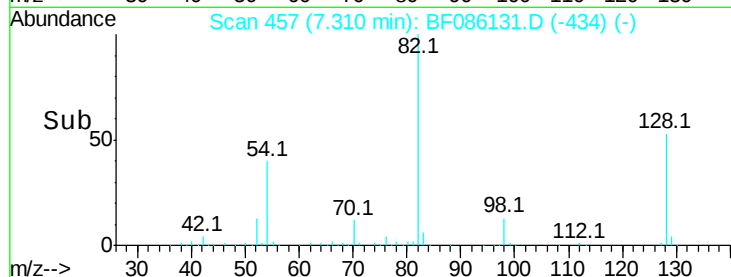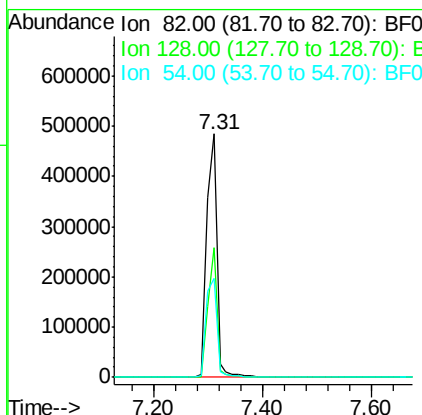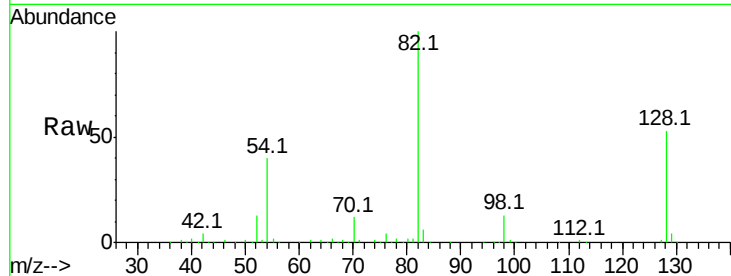

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.77 min Scan# 672
 Delta R.T. -0.05 min
 Lab File: BF086131.D
 Acq: 7 Apr 2016 14:48

Tgt Ion:164 Resp: 172715
 Ion Ratio Lower Upper
 164 100
 162 101.7 82.1 123.1
 160 46.0 37.4 56.2

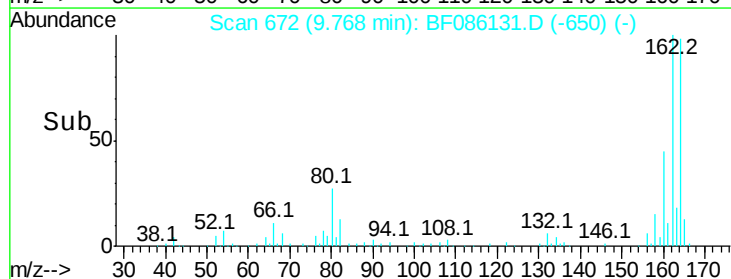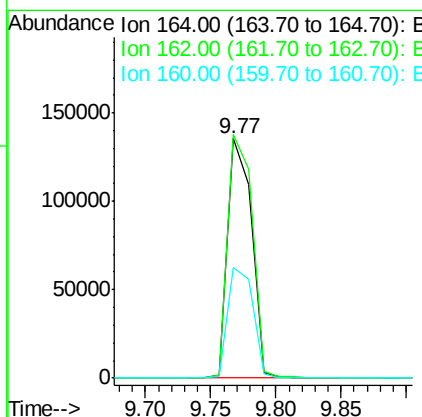


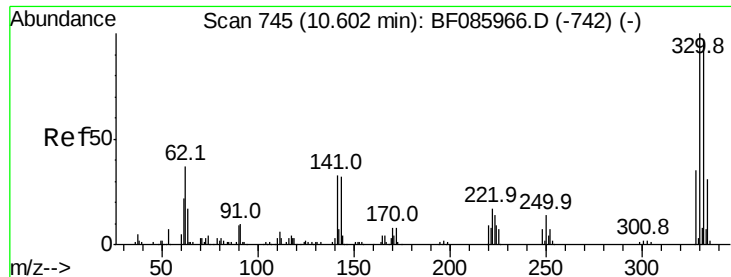



#41
 2,4,6-Tribromophenol
 Concen: 168.50 ng
 RT: 10.57 min Scan# 742
 Delta R.T. -0.03 min
 Lab File: BF086131.D
 Acq: 7 Apr 2016 14:48

Instrument :
 BNA_F
 ClientSampleId :
 MW-10-040116

Tot Ion:330 Resp: 273151
 Ion Ratio Lower Upper
 330 100
 332 97.1 78.2 117.2
 141 33.5 31.5 47.3

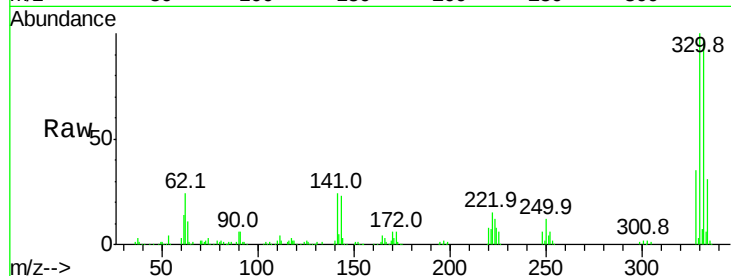


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

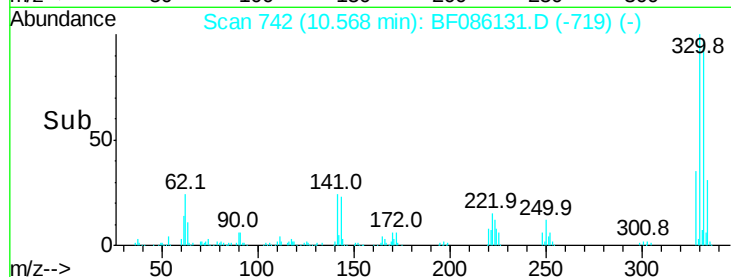
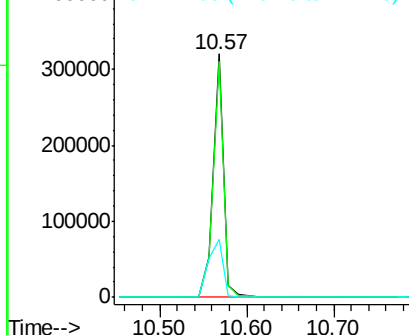



#44
 2-Fluorobiphenyl
 Concen: 103.49 ng
 RT: 9.10 min Scan# 614
 Delta R.T. -0.03 min
 Lab File: BF086131.D
 Acq: 7 Apr 2016 14:48

Tgt Ion:172 Resp: 1075002
 Ion Ratio Lower Upper
 172 100
 171 36.2 29.4 44.2
 170 24.2 19.8 29.6



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

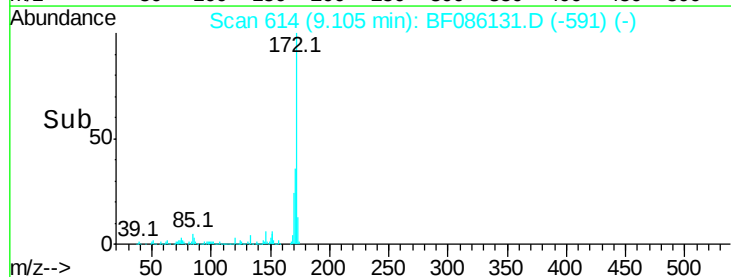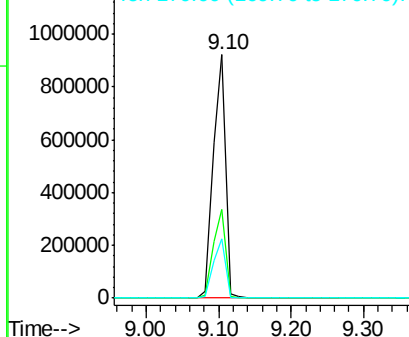


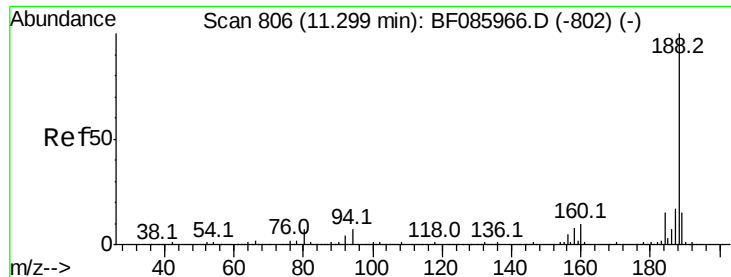




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.25 min Scan# 802
Delta R.T. -0.05 min
Lab File: BF086131.D
Acq: 7 Apr 2016 14:48

Instrument :
BNA_F
ClientSampleId :
MW-10-040116

Tot Ion:188 Resp: 348209
Ion Ratio Lower Upper
188 100
94 11.6 5.4 8.0#
80 12.4 5.5 8.3#

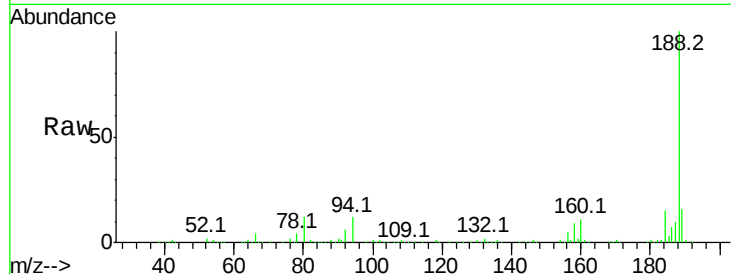


Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

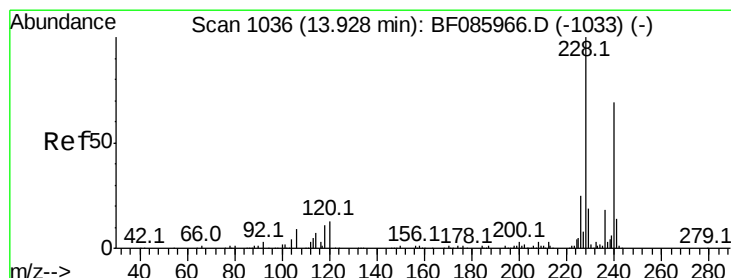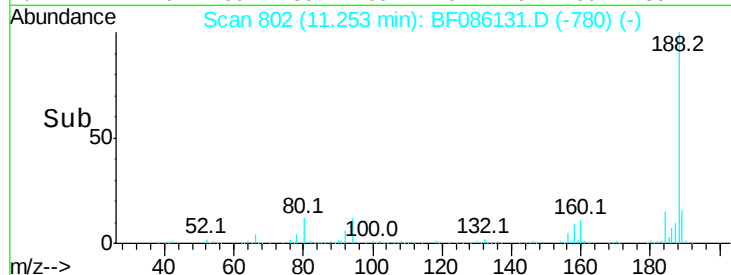
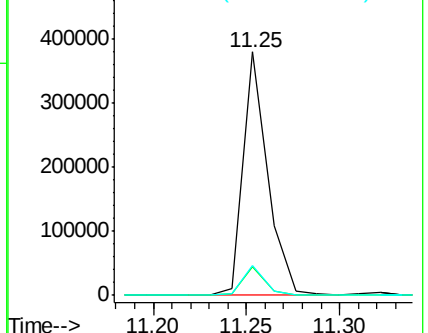



#75
Chrysene-d12
Concen: 20.00 ng
RT: 13.89 min Scan# 1033
Delta R.T. -0.03 min
Lab File: BF086131.D
Acq: 7 Apr 2016 14:48

Tgt Ion:240 Resp: 296029
Ion Ratio Lower Upper
240 100
120 11.0 13.8 20.8#
236 26.7 20.6 30.8



Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

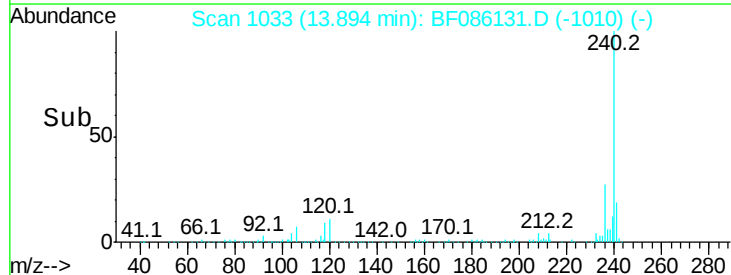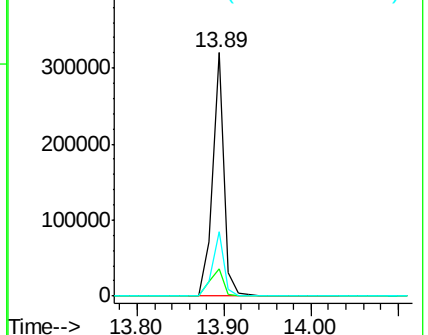

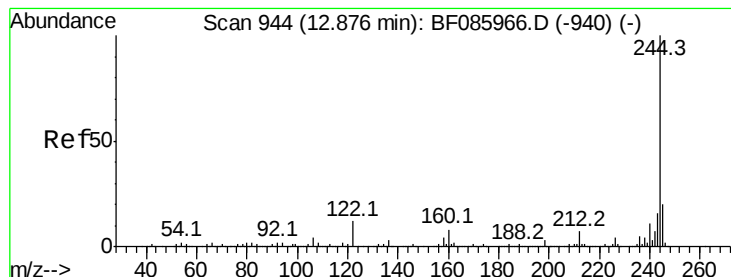

#78

Terphenyl-d14

Concen: 77.37 ng

RT: 12.84 min Scan# 941

Delta R.T. -0.03 min

Lab File: BF086131.D

Acq: 7 Apr 2016 14:48

Instrument :

BNA_F

ClientSampleId :

MW-10-040116


Tot Ion:244 Resp: 974346

Ion Ratio Lower Upper

244 100

212 7.4 6.1 9.1




122 12.1 10.2 15.4



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

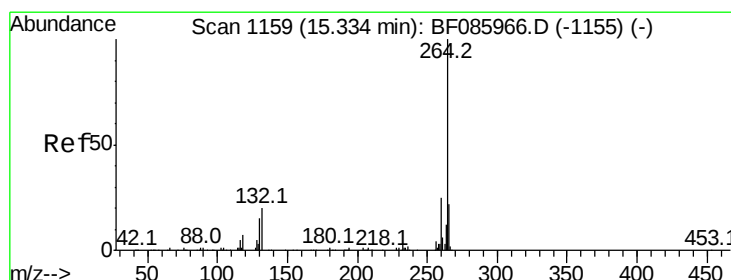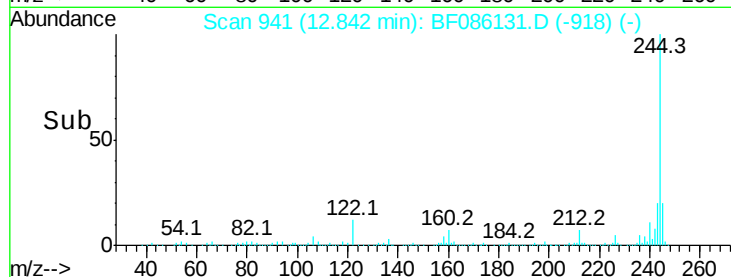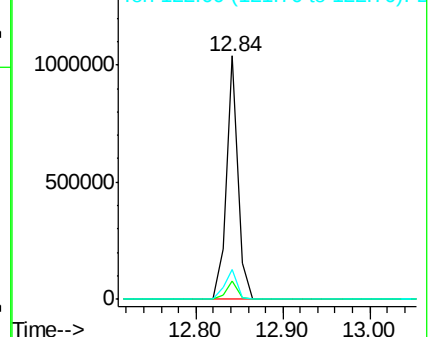

#86

Perylene-d12

Concen: 20.00 ng

RT: 15.29 min Scan# 1155

Delta R.T. -0.05 min

Lab File: BF086131.D

Acq: 7 Apr 2016 14:48


Tgt Ion:264 Resp: 205878

Ion Ratio Lower Upper

264 100

260 24.6 19.4 29.2

265 21.8 17.2 25.8



Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

