

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040716\
 Data File : BF086155.D
 Acq On : 8 Apr 2016 3:13
 Operator : UM/SJ
 Sample : H2282-16
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 AMBOY-SB-37(0.5-15.0)

Quant Time: Apr 08 04:07:16 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Apr 01 23:17:06 2016
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.74	152	107202	20.00	ng	-0.03
21) Naphthalene-d8	8.02	136	448170	20.00	ng	-0.05
38) Acenaphthene-d10	9.77	164	195084	20.00	ng	-0.05
63) Phenanthrene-d10	11.25	188	386636	20.00	ng	-0.05
75) Chrysene-d12	13.89	240	259803	20.00	ng	-0.03
86) Perylene-d12	15.29	264	201184	20.00	ng	-0.05
System Monitoring Compounds						
5) 2-Fluorophenol	5.33	112	780864	124.51	ng	-0.03
7) Phenol-d6	6.38	99	1015208	127.44	ng	-0.03
23) Nitrobenzene-d5	7.30	82	589632	77.59	ng	-0.05
41) 2,4,6-Tribromophenol	10.57	330	245038	133.82	ng	-0.03
44) 2-Fluorobiphenyl	9.09	172	894217	76.21	ng	-0.05
78) Terphenyl-d14	12.84	244	970131	87.78	ng	-0.03
Target Compounds						Qvalue
49) Dimethylphthalate	9.49	163	126245	8.73	ng	# 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA F\DATA\BF040716\
Data File : BF086155.D
Acq On : 8 Apr 2016 3:13
Operator : UM/SJ
Sample : H2282-16
Misc :
ALS Vial : 32 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
AMBOY-SB-37(0.5-15.0)

Quant Time: Apr 08 04:07:16 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF040216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Apr 01 23:17:06 2016
Response via : Initial Calibration

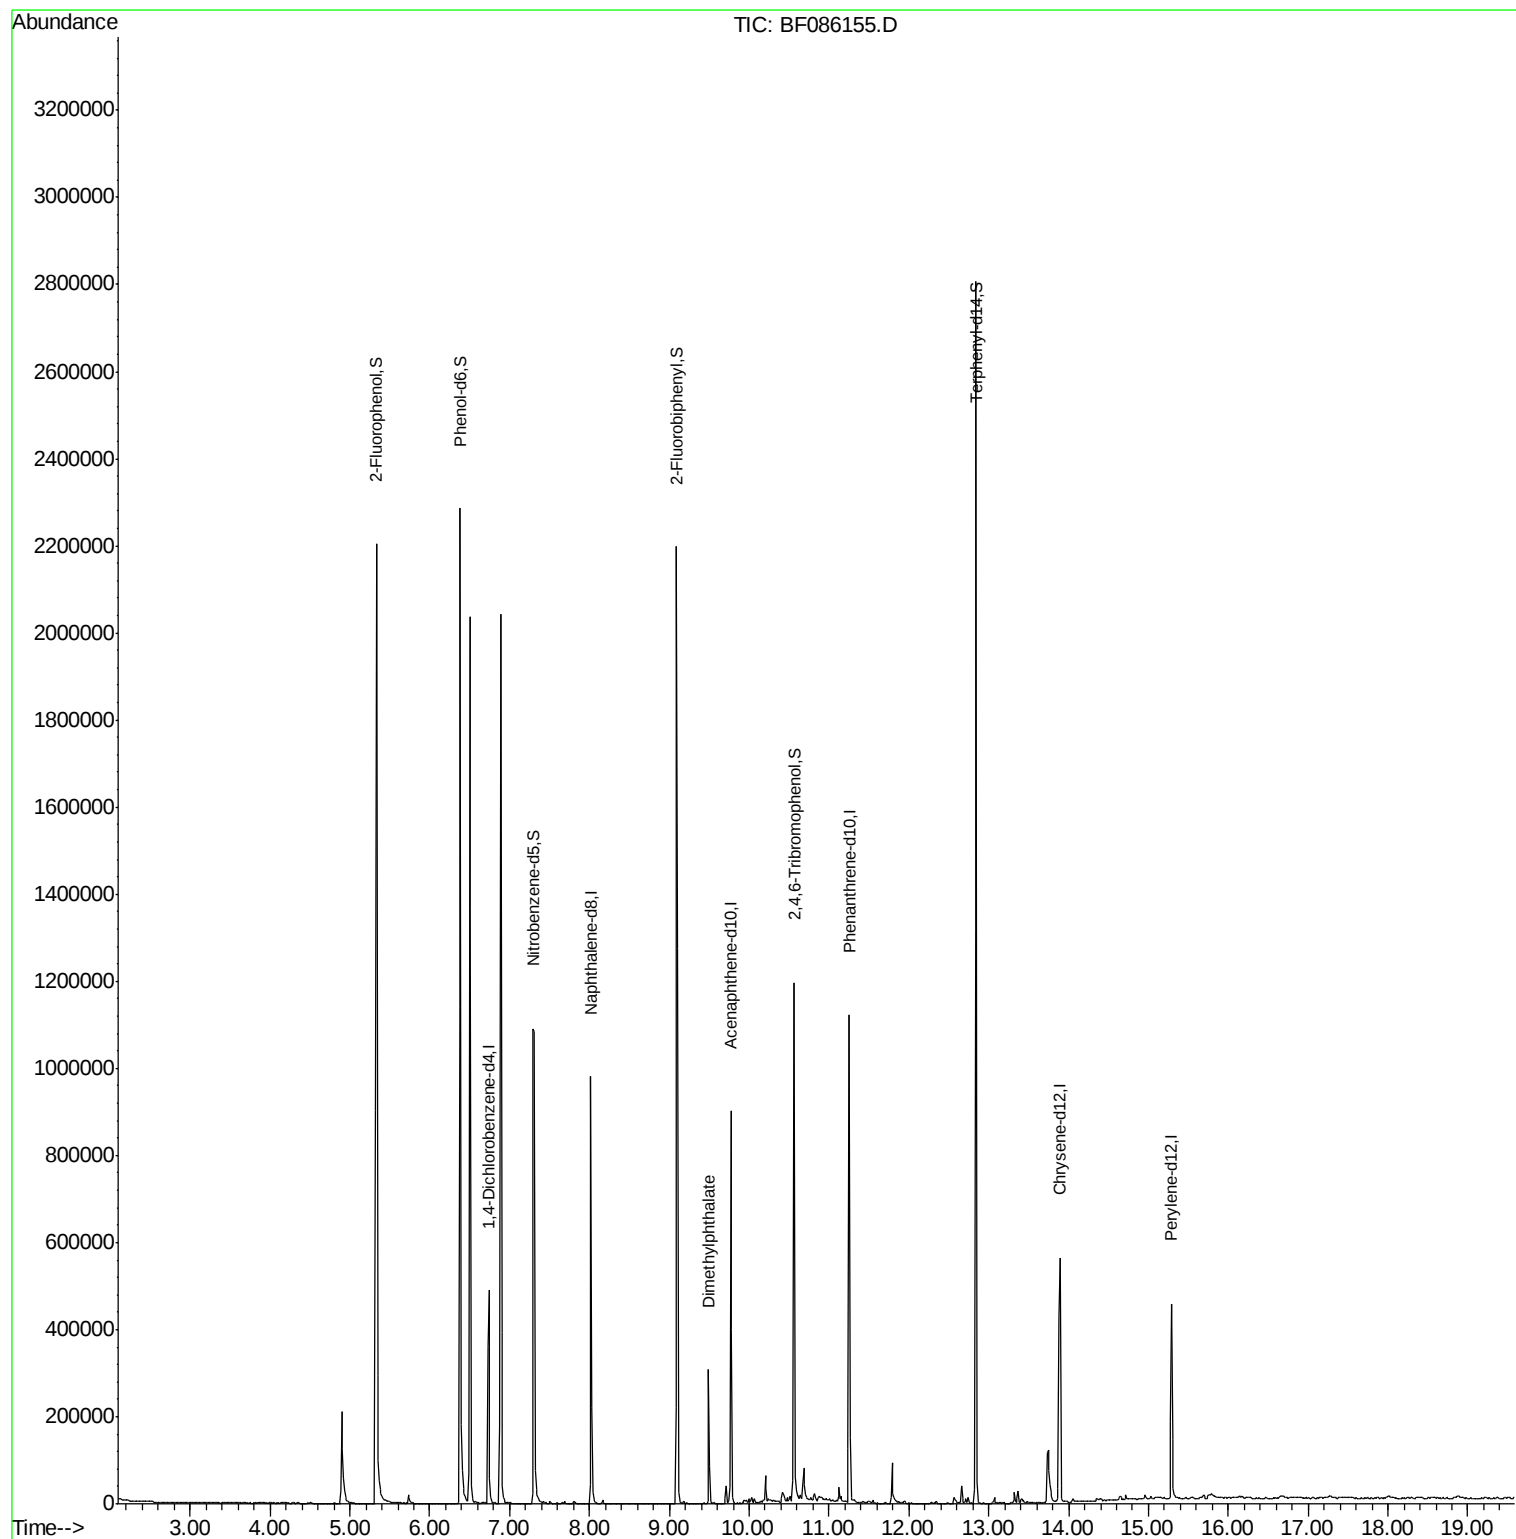

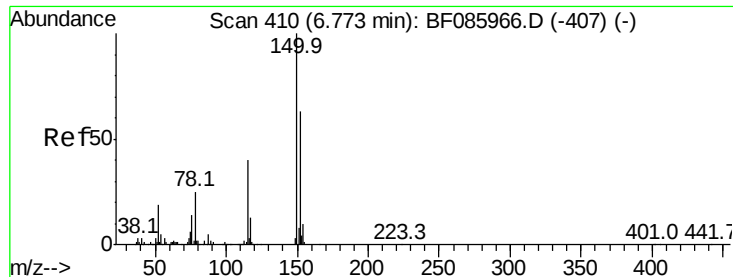

#1

1,4-Dichlorobenzene-d4

Concen: 20.00 ng

RT: 6.74 min Scan# 407

Delta R.T. -0.03 min

Lab File: BF086155.D

Acq: 8 Apr 2016 3:13

Instrument :

BNA_F

ClientSampleId :

AMBOY-SB-37(0.5-15.0)





Tot Ion:152 Resp: 107202

Ion Ratio Lower Upper

152 100

150 155.6 124.2 186.2

115 55.9 47.0 70.6

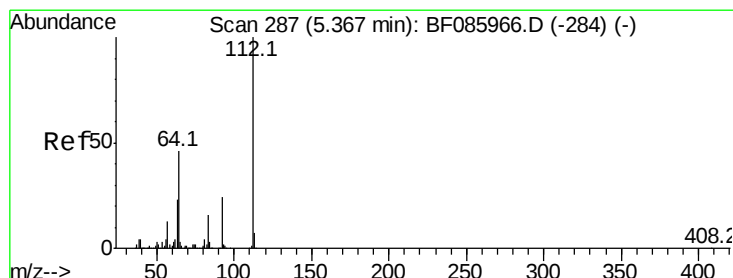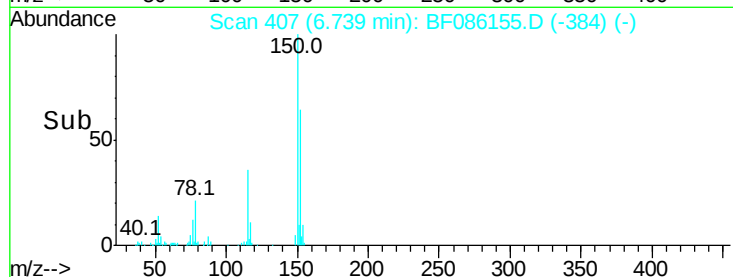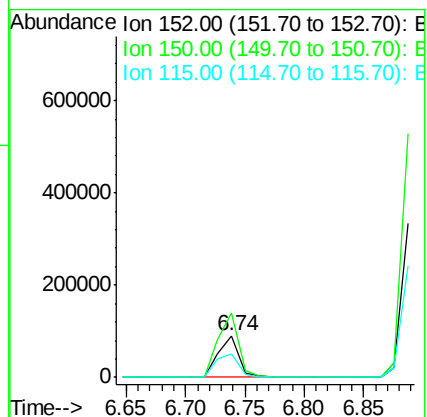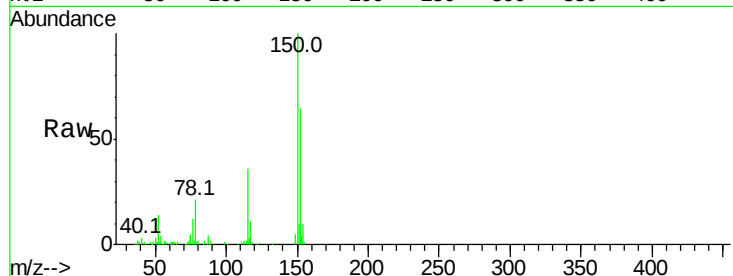

#5

2-Fluorophenol

Concen: 124.51 ng

RT: 5.33 min Scan# 284

Delta R.T. -0.03 min

Lab File: BF086155.D

Acq: 8 Apr 2016 3:13




Tgt Ion:112 Resp: 780864


Ion Ratio Lower Upper

112 100

64 51.4 39.9 59.9

63 26.0 20.2 30.2

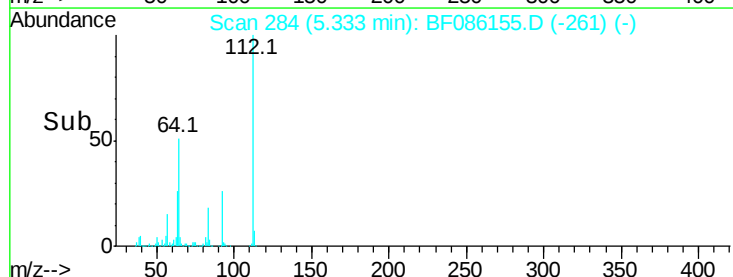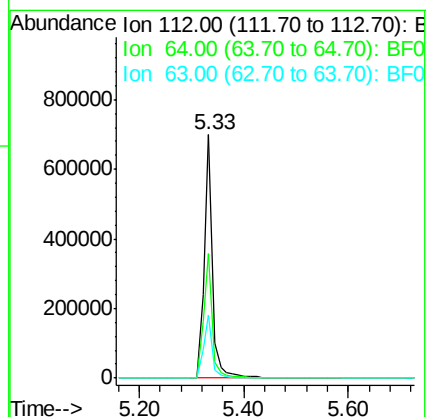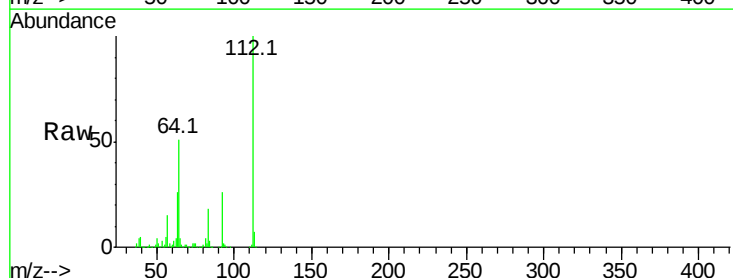

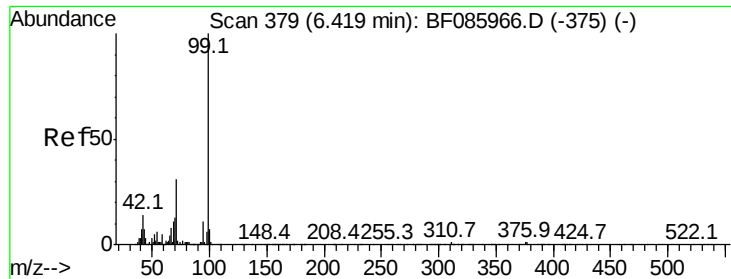

#7

Phenol-d6

Concen: 127.44 ng

RT: 6.38 min Scan# 376

Delta R.T. -0.03 min

Lab File: BF086155.D

Acq: 8 Apr 2016 3:13

Instrument :

BNA_F

ClientSampleId :

AMBOY-SB-37(0.5-15.0)





Tot Ion: 99 Resp: 1015208

Ion Ratio Lower Upper

99 100

42 14.4 11.1 16.7

71 32.1 24.9 37.3

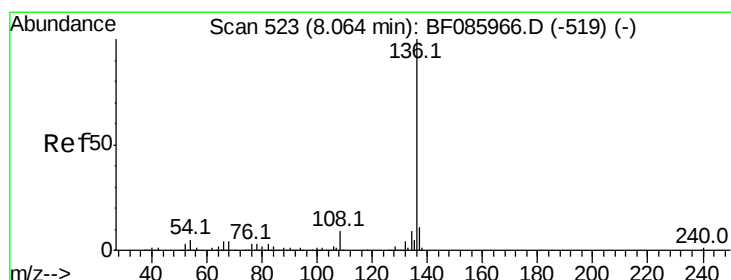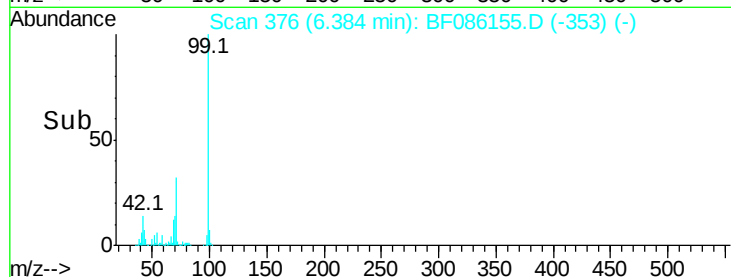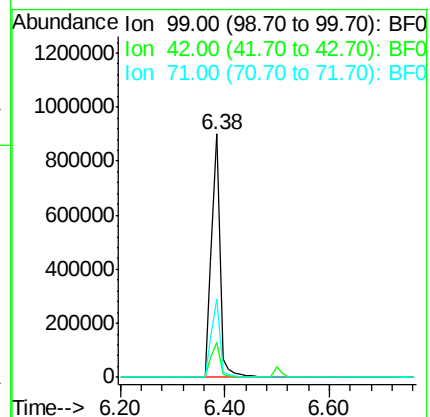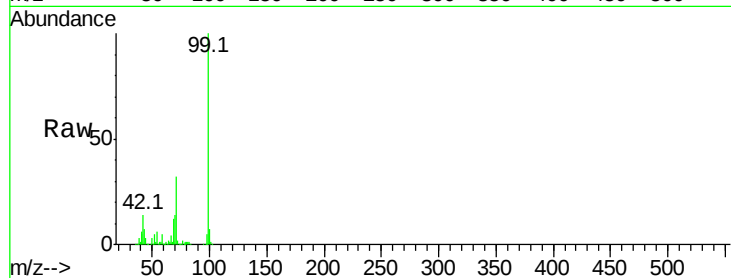

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.02 min Scan# 519

Delta R.T. -0.05 min

Lab File: BF086155.D

Acq: 8 Apr 2016 3:13

Tgt Ion: 136 Resp: 448170




Ion Ratio Lower Upper


136 100

137 11.3 9.1 13.7

54 7.7 7.4 11.0

68 6.5 5.8 8.8


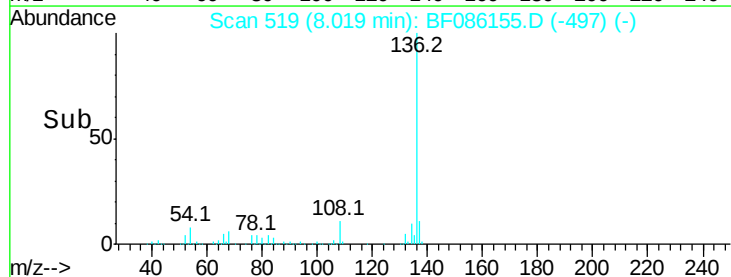
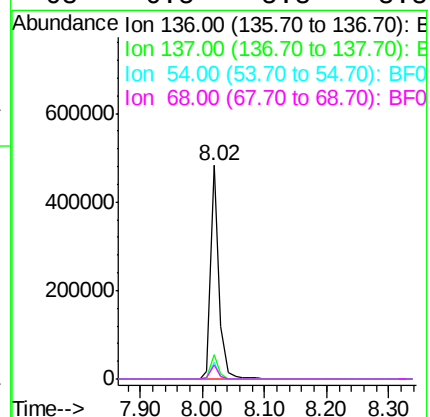
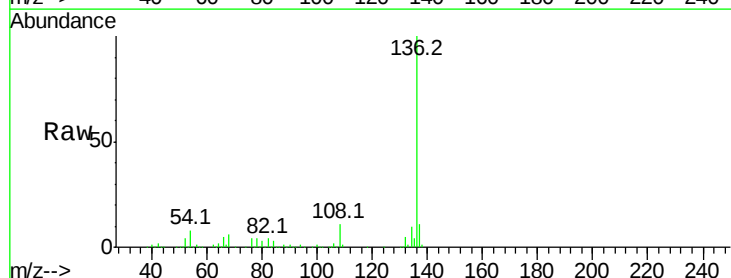


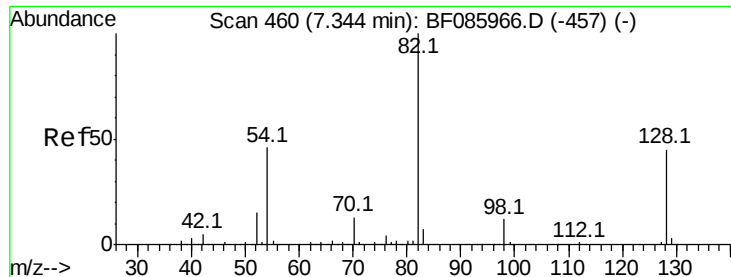

#23
 Nitrobenzene-d5
 Concen: 77.59 ng
 RT: 7.30 min Scan# 456
 Delta R.T. -0.05 min
 Lab File: BF086155.D
 Acq: 8 Apr 2016 3:13




Instrument :
 BNA_F
 ClientSampleId :
 AMBOY-SB-37(0.5-15.0)


Tot Ion: 82 Resp: 589632
 Ion Ratio Lower Upper
 82 100
 128 40.1 41.8 62.8#
 54 47.6 33.4 50.0

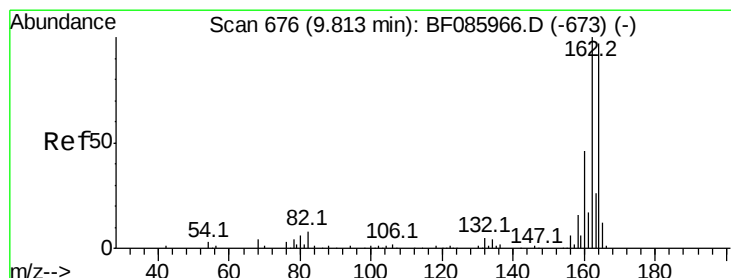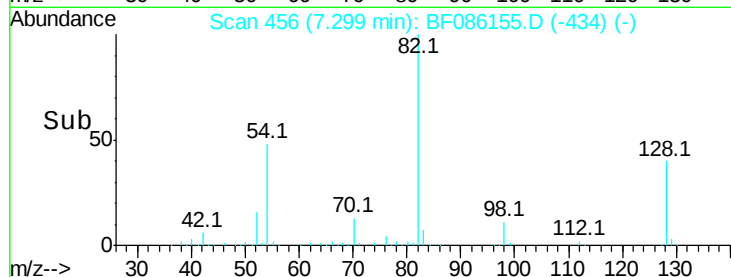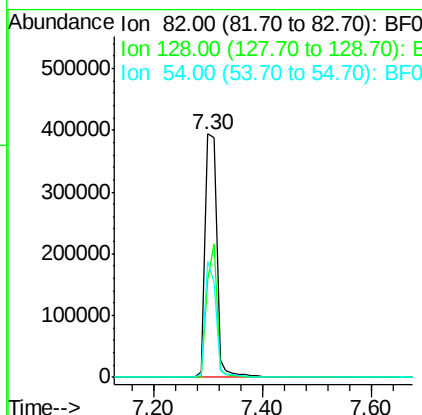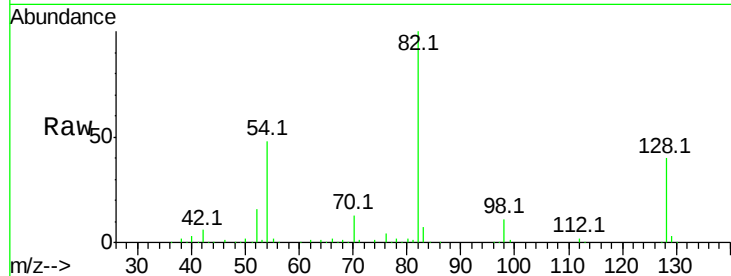

#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 9.77 min Scan# 672
 Delta R.T. -0.05 min
 Lab File: BF086155.D
 Acq: 8 Apr 2016 3:13

Tgt Ion:164 Resp: 195084
 Ion Ratio Lower Upper
 164 100
 162 102.5 82.1 123.1
 160 47.1 37.4 56.2

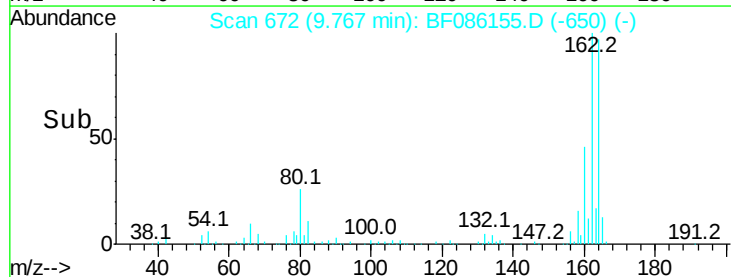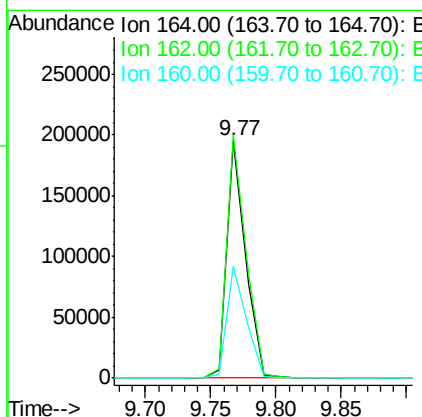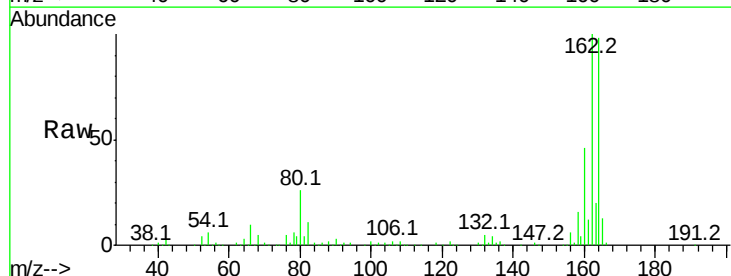


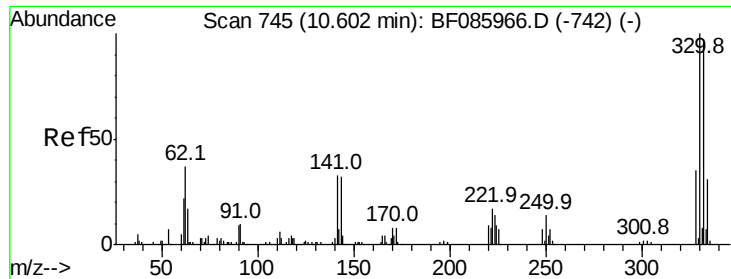




#41
 2,4,6-Tribromophenol
 Concen: 133.82 ng
 RT: 10.57 min Scan# 742
 Delta R.T. -0.03 min
 Lab File: BF086155.D
 Acq: 8 Apr 2016 3:13

Instrument :
 BNA_F
 ClientSampleId :
 AMBOY-SB-37(0.5-15.0)

Tot Ion:330 Resp: 245038
 Ion Ratio Lower Upper
 330 100
 332 96.1 78.2 117.2
 141 31.4 31.5 47.3#

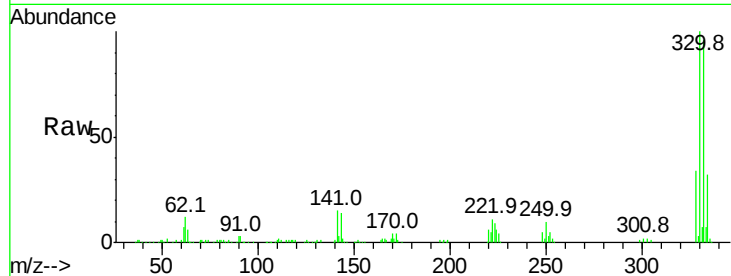


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

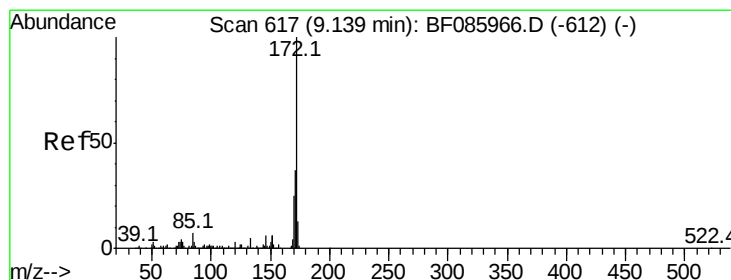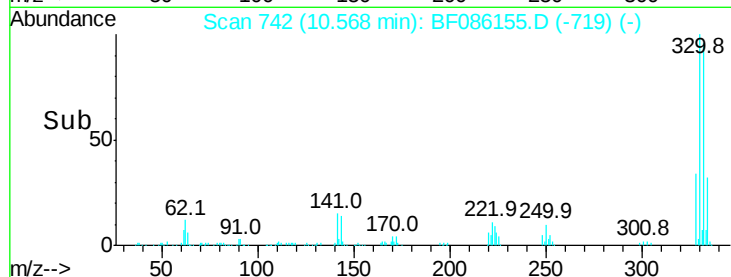
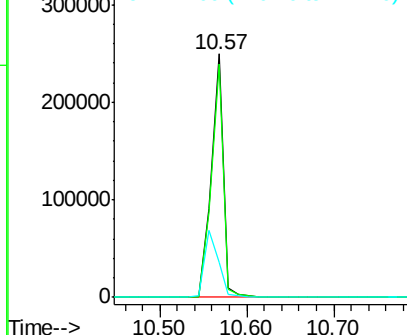



#44
 2-Fluorobiphenyl
 Concen: 76.21 ng
 RT: 9.09 min Scan# 613
 Delta R.T. -0.05 min
 Lab File: BF086155.D
 Acq: 8 Apr 2016 3:13

Tgt Ion:172 Resp: 894217
 Ion Ratio Lower Upper
 172 100
 171 35.7 29.4 44.2
 170 24.1 19.8 29.6

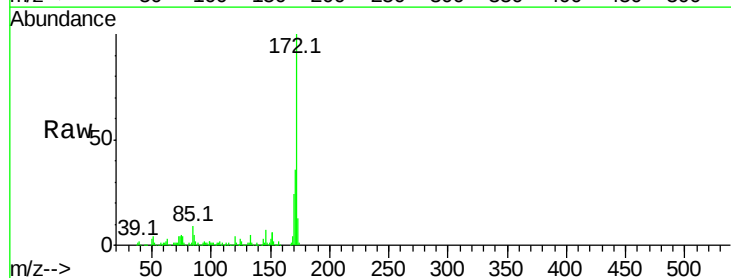

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

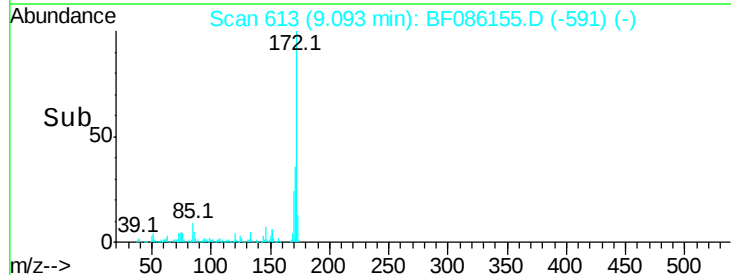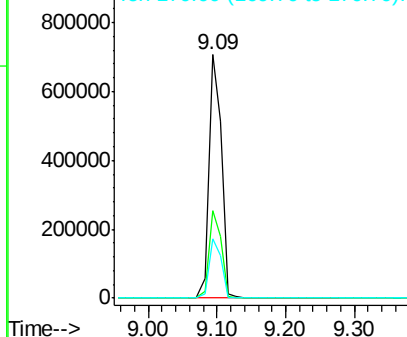

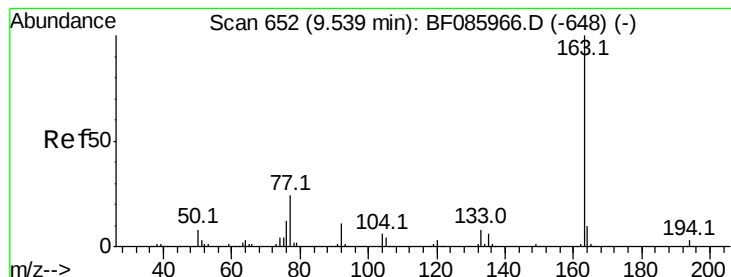

#49

Dimethylphthalate

Concen: 8.73 ng

RT: 9.49 min Scan# 648

Delta R.T. -0.05 min

Lab File: BF086155.D

Acq: 8 Apr 2016 3:13

Instrument :

BNA_F

ClientSampleId :

AMBOY-SB-37(0.5-15.0)


Tot Ion:163 Resp: 126245

Ion Ratio Lower Upper

163 100

194 2.9 2.9 4.3#




164 10.5 8.3 12.5

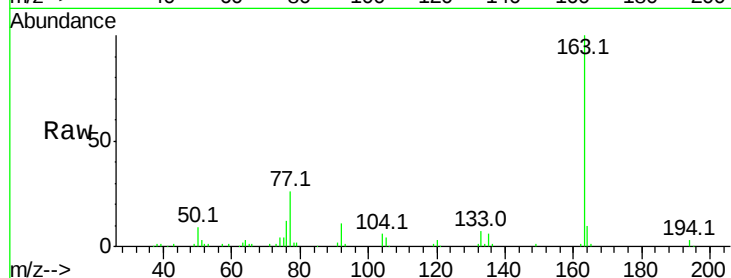

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

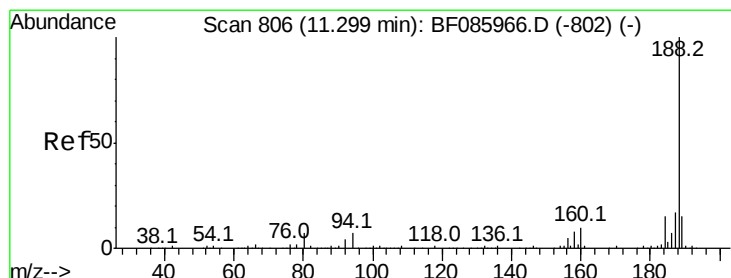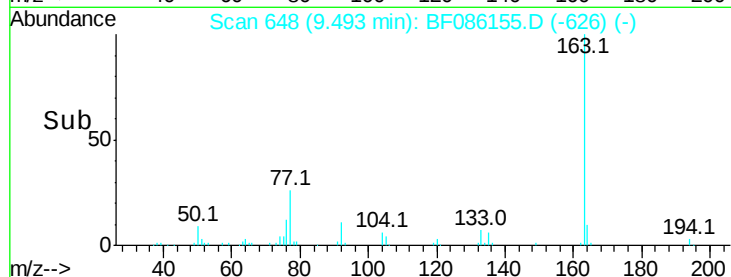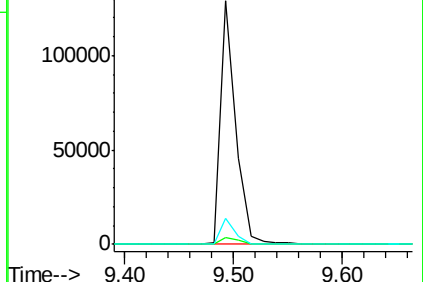

#63

Phenanthrene-d10

Concen: 20.00 ng

RT: 11.25 min Scan# 802

Delta R.T. -0.05 min

Lab File: BF086155.D

Acq: 8 Apr 2016 3:13


Tgt Ion:188 Resp: 386636

Ion Ratio Lower Upper

188 100

94 10.0 5.4 8.0#



80 10.5 5.5 8.3#

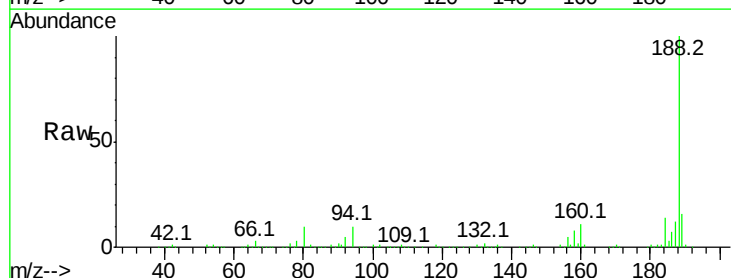


Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF0

Ion 80.00 (79.70 to 80.70): BF0

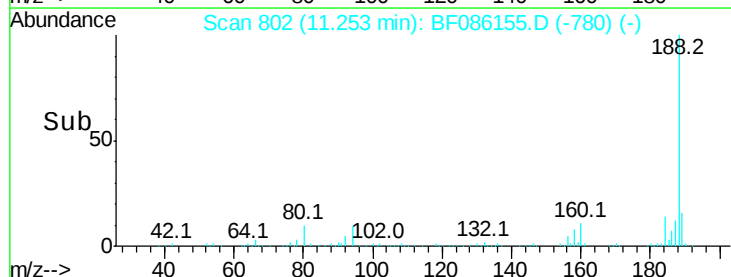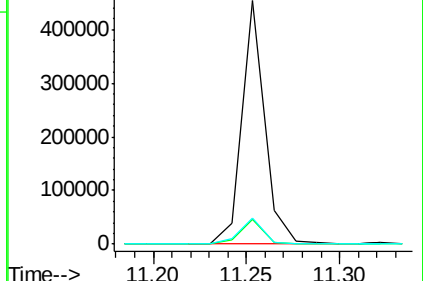

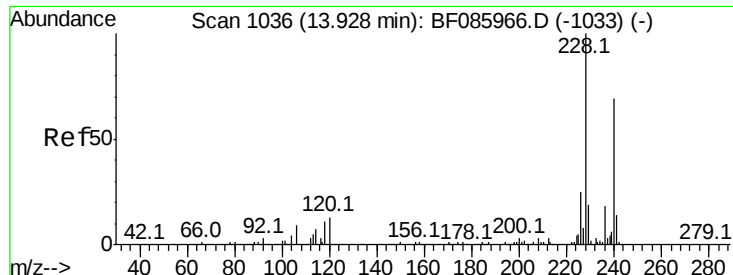

#75

Chrysene-d12

Concen: 20.00 ng

RT: 13.89 min Scan# 1033

Delta R.T. -0.03 min

Lab File: BF086155.D

Acq: 8 Apr 2016 3:13

Instrument :

BNA_F

ClientSampleId :

AMBOY-SB-37(0.5-15.0)


Tot Ion:240 Resp: 259803

Ion Ratio Lower Upper

240 100

120 8.4 13.8 20.8#




236 26.2 20.6 30.8

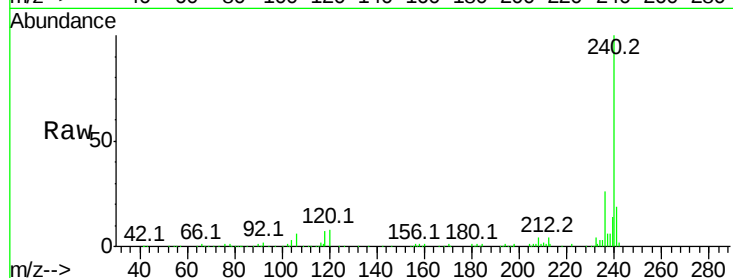

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

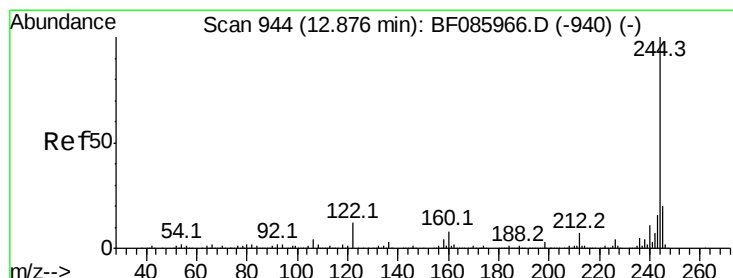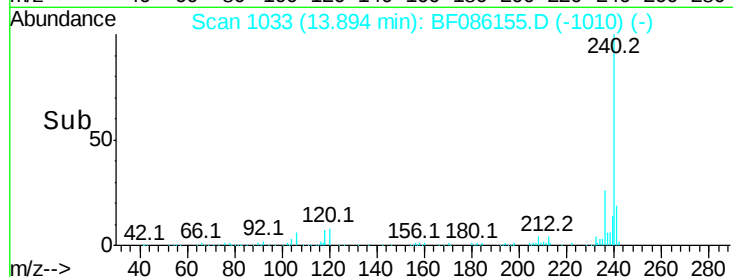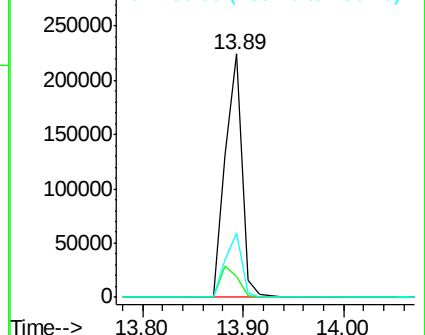

#78

Terphenyl-d14

Concen: 87.78 ng

RT: 12.84 min Scan# 941

Delta R.T. -0.03 min

Lab File: BF086155.D

Acq: 8 Apr 2016 3:13


Tgt Ion:244 Resp: 970131

Ion Ratio Lower Upper

244 100

212 7.0 6.1 9.1



122 9.7 10.2 15.4#

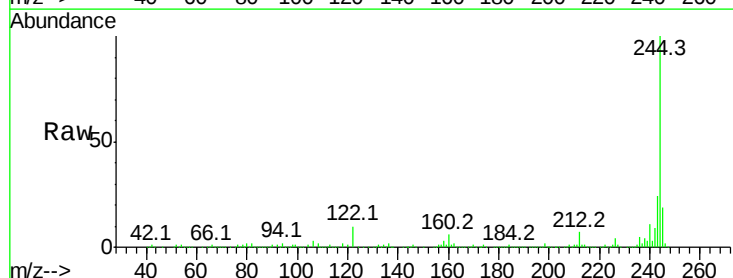


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

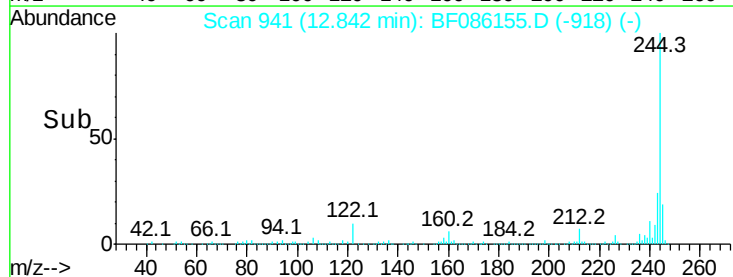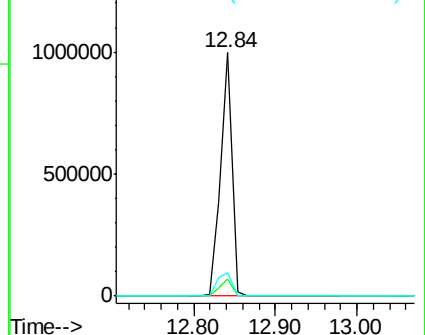


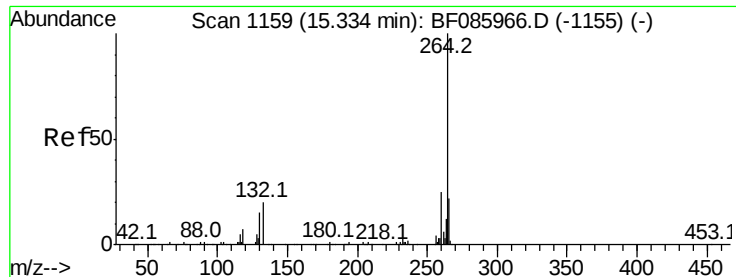

#86
Pervlene-d12
Concen: 20.00 ng
RT: 15.29 min Scan# 1155
Delta R.T. -0.05 min
Lab File: BF086155.D
Acq: 8 Apr 2016 3:13

Instrument :
BNA_F
ClientSampleId :
AMBOY-SB-37(0.5-15.0)

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.0	19.4	29.2
265	21.2	17.2	25.8

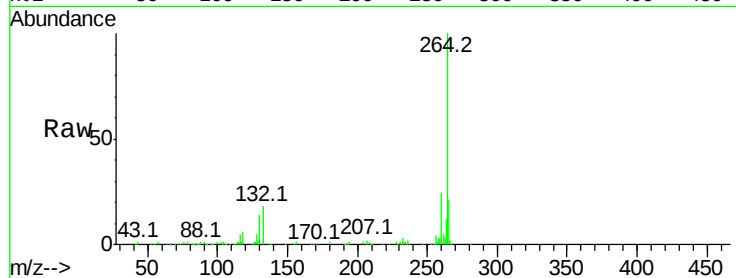

Abundance

Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

