


Data Path : Z:\HPCHEM1\BNA F\Data\BF040716\
 Data File : BF086124.D
 Acq On : 7 Apr 2016 11:27
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF040216.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Apr 01 23:17:06 2016

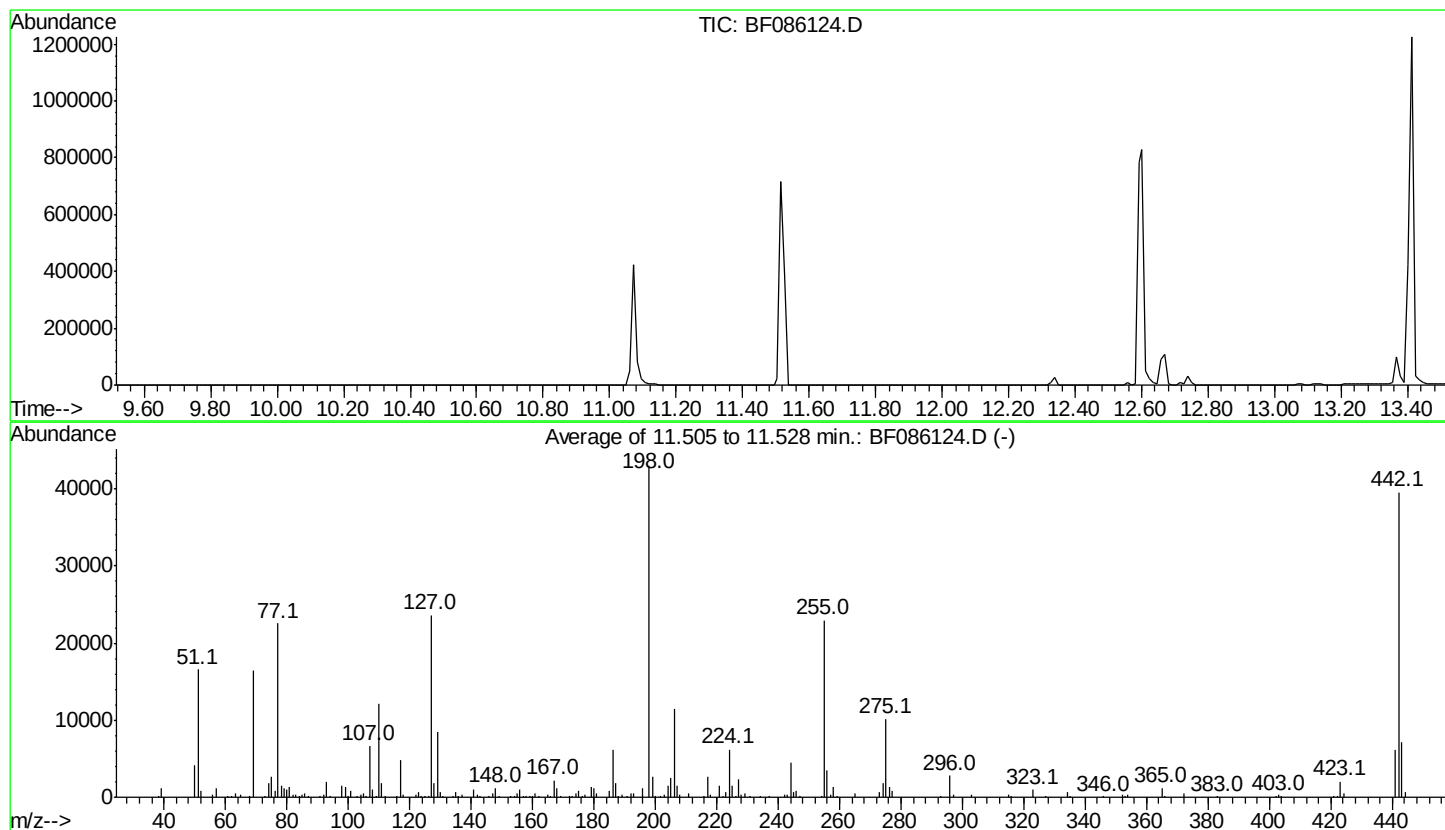

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.6	16587	PASS
68	69	0.00	2	1.4	237	PASS
69	198	0.00	100	38.1	16368	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	54.9	23617	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	43016	PASS
199	198	5	9	6.4	2745	PASS
275	198	10	60	23.6	10170	PASS
365	198	1	100	2.8	1193	PASS
441	442	0.01	24	15.5	6132	PASS
442	198	50	100	92.0	39570	PASS
443	442	15	24	18.2	7197	PASS