


Data Path : Z:\HPCHEM1\BNA F\DATA\BF040716\  
Data File : BF086146.D  
Acq On : 7 Apr 2016 22:57  
Operator : UM/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA\_F\METHODS\8270-BF040216.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Fri Apr 01 23:17:06 2016

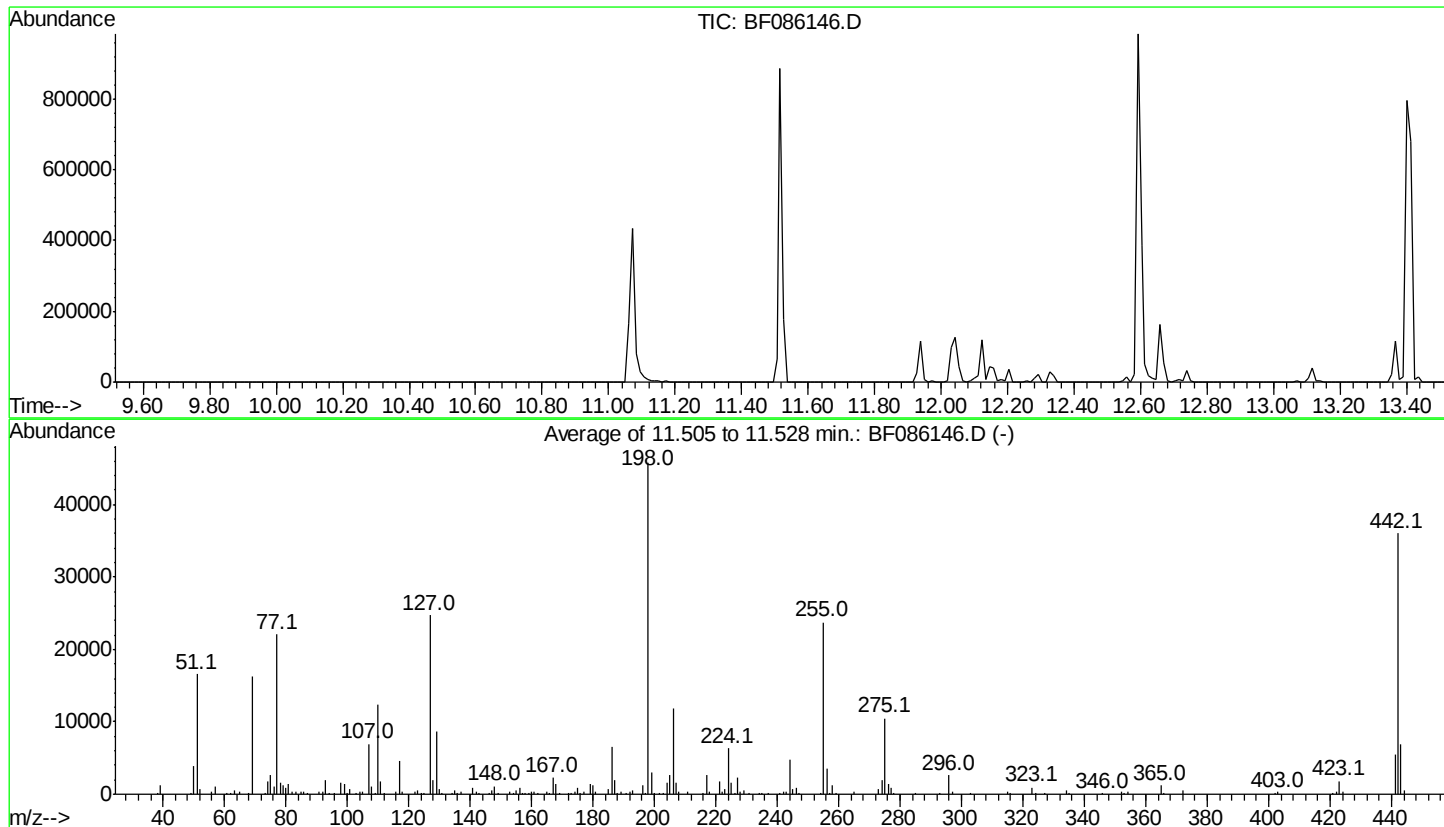

AutoFind: Scans 824, 825, 826; Background Corrected with Scan 821

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 36.2         | 16571      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.3          | 210        | PASS                |
| 69             | 198             | 0.00            | 100             | 35.6         | 16318      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.0          | 0          | PASS                |
| 127            | 198             | 10              | 80              | 54.0         | 24753      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.6          | 263        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 45804      | PASS                |
| 199            | 198             | 5               | 9               | 6.5          | 2997       | PASS                |
| 275            | 198             | 10              | 60              | 22.9         | 10498      | PASS                |
| 365            | 198             | 1               | 100             | 2.7          | 1222       | PASS                |
| 441            | 442             | 0.01            | 24              | 15.2         | 5476       | PASS                |
| 442            | 198             | 50              | 100             | 78.6         | 35989      | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 6918       | PASS                |