
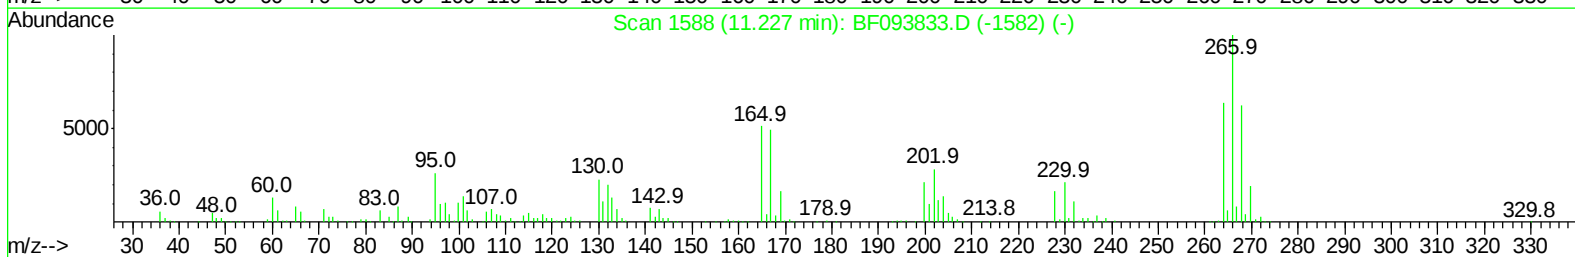
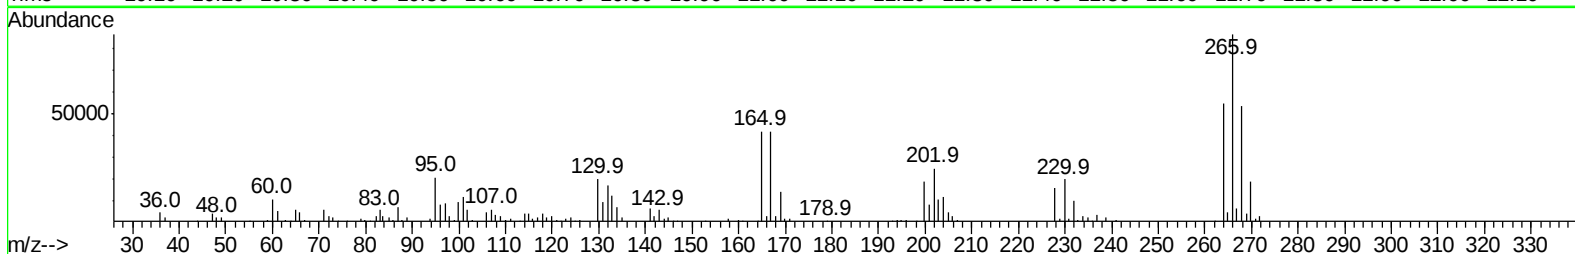


Data Path : Z:\HPCHEM1\BNA F\Data\BF040717\
Data File : BF094266.D
Acq On : 7 Apr 2017 11:54
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 07:21:44 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 13:20:29 2017
Response via : Initial Calibration

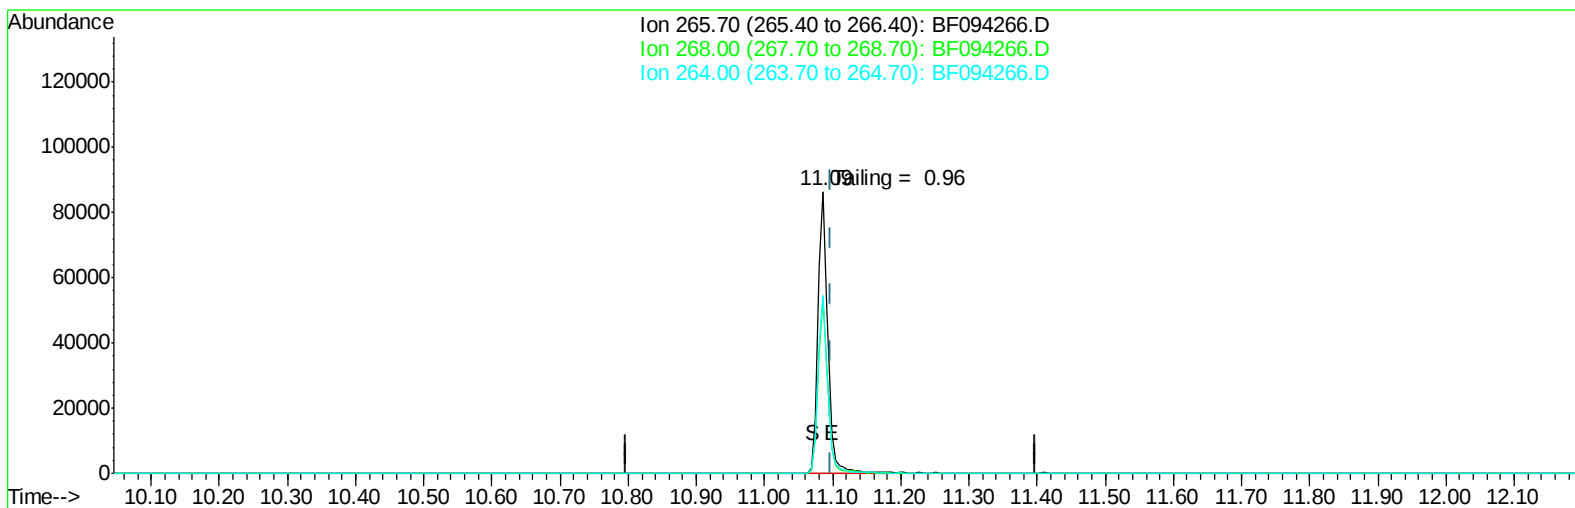

TIC: BF094266.D

(69) Pentachlorophenol (C)




11.086min (-0.012) 0.00ng

response 86833

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.07
264.00	64.60	63.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF040717\
Data File : BF094266.D
Acq On : 7 Apr 2017 11:54
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Apr 10 07:21:44 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Apr 06 13:20:29 2017
Response via : Initial Calibration

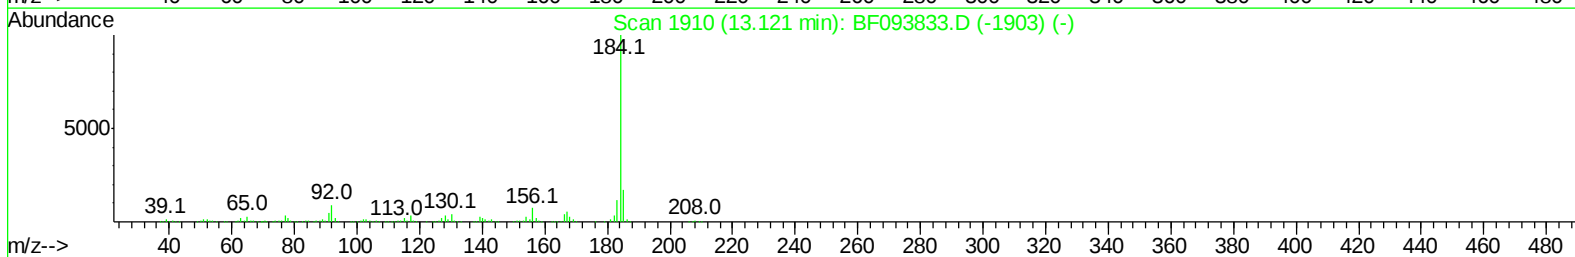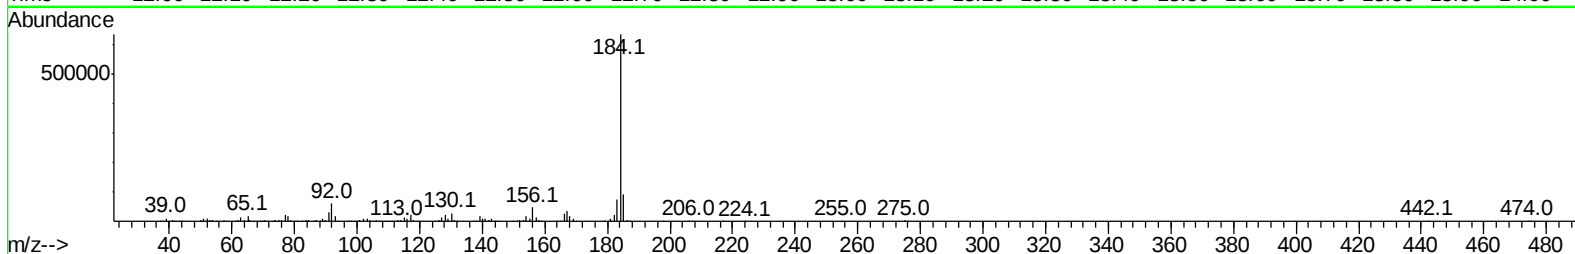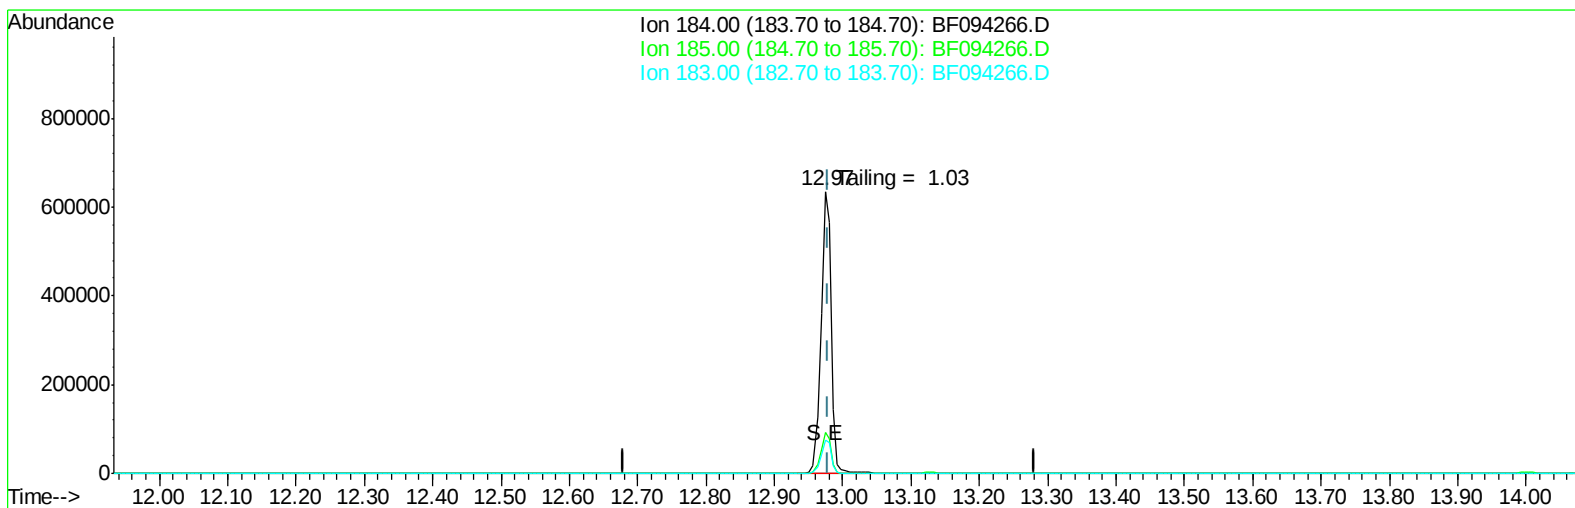

TIC: BF094266.D

(76) Benzidine

12.974min (-0.006) 148074.07ng

response 673959

Ion	Exp%	Act%
184.00	100	100
185.00	19.40	14.48#
183.00	12.20	11.78
0.00	0.00	0.00